

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
 Data File : BG047476.D
 Acq On : 27 Nov 2020 11:08
 Operator : CG/JU
 Sample : PB133234BL
 Misc : MDL-WATER-BL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.438	15	17	18	rBV2	2830	2246	0.16%	0.017%
2	3.526	30	32	33	rBV2	2789	2622	0.19%	0.020%
3	3.609	41	46	50	rBV3	8992	14820	1.08%	0.114%
4	3.673	55	57	58	rBV2	2949	2068	0.15%	0.016%
5	3.844	83	86	87	rBV2	2709	2623	0.19%	0.020%
6	4.032	116	118	133	rBV	127387	229013	16.70%	1.758%
7	4.378	175	177	181	rVB5	4544	4501	0.33%	0.035%
8	4.649	220	223	224	rBV2	2976	2801	0.20%	0.022%
9	4.860	256	259	260	rBV2	3048	2223	0.16%	0.017%
10	4.907	263	267	268	rBV	1732	1939	0.14%	0.015%
11	5.036	286	289	291	rVB2	1896	1994	0.15%	0.015%
12	5.571	378	380	383	rVB2	1983	1873	0.14%	0.014%
13	5.700	400	402	405	rVB2	2054	2119	0.15%	0.016%
14	5.724	405	406	409	rBV2	2152	2036	0.15%	0.016%
15	5.947	441	444	447	rVB2	1556	1821	0.13%	0.014%
16	6.082	466	467	472	rVB	1851	2082	0.15%	0.016%
17	6.229	489	492	493	rBV	2802	1869	0.14%	0.014%
18	6.934	609	612	614	rVB	1708	1828	0.13%	0.014%
19	6.958	614	616	618	rBV	1664	1980	0.14%	0.015%
20	7.398	685	691	702	rVB2	203466	358523	26.14%	2.753%
21	7.580	715	722	729	rVV	122217	211723	15.44%	1.626%
22	7.639	729	732	734	rVB	2260	2018	0.15%	0.015%
23	7.792	750	758	767	rBV2	206900	366821	26.75%	2.816%
24	8.268	829	839	847	rBV	119811	209584	15.28%	1.609%
25	8.897	945	946	949	rBV	2020	1895	0.14%	0.015%
26	8.955	949	956	968	rVV	243482	431338	31.45%	3.312%
27	9.431	1028	1037	1047	rBV	194703	366387	26.71%	2.813%
28	10.160	1154	1161	1170	rBV2	192578	346446	25.26%	2.660%
29	10.700	1246	1253	1260	rBV	261804	482420	35.17%	3.704%
30	11.094	1313	1320	1330	rVB	153604	274151	19.99%	2.105%
31	11.217	1334	1341	1352	rVB	239864	436382	31.82%	3.351%
32	11.576	1399	1402	1404	rBV	1734	2080	0.15%	0.016%
33	12.669	1580	1588	1589	rBV2	4541	7823	0.57%	0.060%
34	13.603	1745	1747	1751	rBV	2170	2372	0.17%	0.018%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
 Data File : BG047476.D
 Acq On : 27 Nov 2020 11:08
 Operator : CG/JU
 Sample : PB133234BL
 Misc : MDL-WATER-BL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	13.820	1781	1784	1788	rVB	1624	2094	0.15%	0.016%
36	13.885	1793	1795	1798	rVB	1902	1933	0.14%	0.015%
37	14.273	1853	1861	1867	rBV	524874	767227	55.94%	5.891%
38	14.578	1906	1913	1920	rBV	493937	778428	56.76%	5.977%
39	14.643	1922	1924	1929	rVB	2180	2289	0.17%	0.018%
40	14.754	1942	1943	1948	rVB	1862	2347	0.17%	0.018%
41	14.813	1952	1953	1957	rBV	2668	2039	0.15%	0.016%
42	14.878	1957	1964	1973	rVB3	240503	402132	29.32%	3.088%
43	15.042	1984	1992	2005	rBV	236105	420948	30.69%	3.232%
44	15.224	2021	2023	2025	rVB2	4219	2817	0.21%	0.022%
45	15.242	2025	2026	2029	rBV2	2380	2349	0.17%	0.018%
46	15.266	2029	2030	2037	rVB	2299	2773	0.20%	0.021%
47	15.424	2055	2057	2060	rBV	2285	2559	0.19%	0.020%
48	15.565	2079	2081	2085	rBV	1899	2773	0.20%	0.021%
49	15.642	2092	2094	2098	rVB	1858	2100	0.15%	0.016%
50	15.865	2124	2132	2139	rBV	637047	974641	71.06%	7.483%
51	15.965	2143	2149	2159	rBV2	196619	301560	21.99%	2.315%
52	16.100	2168	2172	2179	rVB4	7883	14162	1.03%	0.109%
53	16.358	2213	2216	2218	rBV	2025	1966	0.14%	0.015%
54	16.646	2260	2265	2267	rBV2	5135	6302	0.46%	0.048%
55	17.234	2362	2365	2369	rBV	2388	2791	0.20%	0.021%
56	17.293	2371	2375	2379	rVB	2149	3750	0.27%	0.029%
57	17.398	2390	2393	2395	rBV3	2601	2071	0.15%	0.016%
58	17.533	2411	2416	2417	rBV	2508	2649	0.19%	0.020%
59	17.616	2421	2430	2440	rVV	348436	547347	39.91%	4.202%
60	17.716	2440	2447	2457	rVV2	710903	1124051	81.96%	8.630%
61	17.939	2480	2485	2488	rBV2	2078	3190	0.23%	0.024%
62	17.974	2488	2491	2496	rVV	2036	3028	0.22%	0.023%
63	18.156	2518	2522	2524	rVB	2168	2634	0.19%	0.020%
64	18.233	2530	2535	2538	rBV	1870	3505	0.26%	0.027%
65	18.280	2541	2543	2546	rVB3	1781	1991	0.15%	0.015%
66	18.509	2580	2582	2584	rVB3	3499	2396	0.17%	0.018%
67	18.532	2584	2586	2588	rBV	2552	2026	0.15%	0.016%
68	18.632	2600	2603	2604	rBV	2313	2032	0.15%	0.016%
69	18.714	2615	2617	2619	rBV2	3079	3066	0.22%	0.024%
70	18.832	2634	2637	2638	rBV3	2791	3181	0.23%	0.024%
71	18.961	2656	2659	2662	rBV2	2445	2998	0.22%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
 Data File : BG047476.D
 Acq On : 27 Nov 2020 11:08
 Operator : CG/JU
 Sample : PB133234BL
 Misc : MDL-WATER-BL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

72	19.231	2703	2705	2706	rBV2	3213	1872	0.14%	0.014%
73	19.361	2725	2727	2730	rVB	3310	2318	0.17%	0.018%
74	19.425	2736	2738	2739	rBV2	2797	2620	0.19%	0.020%
75	19.467	2742	2745	2747	rVV2	3217	3787	0.28%	0.029%
76	19.578	2762	2764	2767	rBV3	2909	3693	0.27%	0.028%
77	19.625	2767	2772	2776	rVV4	8980	14111	1.03%	0.108%
78	19.690	2779	2783	2784	rBV3	3398	4593	0.33%	0.035%
79	19.843	2807	2809	2810	rBV	3799	1886	0.14%	0.014%
80	19.866	2810	2813	2820	rVB3	10592	16490	1.20%	0.127%
81	19.978	2822	2832	2840	rBV	951596	1371539	100.00%	10.531%
82	20.195	2867	2869	2871	rBV3	3527	3290	0.24%	0.025%
83	20.307	2886	2888	2890	rVB2	4514	2497	0.18%	0.019%
84	20.342	2892	2894	2895	rBV2	4037	2946	0.21%	0.023%
85	21.893	3152	3158	3167	rVB	340614	610116	44.48%	4.684%
86	25.066	3688	3698	3713	rVB2	436533	1254779	91.49%	9.634%
87	25.295	3728	3737	3749	rBV	176407	539262	39.32%	4.140%


Sum of corrected areas: 13024365

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
Data File : BG047476.D
Acq On : 27 Nov 2020 11:08
Operator : CG/JU
Sample : PB133234BL
Misc : MDL-WATER-BL-04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK234

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

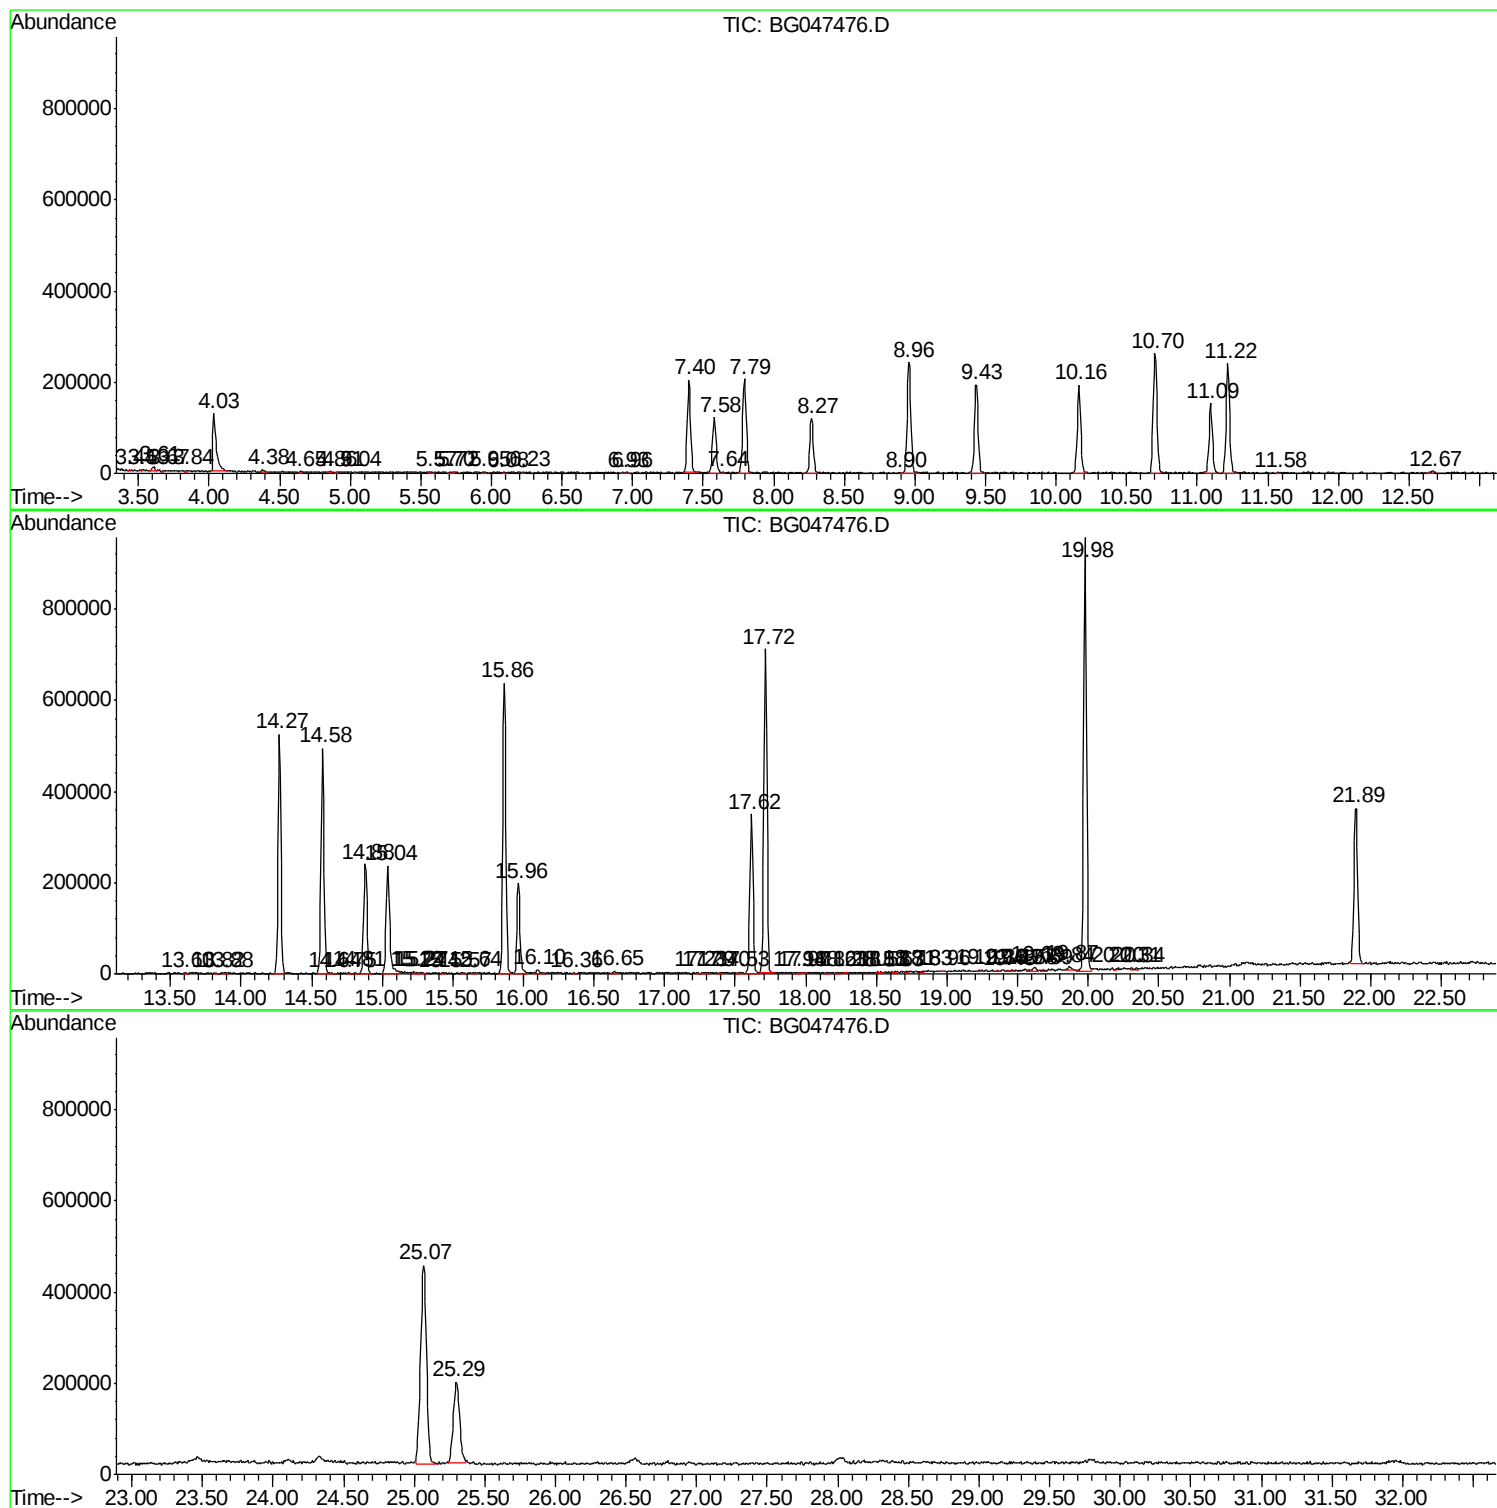

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112720\
Data_File : BG047476.D
Acq_On : 27 Nov 2020 11:088
Operator : CG/JUU
Sample : PB133234BLL
Misc : MDL-WATER-BL-044
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK234

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
