

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
 Data File : BG047478.D
 Acq On : 27 Nov 2020 12:44
 Operator : CG/JU
 Sample : PB133234BL
 Misc : MDL-WATER-BL-05
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.609	43	46	54	rVB5	8496	15315	1.04%	0.111%
2	4.037	115	119	131	rBV	129677	236842	16.15%	1.716%
3	4.390	174	179	184	rVB2	5004	7504	0.51%	0.054%
4	4.472	190	193	197	rBV	1631	2628	0.18%	0.019%
5	4.578	207	211	214	rVB2	1841	2296	0.16%	0.017%
6	4.707	231	233	236	rBV	2043	2265	0.15%	0.016%
7	5.242	322	324	328	rBV	1953	3286	0.22%	0.024%
8	6.658	560	565	566	rBV	1621	2284	0.16%	0.017%
9	6.693	569	571	576	rVB	2528	2733	0.19%	0.020%
10	7.210	657	659	663	rBV	1926	3207	0.22%	0.023%
11	7.281	667	671	675	rBV	1337	2433	0.17%	0.018%
12	7.398	684	691	701	rBV	208880	383247	26.13%	2.777%
13	7.580	715	722	731	rBV	125204	216725	14.77%	1.570%
14	7.792	751	758	766	rBV2	222970	380065	25.91%	2.754%
15	8.268	833	839	845	rBV	127752	224811	15.33%	1.629%
16	8.697	907	912	915	rBV	1631	2400	0.16%	0.017%
17	8.955	949	956	970	rVB	248352	439618	29.97%	3.185%
18	9.290	1010	1013	1016	rVB	1917	2028	0.14%	0.015%
19	9.437	1030	1038	1046	rVB	210618	383079	26.12%	2.776%
20	10.160	1153	1161	1169	rBV	197584	365147	24.89%	2.646%
21	10.336	1188	1191	1194	rVB	1723	2067	0.14%	0.015%
22	10.589	1230	1234	1235	rBV	2109	2017	0.14%	0.015%
23	10.700	1245	1253	1265	rBV2	273421	502967	34.29%	3.644%
24	11.094	1312	1320	1327	rBV	153134	284132	19.37%	2.059%
25	11.217	1333	1341	1348	rBV	237655	444502	30.30%	3.221%
26	12.657	1580	1586	1590	rBV	6200	8895	0.61%	0.064%
27	13.238	1681	1685	1686	rVB	1808	2069	0.14%	0.015%
28	13.914	1798	1800	1804	rVB	2128	2372	0.16%	0.017%
29	14.273	1855	1861	1869	rVB	543852	790185	53.87%	5.725%
30	14.578	1902	1913	1919	rBV	485436	802227	54.69%	5.813%
31	14.878	1957	1964	1972	rBV2	243317	399263	27.22%	2.893%
32	15.042	1984	1992	2004	rBV	266149	449059	30.61%	3.254%
33	15.600	2085	2087	2093	rVB	2303	2937	0.20%	0.021%
34	15.865	2125	2132	2139	rBV	651906	1012552	69.03%	7.337%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
 Data File : BG047478.D
 Acq On : 27 Nov 2020 12:44
 Operator : CG/JU
 Sample : PB133234BL
 Misc : MDL-WATER-BL-05
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	15.965	2143	2149	2156	rBV2	231505	337745	23.02%	2.447%
36	16.100	2169	2172	2178	rVB2	8858	14269	0.97%	0.103%
37	16.229	2190	2194	2197	rBV2	1777	3267	0.22%	0.024%
38	16.634	2260	2263	2265	rBV	2832	3768	0.26%	0.027%
39	17.104	2340	2343	2347	rVB	2122	2828	0.19%	0.020%
40	17.398	2390	2393	2395	rBV	2175	2133	0.15%	0.015%
41	17.616	2422	2430	2437	rBV	362499	567773	38.71%	4.114%
42	17.710	2440	2446	2456	rVB2	735799	1186676	80.90%	8.598%
43	17.862	2471	2472	2476	rBV	2208	2624	0.18%	0.019%
44	17.898	2476	2478	2481	rVB	2031	2139	0.15%	0.015%
45	18.062	2502	2506	2508	rBV	1853	2324	0.16%	0.017%
46	18.221	2531	2533	2535	rBV	2276	2408	0.16%	0.017%
47	18.303	2545	2547	2550	rVB2	2493	2627	0.18%	0.019%
48	18.920	2650	2652	2654	rVB	3191	2076	0.14%	0.015%
49	19.108	2683	2684	2690	rBV	2118	3483	0.24%	0.025%
50	19.220	2702	2703	2706	rBV2	3051	2585	0.18%	0.019%
51	19.613	2766	2770	2775	rBV3	9948	14996	1.02%	0.109%
52	19.684	2779	2782	2783	rBV	2546	3113	0.21%	0.023%
53	19.772	2795	2797	2799	rBV2	2411	2142	0.15%	0.016%
54	19.872	2809	2814	2817	rBV5	9209	13951	0.95%	0.101%
55	19.978	2825	2832	2841	rBV	1036107	1466877	100.00%	10.628%
56	20.401	2902	2904	2907	rBV3	3214	2496	0.17%	0.018%
57	20.753	2962	2964	2966	rBV3	4712	3886	0.26%	0.028%
58	20.888	2985	2987	2988	rBV2	5361	4211	0.29%	0.031%
59	21.893	3152	3158	3165	rVB	387362	648924	44.24%	4.702%
60	22.081	3188	3190	3191	rBV2	7028	5052	0.34%	0.037%
61	24.325	3567	3572	3583	rVB6	32050	67041	4.57%	0.486%
62	25.060	3686	3697	3709	rVB	452742	1353626	92.28%	9.808%
63	25.295	3728	3737	3753	rVB2	190279	690731	47.09%	5.005%
64	32.081	4891	4892	4893	rBV	6023	2585	0.18%	0.019%


Sum of corrected areas: 13801513

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112720\
Data File : BG047478.D
Acq On : 27 Nov 2020 12:44
Operator : CG/JU
Sample : PB133234BL
Misc : MDL-WATER-BL-05
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK234

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

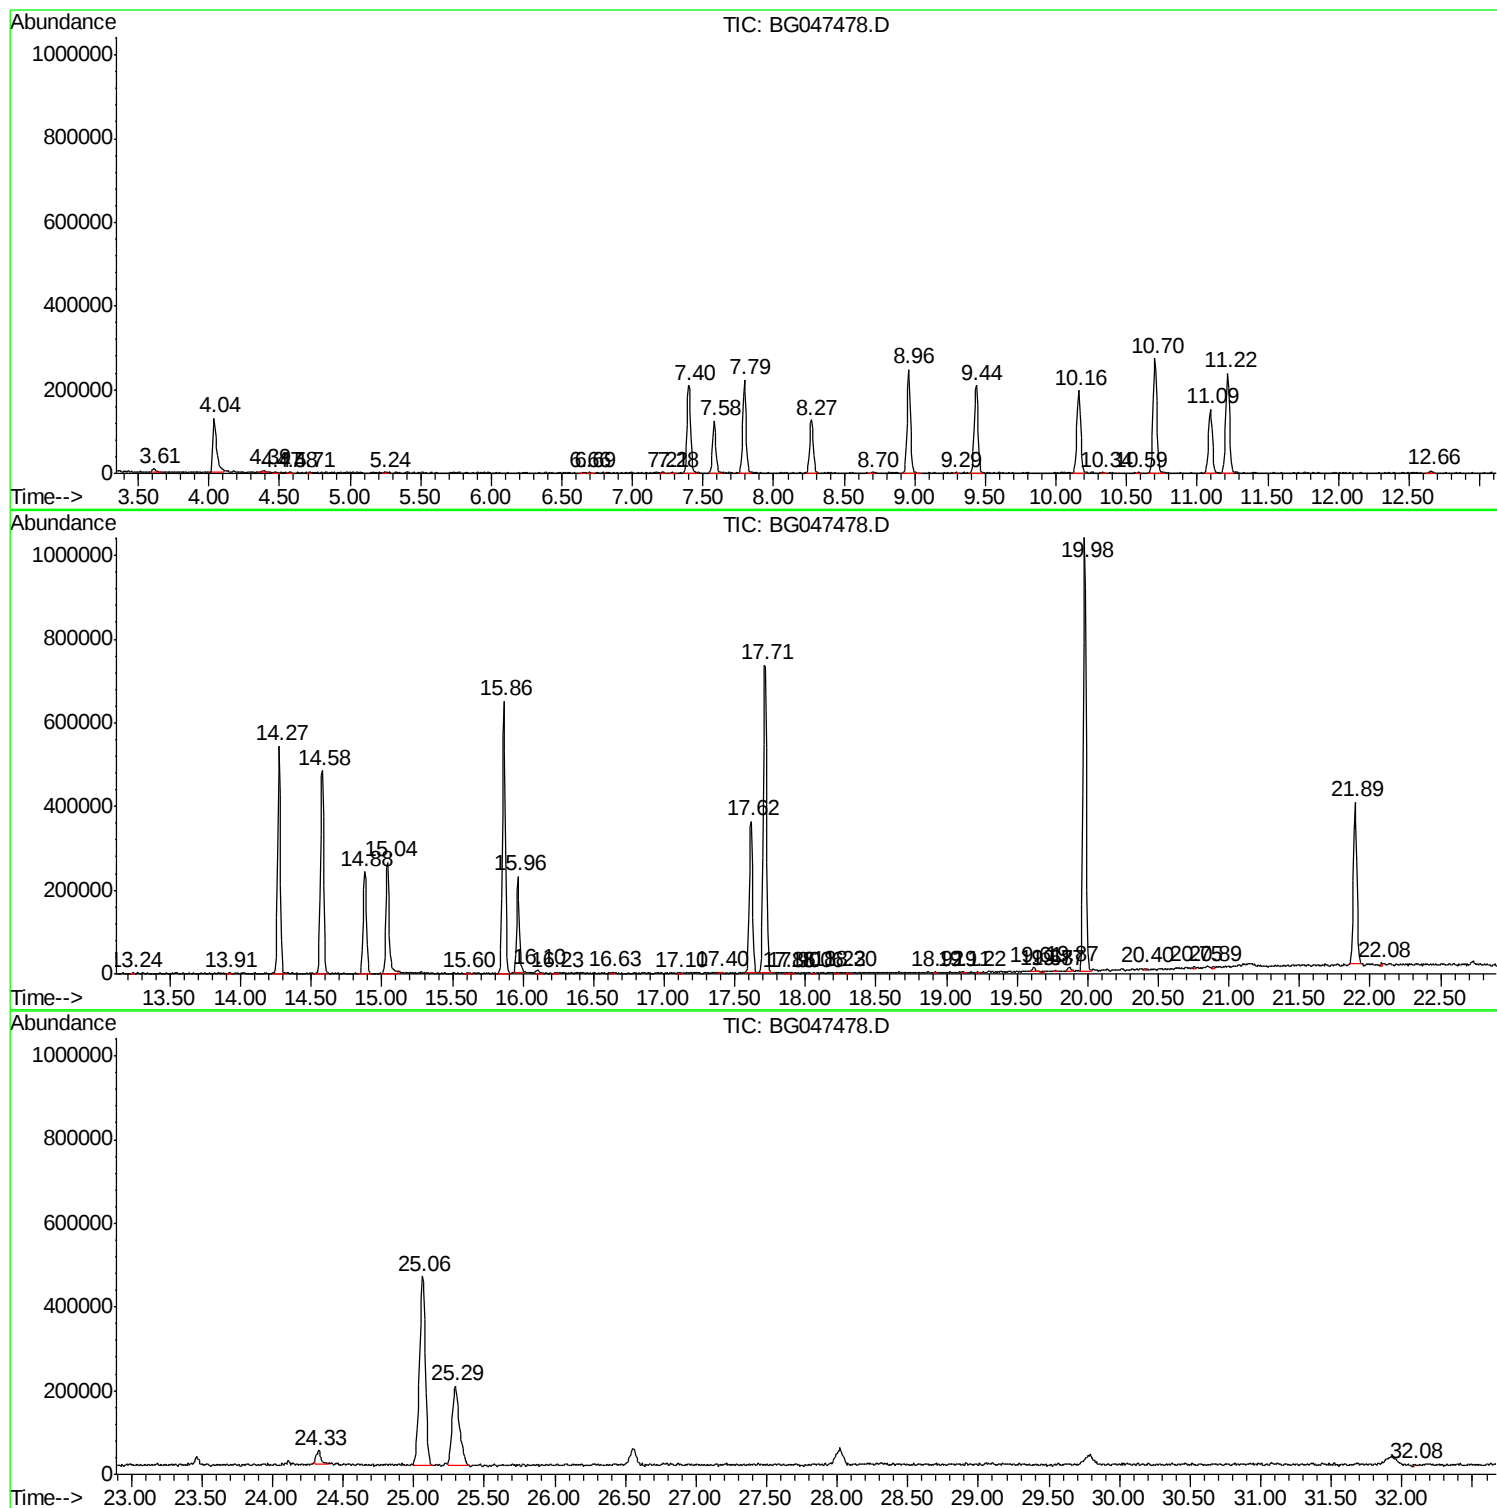

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112720\
Data_File : BG047478.D
Acq_On : 27 Nov 2020 12:444
Operator : CG/JUU
Sample : PB133234BLL
Misc : MDL-WATER-BL-055
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK234

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
