
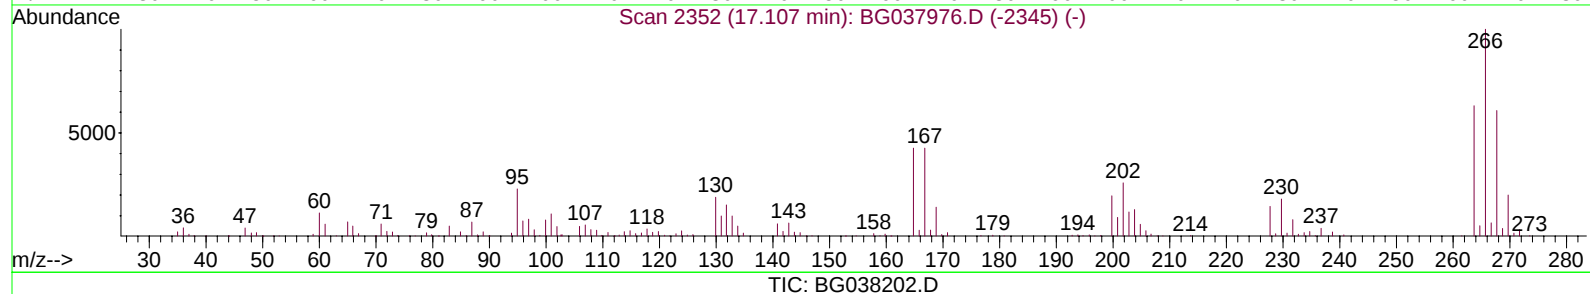
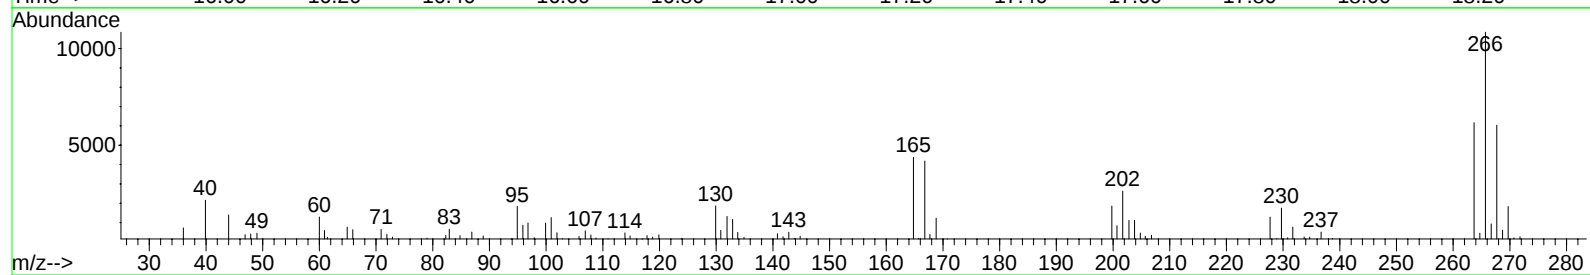


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112818\
Data File : BG038202.D
Acq On : 28 Nov 2018 16:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 18:16:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

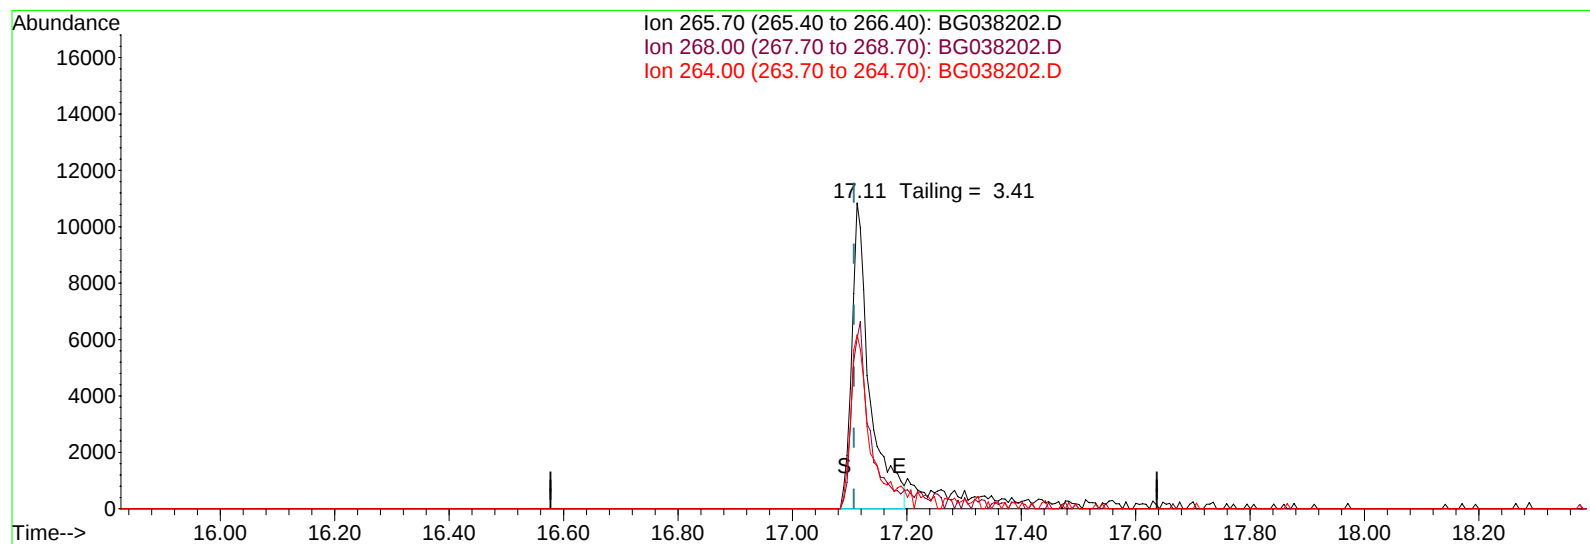

(70) Pentachlorophenol (C)




17.113min (+0.006) 23306.52ng

response 23851

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	61.32
264.00	73.60	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112818\
Data File : BG038202.D
Acq On : 28 Nov 2018 16:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 18:16:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

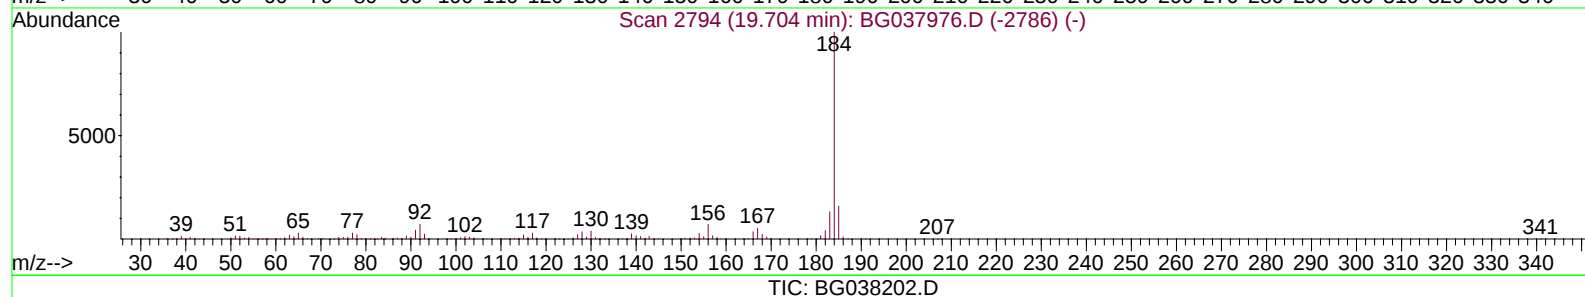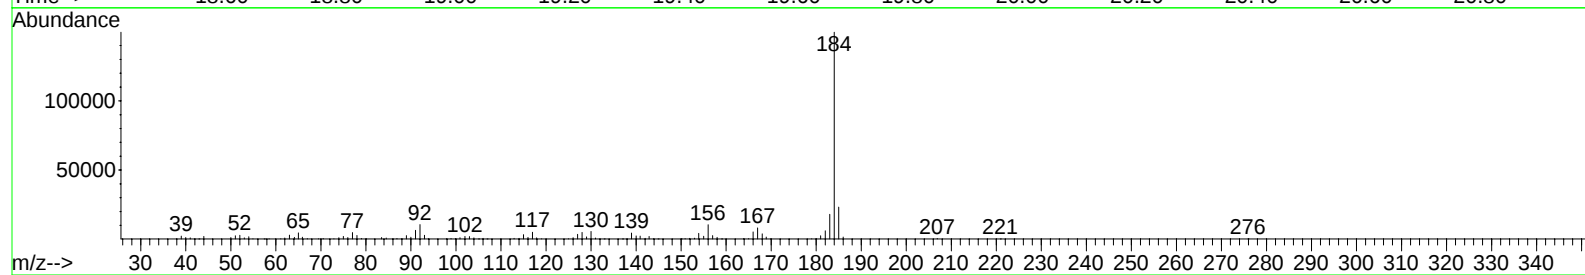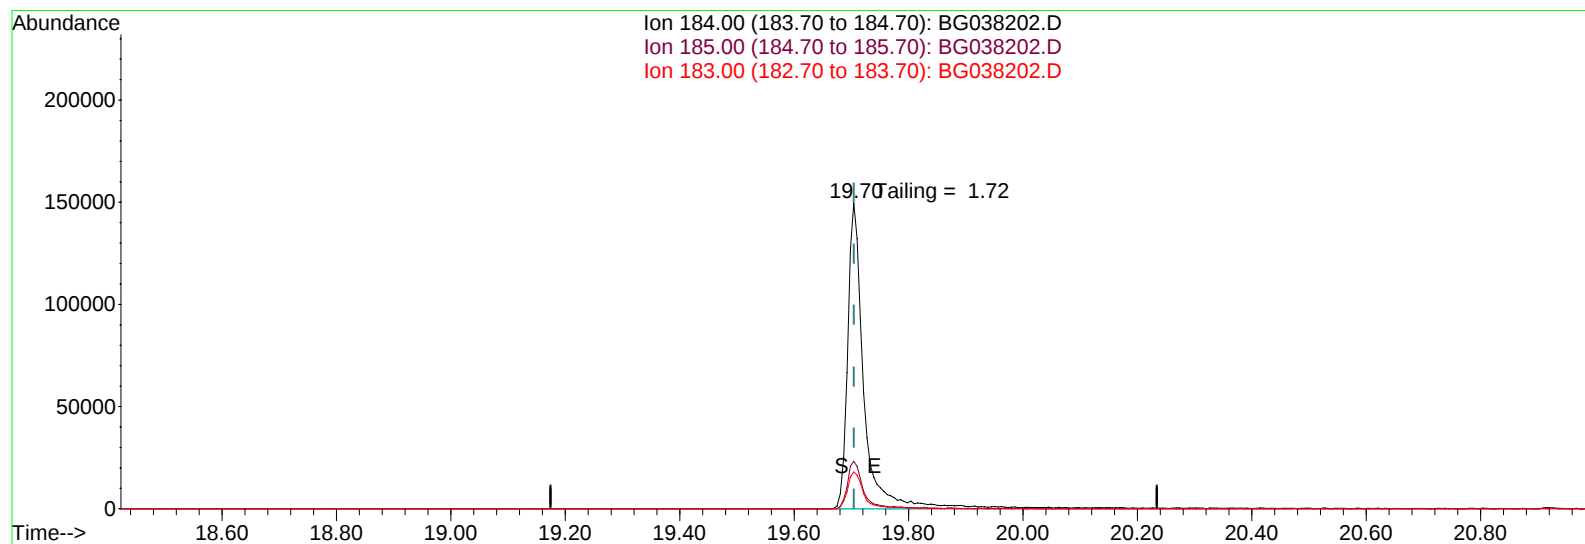

(77) Benzidine

19.704min (-0.000) 0.00ng

response 288239

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.52
183.00	12.70	12.06
0.00	0.00	0.00