
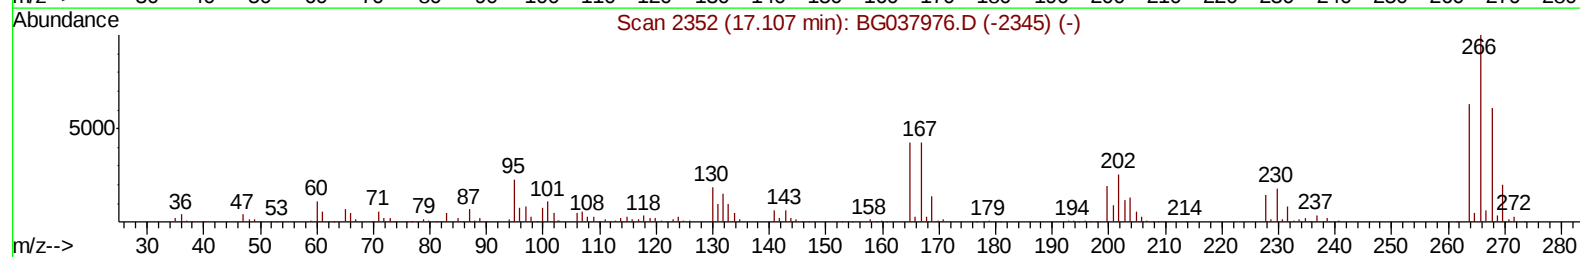
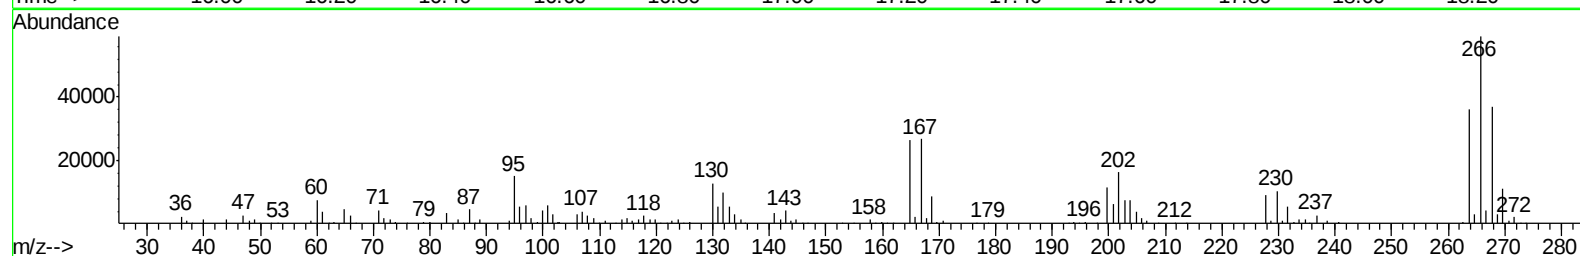


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112818\
Data File : BG038221.D
Acq On : 29 Nov 2018 5:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:19:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

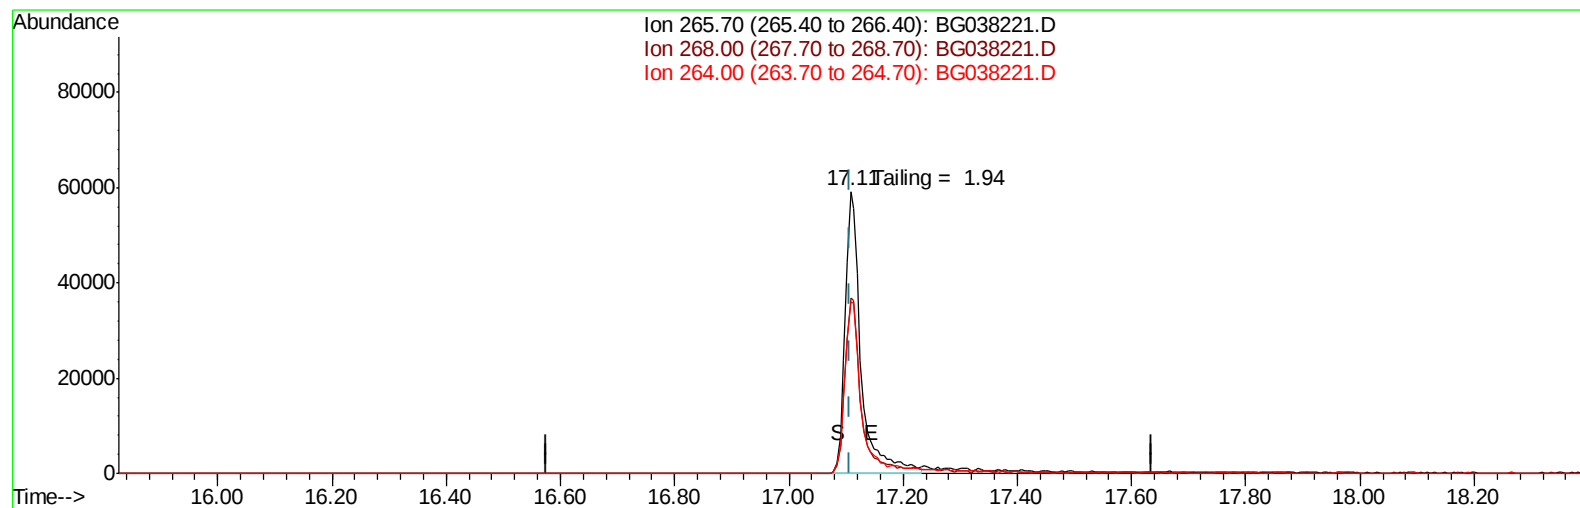

TIC: BG038221.D

(70) Pentachlorophenol (C)




17.108min (+0.000) 48869.38ng

response 115063

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.73
264.00	73.60	66.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112818\
Data File : BG038221.D
Acq On : 29 Nov 2018 5:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 07:19:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

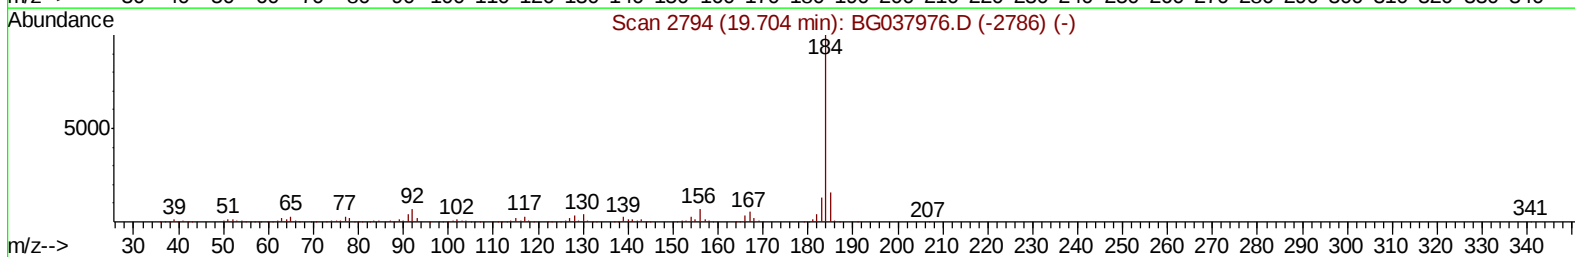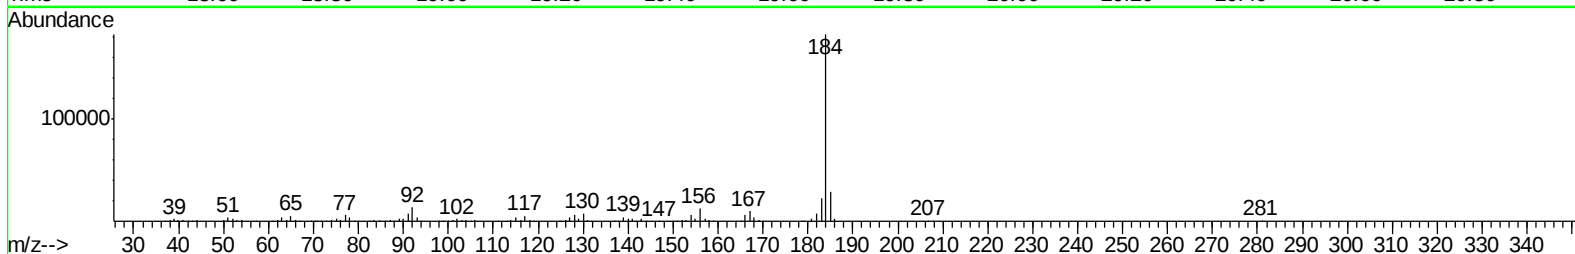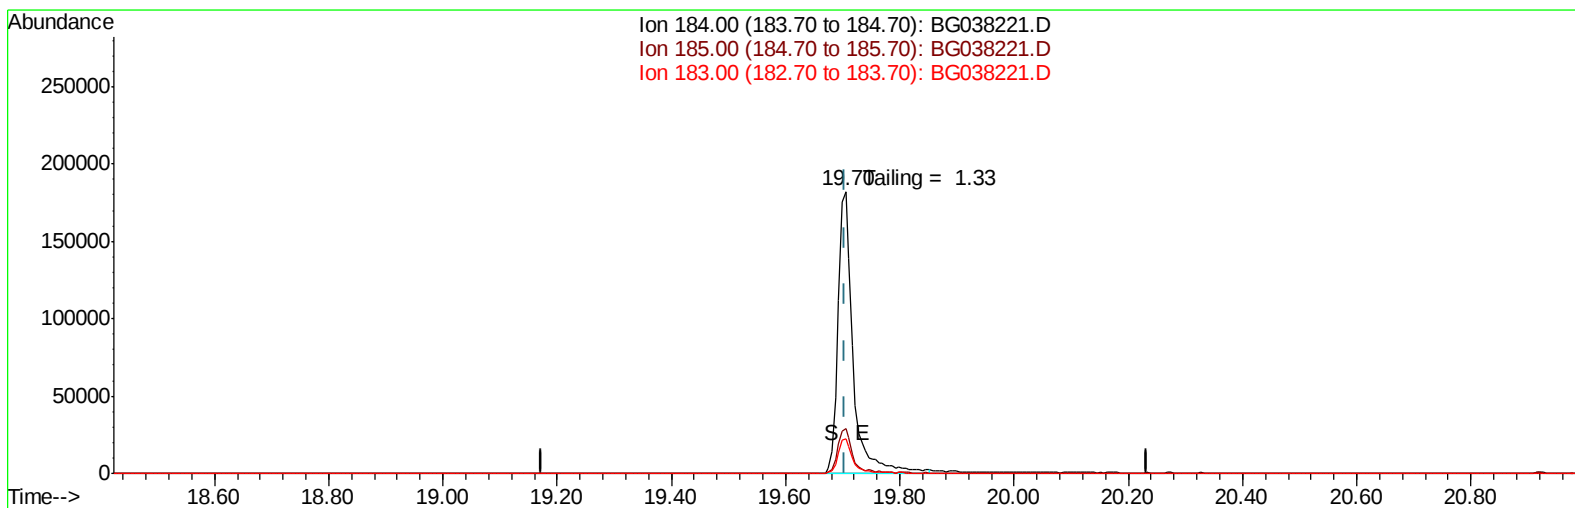

TIC: BG038221.D

(77) Benzidine

19.705min (+0.000) 0.00ng

response 332469

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.10
183.00	12.70	12.35
0.00	0.00	0.00