


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112818\
 Data File : BG038202.D
 Acq On : 28 Nov 2018 16:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

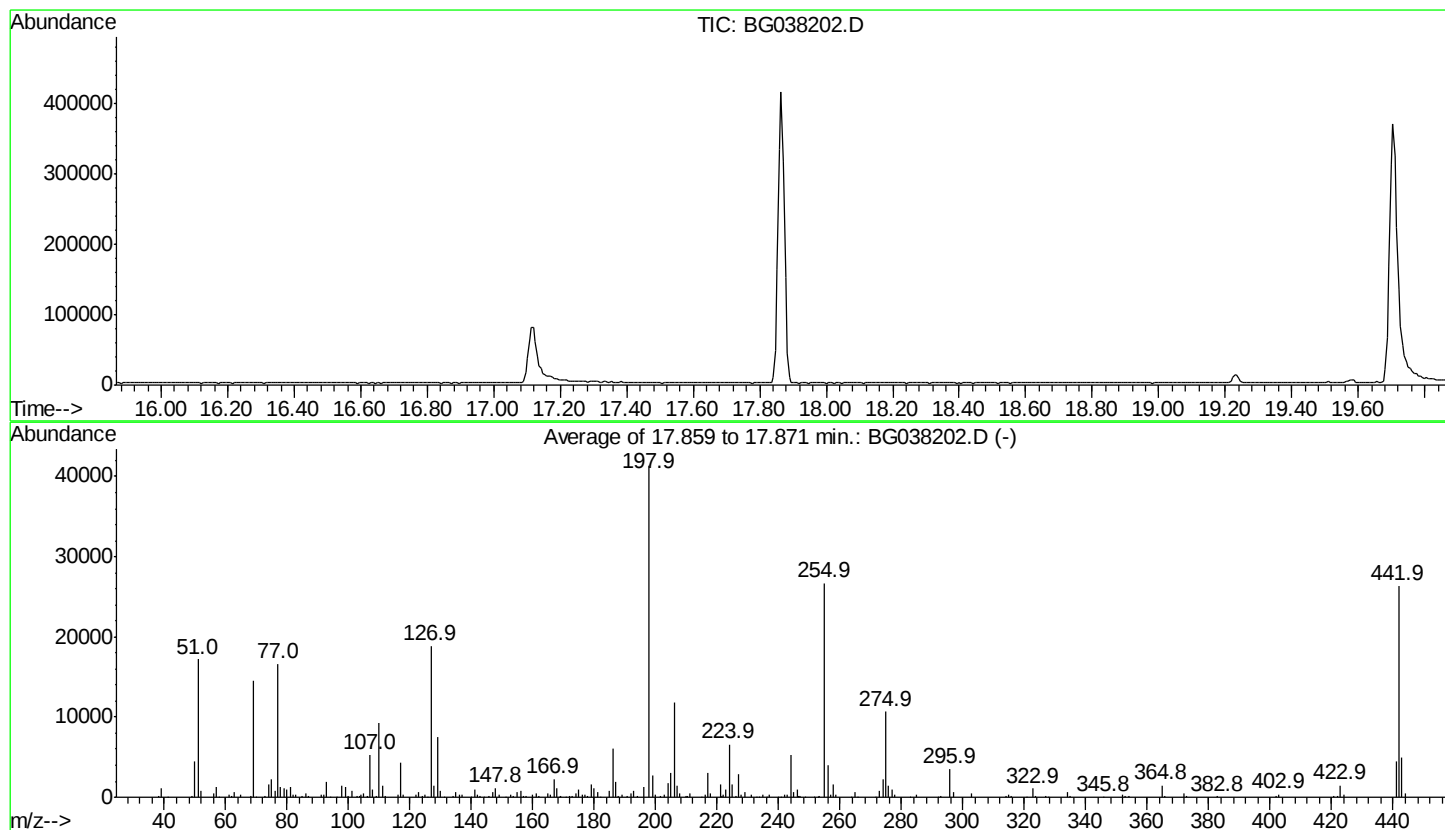

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	17221	PASS
68	69	0.00	2	0.9	126	PASS
69	198	0.00	100	35.1	14502	PASS
70	69	0.00	2	0.5	70	PASS
127	198	10	80	45.7	18900	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41354	PASS
199	198	5	9	6.4	2648	PASS
275	198	10	60	25.9	10693	PASS
365	198	1	100	3.5	1440	PASS
441	198	0.01	100	10.9	4518	PASS
442	198	50	100	63.9	26405	PASS
443	442	15	24	18.9	4996	PASS