


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112818\
 Data File : BG038221.D
 Acq On : 29 Nov 2018 5:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

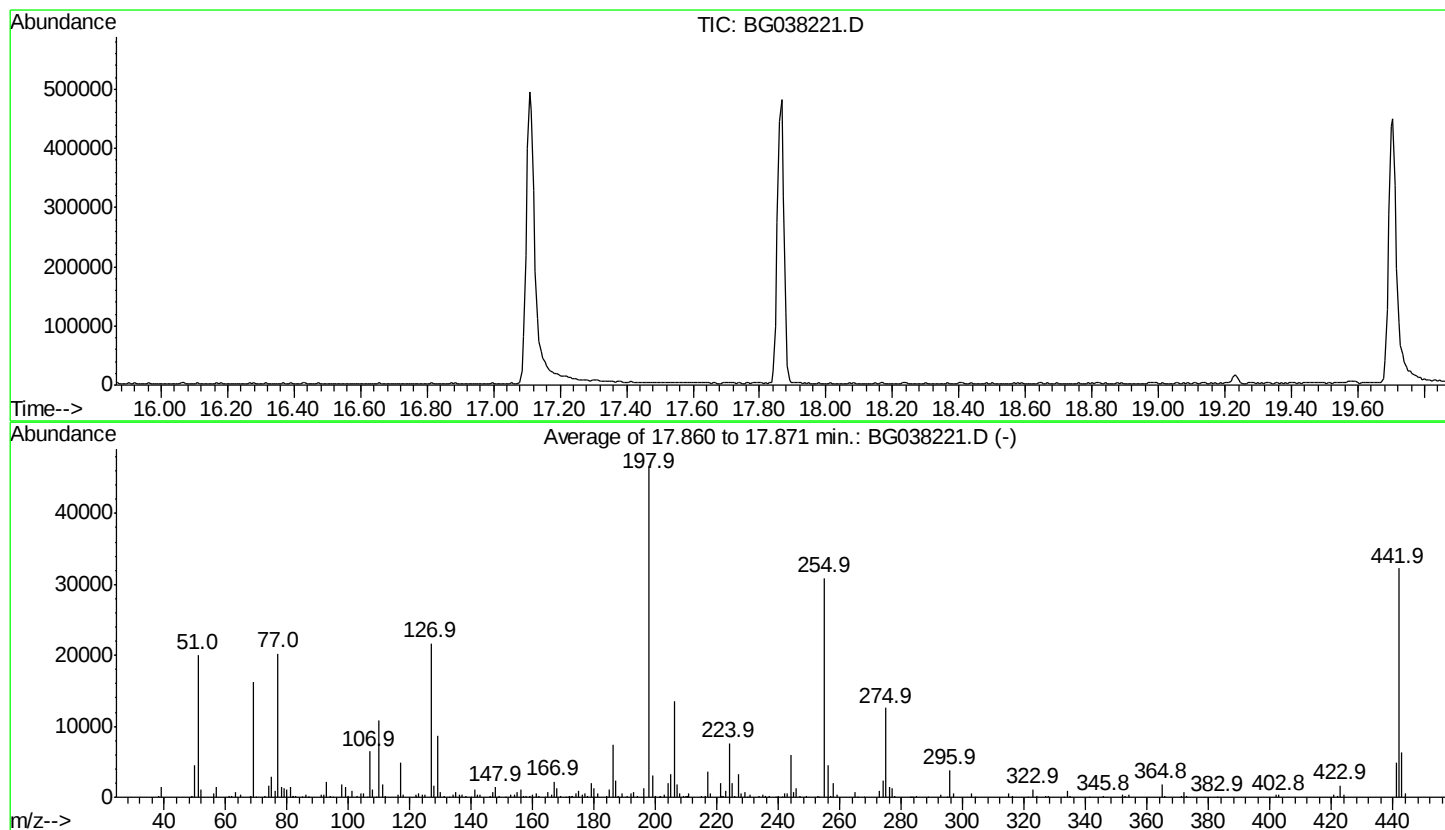

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	20082	PASS
68	69	0.00	2	0.8	123	PASS
69	198	0.00	100	34.8	16288	PASS
70	69	0.00	2	0.4	63	PASS
127	198	10	80	46.4	21689	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46749	PASS
199	198	5	9	6.4	3007	PASS
275	198	10	60	27.0	12627	PASS
365	198	1	100	4.0	1878	PASS
441	198	0.01	100	10.3	4812	PASS
442	198	50	100	69.1	32288	PASS
443	442	15	24	19.5	6292	PASS