

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
 Data File : BG031282.D
 Acq On : 29 Nov 2017 22:15
 Operator : SJ/JU
 Sample : I6306-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 30 03:09:47 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	51550	20.00	ng	-0.02
21) Naphthalene-d8	10.95	136	218082	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	149868	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	437373	20.00	ng	-0.02
75) Chrysene-d12	21.77	240	513026	20.00	ng	-0.02
86) Perylene-d12	25.06	264	489940	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	394503	131.23	ng	-0.02
7) Phenol-d6	7.29	99	462397	114.17	ng	-0.01
23) Nitrobenzene-d5	9.30	82	340195	92.44	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	318386	131.33	ng	-0.02
44) 2-Fluorobiphenyl	13.38	172	1044668	100.16	ng	-0.02
78) Terphenyl-d14	20.09	244	2185802	94.08	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
Data File : BG031282.D
Acq On : 29 Nov 2017 22:15
Operator : SJ/JU
Sample : I6306-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 30 03:09:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

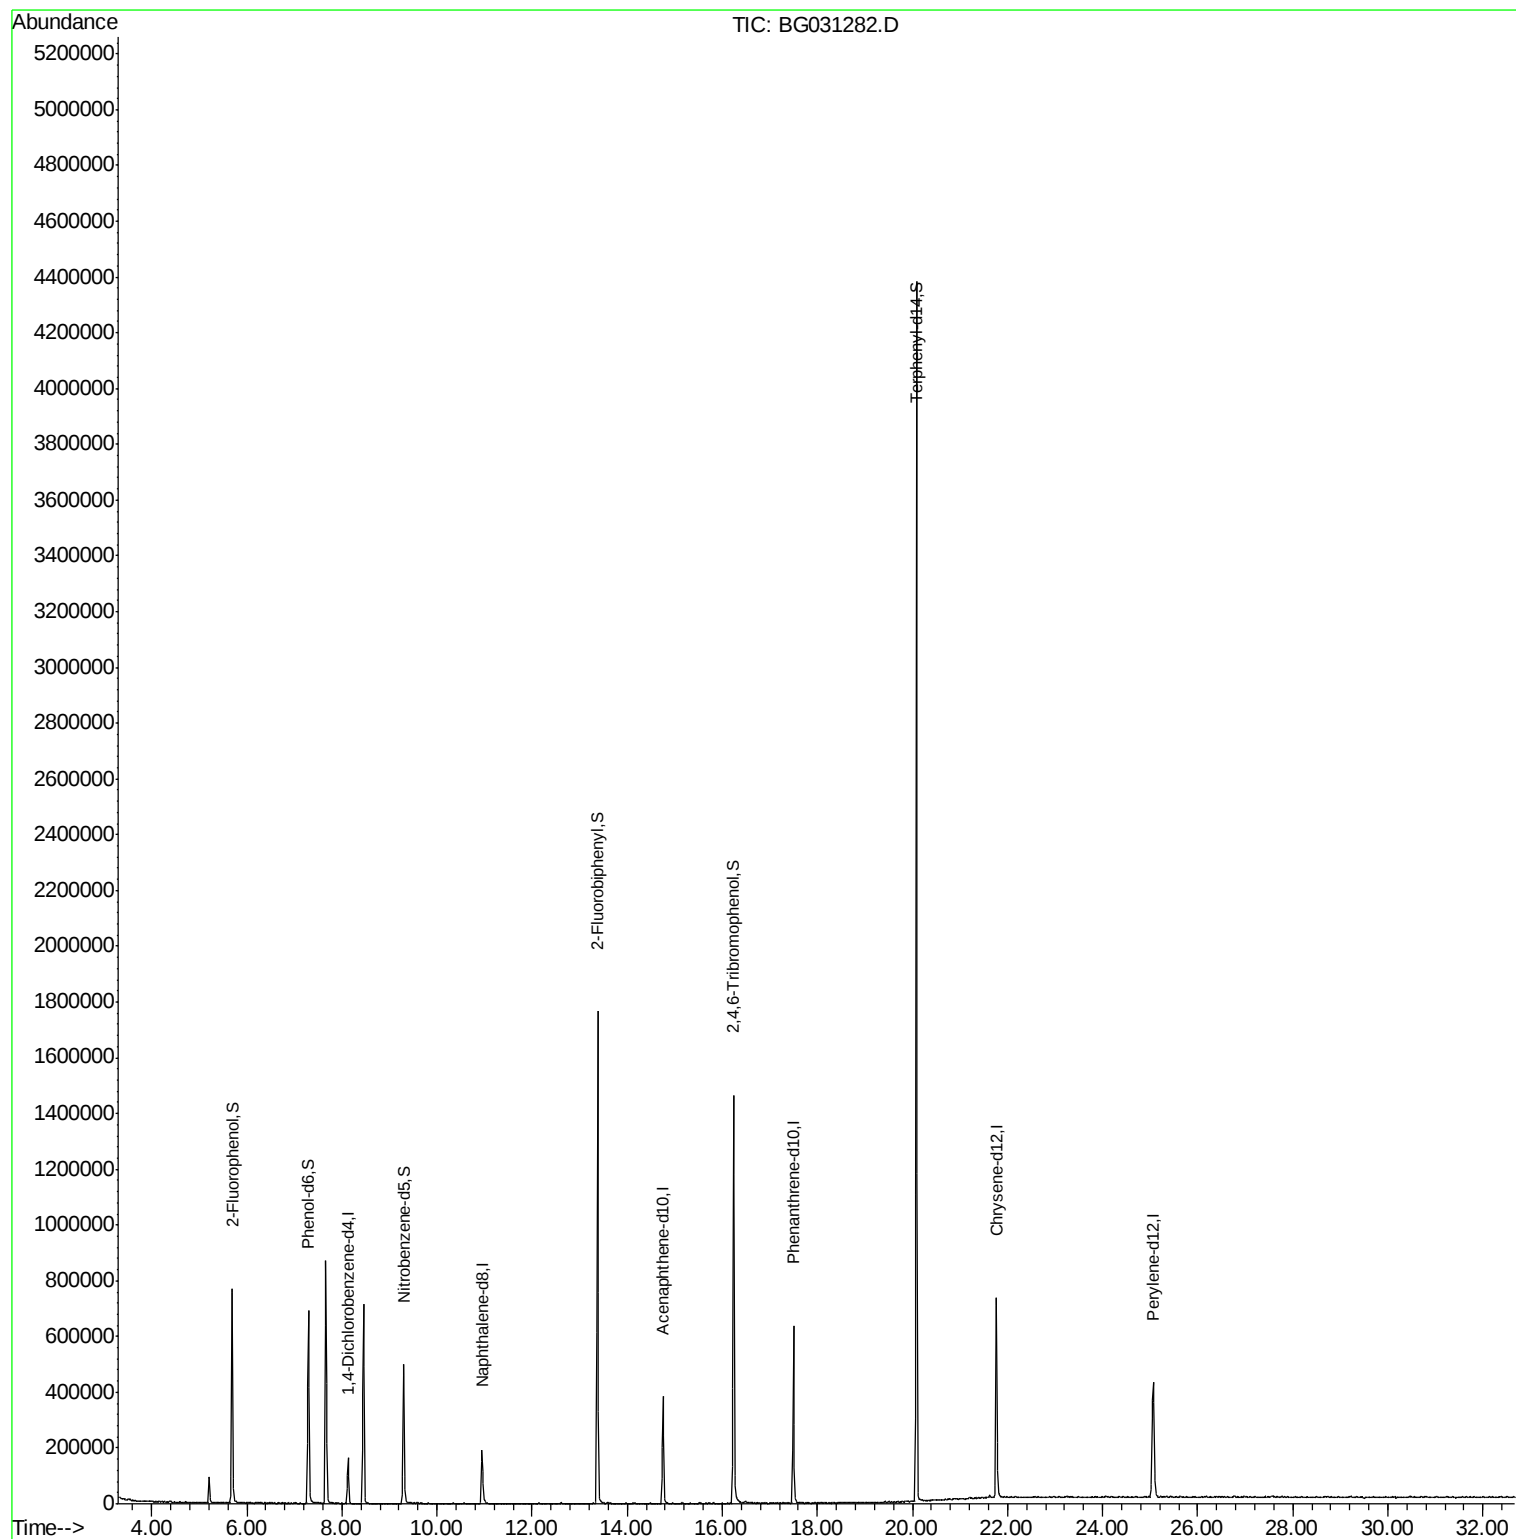

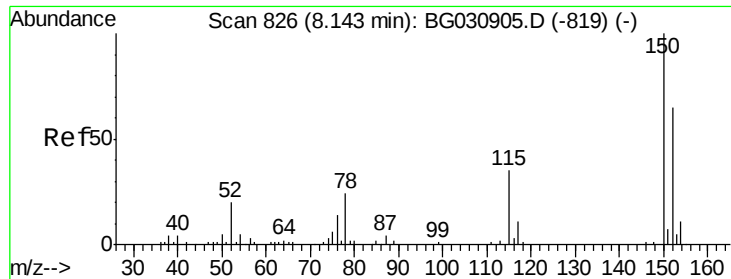

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.13 min Scan# 824

Delta R.T. -0.02 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15

Instrument :

BNA_G

ClientSampled :


Tot Ion:152 Resp: 51550

Ion Ratio Lower Upper

152 100

150 151.5 126.6 189.8




115 55.6 53.0 79.4

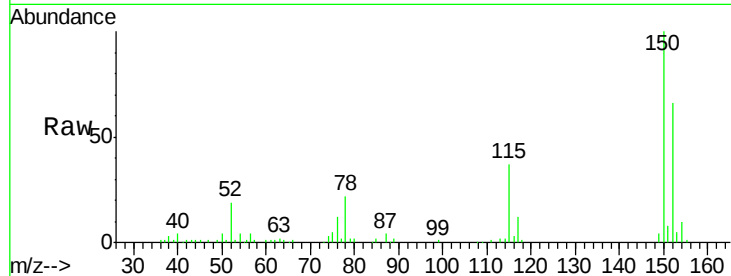

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

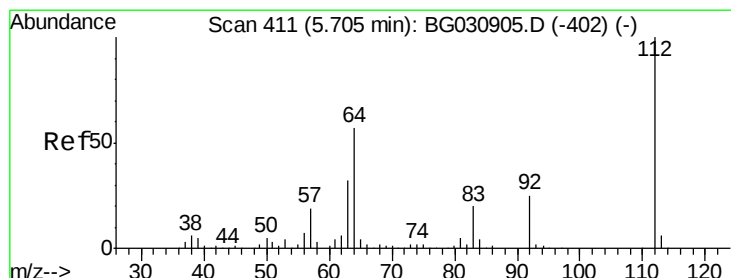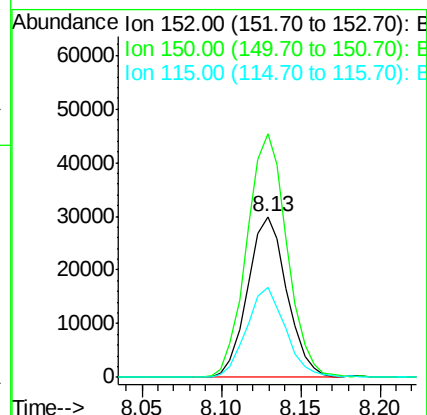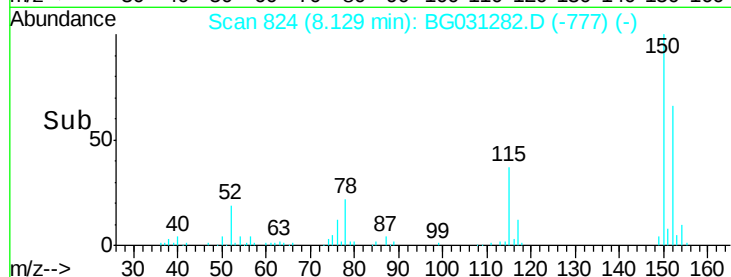

#5

2-Fluorophenol

Concen: 131.23 ng

RT: 5.69 min Scan# 409

Delta R.T. -0.02 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15


Tgt Ion:112 Resp: 394503

Ion Ratio Lower Upper

112 100

64 54.8 56.3 84.5#



63 28.0 30.1 45.1#

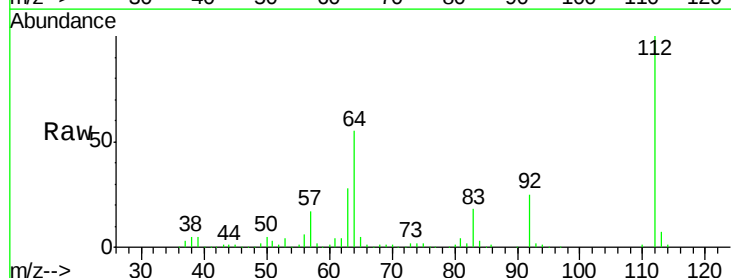


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

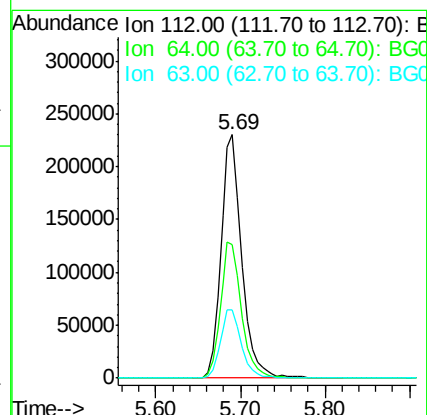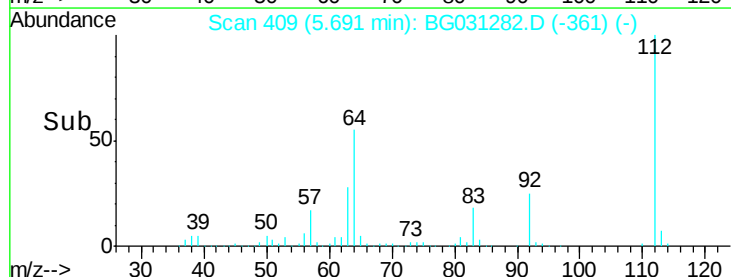

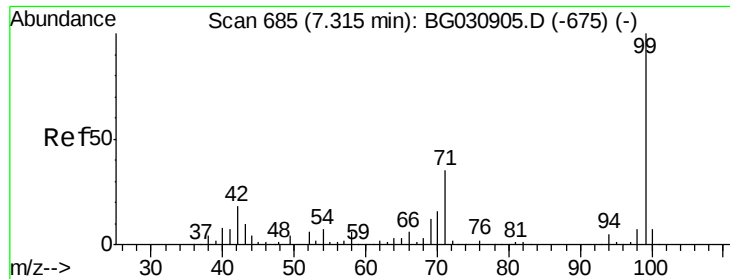

#7

Phenol-d6

Concen: 114.17 ng

RT: 7.29 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 462397

Ion Ratio Lower Upper




99 100

42 16.8 14.1 21.1

71 34.4 26.1 39.1

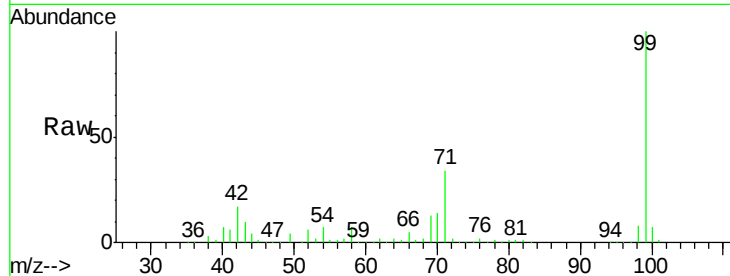

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

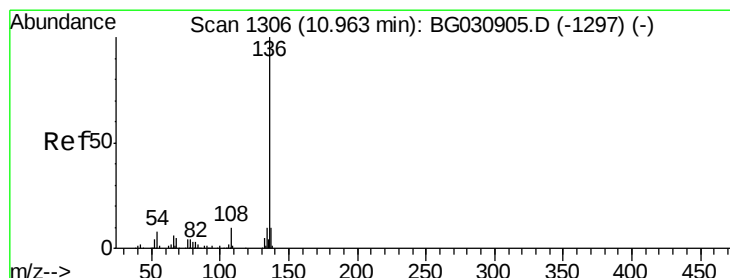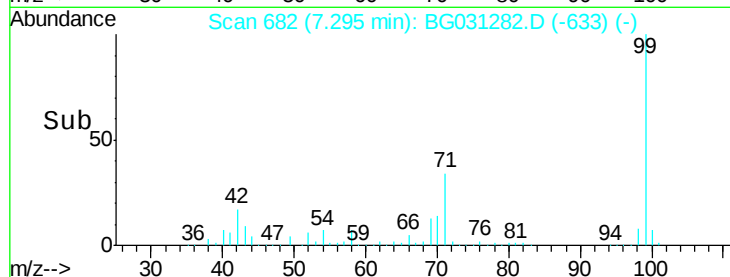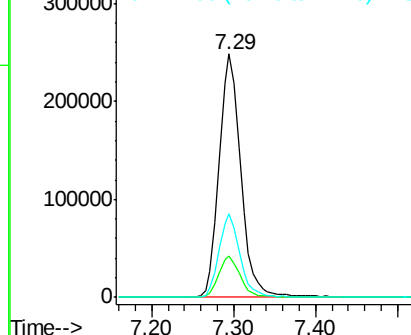

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.95 min Scan# 1304

Delta R.T. -0.02 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15

Tgt Ion: 136 Resp: 218082


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8

54 6.8 10.3 15.5#

68 5.1 4.5 6.7

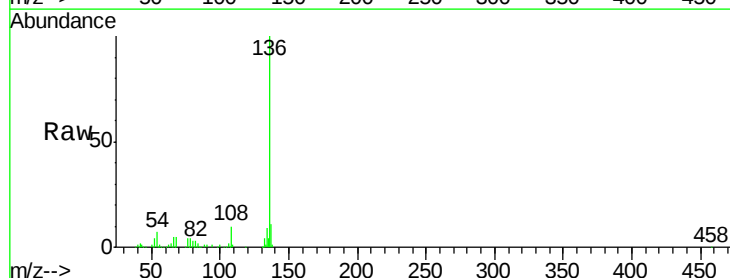

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

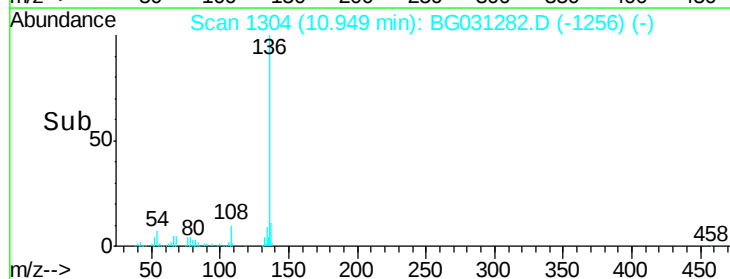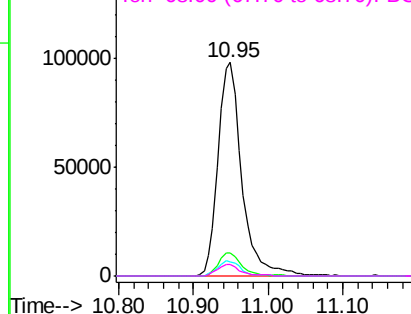







#23
Nitrobenzene-d5
Concen: 92.44 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031282.D
Acq: 29 Nov 2017 22:15

Instrument :
BNA_G
ClientSampleId :

Tot Ion	82	Resp	340195
Ion Ratio	100		
128	46.4	29.7	44.5#
54	47.5	43.1	64.7

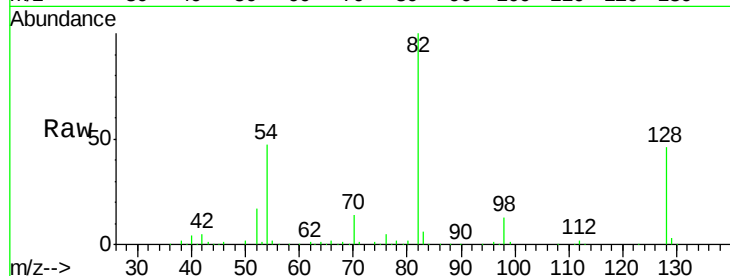


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

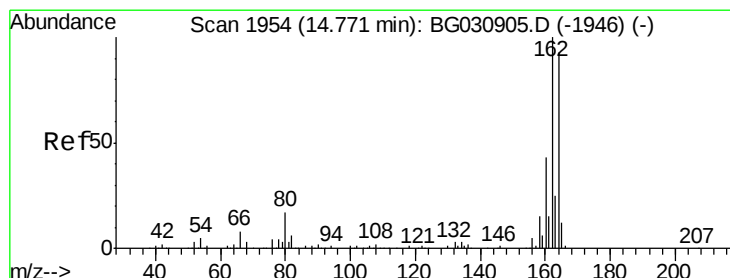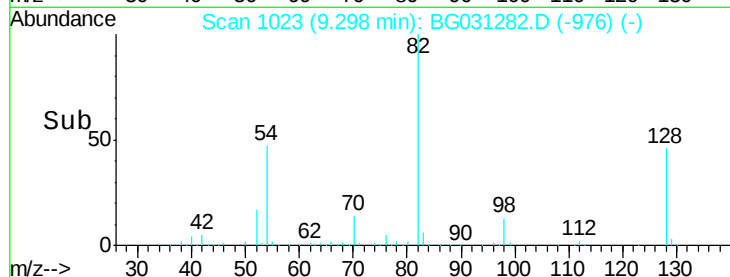
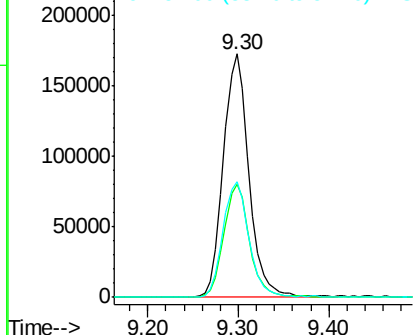


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031282.D
Acq: 29 Nov 2017 22:15

Tgt Ion	164	Resp	149868
Ion Ratio	100		
162	104.7	78.8	118.2
160	45.1	35.4	53.0

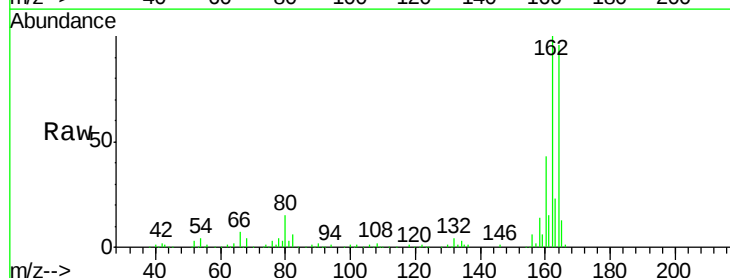

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC



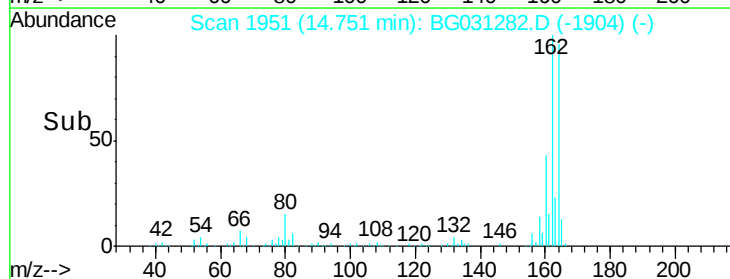
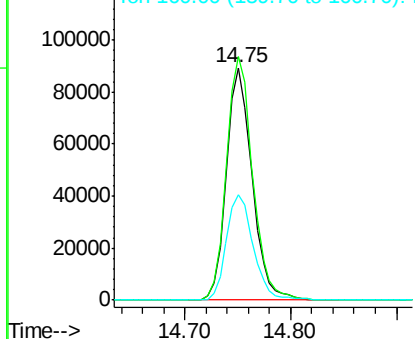




#41
 2,4,6-Tribromophenol
 Concen: 131.33 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031282.D
 Acq: 29 Nov 2017 22:15




Instrument :
 BNA_G
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.6	77.0	115.6
141	34.5	25.2	37.8

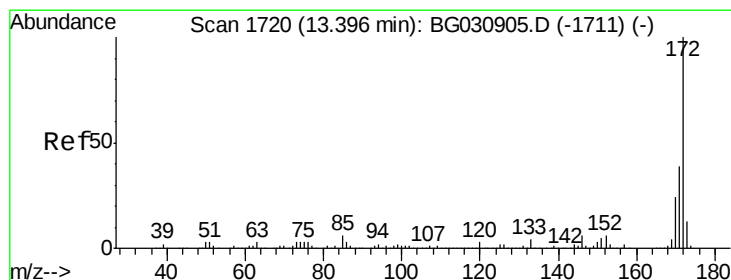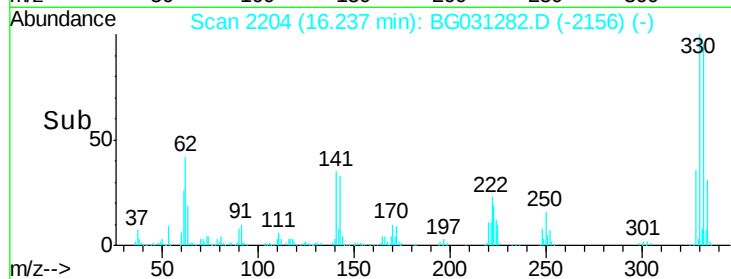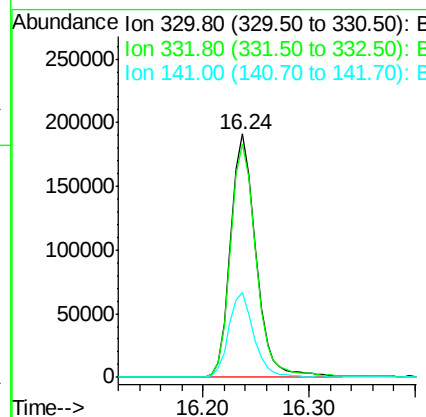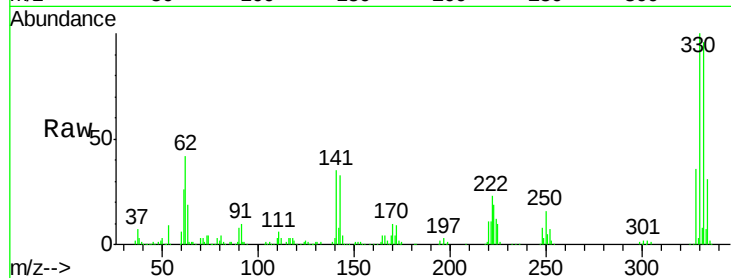

#44
 2-Fluorobiphenyl
 Concen: 100.16 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.02 min
 Lab File: BG031282.D
 Acq: 29 Nov 2017 22:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	30.0	45.0
170	24.6	19.5	29.3


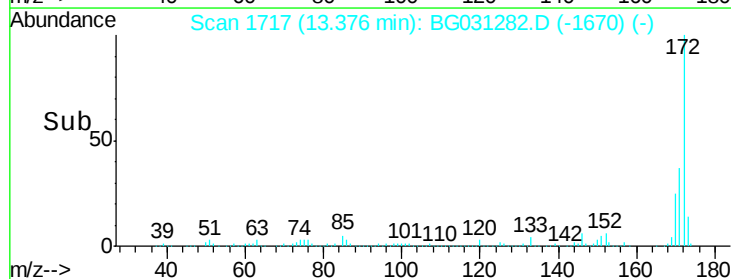
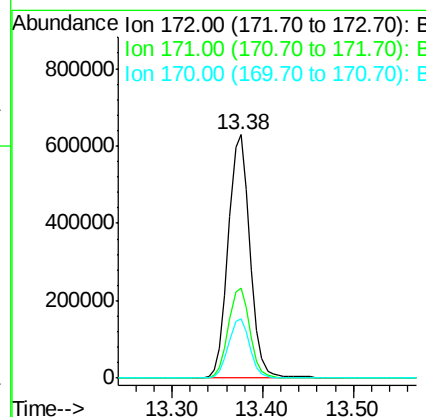
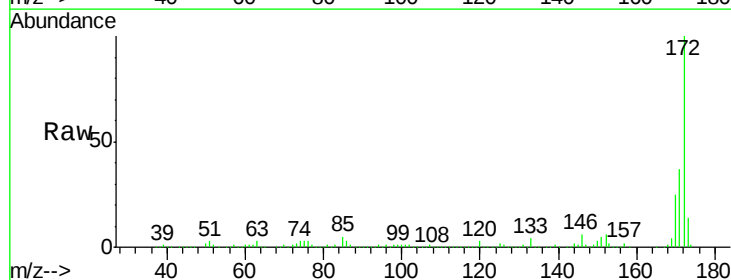


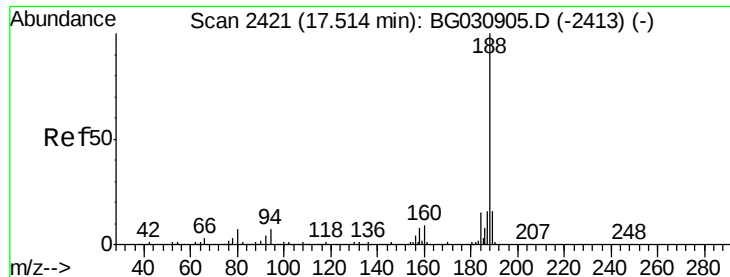

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG031282.D
Acq: 29 Nov 2017 22:15




Instrument :
BNA_G
ClientSampleId :


Tot Ion:188 Resp: 437373
Ion Ratio Lower Upper
188 100
94 7.1 6.9 10.3
80 7.5 7.7 11.5#

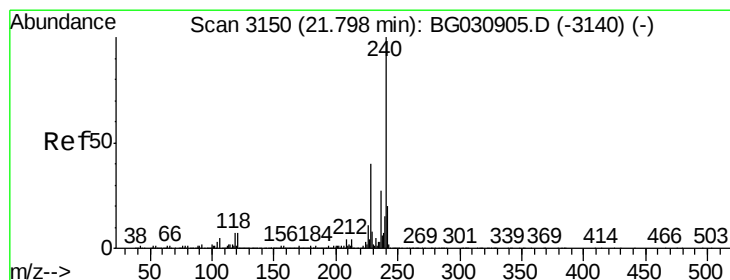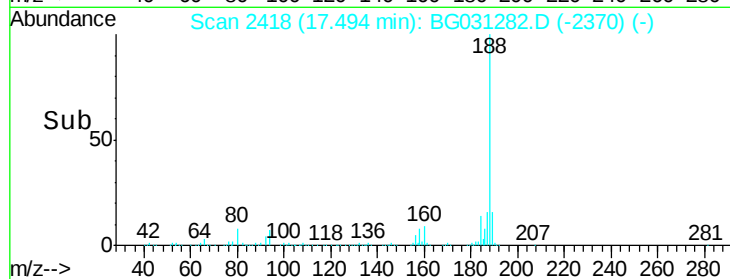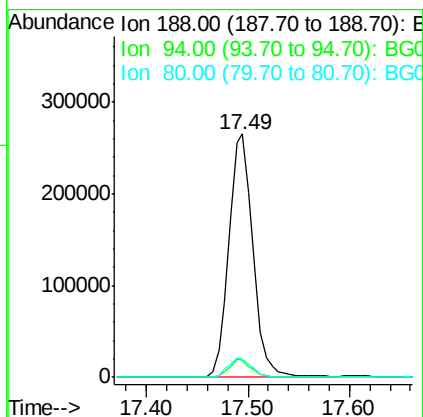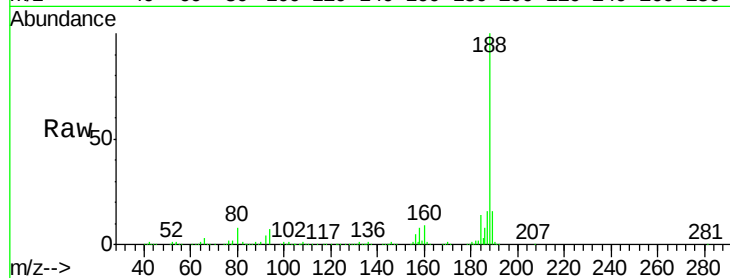

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.02 min
Lab File: BG031282.D
Acq: 29 Nov 2017 22:15

Tgt Ion:240 Resp: 513026
Ion Ratio Lower Upper
240 100
120 7.9 6.8 10.2
236 26.6 20.9 31.3

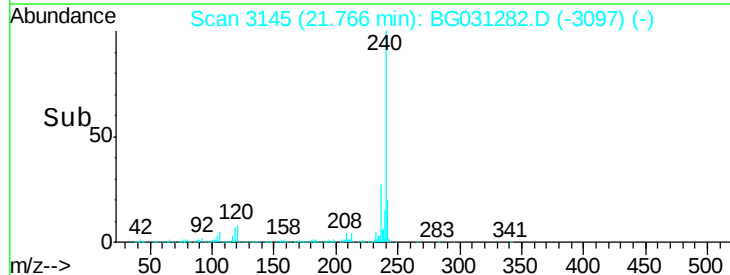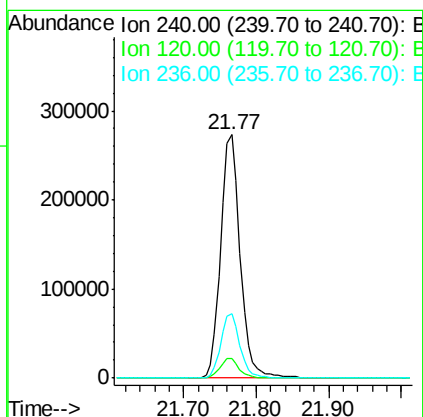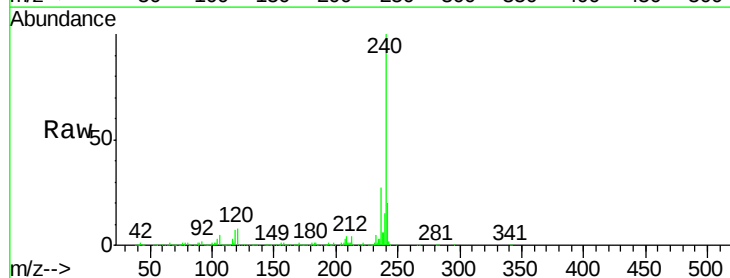

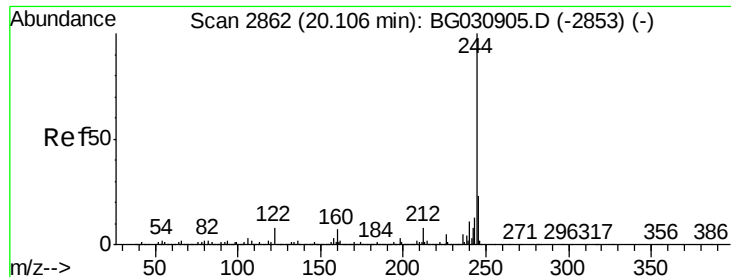

#78

Terphenyl-d14

Concen: 94.08 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 2185802

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 9.2 7.0 10.4

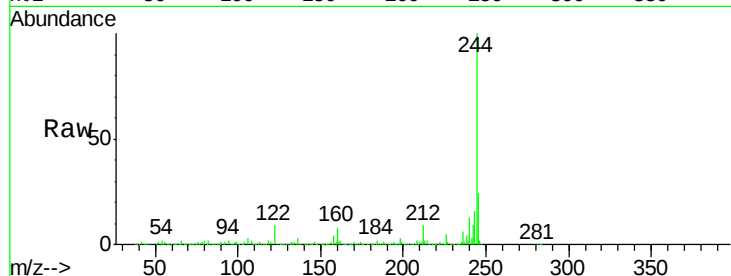

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

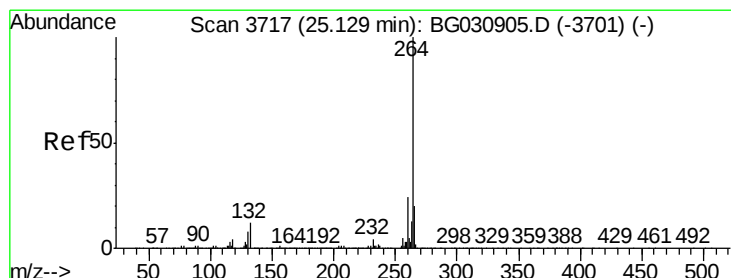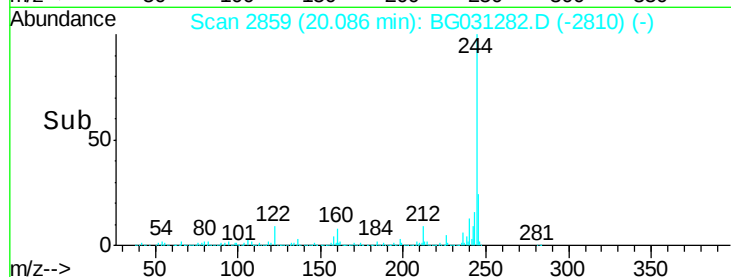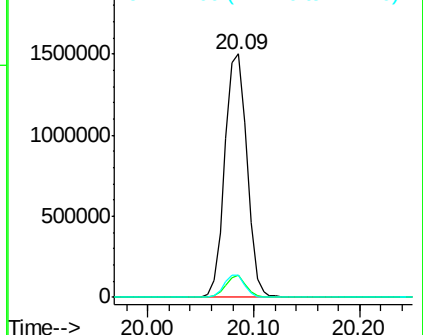

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.03 min

Lab File: BG031282.D

Acq: 29 Nov 2017 22:15


Tgt Ion:264 Resp: 489940

Ion Ratio Lower Upper

264 100

260 22.3 17.4 26.0

265 21.5 17.7 26.5

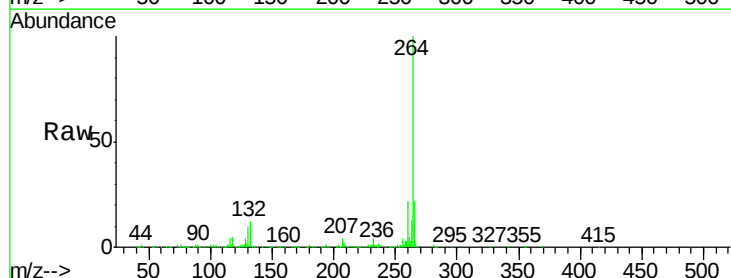

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

