
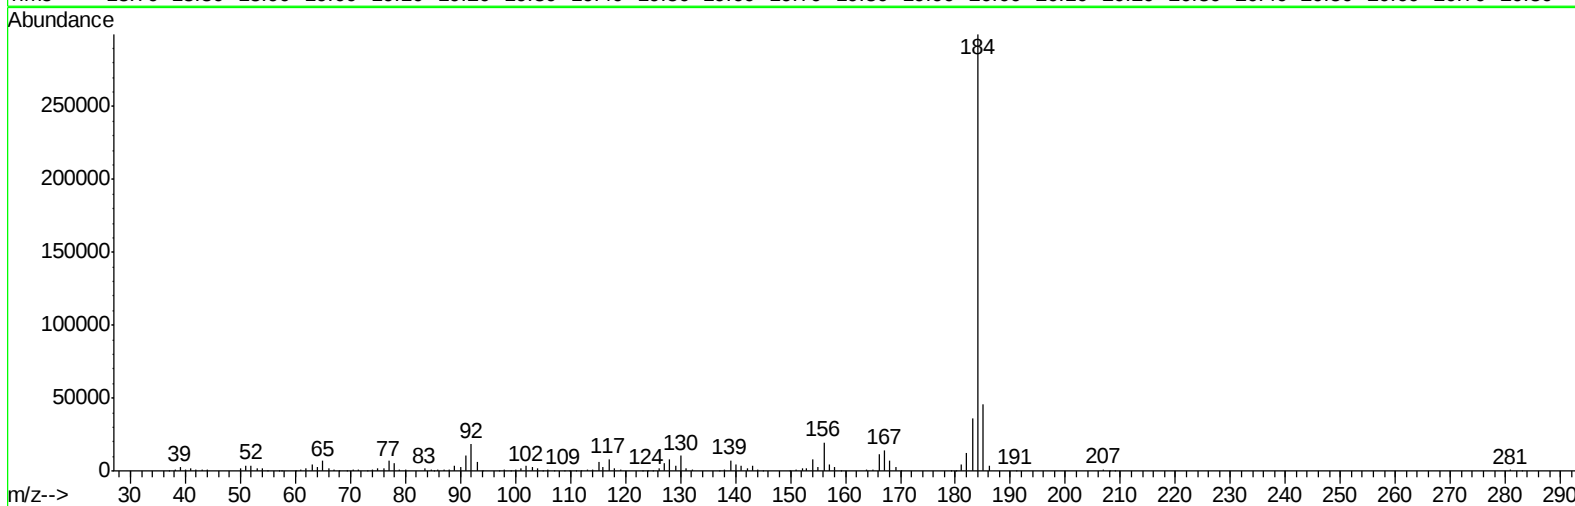


Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
Data File : BG031269.D
Acq On : 29 Nov 2017 14:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 06:21:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

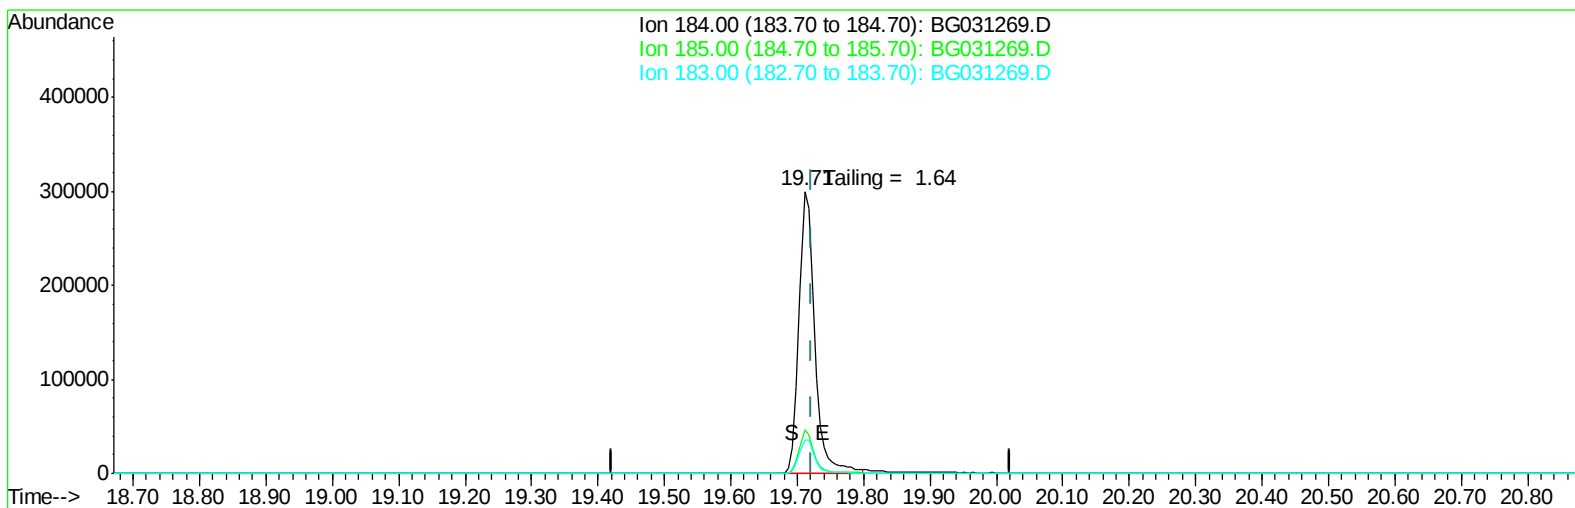

TIC: BG031269.D

(76) Benzidine



19.711min (-0.011) 6628.32ng

response 488002

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.30
183.00	13.30	12.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
Data File : BG031269.D
Acq On : 29 Nov 2017 14:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 06:21:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

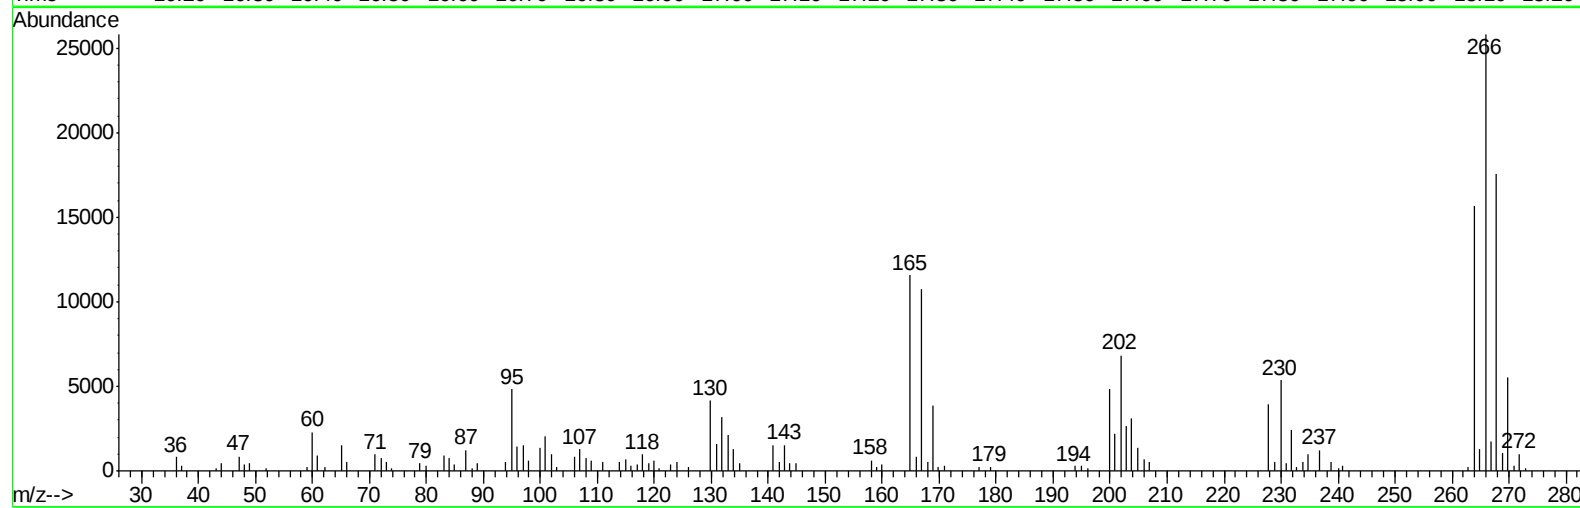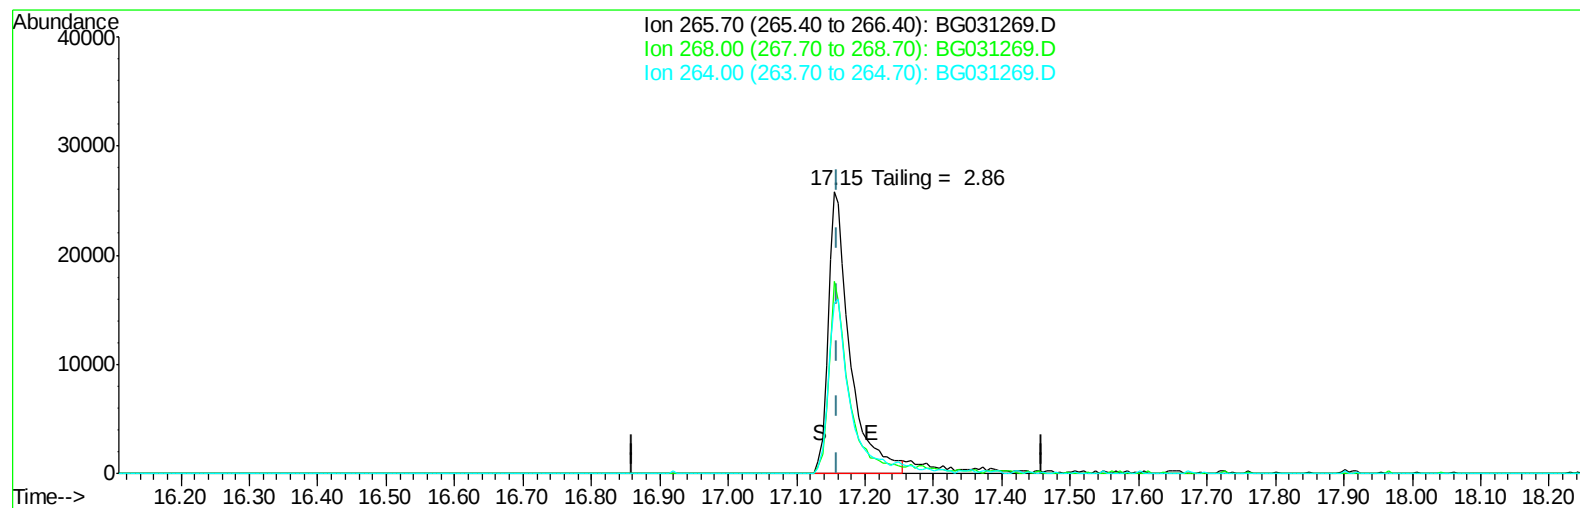

TIC: BG031269.D

(69) Pentachlorophenol (C)

17.155min (-0.005) 110870.40ng

response 56909

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.01
264.00	62.00	60.61
0.00	0.00	0.00