

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
 Data File : BG031279.D
 Acq On : 29 Nov 2017 20:22
 Operator : SJ/JU
 Sample : I6304-27
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-112817-C

Quant Time: Nov 30 03:09:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	47337	20.00	ng	-0.02
21) Naphthalene-d8	10.95	136	205799	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	145363	20.00	ng	-0.02
63) Phenanthrene-d10	17.50	188	459244	20.00	ng	-0.02
75) Chrysene-d12	21.77	240	550892	20.00	ng	-0.02
86) Perylene-d12	25.06	264	539108	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	407772	147.71	ng	-0.02
7) Phenol-d6	7.30	99	499392	134.28	ng	-0.01
23) Nitrobenzene-d5	9.30	82	341351	98.29	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	351518	149.49	ng	-0.02
44) 2-Fluorobiphenyl	13.38	172	1041939	102.99	ng	-0.02
78) Terphenyl-d14	20.09	244	2350206	94.20	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
Data File : BG031279.D
Acq On : 29 Nov 2017 20:22
Operator : SJ/JU
Sample : I6304-27
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-112817-C

Quant Time: Nov 30 03:09:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

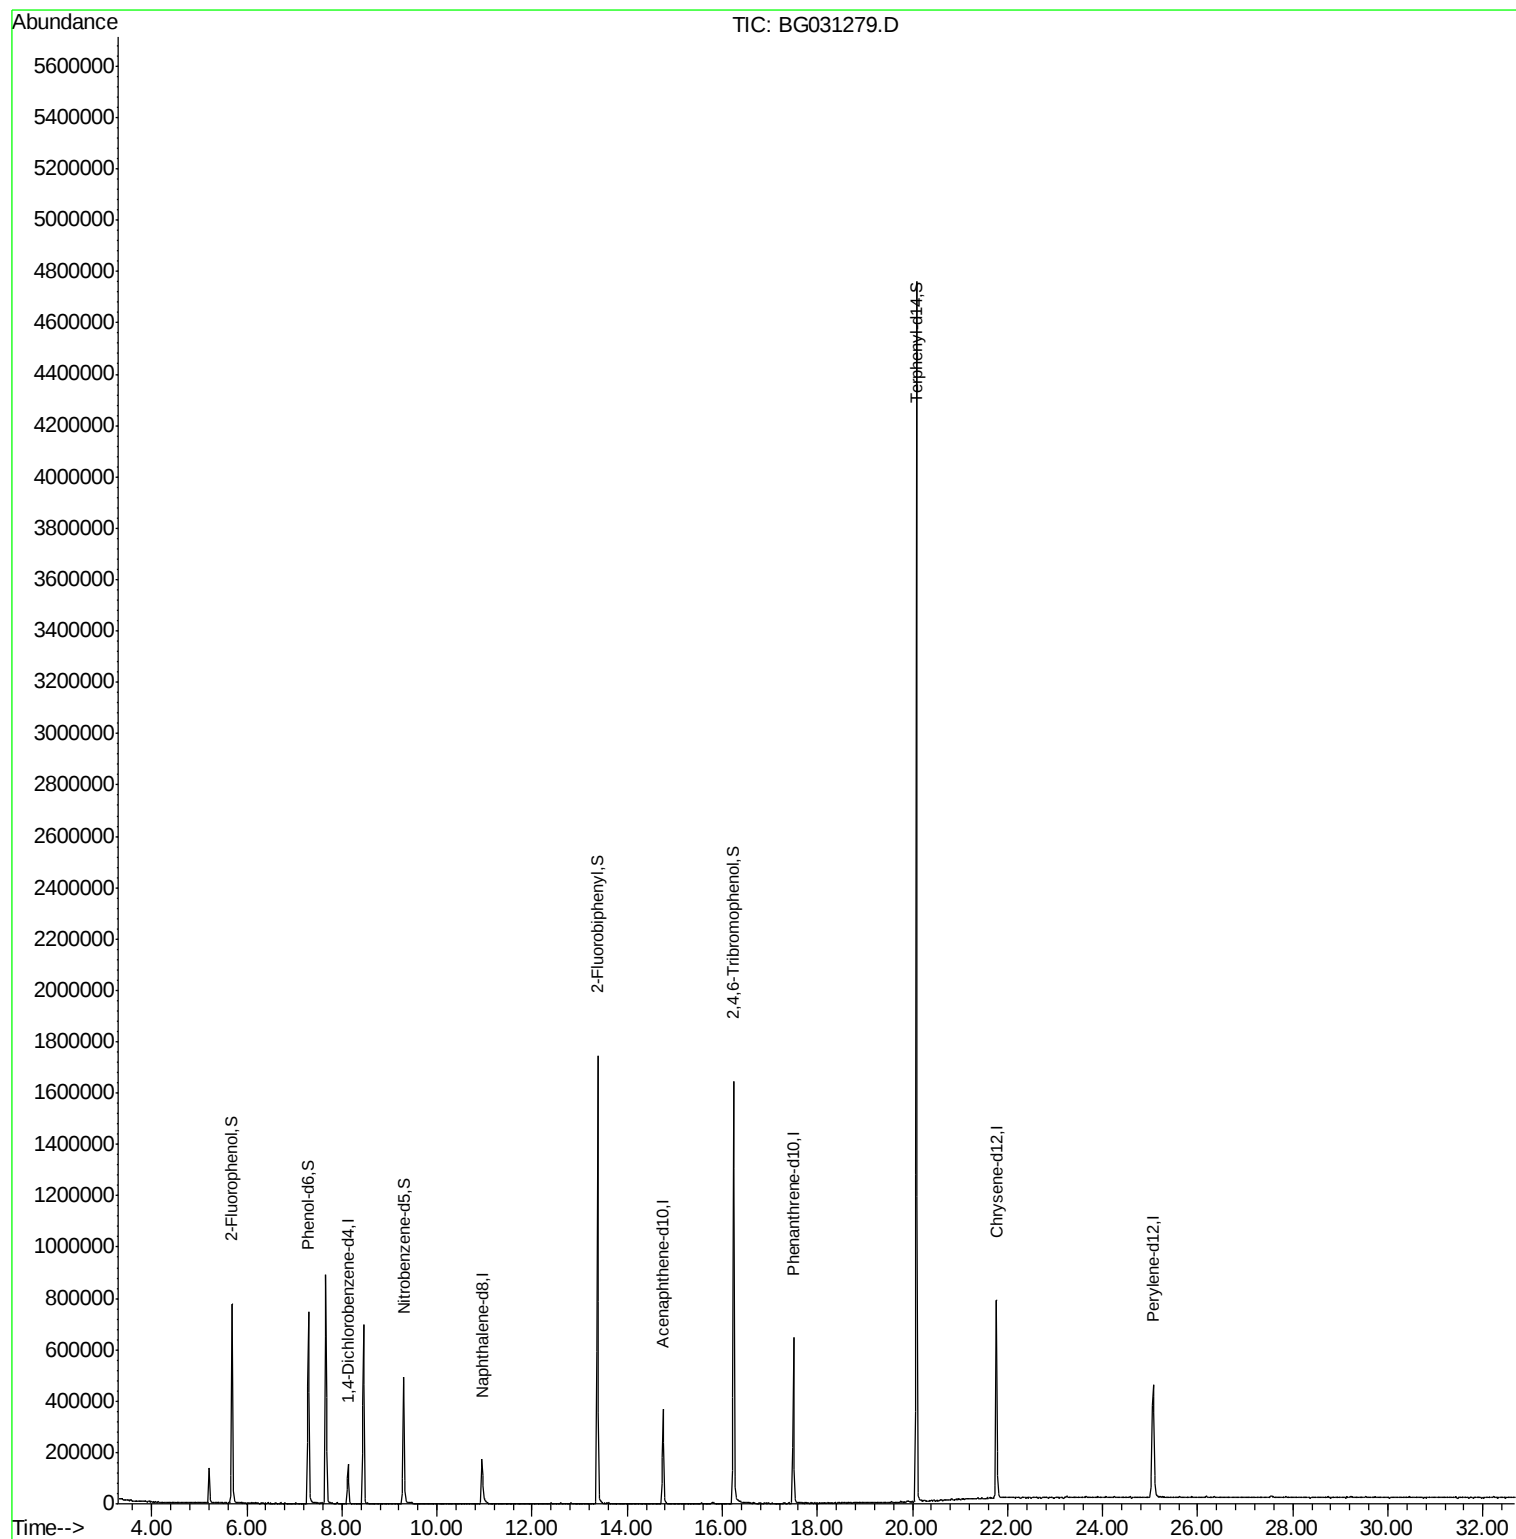




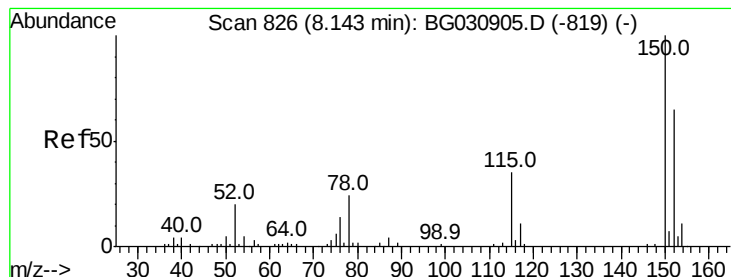


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.13 min Scan# 824
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22

Instrument :
BNA_G
ClientSampleId :
CL-02-112817-C




Tot Ion:152 Resp: 47337
Ion Ratio Lower Upper
152 100
150 152.4 126.6 189.8
115 56.3 53.0 79.4

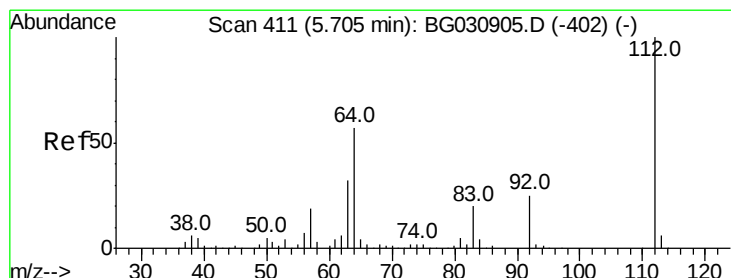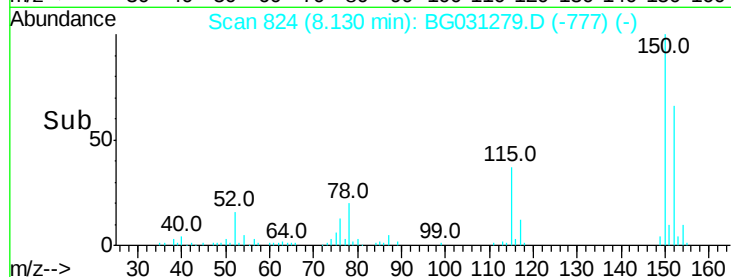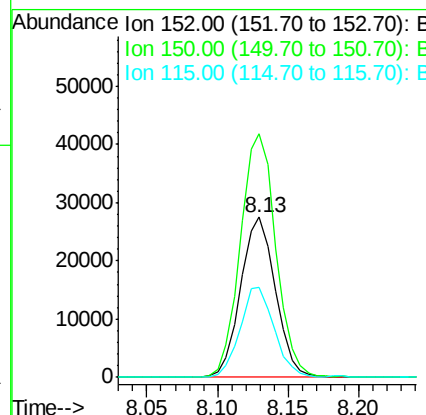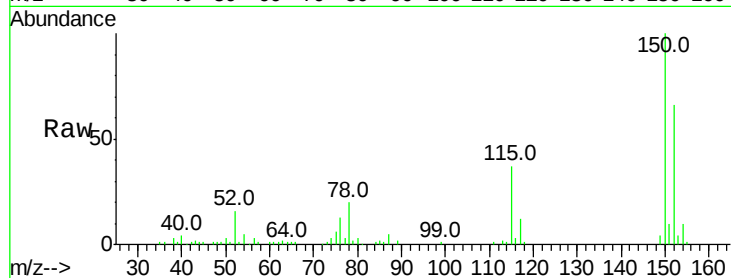


#5

2-Fluorophenol
Concen: 147.713 ng
RT: 5.69 min Scan# 409
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22

Tgt Ion:112 Resp: 407772
Ion Ratio Lower Upper
112 100
64 55.2 56.3 84.5#
63 29.3 30.1 45.1#

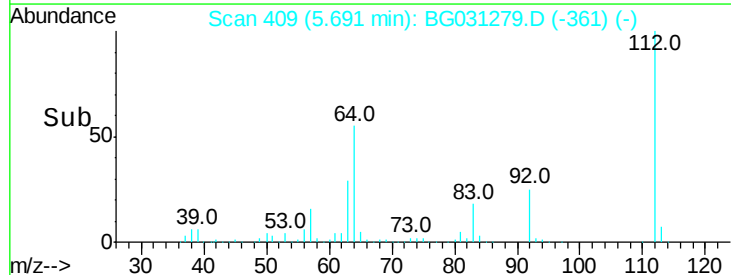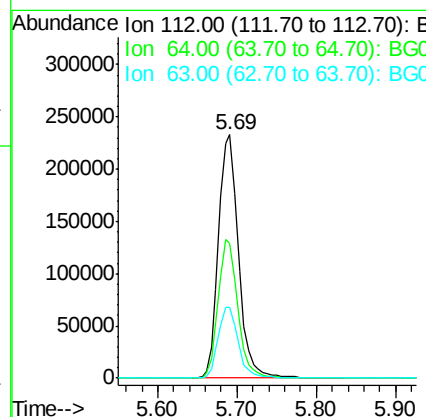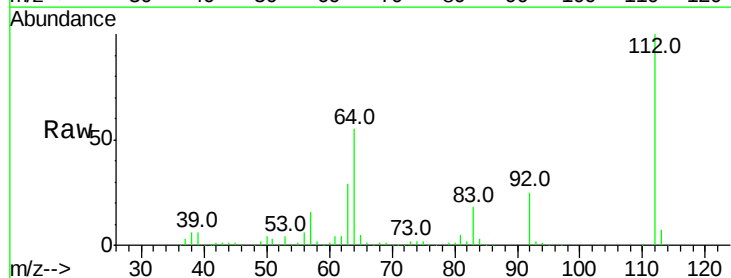

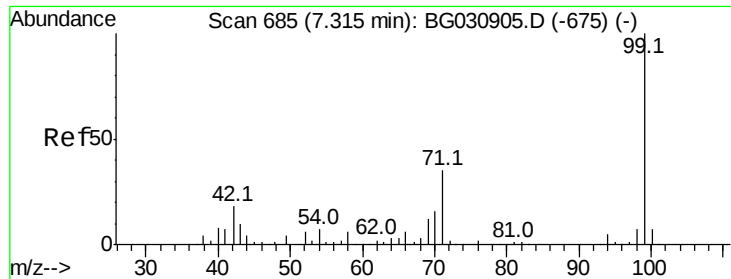

#7

Phenol-d6

Concen: 134.278 ng

RT: 7.30 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031279.D

Acq: 29 Nov 2017 20:22

Instrument :

BNA_G

ClientSampleId :

CL-02-112817-C


Tot Ion: 99 Resp: 499392

Ion Ratio Lower Upper



99 100

42 17.6 14.1 21.1

71 34.4 26.1 39.1

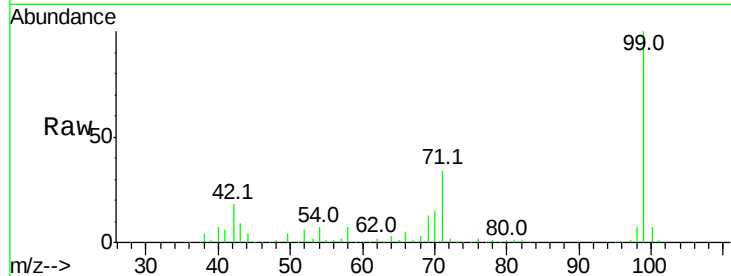

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

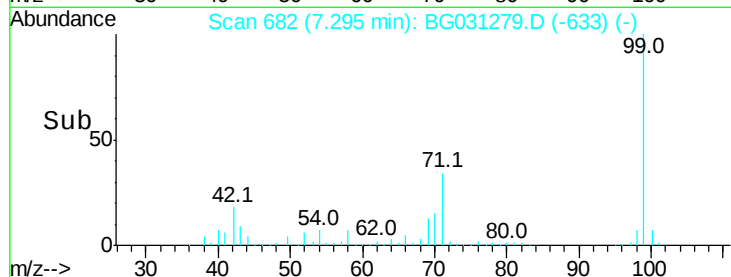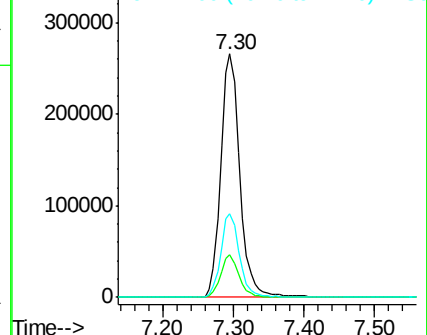

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.95 min Scan# 1304

Delta R.T. -0.02 min

Lab File: BG031279.D

Acq: 29 Nov 2017 20:22

Tgt Ion: 136 Resp: 205799


Ion Ratio Lower Upper

136 100



137 10.5 9.2 13.8

54 7.9 10.3 15.5#

68 4.7 4.5 6.7

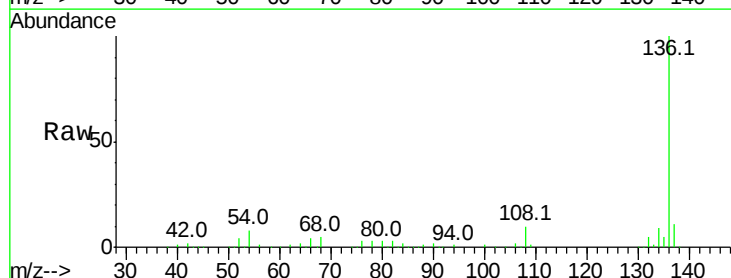

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



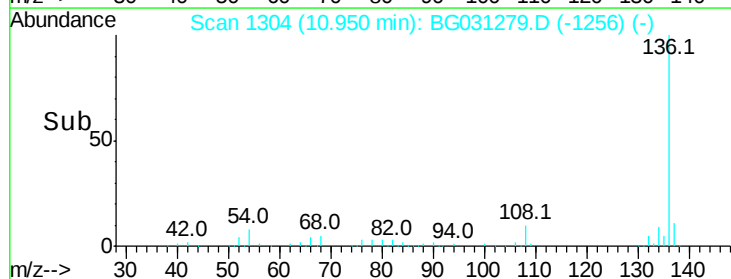
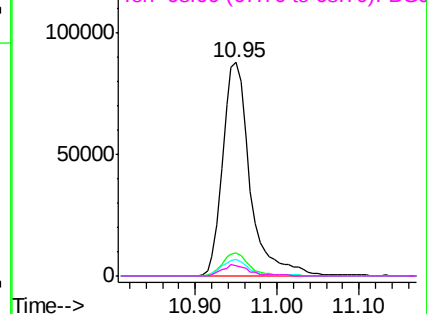




#23
Nitrobenzene-d5
Concen: 98.286 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22




Instrument :
BNA_G
ClientSampleId :
CL-02-112817-C

Tot Ion: 82 Resp: 341351
Ion Ratio Lower Upper
82 100
128 47.2 29.7 44.5#
54 47.9 43.1 64.7

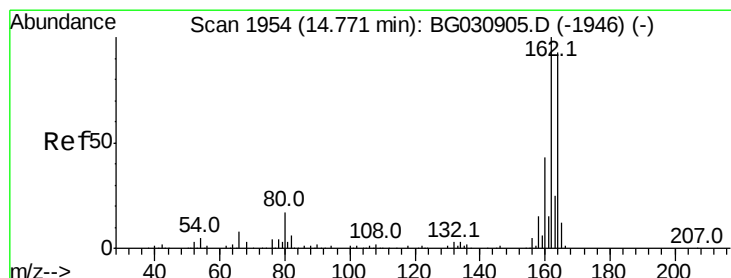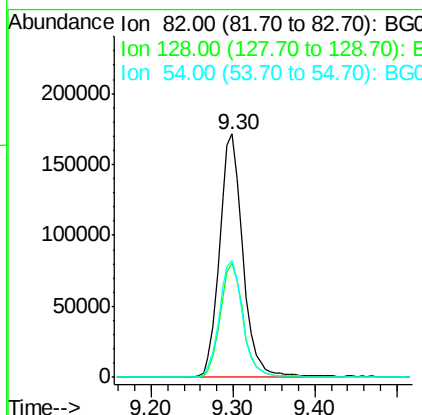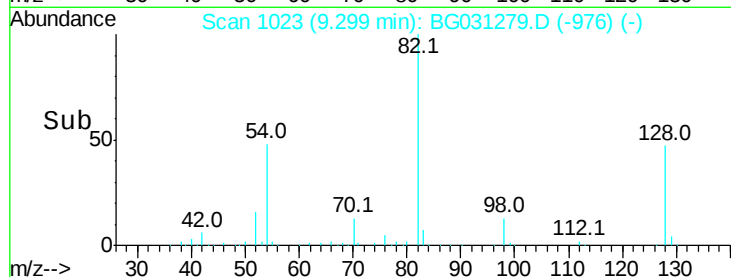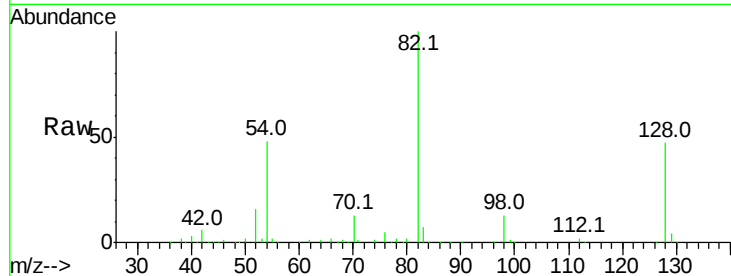

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22

Tgt Ion:164 Resp: 145363
Ion Ratio Lower Upper
164 100
162 105.6 78.8 118.2
160 44.2 35.4 53.0

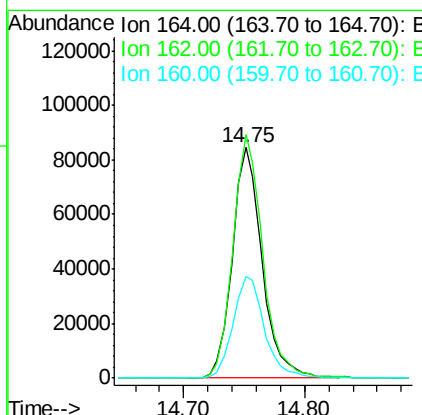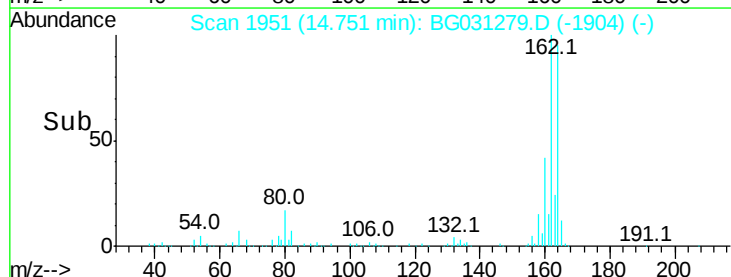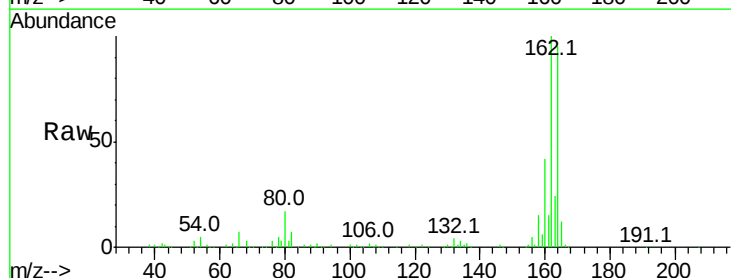







#41
 2,4,6-Tribromophenol
 Concen: 149.487 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031279.D
 Acq: 29 Nov 2017 20:22

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-112817-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	77.0	115.6
141	35.3	25.2	37.8

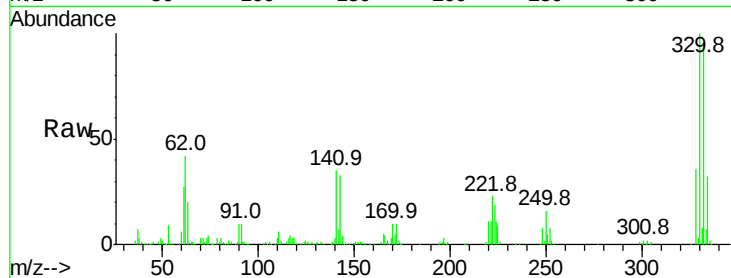


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

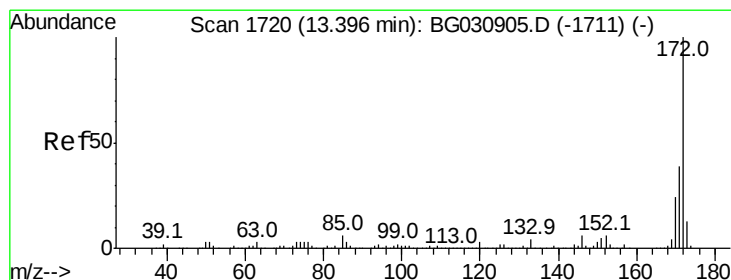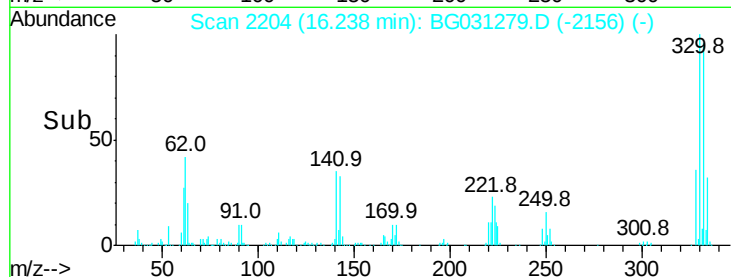
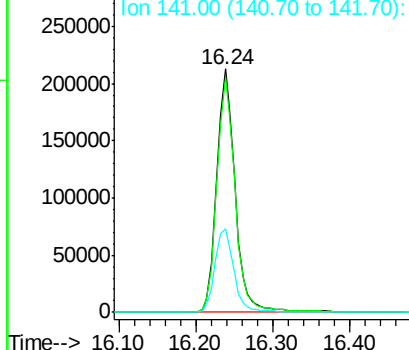



#44
 2-Fluorobiphenyl
 Concen: 102.994 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.02 min
 Lab File: BG031279.D
 Acq: 29 Nov 2017 20:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.0	45.0
170	24.3	19.5	29.3

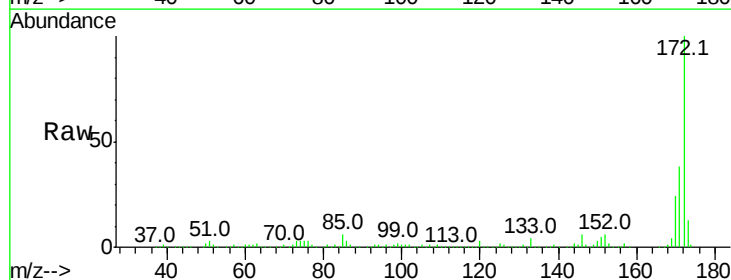

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


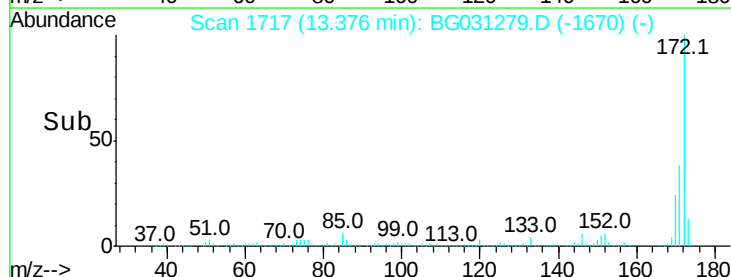
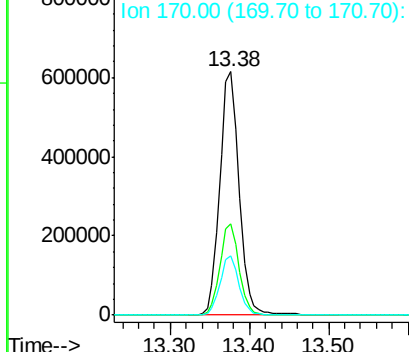


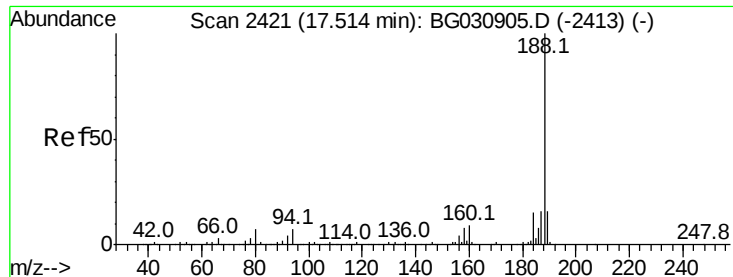

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.50 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22




Instrument :
BNA_G
ClientSampleId :
CL-02-112817-C

Tot Ion:188 Resp: 459244
Ion Ratio Lower Upper
188 100
94 7.3 6.9 10.3
80 7.6 7.7 11.5#

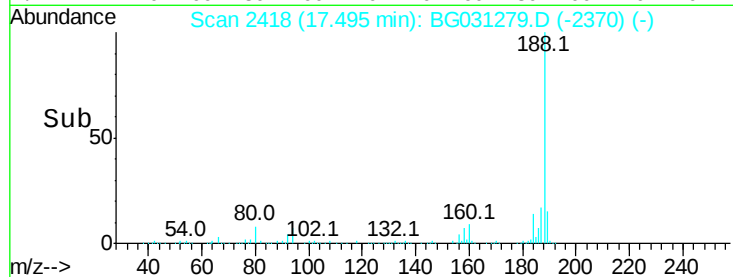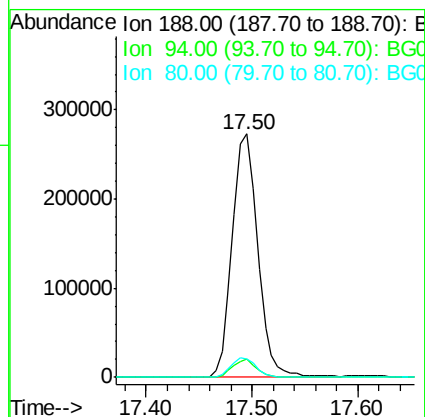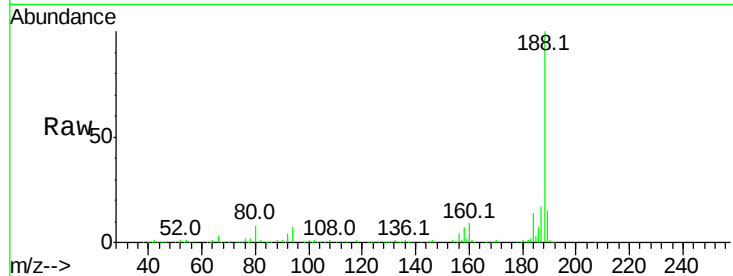

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.02 min
Lab File: BG031279.D
Acq: 29 Nov 2017 20:22

Tgt Ion:240 Resp: 550892
Ion Ratio Lower Upper
240 100
120 6.9 6.8 10.2
236 26.7 20.9 31.3

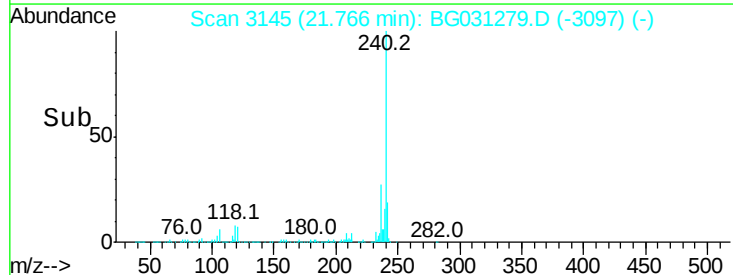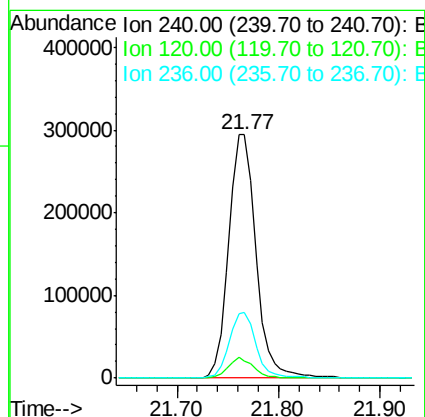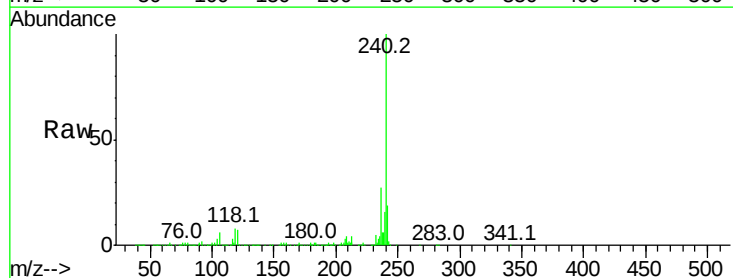



#78

Terphenyl-d14

Concen: 94.201 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031279.D

Acq: 29 Nov 2017 20:22

Instrument :

BNA_G

ClientSampleId :

CL-02-112817-C


Tot Ion:244 Resp: 2350206

Ion Ratio Lower Upper

244 100

212 9.2 5.8 8.8#



122 8.9 7.0 10.4

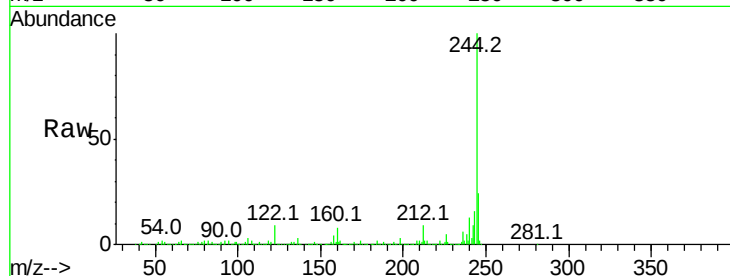

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

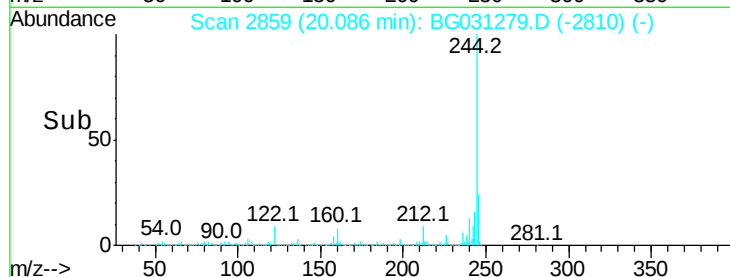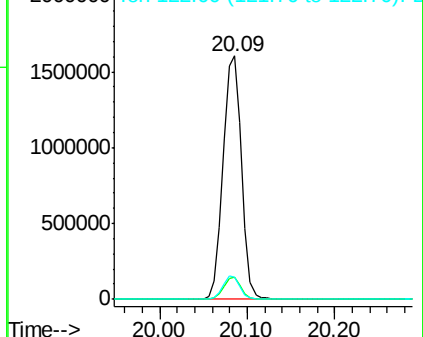

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.03 min

Lab File: BG031279.D

Acq: 29 Nov 2017 20:22


Tgt Ion:264 Resp: 539108

Ion Ratio Lower Upper

264 100

260 22.8 17.4 26.0

265 21.7 17.7 26.5

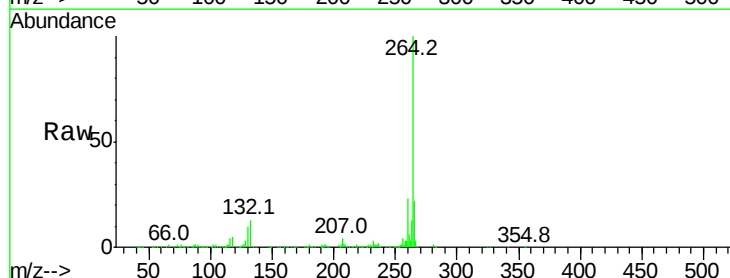

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

