

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
 Data File : BG031283.D
 Acq On : 29 Nov 2017 22:52
 Operator : SJ/JU
 Sample : I6306-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-112817-B

Quant Time: Nov 30 03:10:01 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	58952	20.00	ng	-0.02
21) Naphthalene-d8	10.94	136	235751	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	156035	20.00	ng	-0.02
63) Phenanthrene-d10	17.50	188	435232	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	533651	20.00	ng	-0.02
86) Perylene-d12	25.06	264	512125	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	461135	134.13	ng	-0.02
7) Phenol-d6	7.30	99	523665	113.06	ng	-0.01
23) Nitrobenzene-d5	9.30	82	384342	96.60	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	337735	133.80	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	1116497	102.82	ng	-0.03
78) Terphenyl-d14	20.09	244	2318092	95.92	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112917\
Data File : BG031283.D
Acq On : 29 Nov 2017 22:52
Operator : SJ/JU
Sample : I6306-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NB-08-112817-B

Quant Time: Nov 30 03:10:01 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

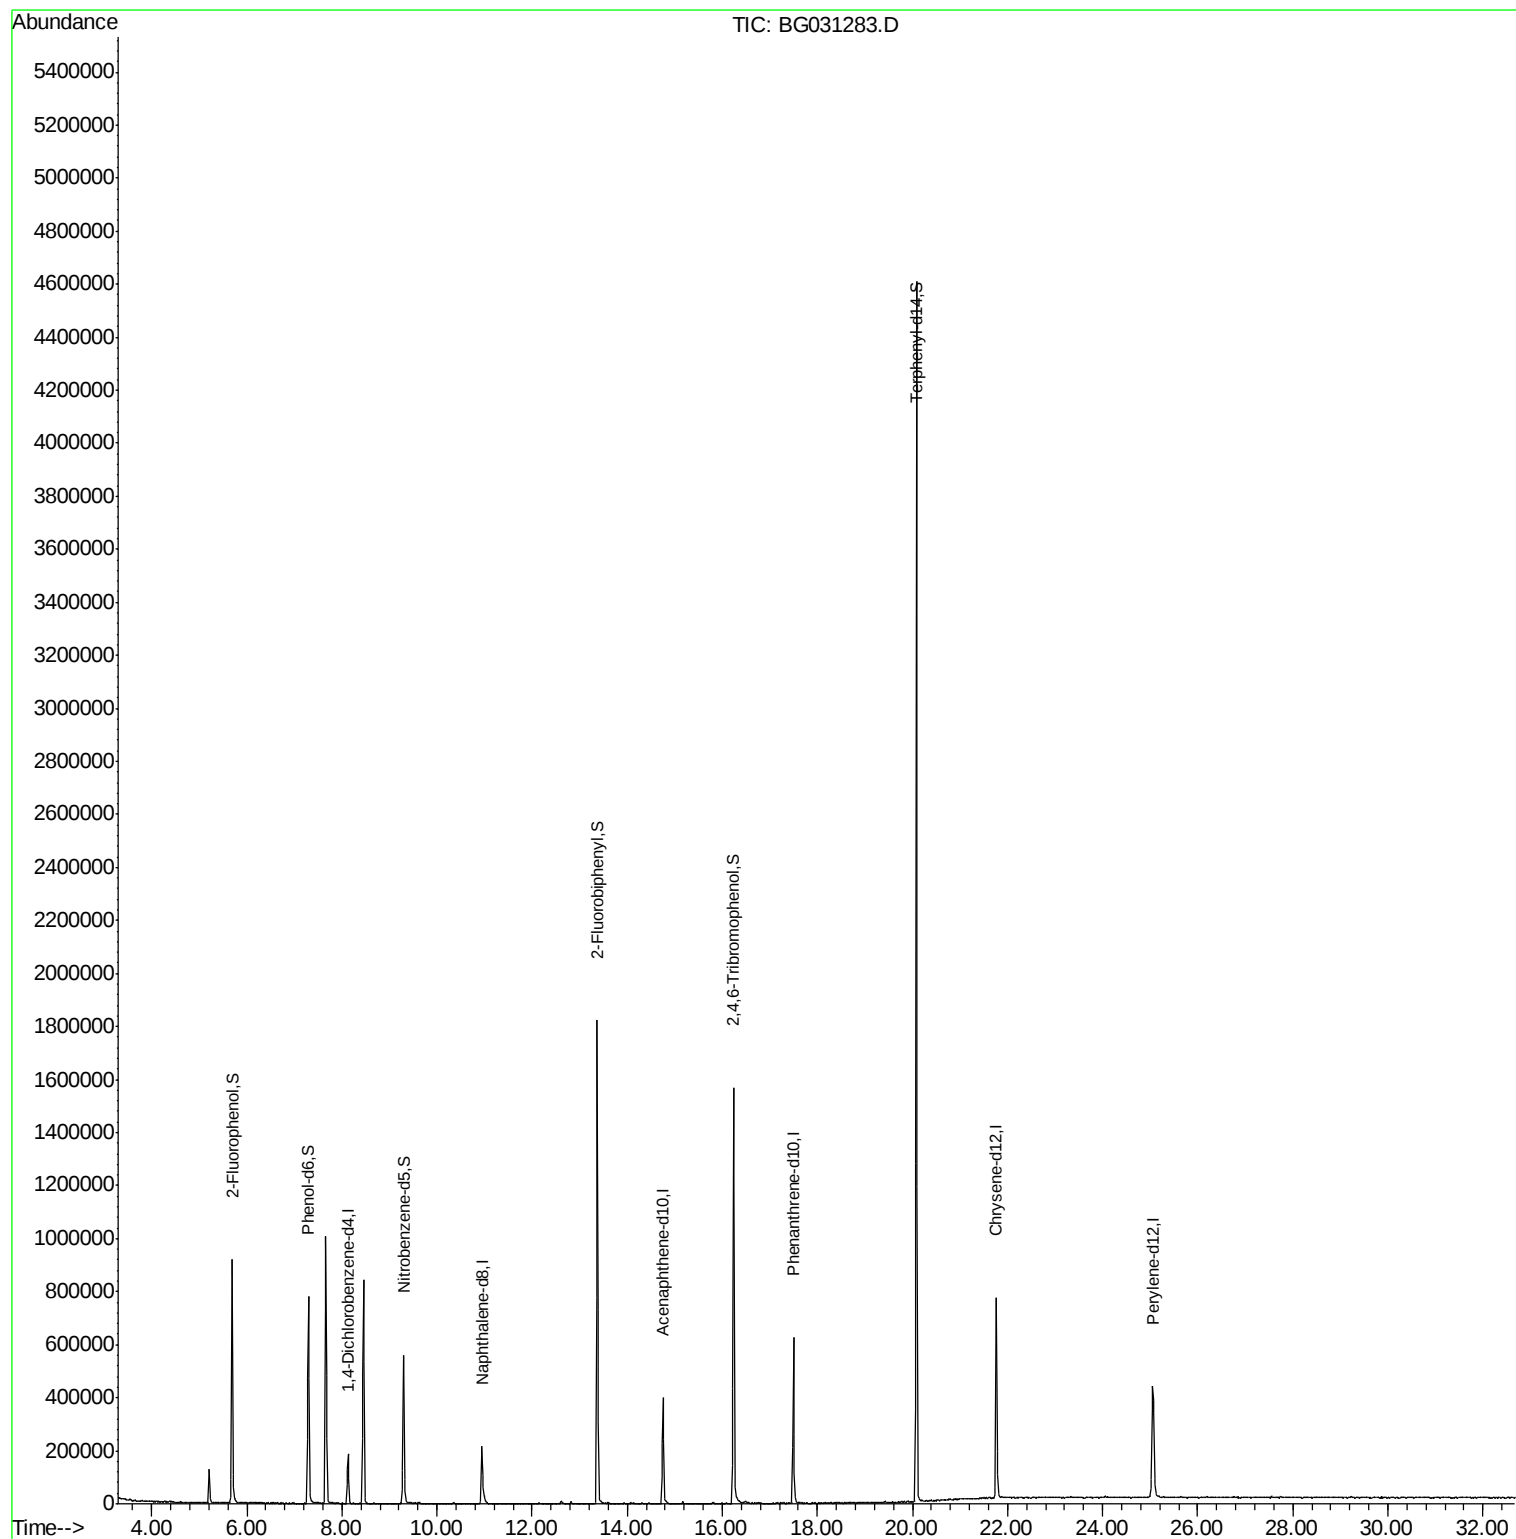

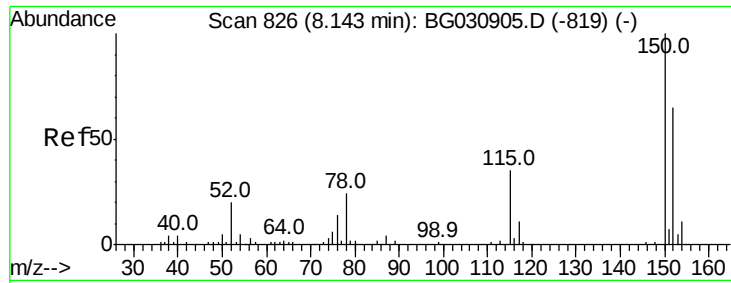


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.13 min Scan# 824
 Delta R.T. -0.02 min
 Lab File: BG031283.D
 Acq: 29 Nov 2017 22:52

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-112817-B

Tot Ion:152 Resp: 58952
 Ion Ratio Lower Upper
 152 100
 150 154.8 126.6 189.8
 115 57.1 53.0 79.4

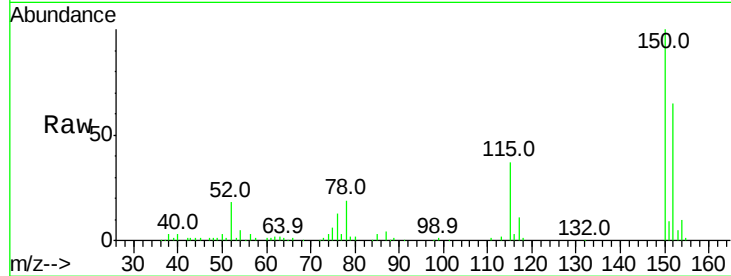


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

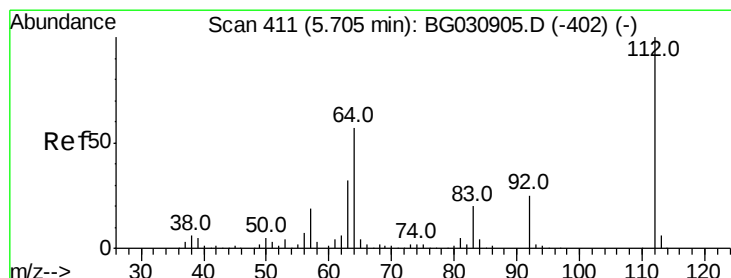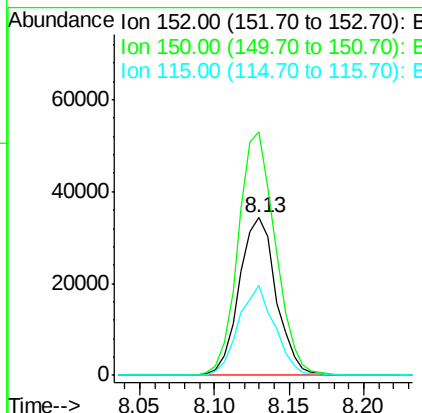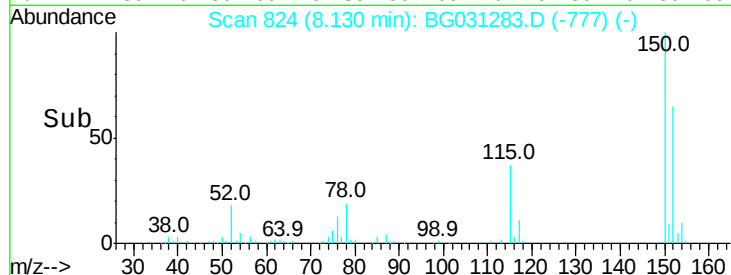



#5


2-Fluorophenol
 Concen: 134.132 ng
 RT: 5.69 min Scan# 409
 Delta R.T. -0.02 min
 Lab File: BG031283.D
 Acq: 29 Nov 2017 22:52

Tgt Ion:112 Resp: 461135
 Ion Ratio Lower Upper
 112 100
 64 58.0 56.3 84.5
 63 29.1 30.1 45.1#

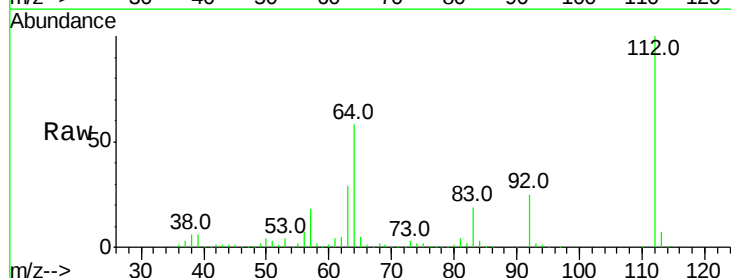

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

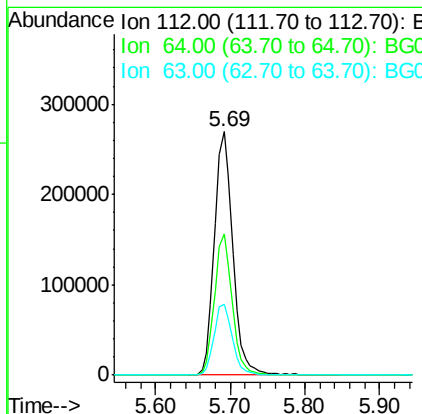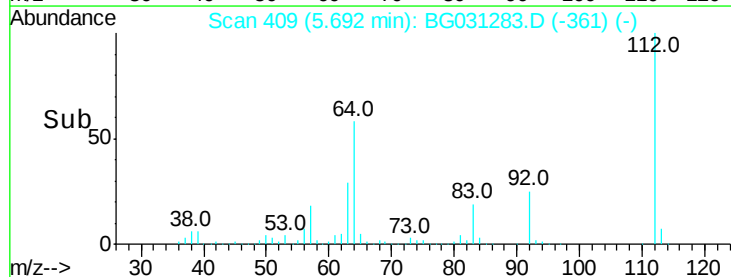

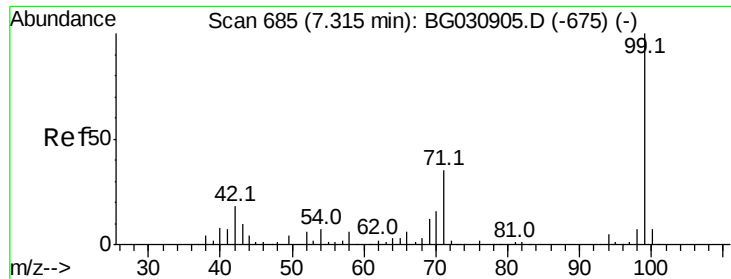

#7

Phenol-d6

Concen: 113.063 ng

RT: 7.30 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52

Instrument :

BNA_G

ClientSampleId :

NB-08-112817-B


Tot Ion: 99 Resp: 523665

Ion Ratio Lower Upper




99 100

42 16.8 14.1 21.1

71 33.3 26.1 39.1

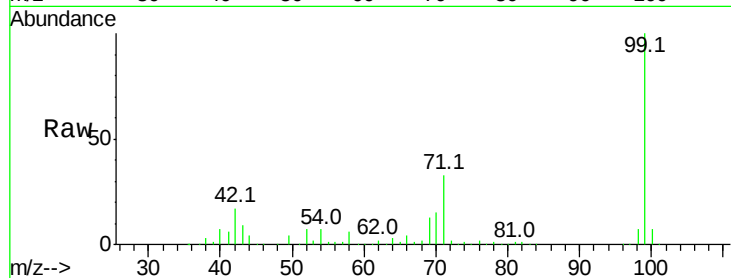

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

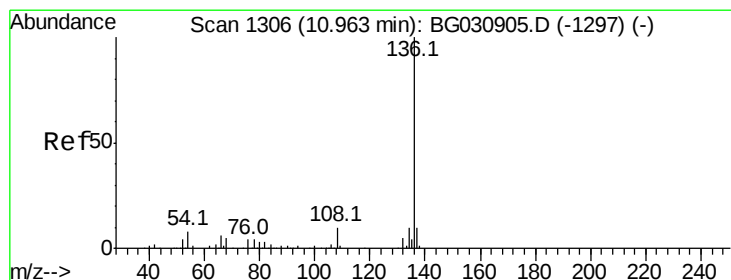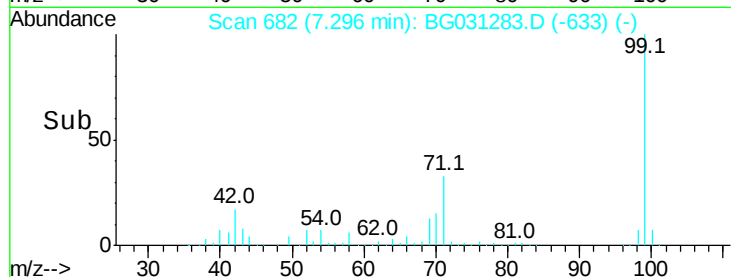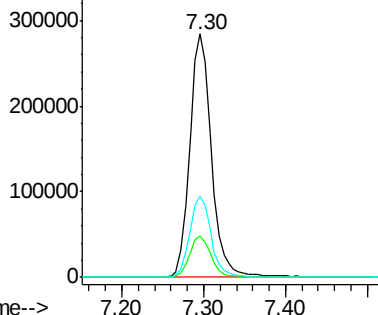

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1303

Delta R.T. -0.02 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52

Tgt Ion: 136 Resp: 235751


Ion Ratio Lower Upper

136 100



137 10.3 9.2 13.8


54 7.5 10.3 15.5#

68 6.0 4.5 6.7

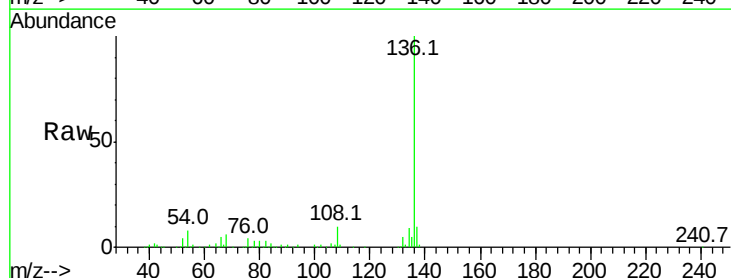

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



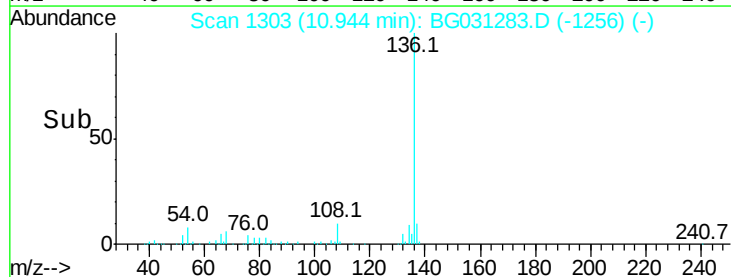
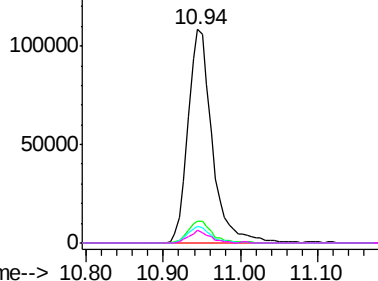


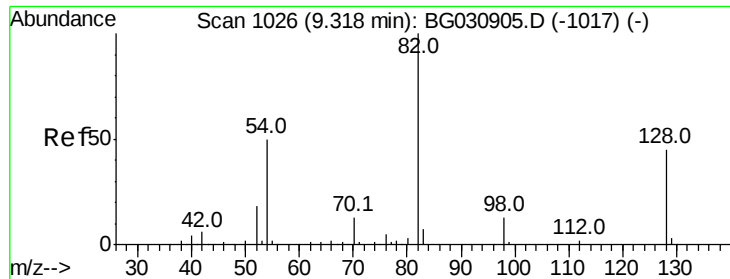

#23
Nitrobenzene-d5
Concen: 96.605 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031283.D
Acq: 29 Nov 2017 22:52




Instrument :
BNA_G
ClientSampleId :
NB-08-112817-B


Tot Ion: 82 Resp: 384342
Ion Ratio Lower Upper
82 100
128 46.0 29.7 44.5#
54 45.9 43.1 64.7

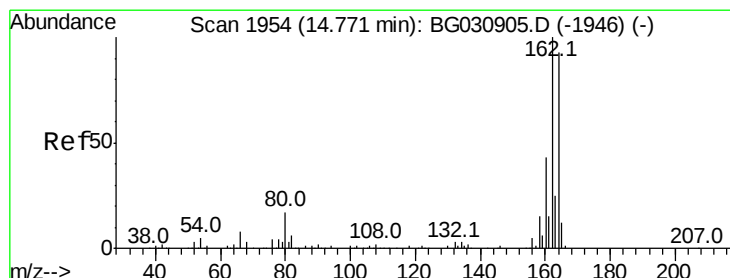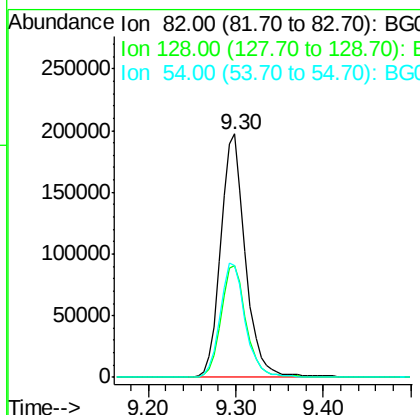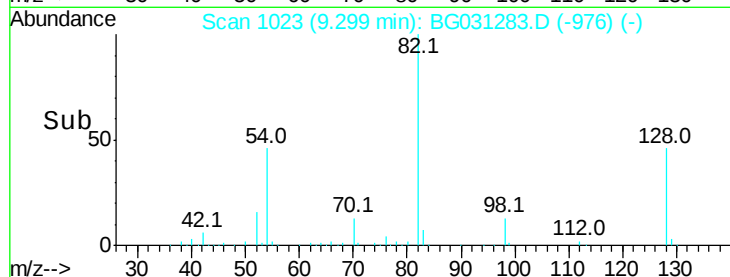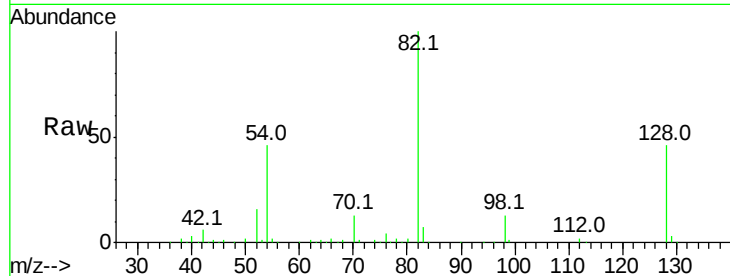

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031283.D
Acq: 29 Nov 2017 22:52

Tgt Ion:164 Resp: 156035
Ion Ratio Lower Upper
164 100
162 103.8 78.8 118.2
160 46.4 35.4 53.0

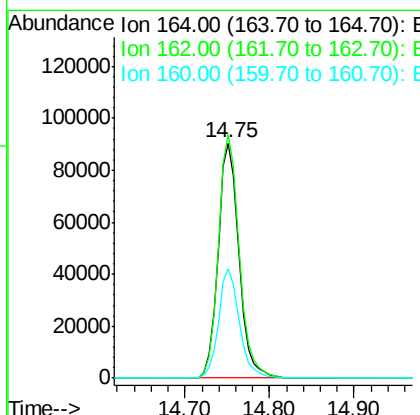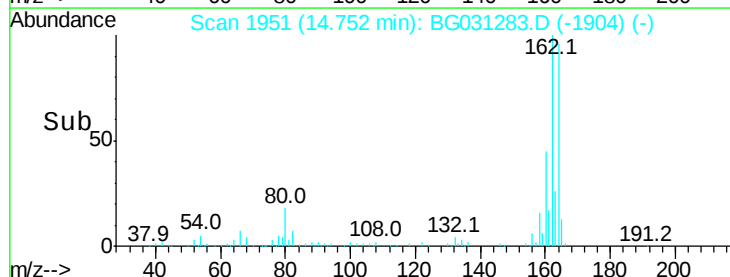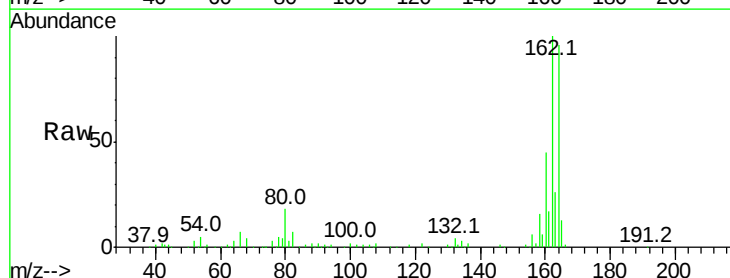


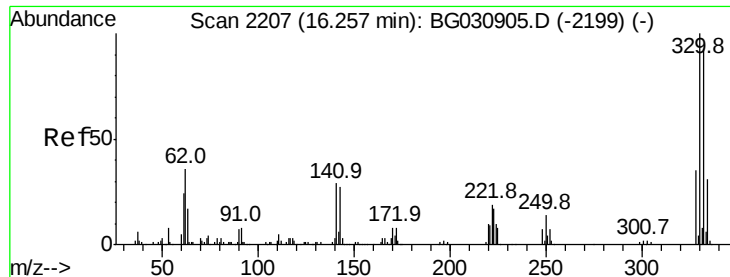




#41
 2,4,6-Tribromophenol
 Concen: 133.802 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031283.D
 Acq: 29 Nov 2017 22:52

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-112817-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.1	77.0	115.6
141	35.0	25.2	37.8

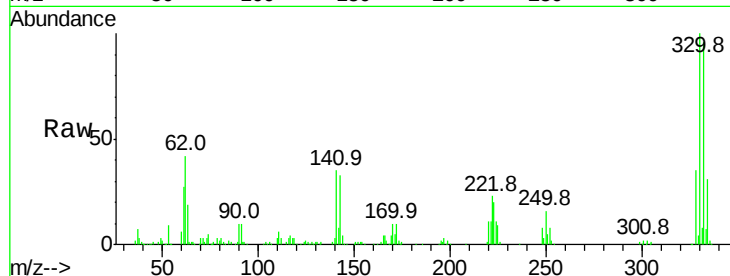


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

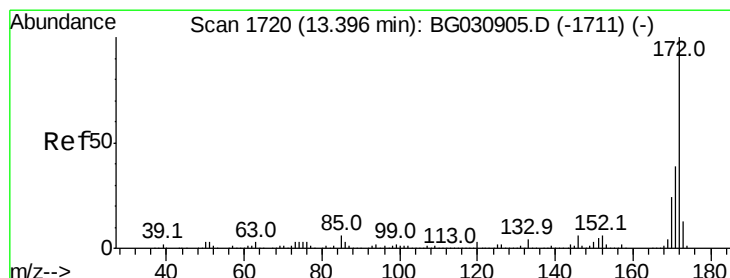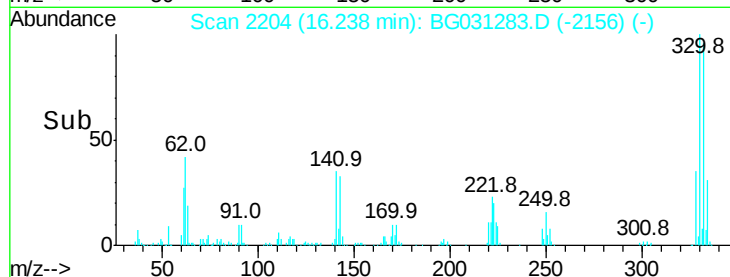
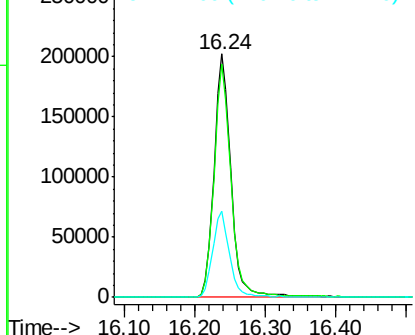



#44
 2-Fluorobiphenyl
 Concen: 102.816 ng
 RT: 13.37 min Scan# 1716
 Delta R.T. -0.03 min
 Lab File: BG031283.D
 Acq: 29 Nov 2017 22:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.0	30.0	45.0
170	24.1	19.5	29.3

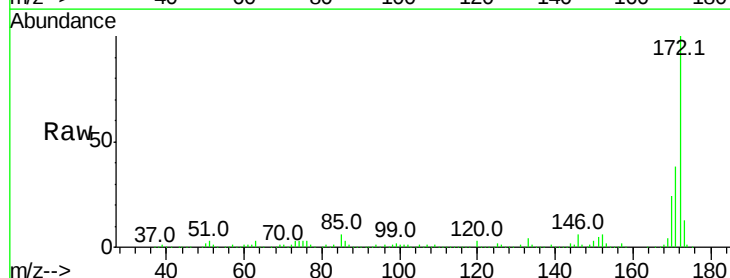

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

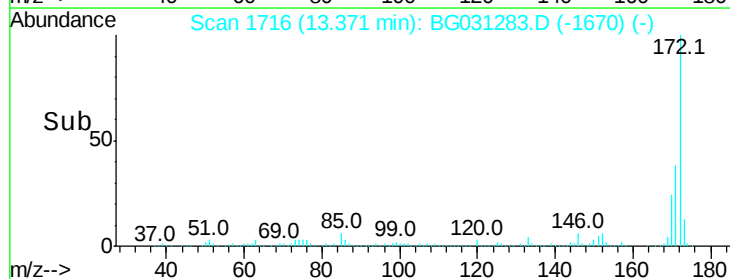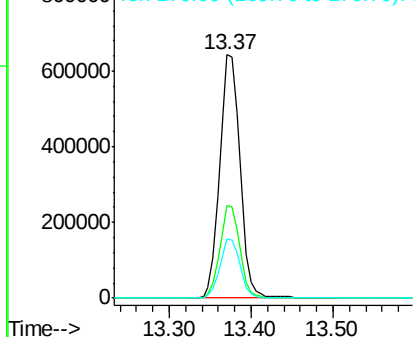

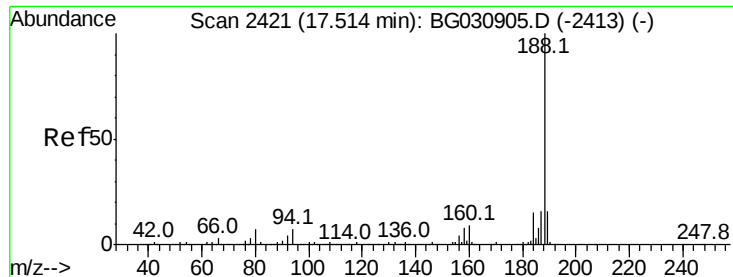

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.50 min Scan# 2418

Delta R.T. -0.02 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52

Instrument :

BNA_G

ClientSampleId :

NB-08-112817-B


Tot Ion:188 Resp: 435232

Ion Ratio Lower Upper

188 100

94 6.9 6.9 10.3




80 7.4 7.7 11.5#

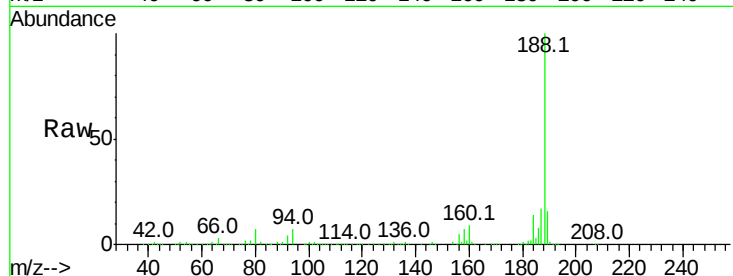

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

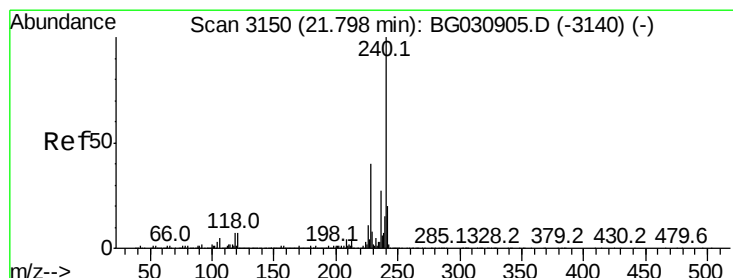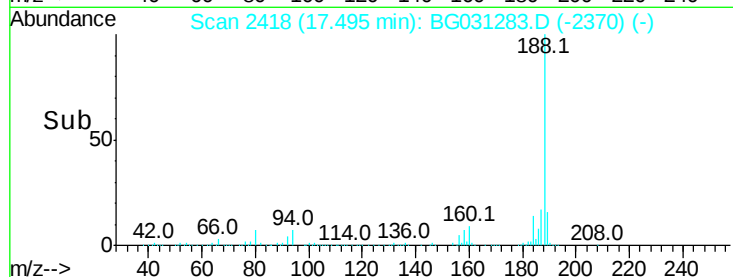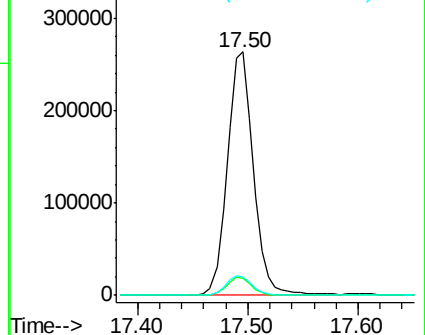

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.76 min Scan# 3144

Delta R.T. -0.02 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52


Tgt Ion:240 Resp: 533651

Ion Ratio Lower Upper

240 100

120 8.0 6.8 10.2



236 26.1 20.9 31.3

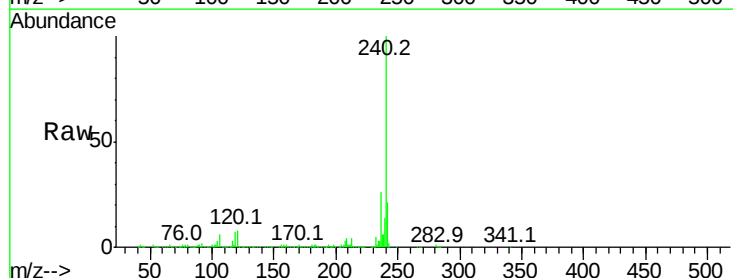


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

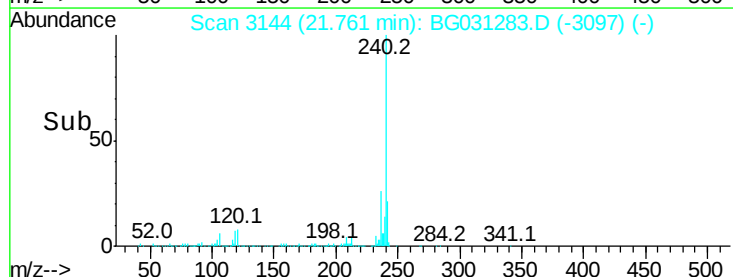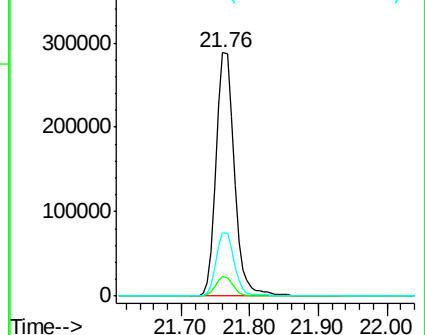

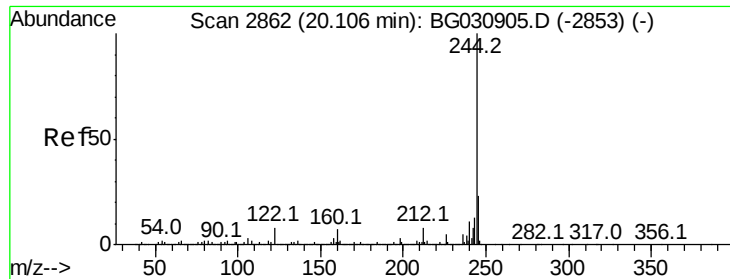

#78

Terphenyl-d14

Concen: 95.916 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52

Instrument :

BNA_G

ClientSampleId :

NB-08-112817-B


Tot Ion:244 Resp: 2318092

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#




122 9.0 7.0 10.4

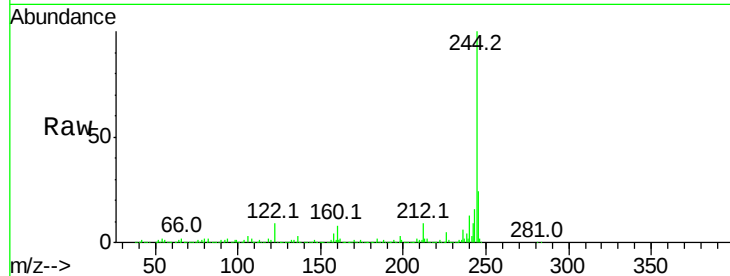

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

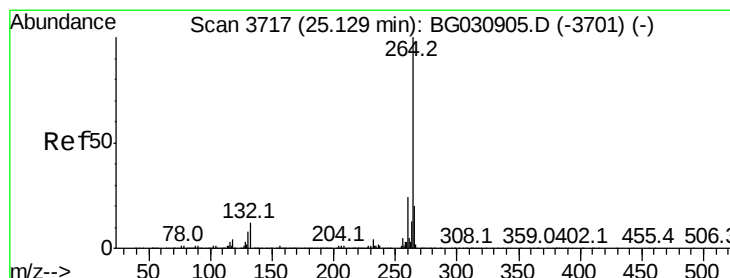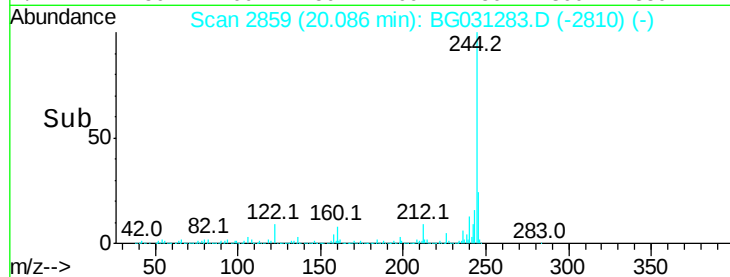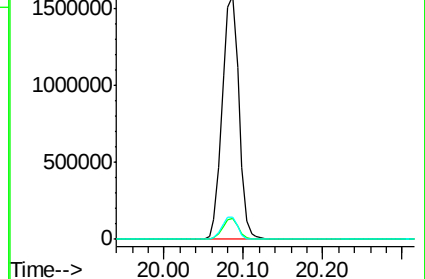

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3705

Delta R.T. -0.03 min

Lab File: BG031283.D

Acq: 29 Nov 2017 22:52


Tgt Ion:264 Resp: 512125

Ion Ratio Lower Upper

264 100

260 22.9 17.4 26.0

265 20.6 17.7 26.5

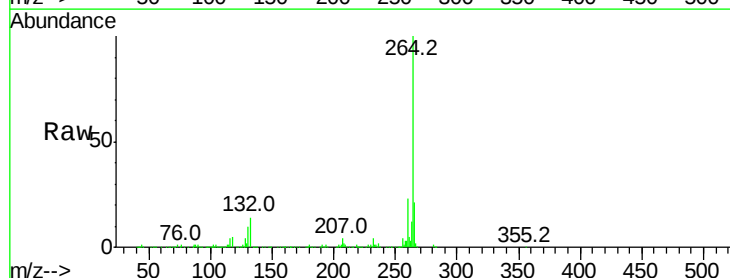

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

