


Data Path : Z:\HPCHEM1\BNA G\Data\BG112917\
 Data File : BG031269.D
 Acq On : 29 Nov 2017 14:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

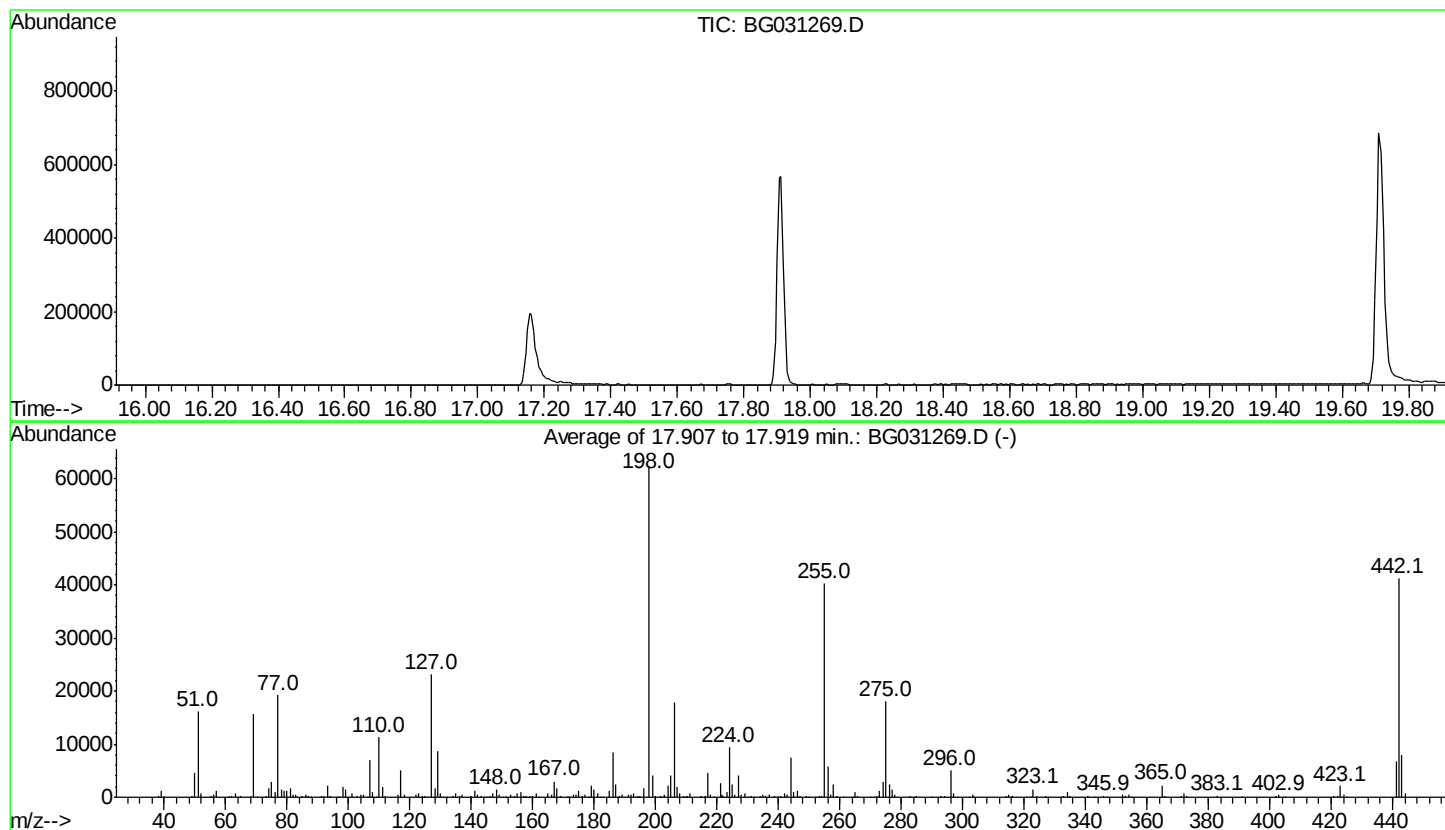

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	16049	PASS
68	69	0.00	2	1.0	163	PASS
69	198	0.00	100	25.1	15661	PASS
70	69	0.00	2	0.5	84	PASS
127	198	10	80	37.0	23144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62482	PASS
199	198	5	9	6.7	4217	PASS
275	198	10	60	28.9	18084	PASS
365	198	1	100	3.6	2263	PASS
441	442	0.01	24	16.2	6664	PASS
442	198	50	100	66.0	41210	PASS
443	442	15	24	19.5	8025	PASS