


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112918\
 Data File : BG038233.D
 Acq On : 29 Nov 2018 15:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

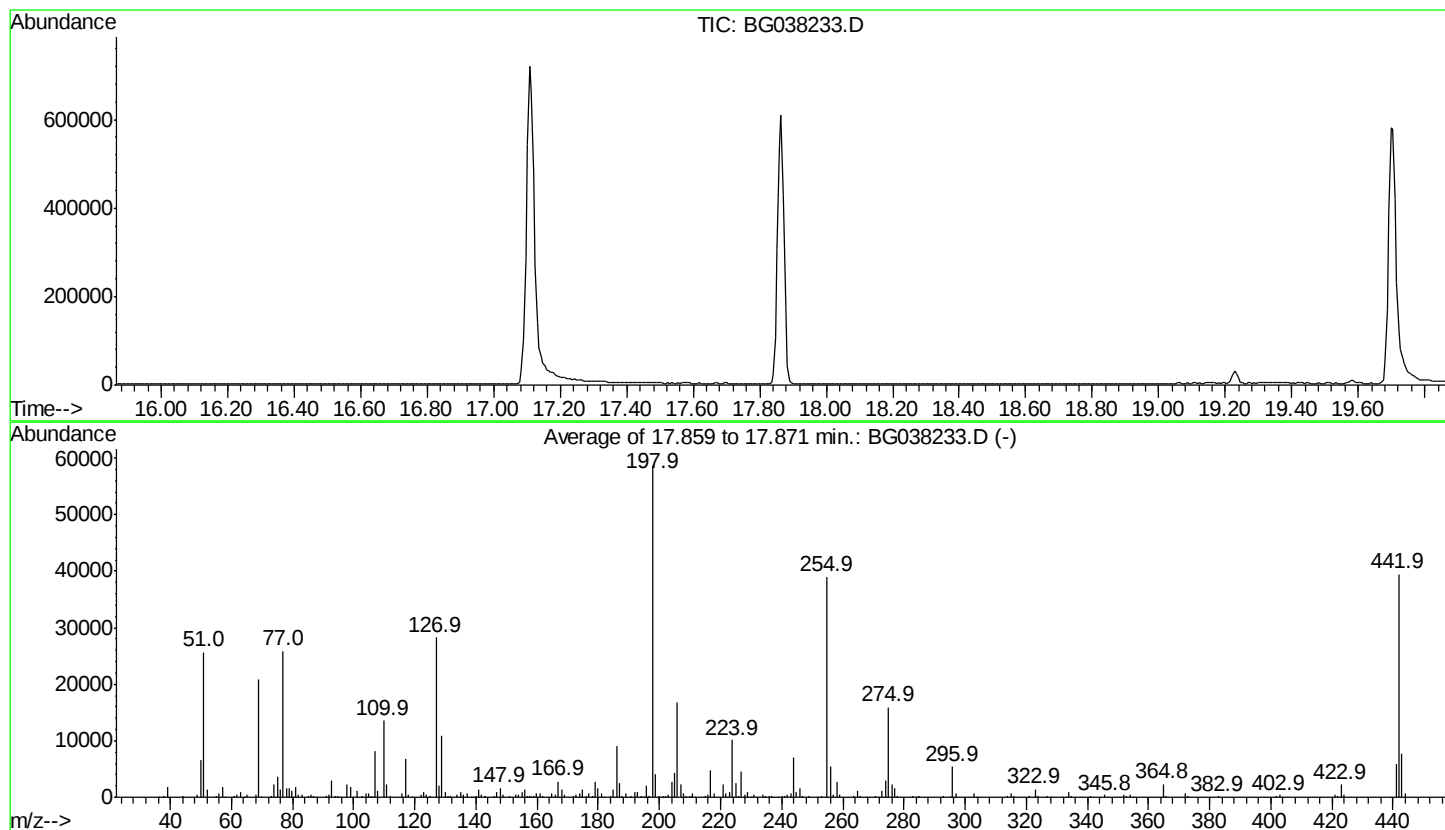

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	25610	PASS
68	69	0.00	2	1.8	370	PASS
69	198	0.00	100	35.5	20806	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	48.2	28269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58658	PASS
199	198	5	9	7.0	4103	PASS
275	198	10	60	27.1	15883	PASS
365	198	1	100	4.0	2327	PASS
441	198	0.01	100	10.1	5934	PASS
442	198	50	100	67.3	39474	PASS
443	442	15	24	19.6	7727	PASS