
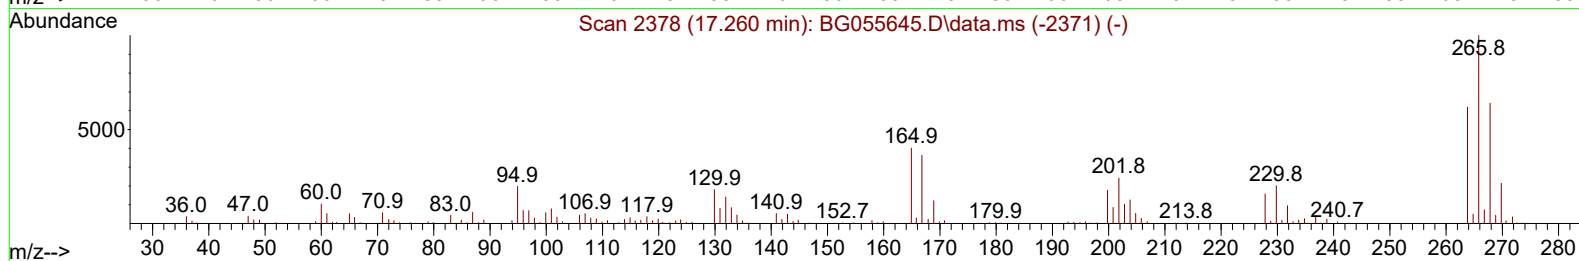
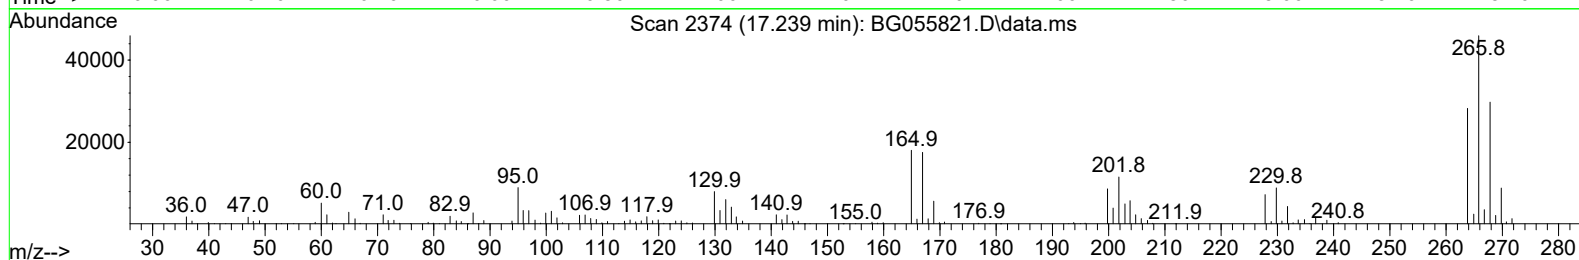


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112922\
Data File : BG055821.D
Acq On : 29 Nov 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 10:11:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

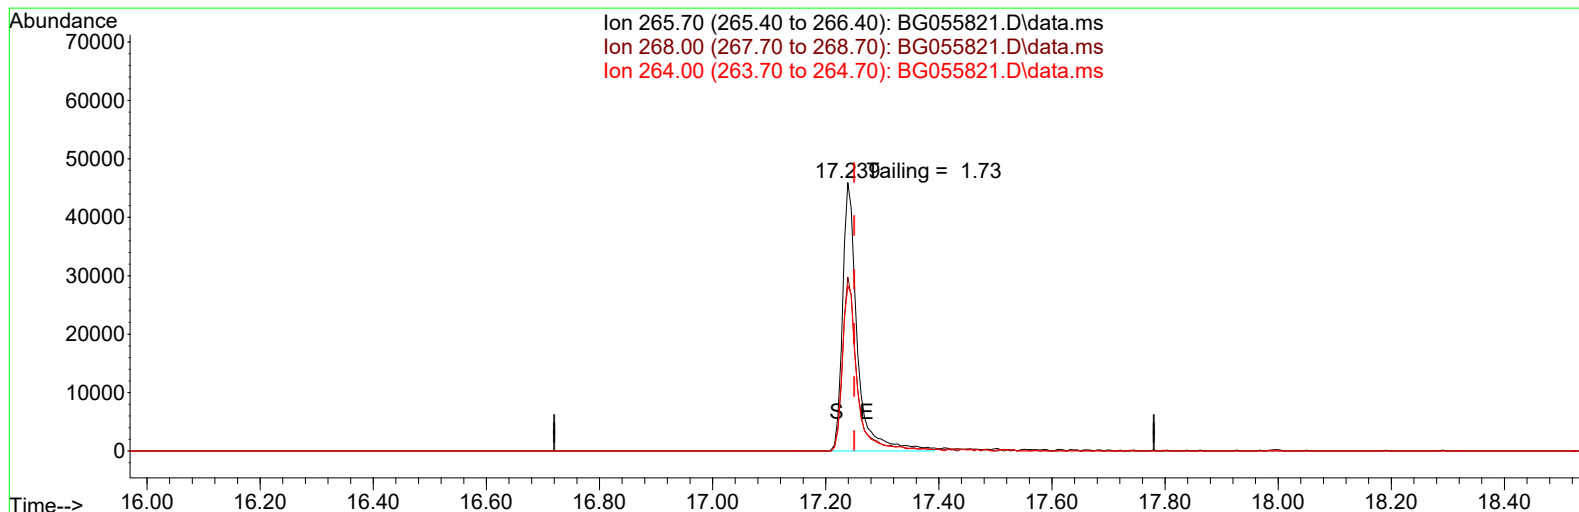

TIC: BG055821.D\data.ms

(70) Pentachlorophenol (C)




17.239min (-0.011) 58507.56 ng

response 83653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.77
264.00	61.90	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112922\
 Data File : BG055821.D
 Acq On : 29 Nov 2022 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 10:11:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 02:02:15 2022
 Response via : Initial Calibration

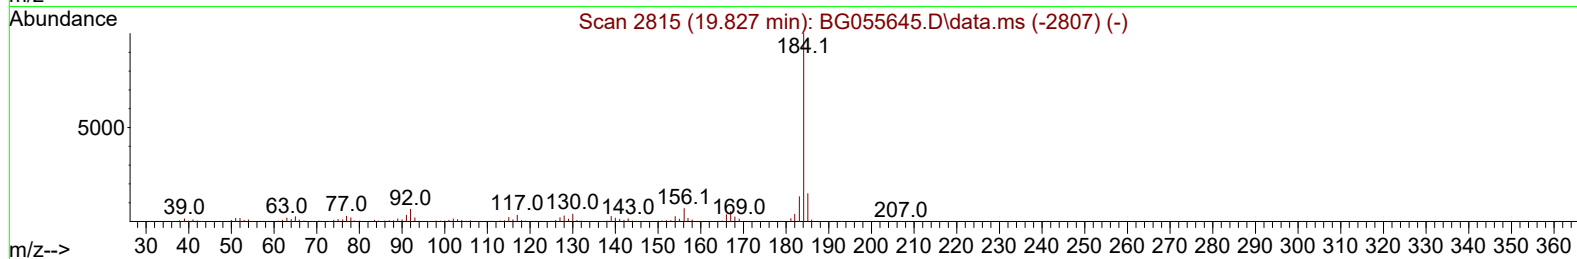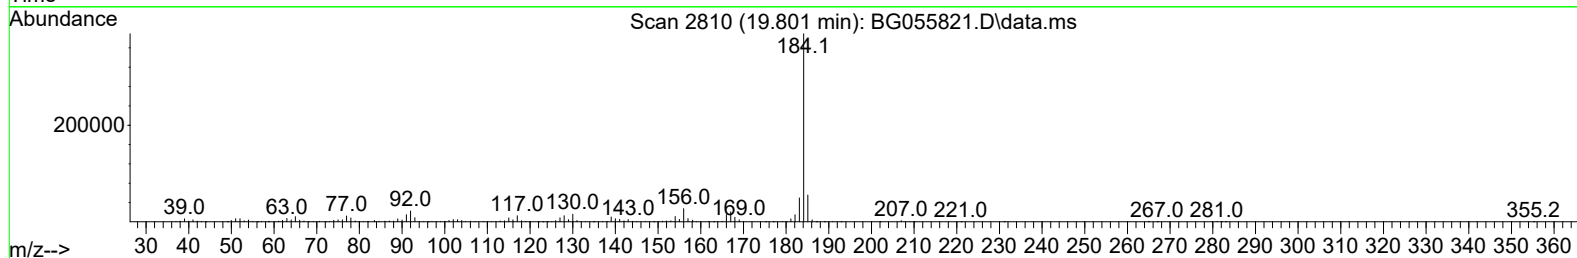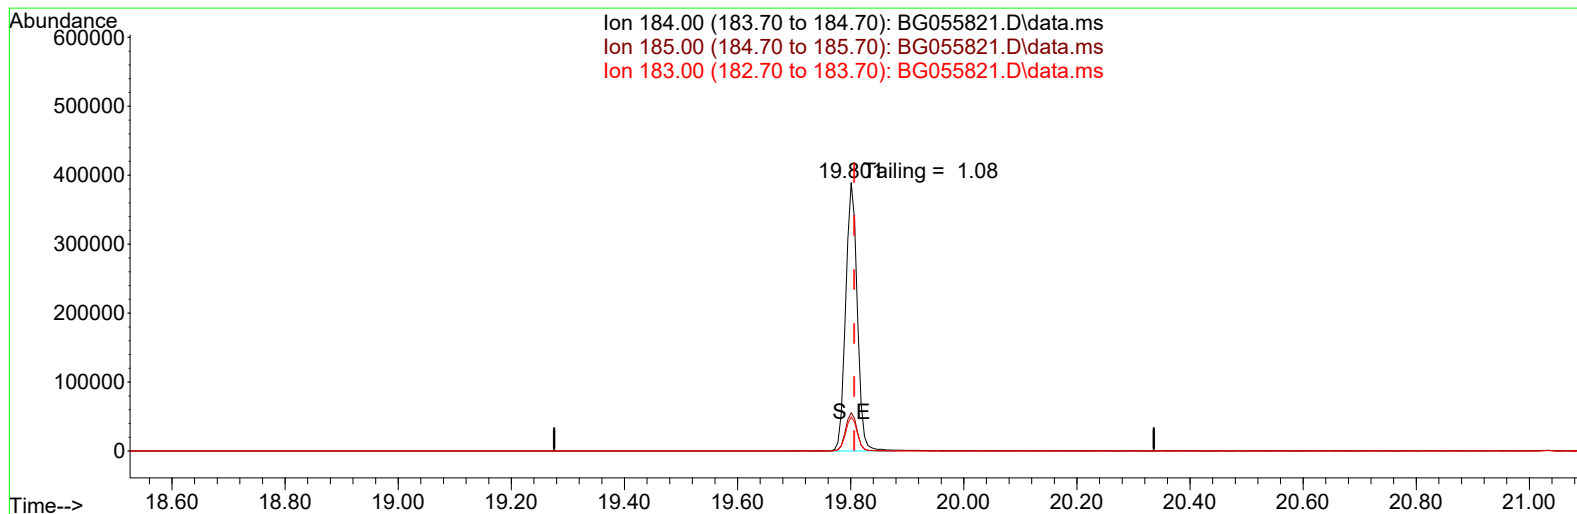

TIC: BG055821.D\data.ms

(77) Benzidine**19.801min (-0.005) 402275.44 ng****response 558386**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.25
183.00	13.20	12.72
0.00	0.00	0.00