


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112922\
 Data File : BG055821.D
 Acq On : 29 Nov 2022 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 30 02:01:09 2022

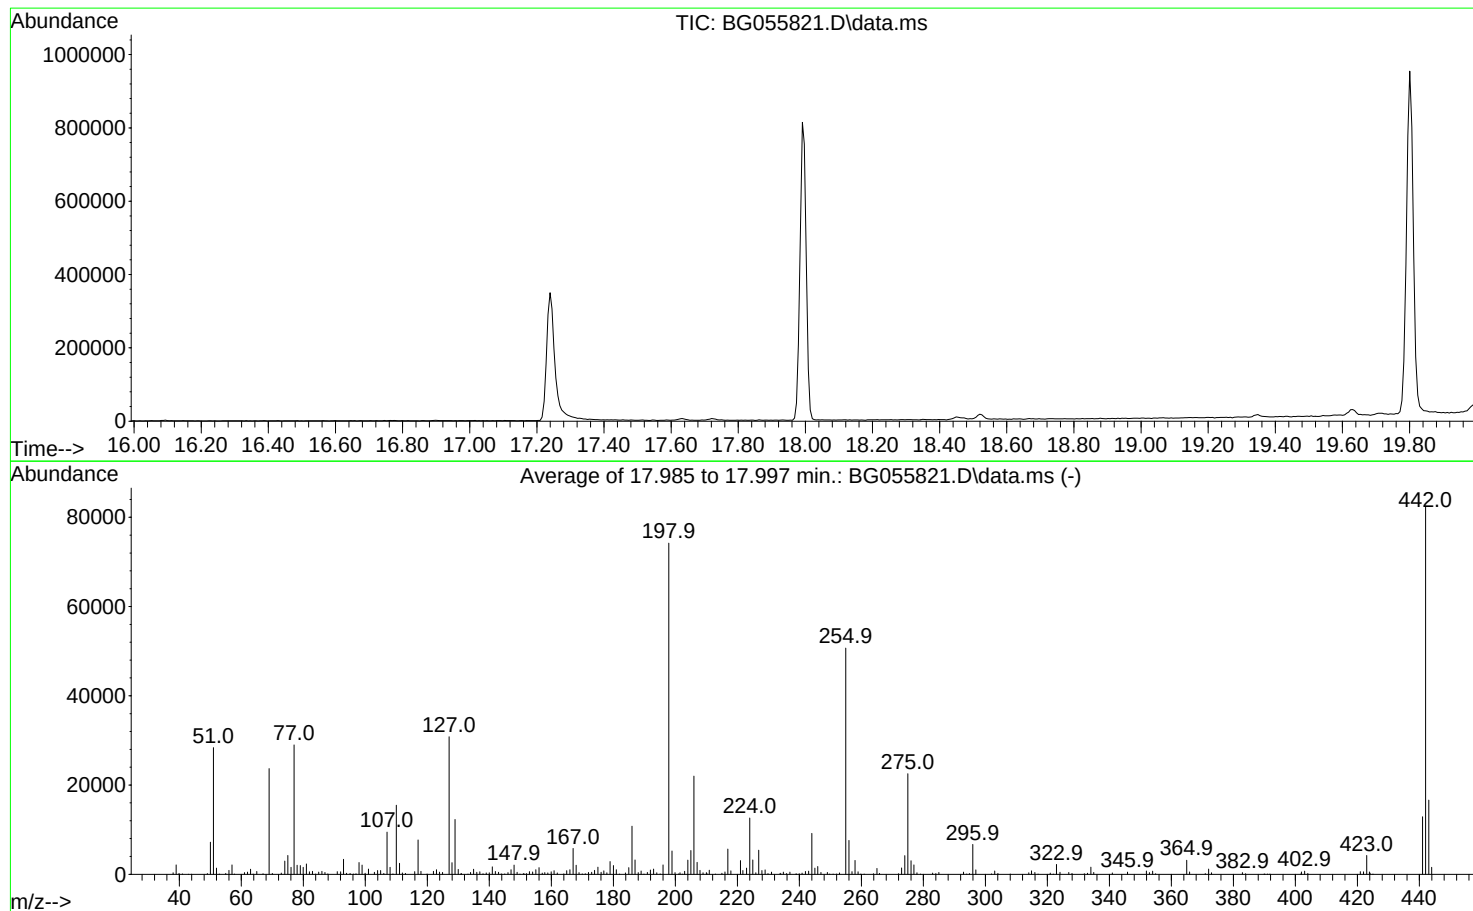




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	28395	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.9	23672	PASS
70	69	0.00	2	0.9	215	PASS
127	198	10	80	41.5	30827	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74216	PASS
199	198	5	9	7.0	5230	PASS
275	198	10	60	30.4	22546	PASS
365	198	1	100	4.2	3151	PASS
441	198	0.01	100	17.4	12892	PASS
442	442	50	100	100.0	82440	PASS
443	442	15	24	20.1	16609	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112922\
Data File : BG055821.D
Acq On : 29 Nov 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 10:11:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

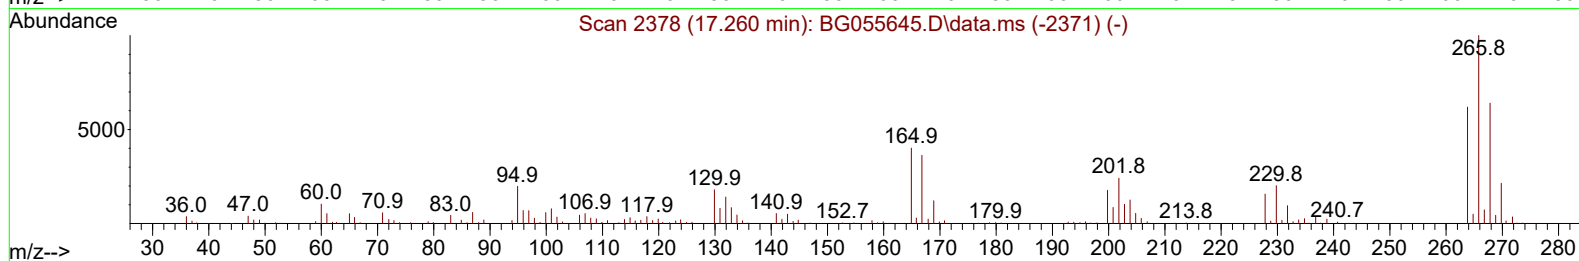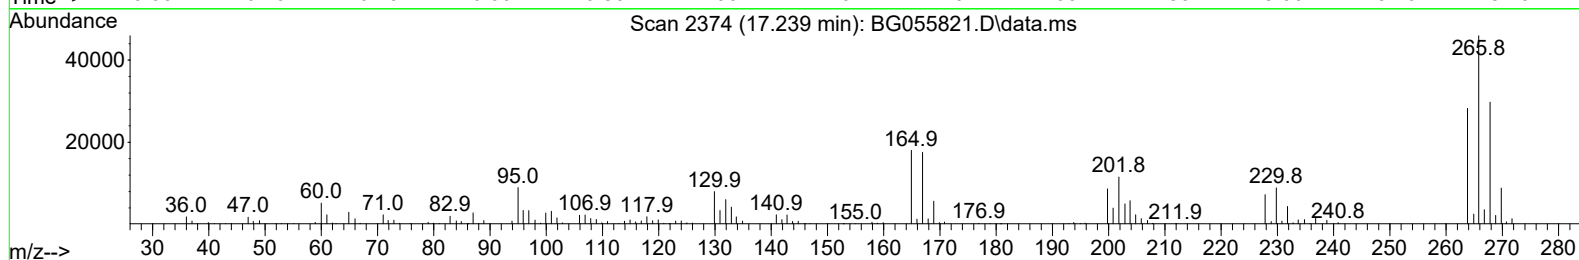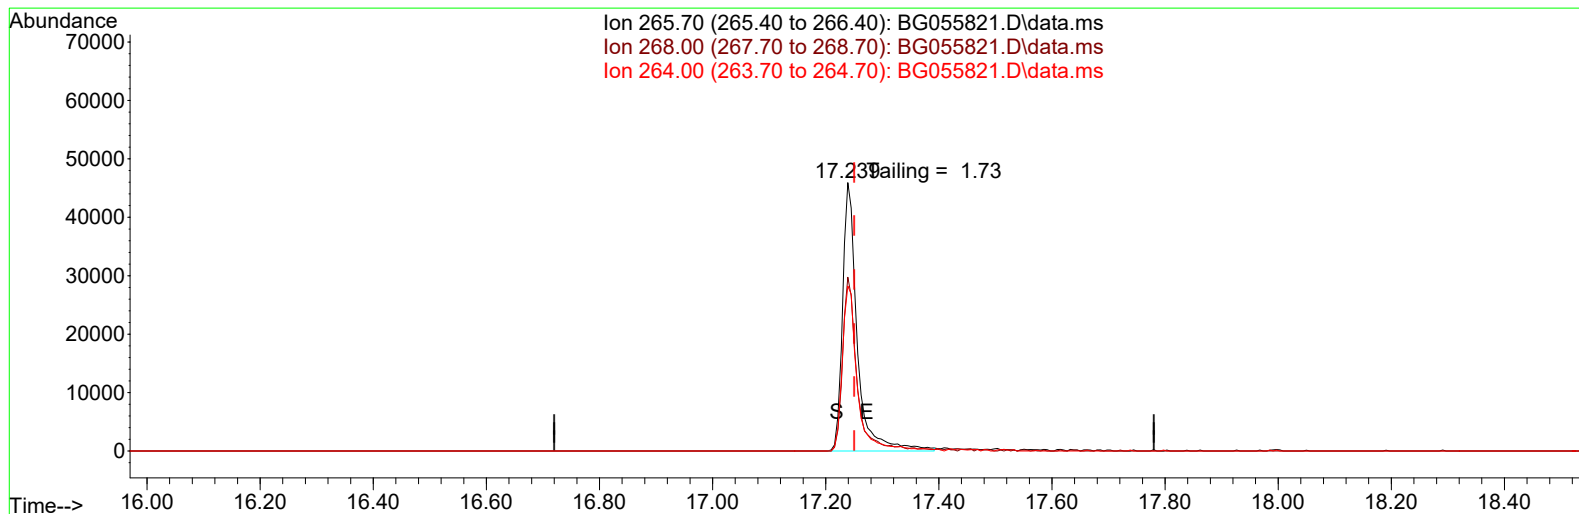

TIC: BG055821.D\data.ms

(70) Pentachlorophenol (C)

17.239min (-0.011) 58507.56 ng




response 83653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.77
264.00	61.90	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112922\
Data File : BG055821.D
Acq On : 29 Nov 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 29 10:11:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 02:02:15 2022
Response via : Initial Calibration

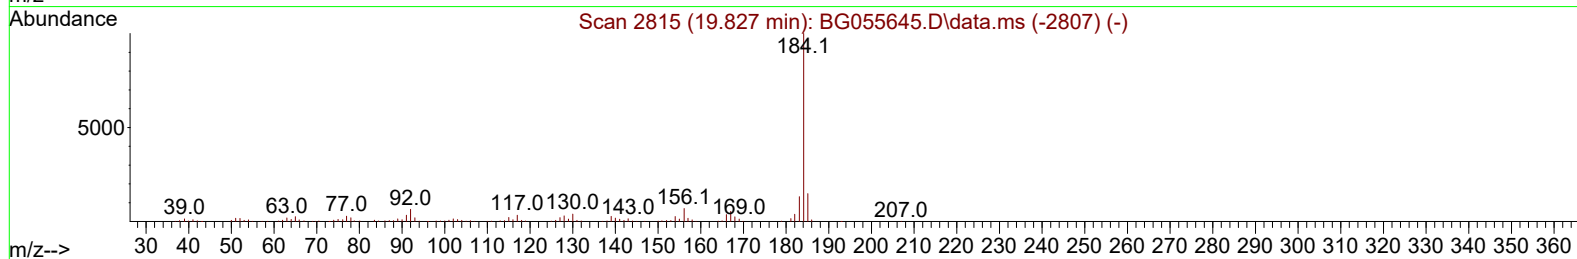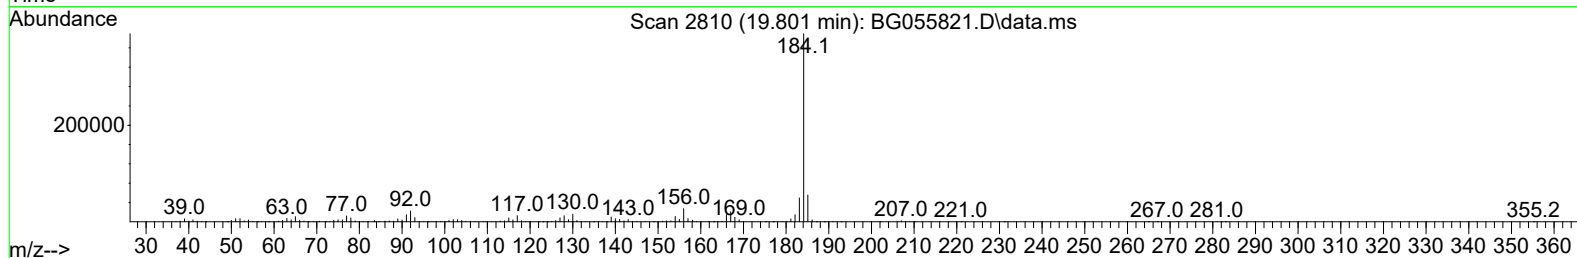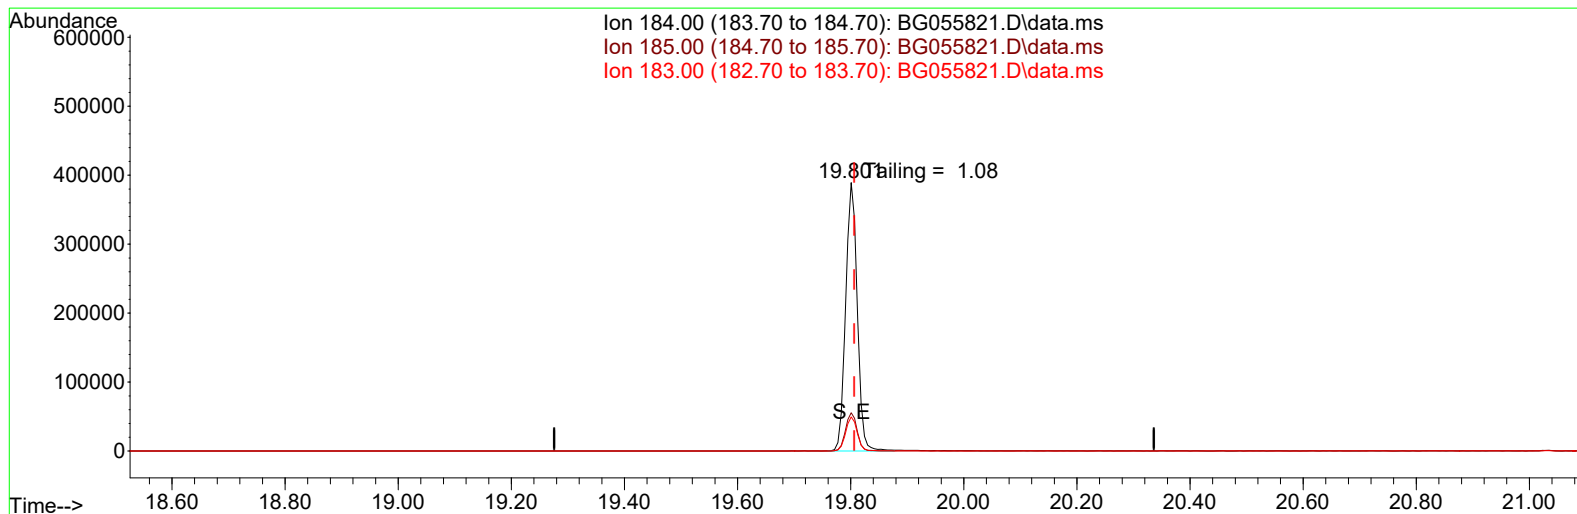

TIC: BG055821.D\data.ms

(77) Benzidine

19.801min (-0.005) 402275.44 ng

response 558386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.25
183.00	13.20	12.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2022	BNA_G	<u>BG055821.D</u>
Compound Name	Response	Retention Time
DDT	268880	21.029
DDD	5168	20.635
DDE	166	20.077
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5334	274214	1.95

Instrument :
BNA_G
ClientSampleId :
DFTPP