

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
 Data File : BG031293.D
 Acq On : 30 Nov 2017 18:30
 Operator : SJ/JU
 Sample : I6634-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 01 03:16:42 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	65179	20.00	ng	-0.02
21) Naphthalene-d8	10.95	136	272987	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	182481	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	477321	20.00	ng	-0.02
75) Chrysene-d12	21.77	240	551151	20.00	ng	-0.02
86) Perylene-d12	25.06	264	530055	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	171291	45.06	ng	-0.02
7) Phenol-d6	7.29	99	137131	26.78	ng	-0.01
23) Nitrobenzene-d5	9.30	82	422087	91.62	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	232739	78.84	ng	-0.02
44) 2-Fluorobiphenyl	13.38	172	1249186	98.36	ng	-0.02
78) Terphenyl-d14	20.09	244	2104070	84.30	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031293.D
Acq On : 30 Nov 2017 18:30
Operator : SJ/JU
Sample : I6634-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 01 03:16:42 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

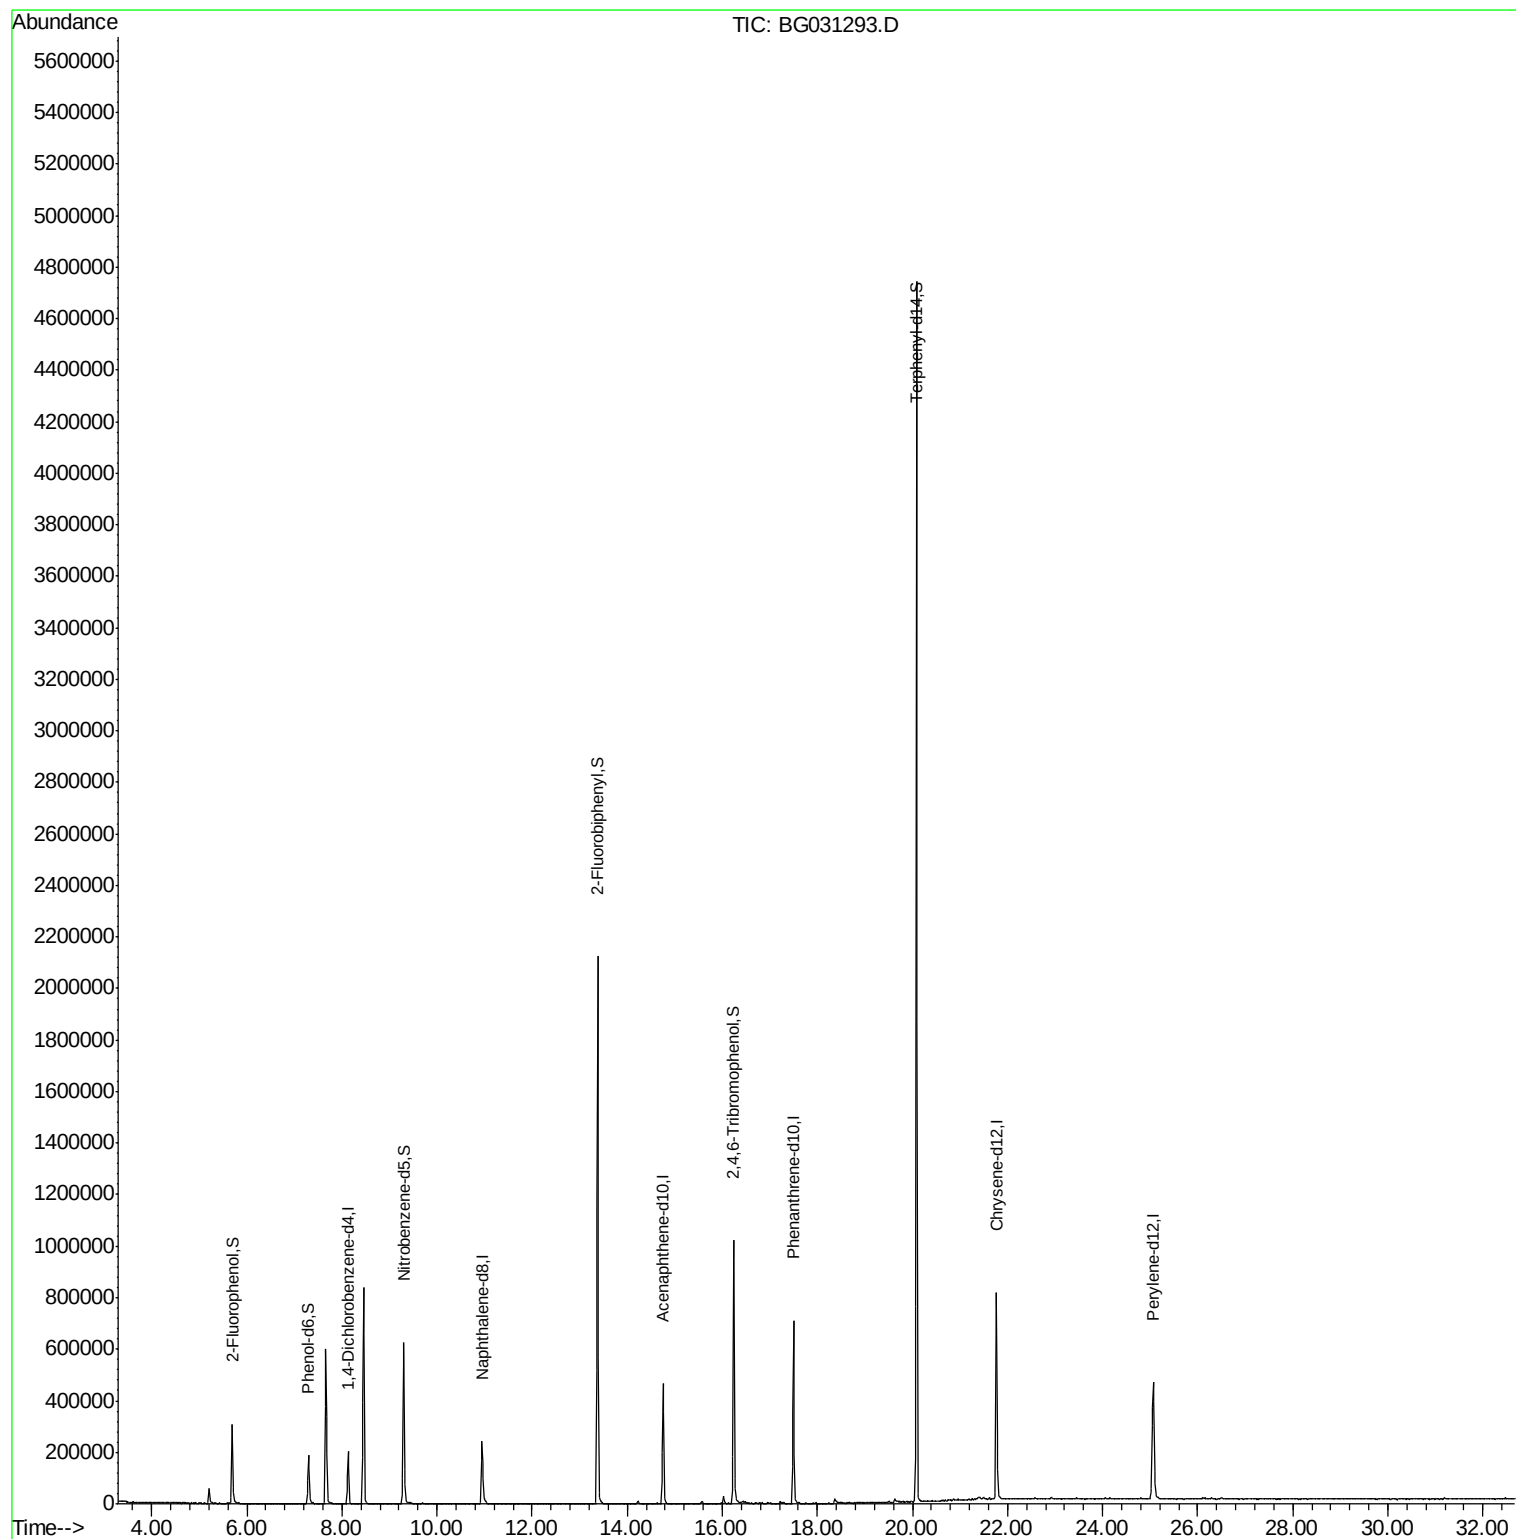




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.13 min Scan# 824
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 65179
Ion Ratio Lower Upper
152 100
150 157.1 126.6 189.8
115 55.3 53.0 79.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

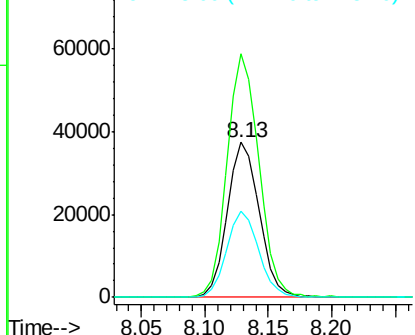



#5


2-Fluorophenol
Concen: 45.06 ng
RT: 5.69 min Scan# 409
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30

Tgt Ion:112 Resp: 171291
Ion Ratio Lower Upper
112 100
64 57.9 56.3 84.5
63 30.2 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

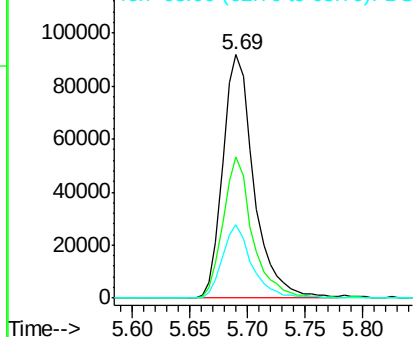

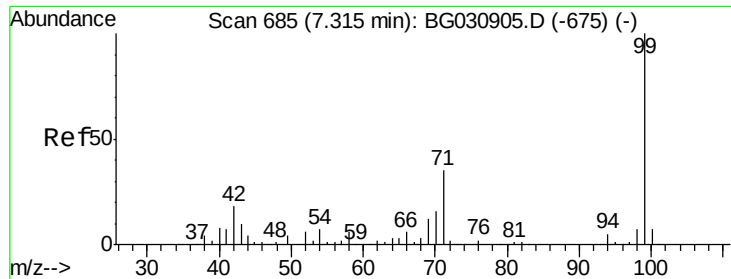

#7

Phenol-d6

Concen: 26.78 ng

RT: 7.29 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031293.D

Acq: 30 Nov 2017 18:30

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 137131

Ion Ratio Lower Upper




99 100

42 14.8 14.1 21.1

71 33.1 26.1 39.1

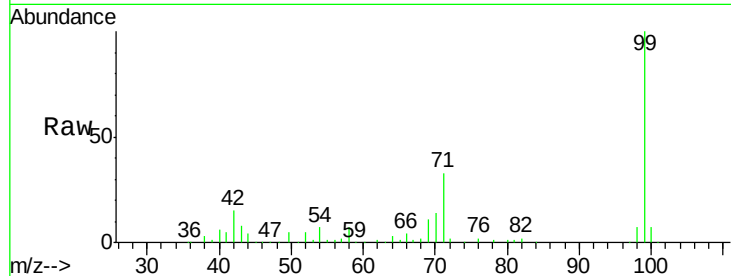

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

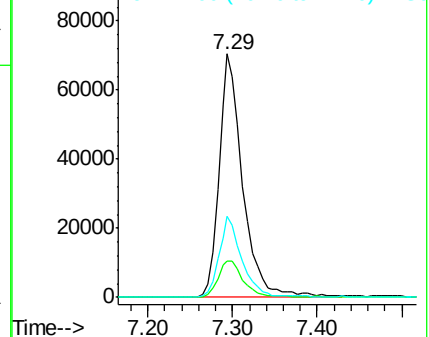

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.95 min Scan# 1304

Delta R.T. -0.02 min

Lab File: BG031293.D

Acq: 30 Nov 2017 18:30

Tgt Ion: 136 Resp: 272987


Ion Ratio Lower Upper

136 100



137 10.2 9.2 13.8


54 7.8 10.3 15.5#

68 5.1 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




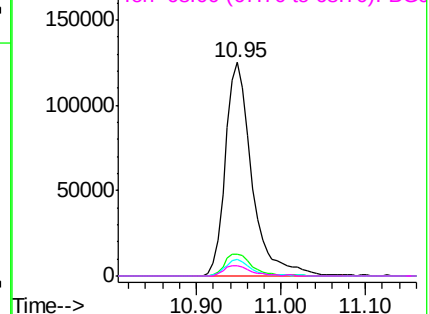




#23
Nitrobenzene-d5
Concen: 91.62 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30




Instrument :
BNA_G
ClientSampled :


Tot Ion: 82 Resp: 422087
Ion Ratio Lower Upper
82 100
128 45.8 29.7 44.5#
54 46.5 43.1 64.7

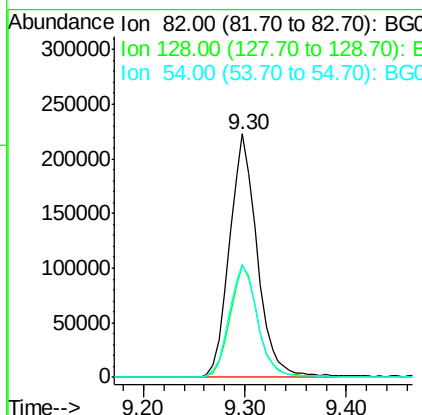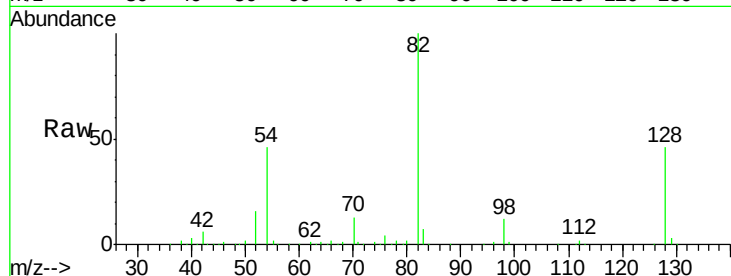

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30

Tgt Ion:164 Resp: 182481
Ion Ratio Lower Upper
164 100
162 103.8 78.8 118.2
160 43.8 35.4 53.0

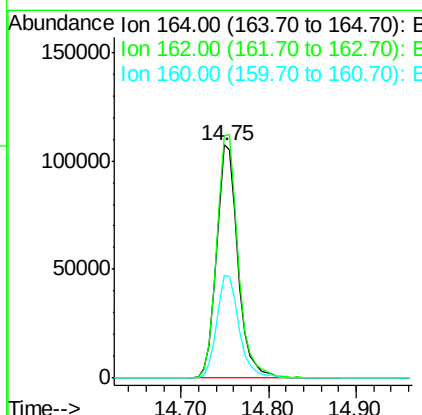


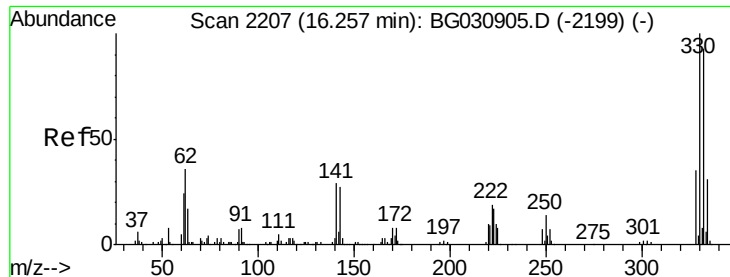




#41
 2,4,6-Tribromophenol
 Concen: 78.84 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031293.D
 Acq: 30 Nov 2017 18:30

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	77.0	115.6
141	33.8	25.2	37.8

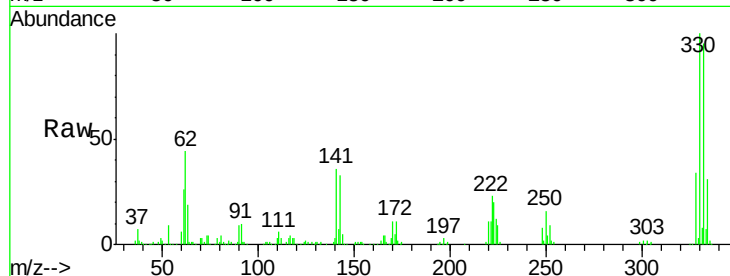


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

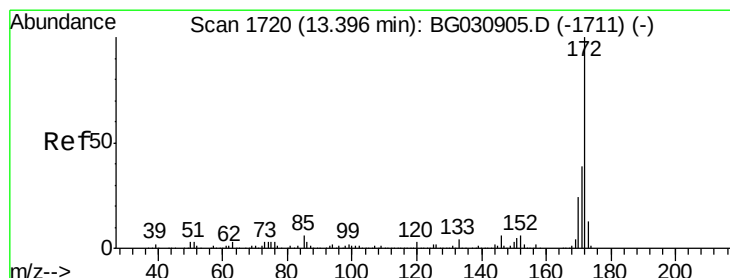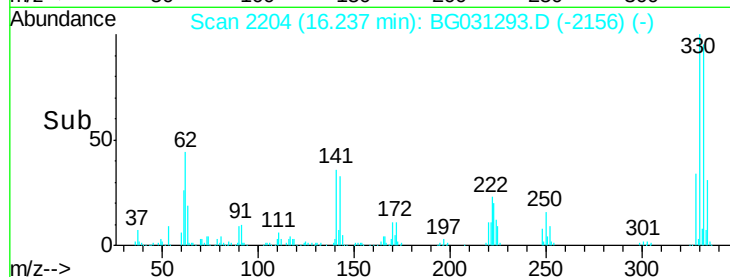
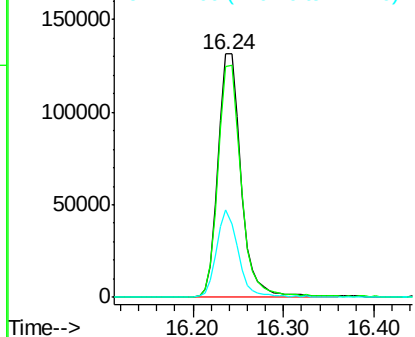



#44
 2-Fluorobiphenyl
 Concen: 98.36 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.02 min
 Lab File: BG031293.D
 Acq: 30 Nov 2017 18:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	30.0	45.0
170	23.8	19.5	29.3

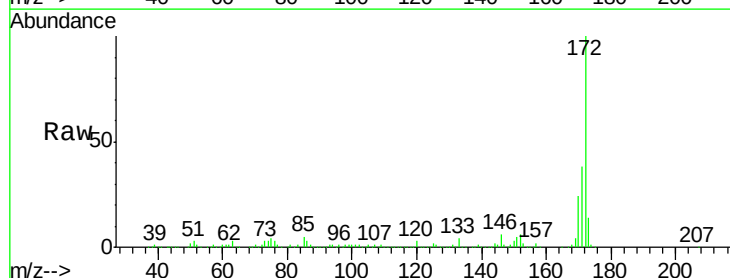

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

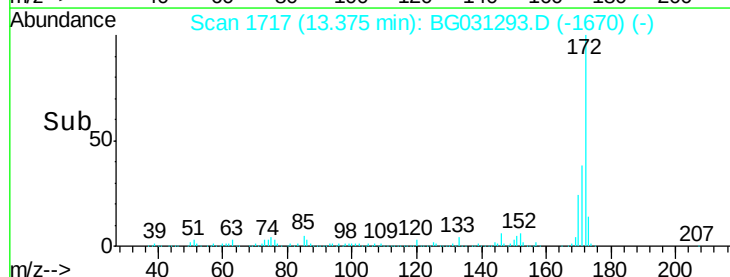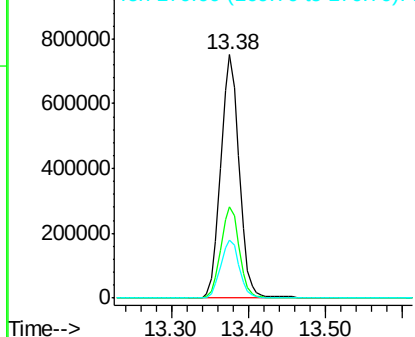







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 477321
Ion Ratio Lower Upper
188 100
94 6.9 6.9 10.3
80 8.2 7.7 11.5

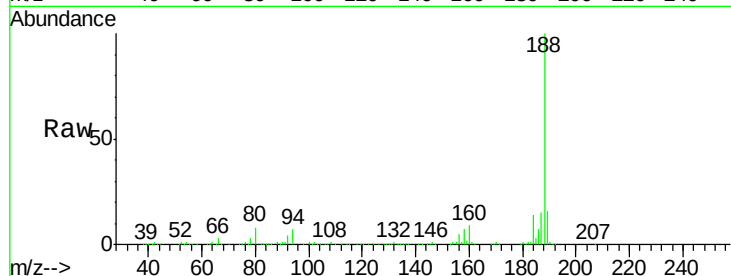


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC


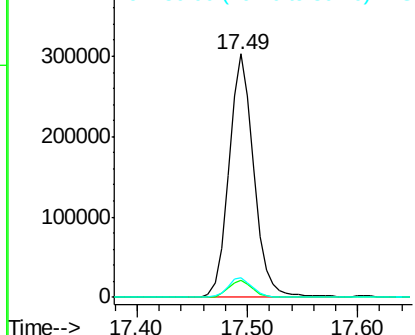



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.02 min
Lab File: BG031293.D
Acq: 30 Nov 2017 18:30

Tgt Ion:240 Resp: 551151
Ion Ratio Lower Upper
240 100
120 7.6 6.8 10.2
236 26.7 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

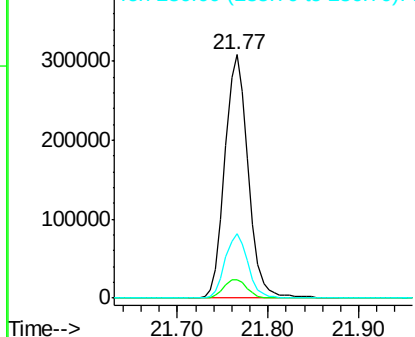

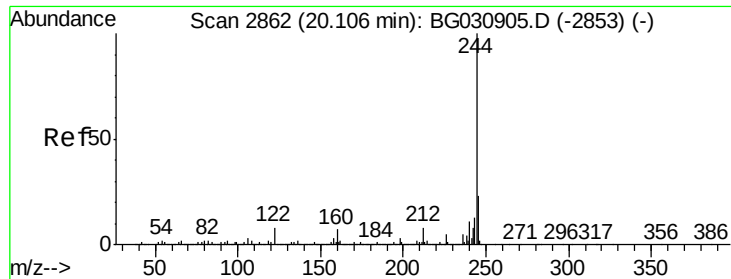

#78

Terphenyl-d14

Concen: 84.30 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031293.D

Acq: 30 Nov 2017 18:30

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 2104070

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 9.1 7.0 10.4

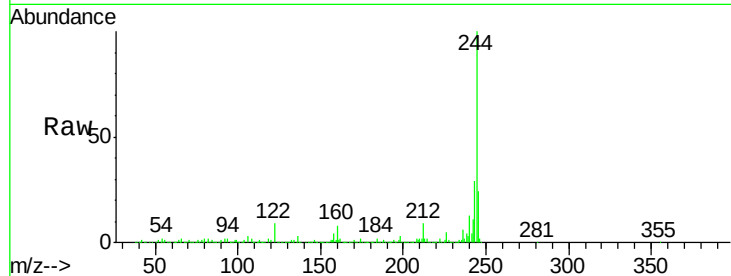

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

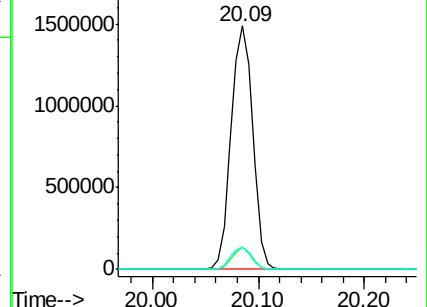

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.03 min

Lab File: BG031293.D

Acq: 30 Nov 2017 18:30


Tgt Ion:264 Resp: 530055

Ion Ratio Lower Upper

264 100

260 25.2 17.4 26.0

265 21.5 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

