

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
 Data File : BG031295.D
 Acq On : 30 Nov 2017 19:45
 Operator : SJ/JU
 Sample : I6634-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 01 03:17:22 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	145808	20.00	ng	-0.02
21) Naphthalene-d8	10.95	136	598069	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	390047	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	976343	20.00	ng	-0.02
75) Chrysene-d12	21.77	240	1102273	20.00	ng	-0.02
86) Perylene-d12	25.06	264	1110185	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	186507	21.93	ng	-0.02
7) Phenol-d6	7.30	99	150554	13.14	ng	0.00
23) Nitrobenzene-d5	9.30	82	476567	47.22	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	253160	40.12	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	1396283	51.44	ng	-0.03
78) Terphenyl-d14	20.09	244	2188186	43.83	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031295.D
Acq On : 30 Nov 2017 19:45
Operator : SJ/JU
Sample : I6634-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 01 03:17:22 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

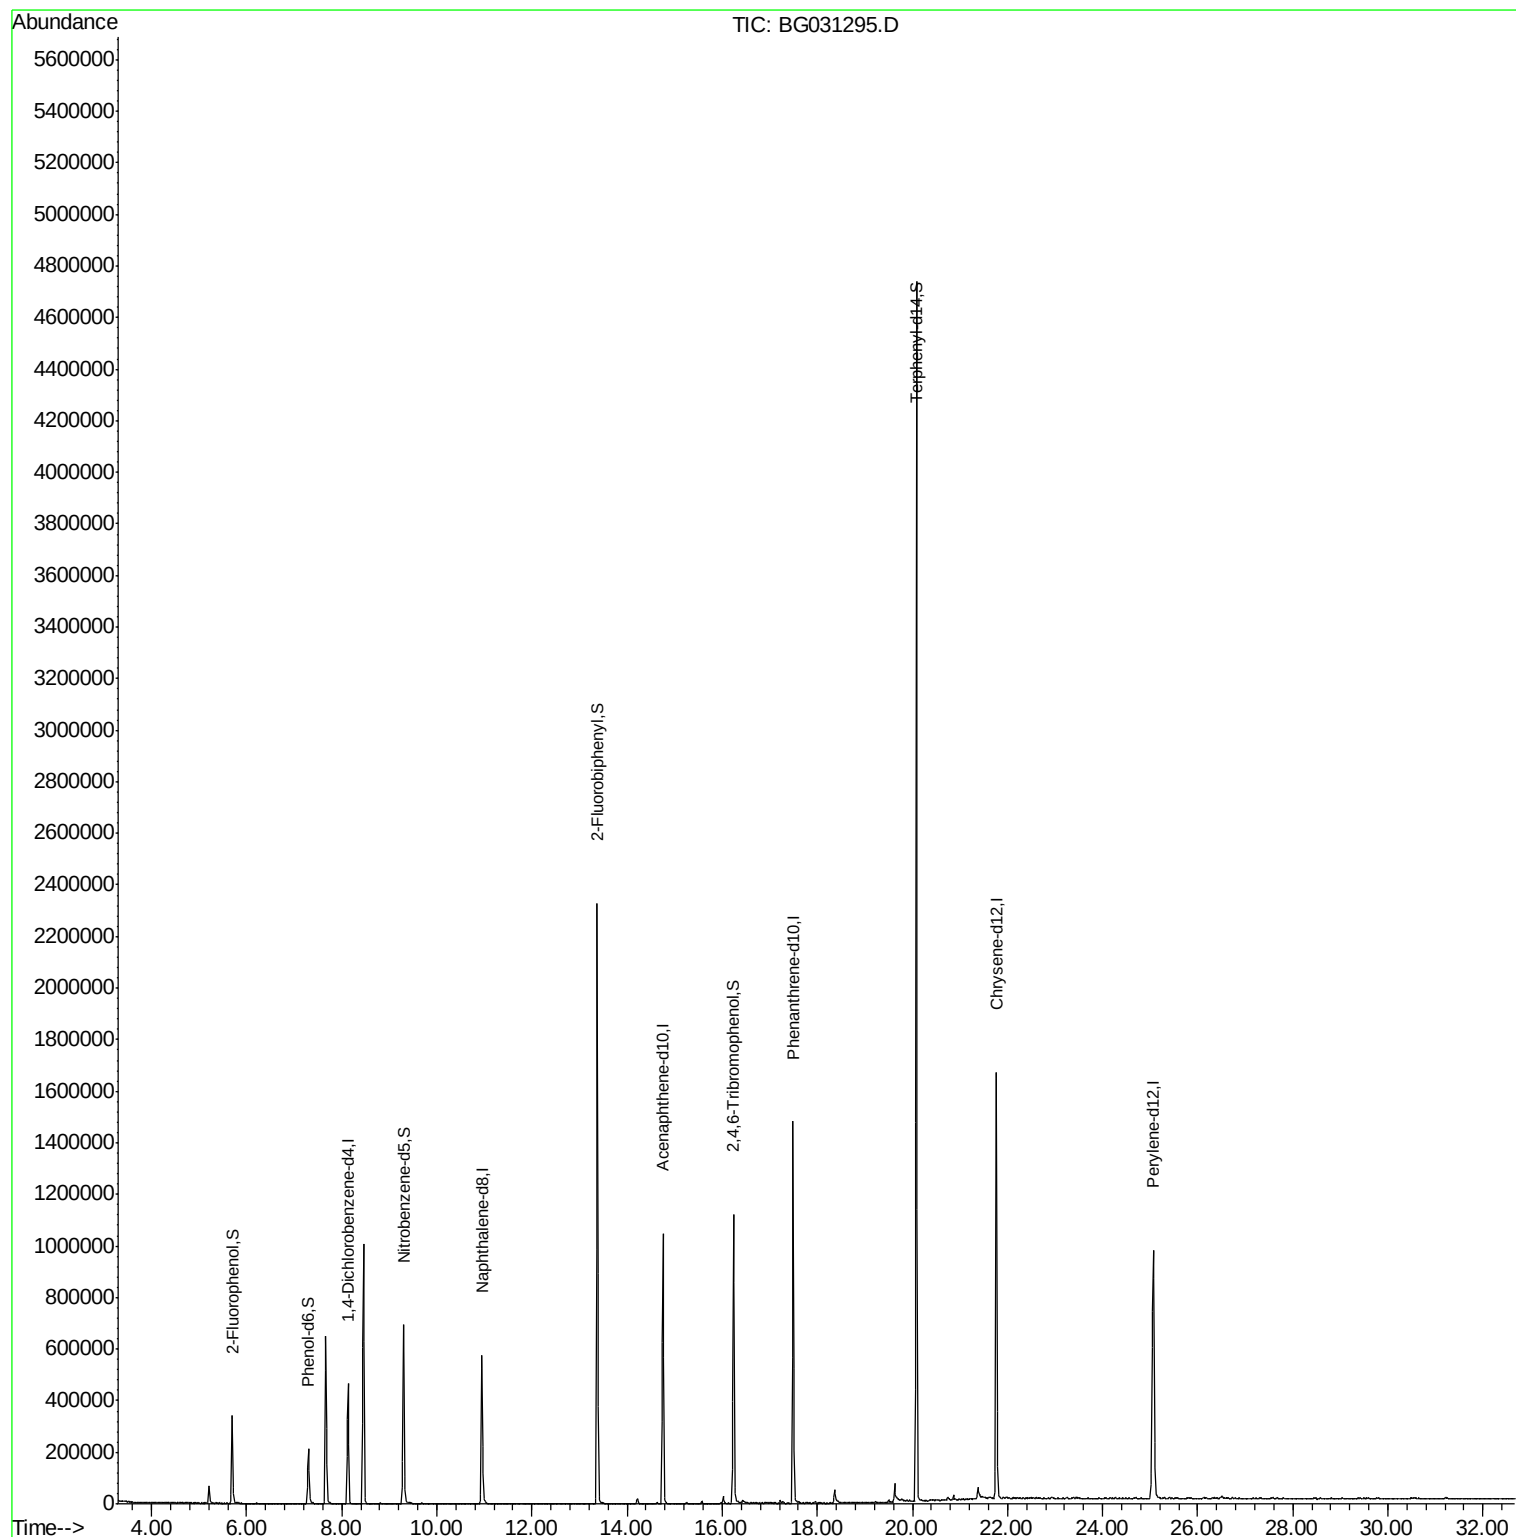

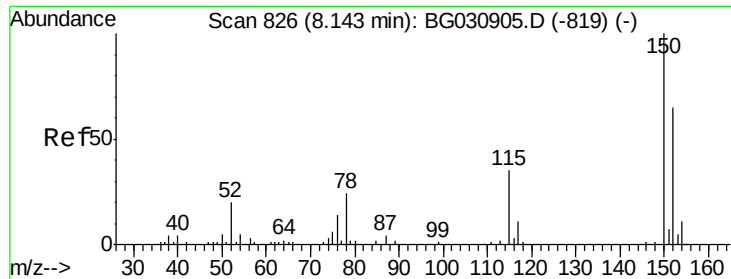


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.13 min Scan# 824
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 145808
Ion Ratio Lower Upper
152 100
150 154.2 126.6 189.8
115 56.3 53.0 79.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

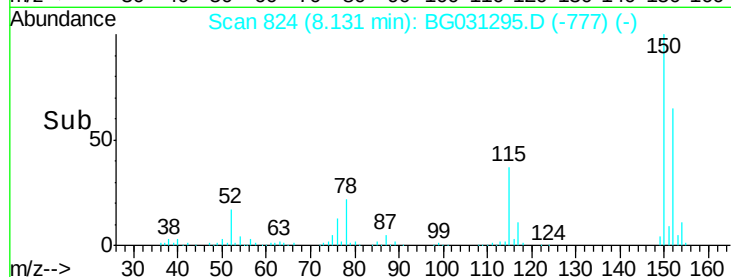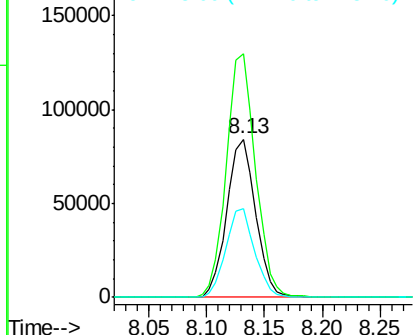



#5


2-Fluorophenol
Concen: 21.93 ng
RT: 5.69 min Scan# 409
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Tgt Ion:112 Resp: 186507
Ion Ratio Lower Upper
112 100
64 55.9 56.3 84.5#
63 27.8 30.1 45.1#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

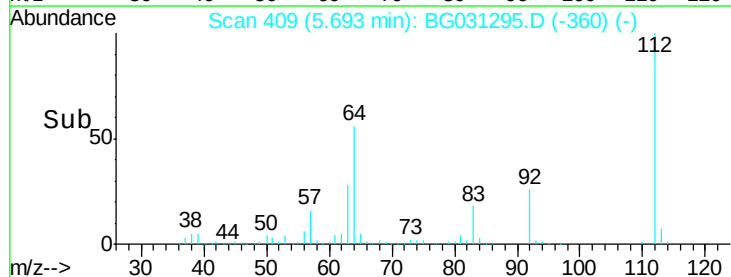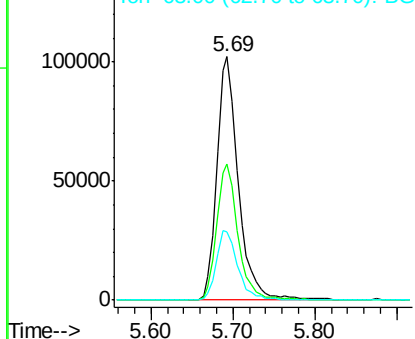

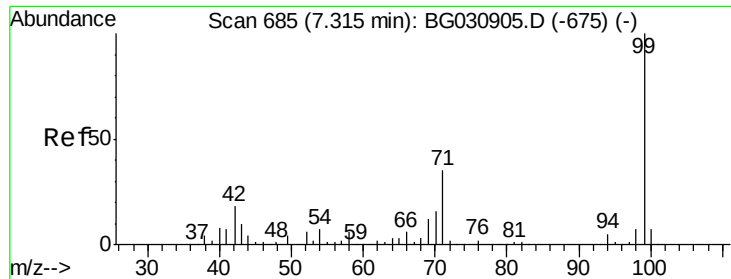

#7

Phenol-d6

Concen: 13.14 ng

RT: 7.30 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031295.D

Acq: 30 Nov 2017 19:45

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 150554

Ion Ratio Lower Upper




99 100

42 17.4 14.1 21.1

71 34.3 26.1 39.1

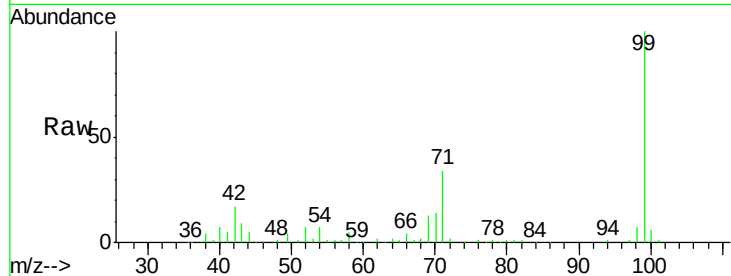

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

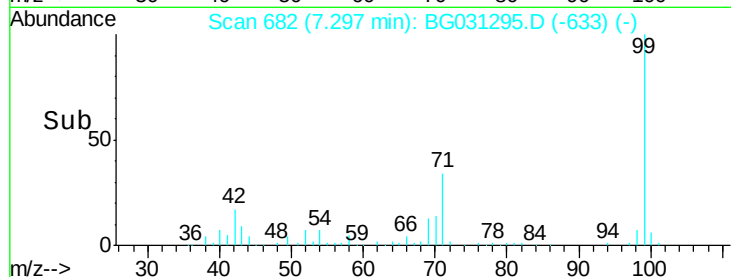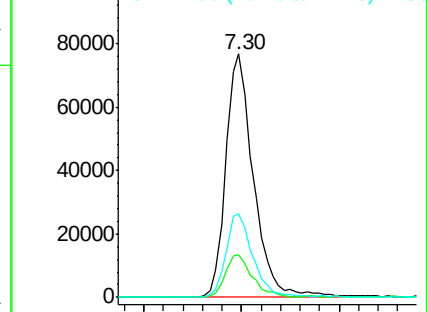

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.95 min Scan# 1303

Delta R.T. -0.02 min

Lab File: BG031295.D

Acq: 30 Nov 2017 19:45

Tgt Ion: 136 Resp: 598069


Ion Ratio Lower Upper

136 100



137 11.4 9.2 13.8


54 7.5 10.3 15.5#

68 5.4 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

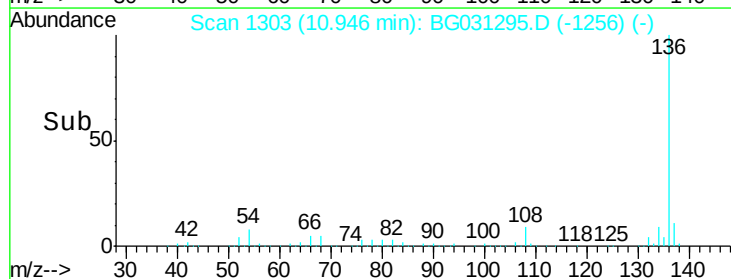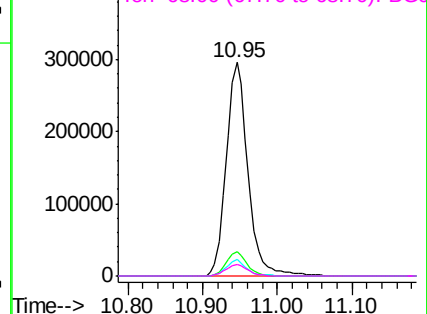


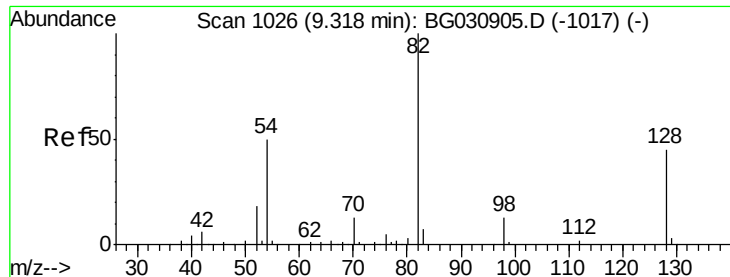




#23
Nitrobenzene-d5
Concen: 47.22 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Instrument :
BNA_G
ClientSampleId :

Tot Ion: 82 Resp: 476567
Ion Ratio Lower Upper
82 100
128 48.5 29.7 44.5#
54 48.1 43.1 64.7

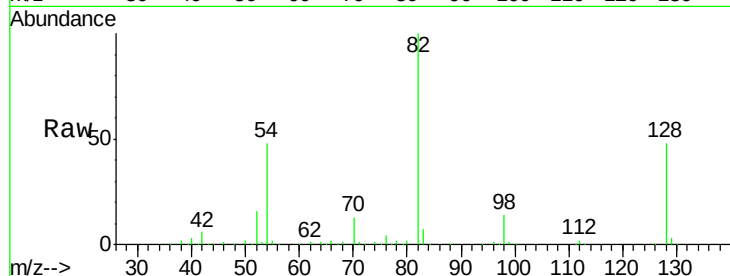


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

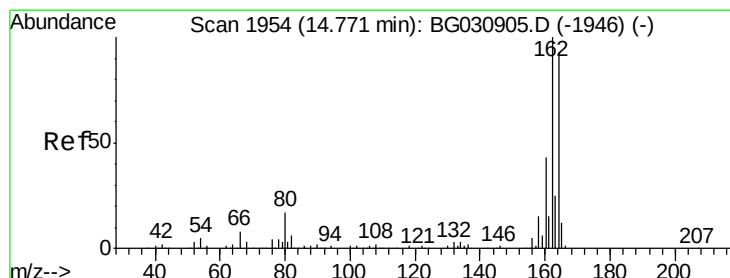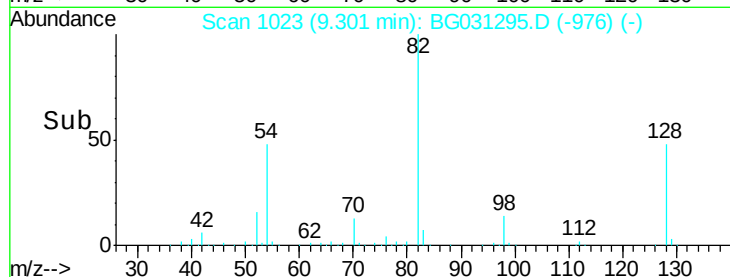
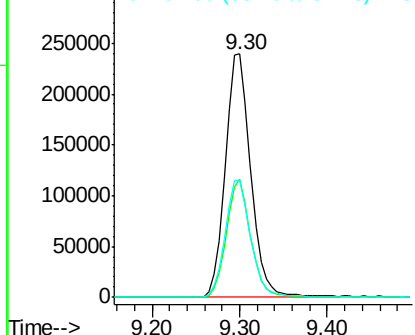



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Tgt Ion:164 Resp: 390047
Ion Ratio Lower Upper
164 100
162 107.1 78.8 118.2
160 46.5 35.4 53.0

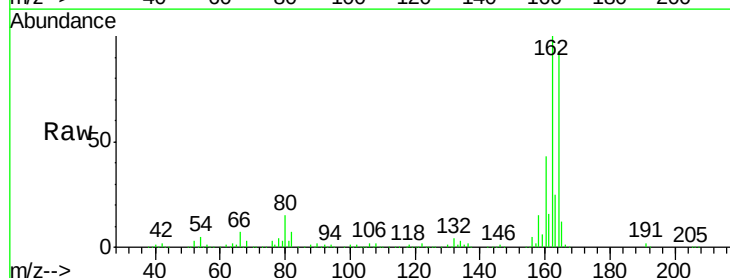

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC



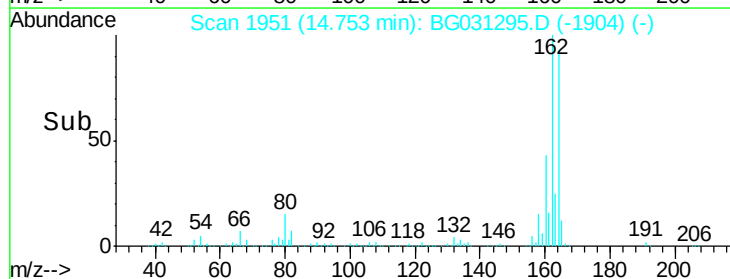
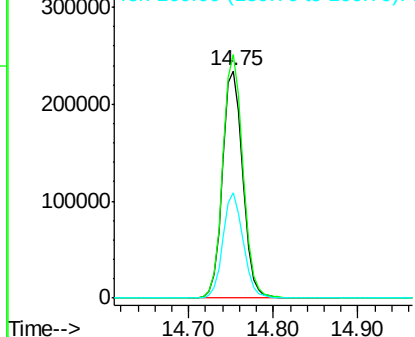


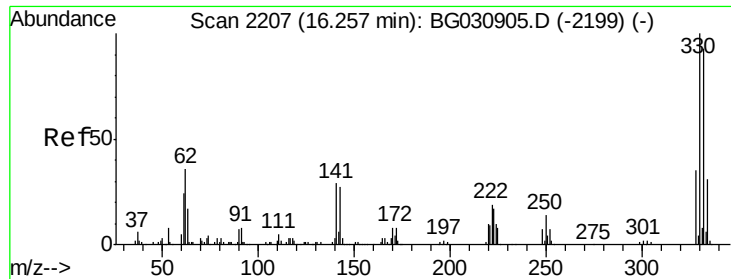

#41
 2,4,6-Tribromophenol
 Concen: 40.12 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031295.D
 Acq: 30 Nov 2017 19:45




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	77.0	115.6
141	34.7	25.2	37.8

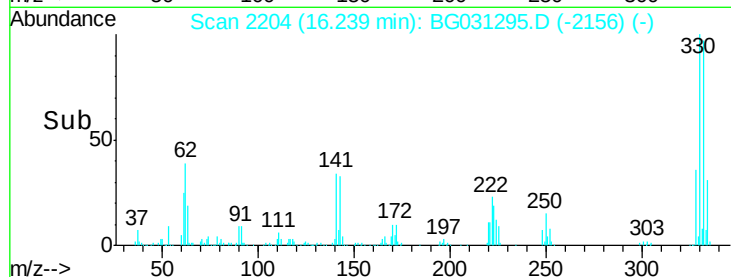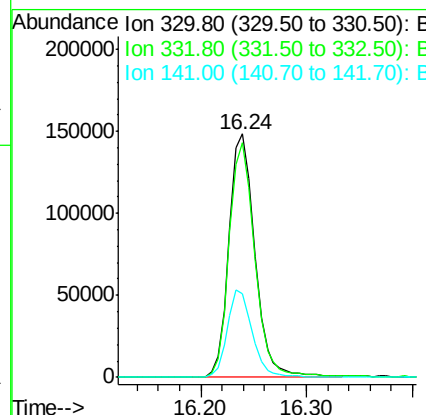

#44
 2-Fluorobiphenyl
 Concen: 51.44 ng
 RT: 13.37 min Scan# 1716
 Delta R.T. -0.03 min
 Lab File: BG031295.D
 Acq: 30 Nov 2017 19:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.1	30.0	45.0
170	24.6	19.5	29.3

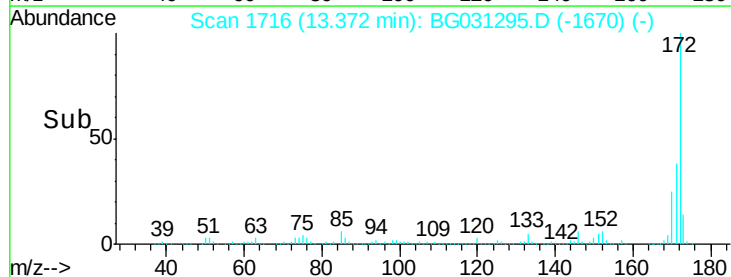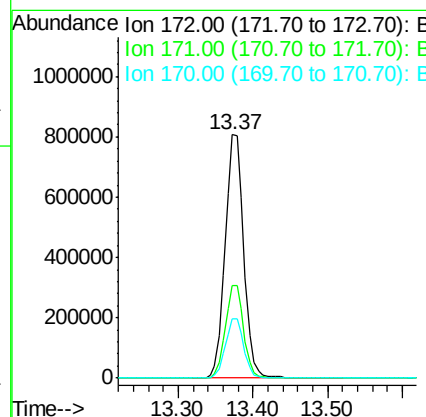


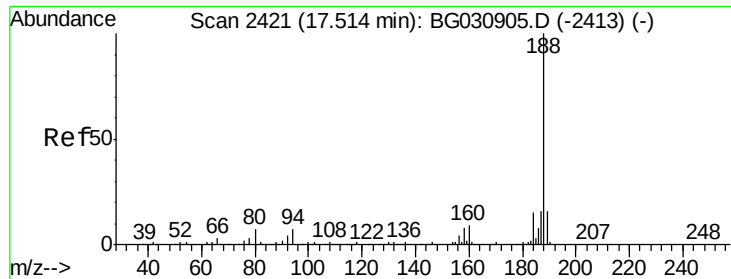




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2417
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 976343
Ion Ratio Lower Upper
188 100
94 6.9 6.9 10.3
80 7.9 7.7 11.5




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

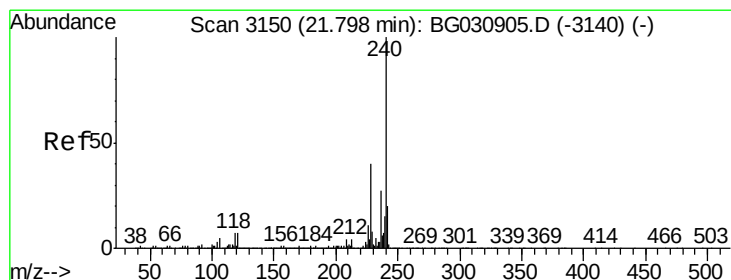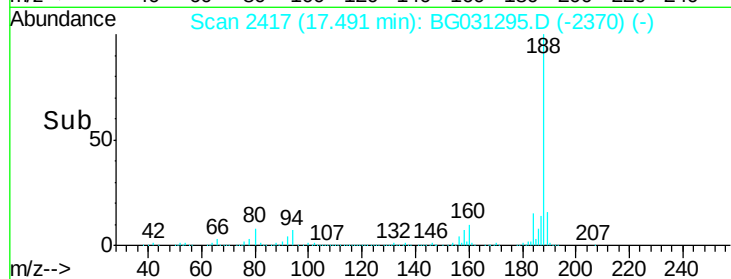
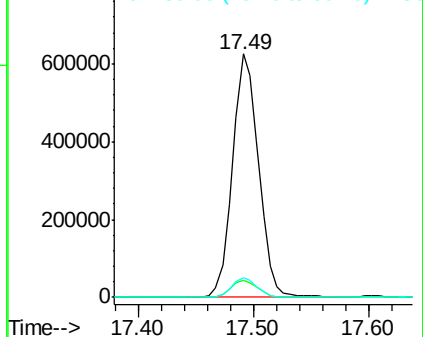



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.02 min
Lab File: BG031295.D
Acq: 30 Nov 2017 19:45

Tgt Ion:240 Resp: 1102273
Ion Ratio Lower Upper
240 100
120 7.7 6.8 10.2
236 27.7 20.9 31.3

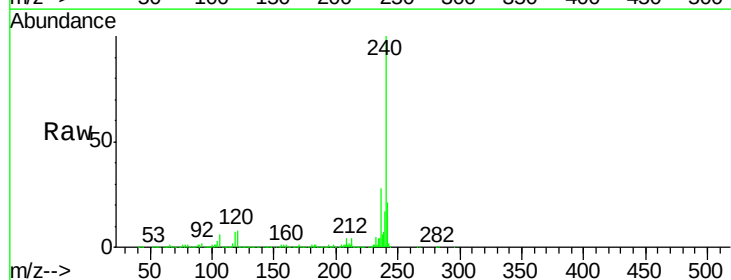

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

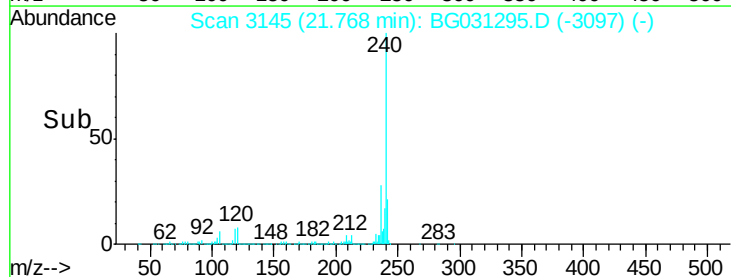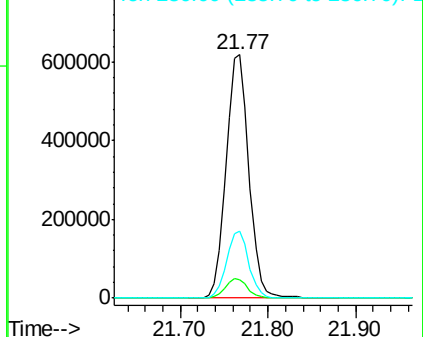

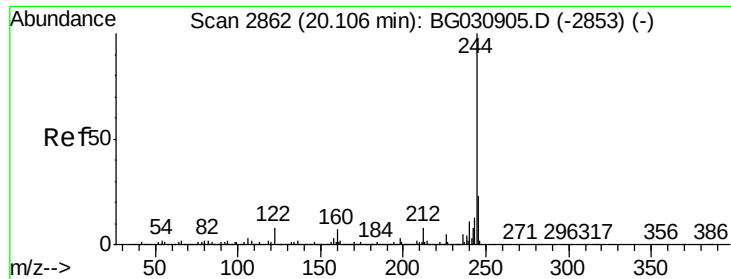

#78

Terphenyl-d14

Concen: 43.83 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031295.D

Acq: 30 Nov 2017 19:45

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 2188186

Ion Ratio Lower Upper

244 100

212 9.2 5.8 8.8#




122 8.8 7.0 10.4

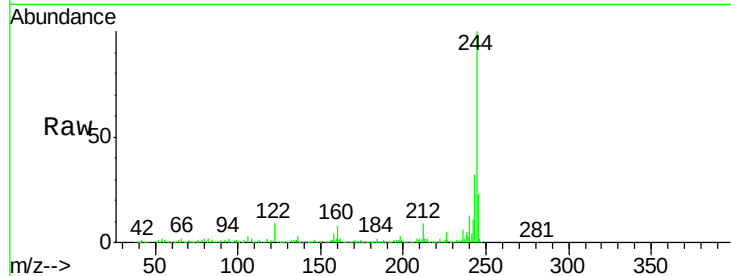

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

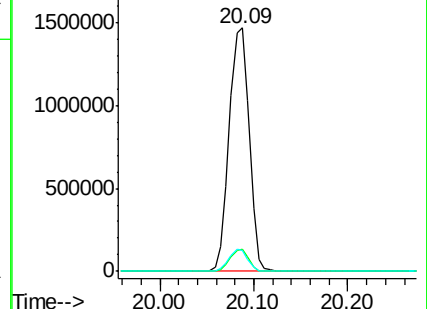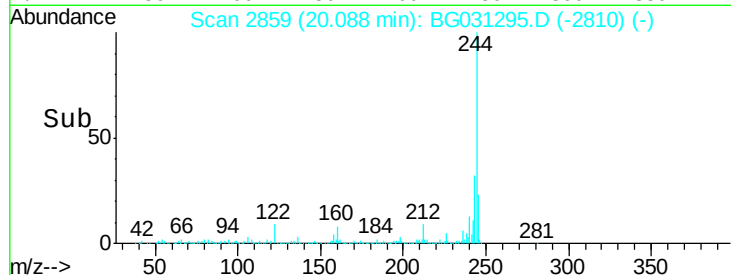

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.03 min

Lab File: BG031295.D

Acq: 30 Nov 2017 19:45


Tgt Ion:264 Resp: 1110185

Ion Ratio Lower Upper

264 100

260 24.4 17.4 26.0

265 23.7 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

