
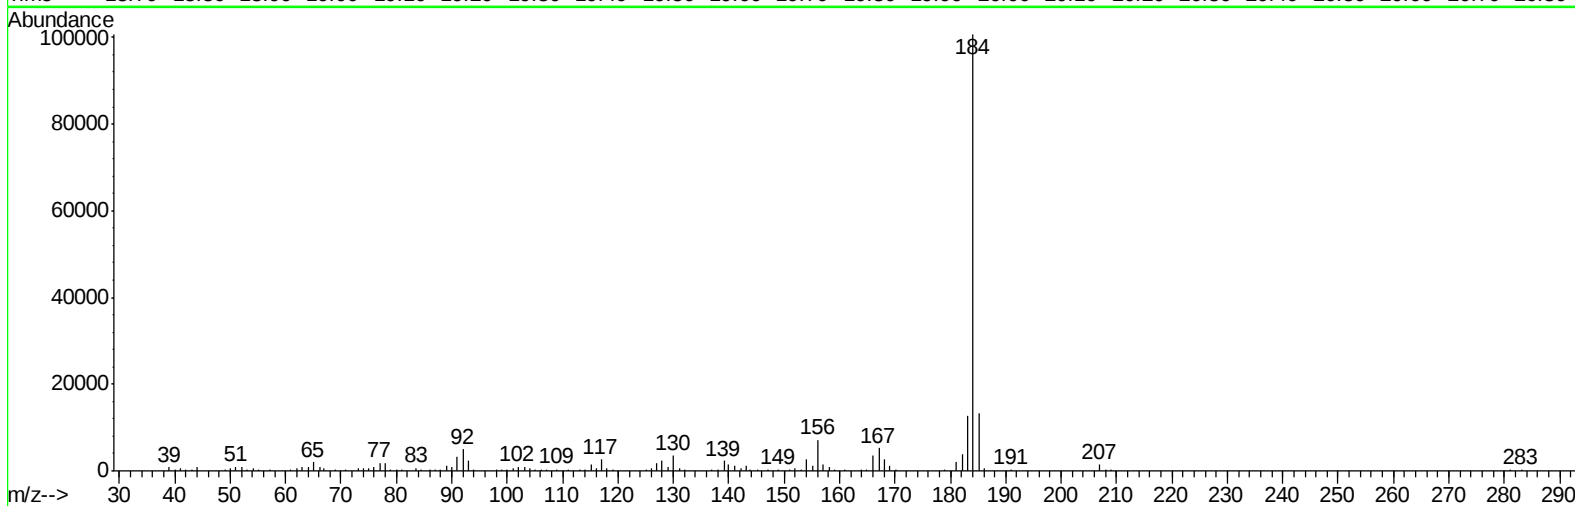


Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031288.D
Acq On : 30 Nov 2017 15:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:56:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

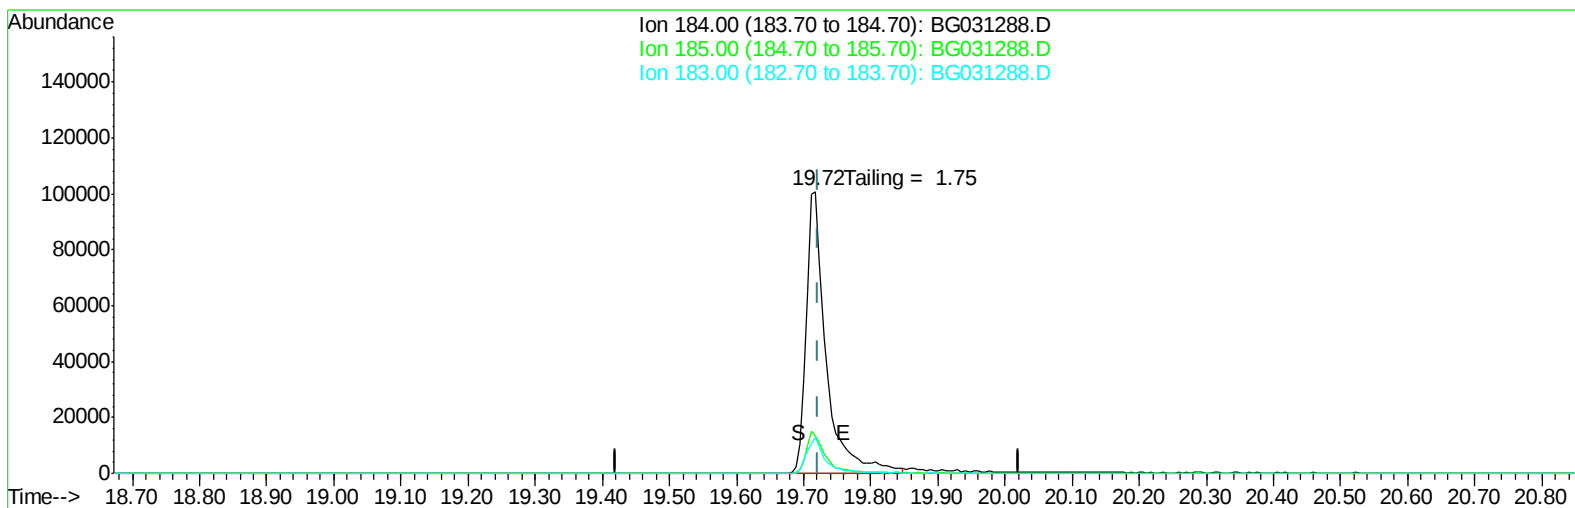

TIC: BG031288.D

(76) Benzidine



19.718min (-0.004) 96005.06ng

response 206620

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.17
183.00	13.30	12.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031288.D
Acq On : 30 Nov 2017 15:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:56:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

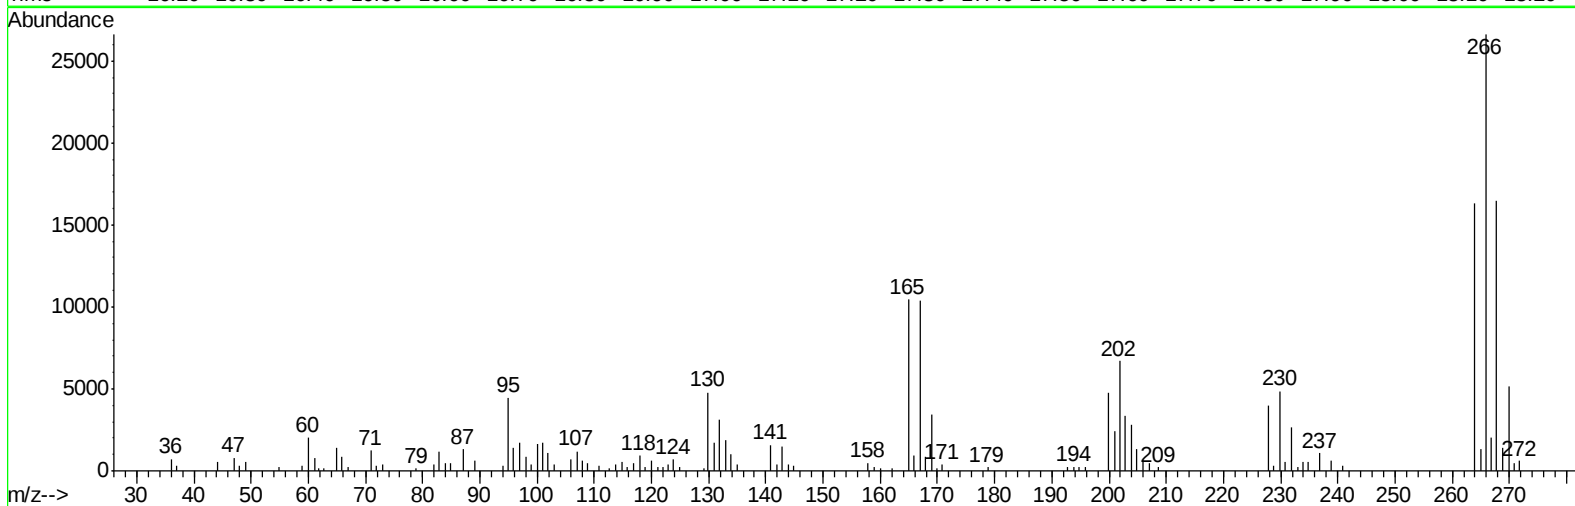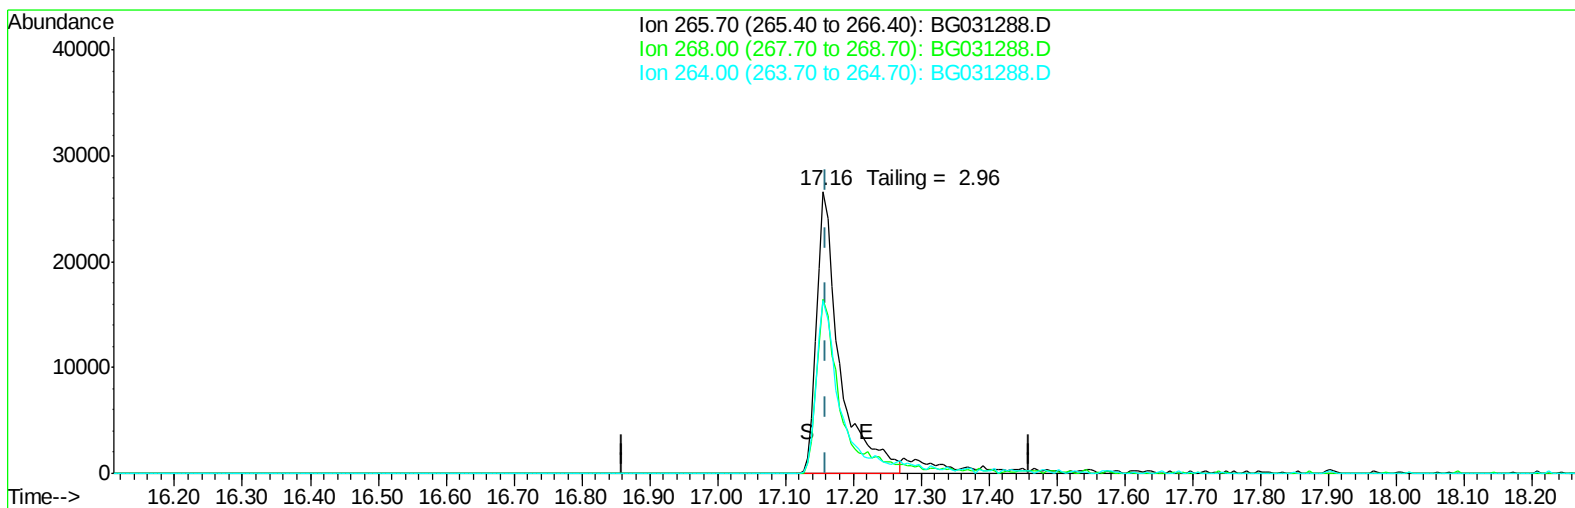

TIC: BG031288.D

(69) Pentachlorophenol (C)

17.156min (-0.004) 0.00ng

response 62327

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.89
264.00	62.00	61.41
0.00	0.00	0.00