
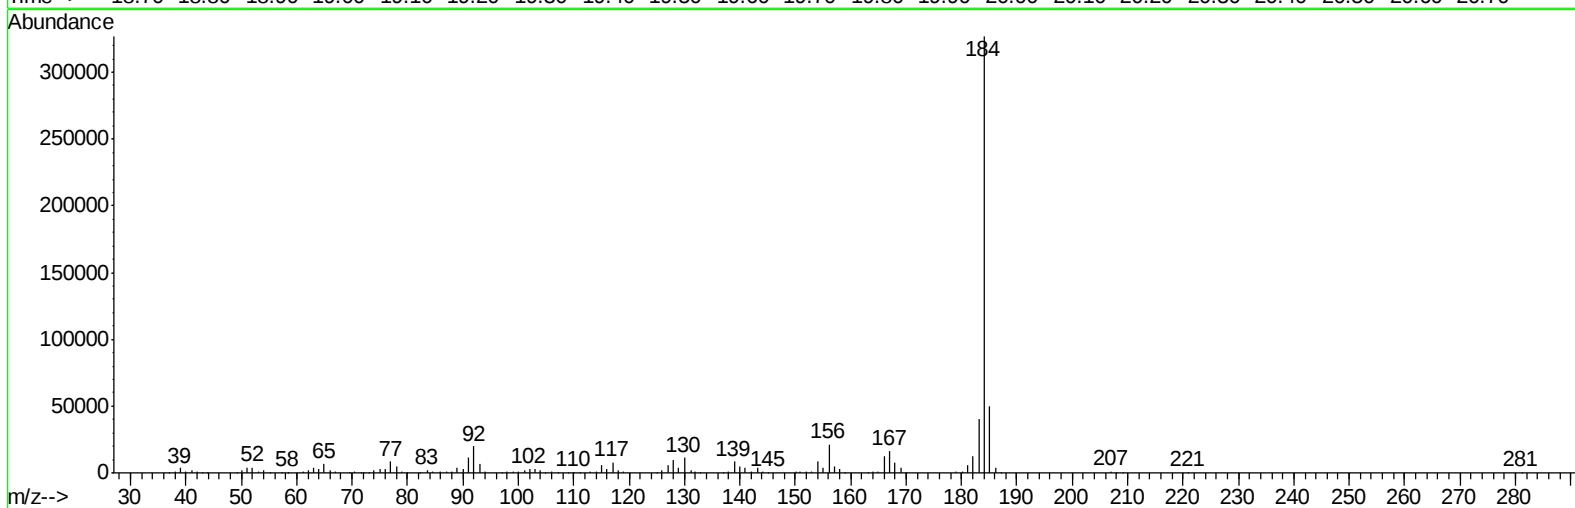


Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031307.D
Acq On : 1 Dec 2017 3:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:57:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

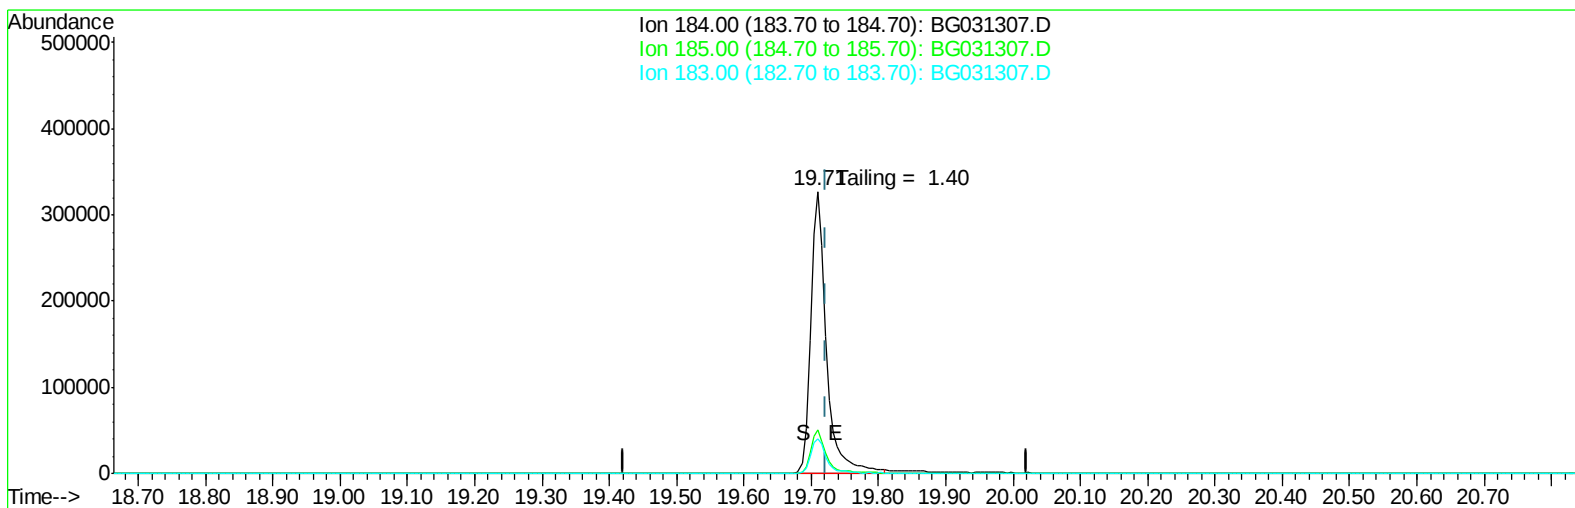

TIC: BG031307.D

(76) Benzidine



19.710min (-0.012) 0.00ng

response 543549

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.27
183.00	13.30	12.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031307.D
Acq On : 1 Dec 2017 3:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:57:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

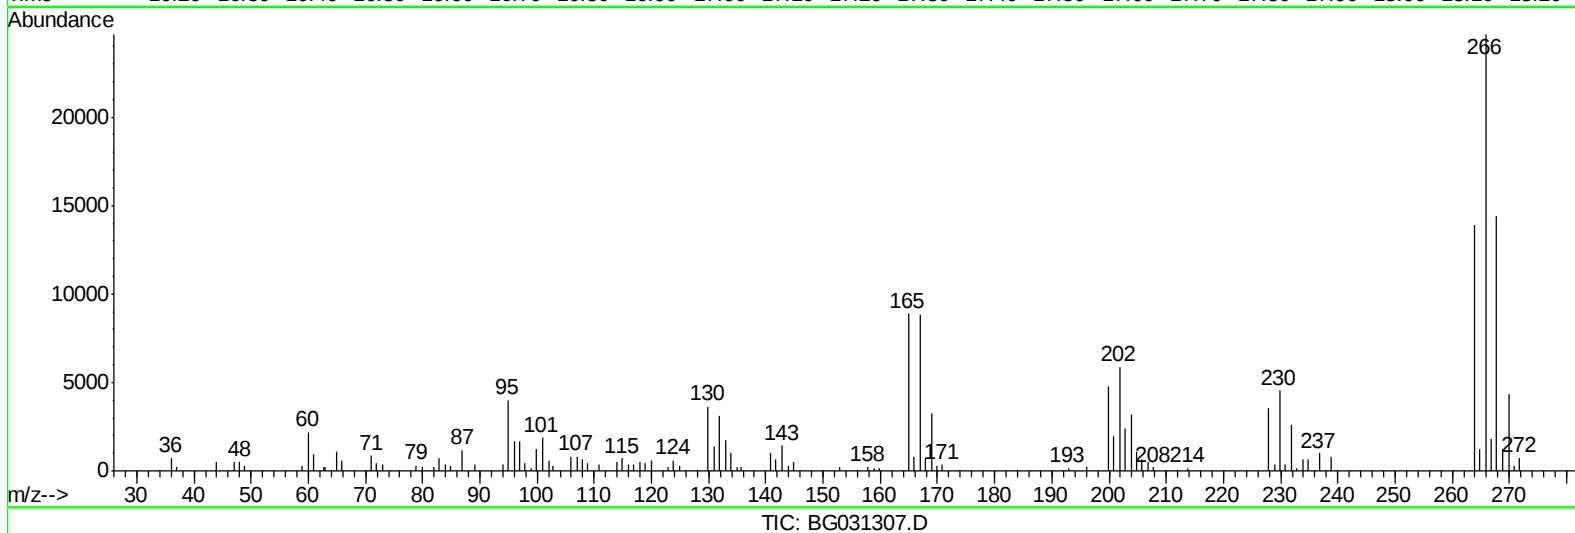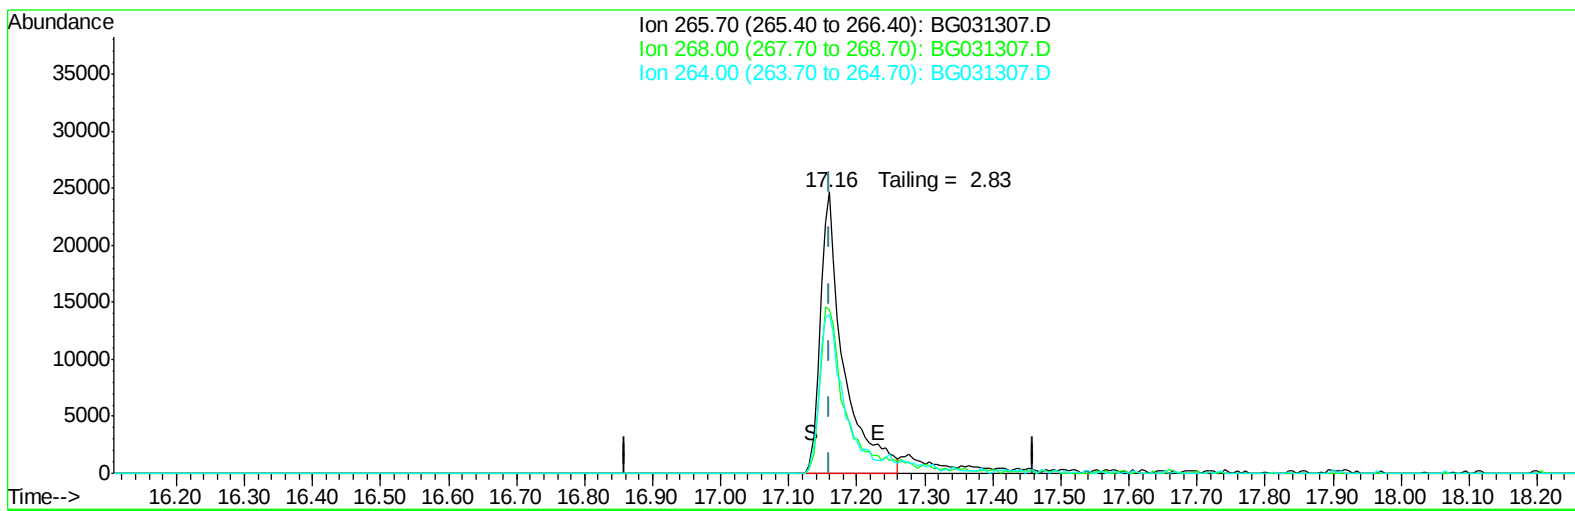

(69) Pentachlorophenol (C)

17.160min (-0.000) 0.00ng

response 58691

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.24
264.00	62.00	56.21
0.00	0.00	0.00