

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
 Data File : BG031309.D
 Acq On : 1 Dec 2017 4:36
 Operator : SJ/JU
 Sample : I6635-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 112817-TIDO-E-U-B

Quant Time: Dec 01 07:28:24 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	65849	20.00	ng	-0.02
21) Naphthalene-d8	10.95	136	269420	20.00	ng	-0.02
38) Acenaphthene-d10	14.76	164	176073	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	479400	20.00	ng	-0.02
75) Chrysene-d12	21.77	240	567086	20.00	ng	-0.02
86) Perylene-d12	25.07	264	543461	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	168737	43.94	ng	-0.02
7) Phenol-d6	7.29	99	129048	24.94	ng	-0.01
23) Nitrobenzene-d5	9.30	82	396321	87.17	ng	-0.02
41) 2,4,6-Tribromophenol	16.24	330	227076	79.72	ng	-0.01
44) 2-Fluorobiphenyl	13.38	172	1149998	93.85	ng	-0.02
78) Terphenyl-d14	20.09	244	2005025	78.07	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG113017\
Data File : BG031309.D
Acq On : 1 Dec 2017 4:36
Operator : SJ/JU
Sample : I6635-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
112817-TIDO-E-U-B

Quant Time: Dec 01 07:28:24 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

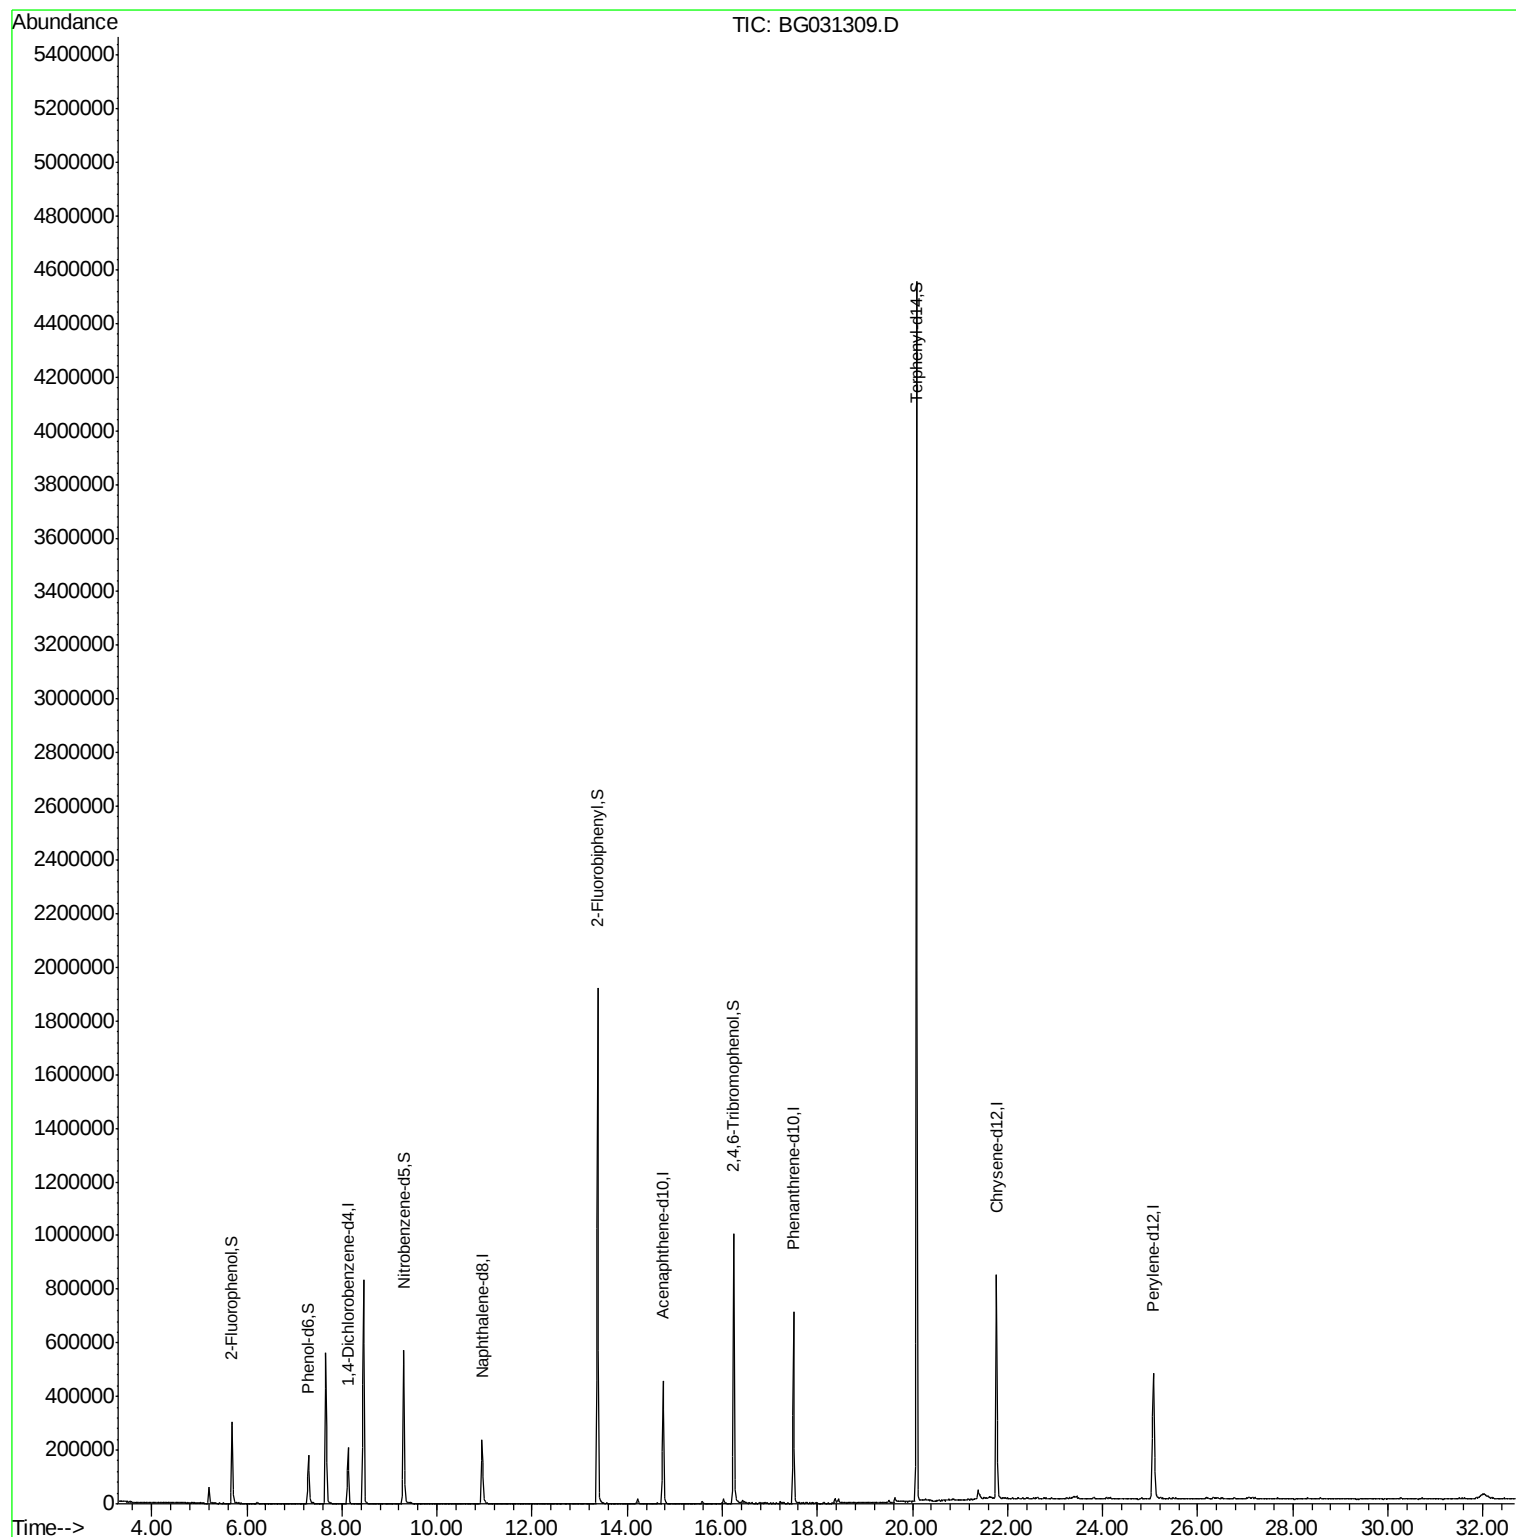




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.13 min Scan# 824
Delta R.T. -0.02 min
Lab File: BG031309.D
Acq: 1 Dec 2017 4:36

Instrument :
BNA_G
ClientSampleId :
112817-TIDO-E-U-B

Tot Ion:152 Resp: 65849
Ion Ratio Lower Upper
152 100
150 153.3 126.6 189.8
115 56.6 53.0 79.4

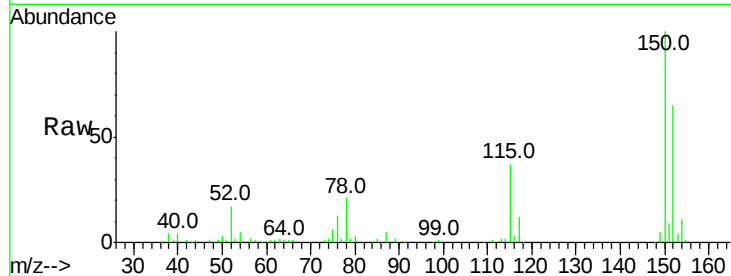


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

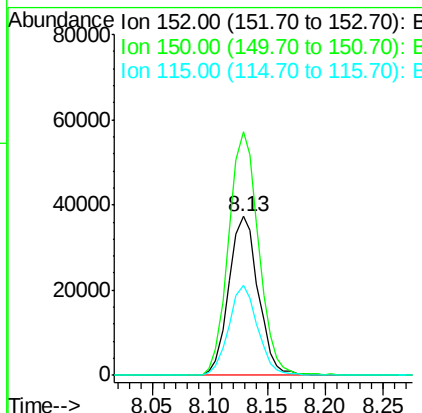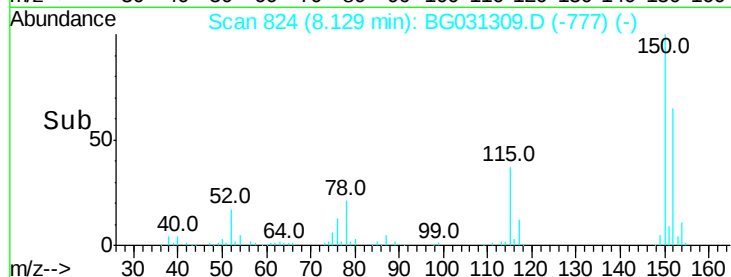



#5


2-Fluorophenol
Concen: 43.940 ng
RT: 5.68 min Scan# 408
Delta R.T. -0.02 min
Lab File: BG031309.D
Acq: 1 Dec 2017 4:36

Tgt Ion:112 Resp: 168737
Ion Ratio Lower Upper
112 100
64 56.9 56.3 84.5
63 28.7 30.1 45.1#

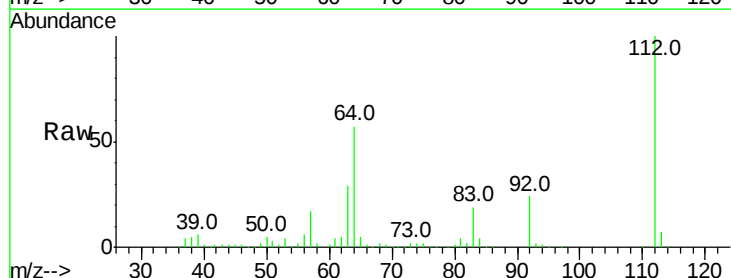

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

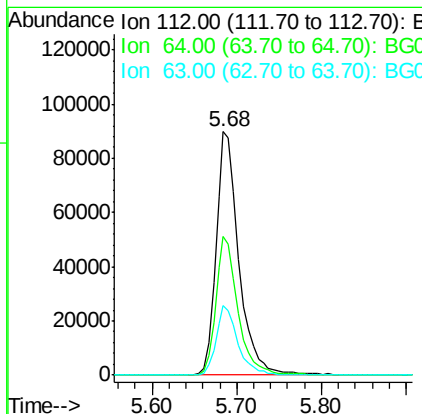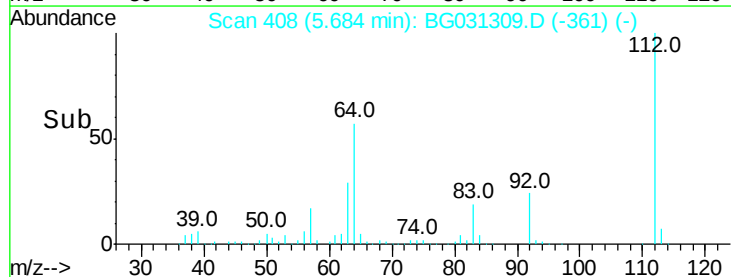

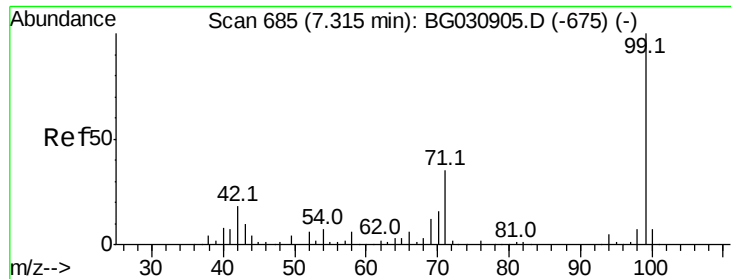

#7

Phenol-d6

Concen: 24.944 ng

RT: 7.29 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36

Instrument :

BNA_G

ClientSampleId :

112817-TIDO-E-U-B


Tot Ion: 99 Resp: 129048

Ion Ratio Lower Upper




99 100

42 16.0 14.1 21.1

71 32.5 26.1 39.1

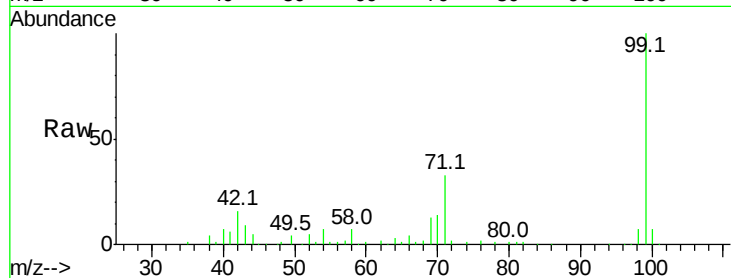

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

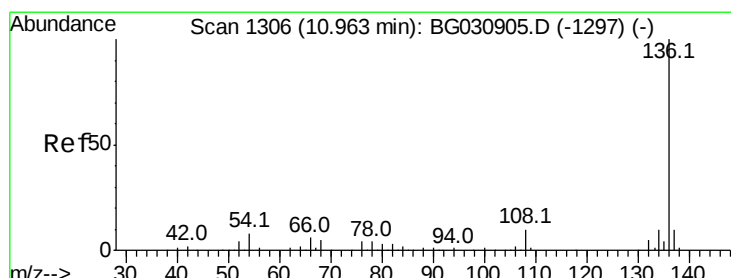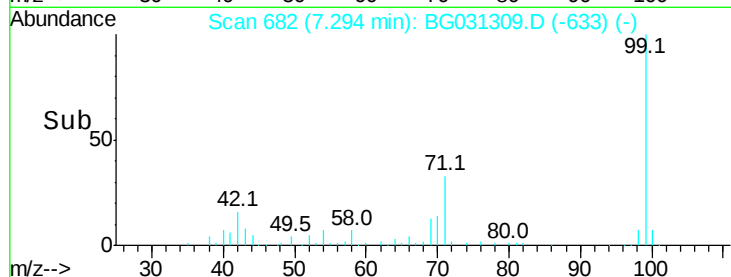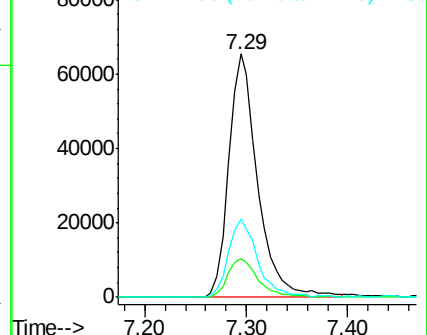

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.95 min Scan# 1304

Delta R.T. -0.02 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36

Tgt Ion: 136 Resp: 269420


Ion Ratio Lower Upper

136 100



137 10.3 9.2 13.8


54 7.5 10.3 15.5#

68 5.1 4.5 6.7

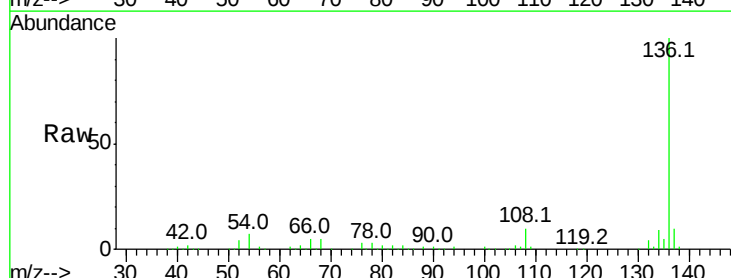

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



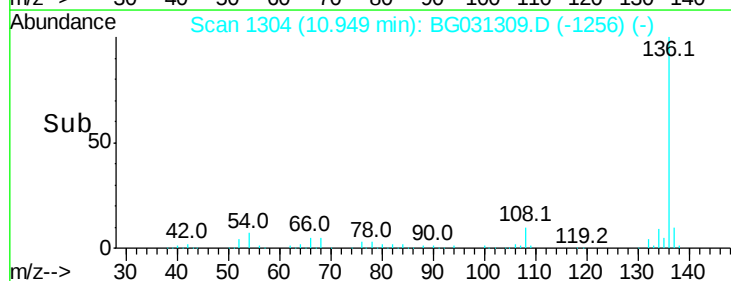
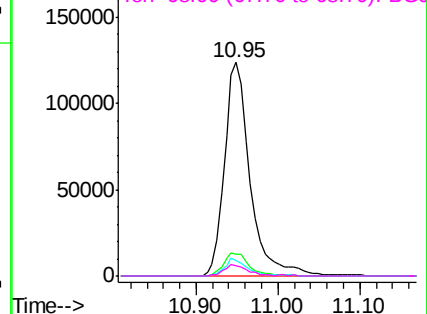


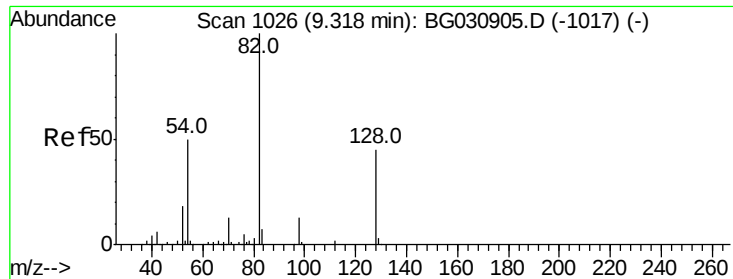

#23
Nitrobenzene-d5
Concen: 87.167 ng
RT: 9.30 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BG031309.D
Acq: 1 Dec 2017 4:36




Instrument :
BNA_G
ClientSampleId :
112817-TIDO-E-U-B

Tot Ion: 82 Resp: 396321
Ion Ratio Lower Upper
82 100
128 47.9 29.7 44.5#
54 47.1 43.1 64.7

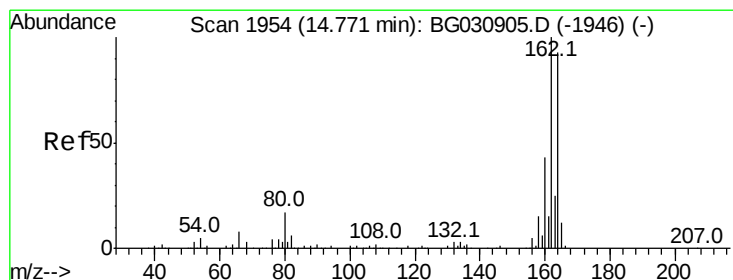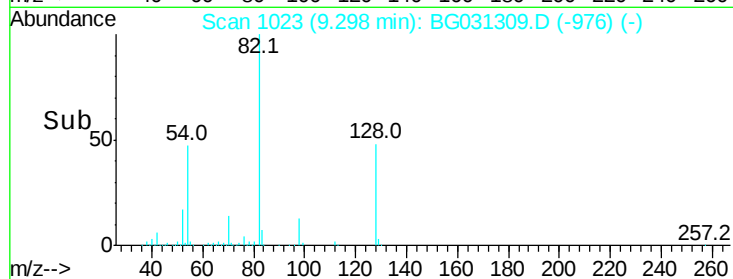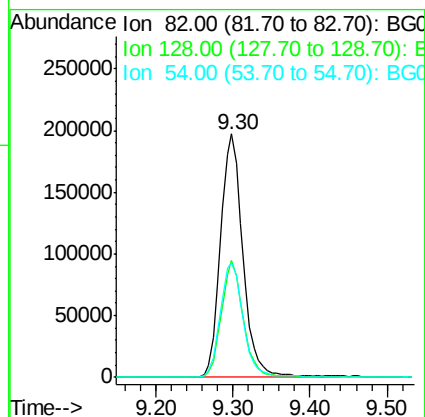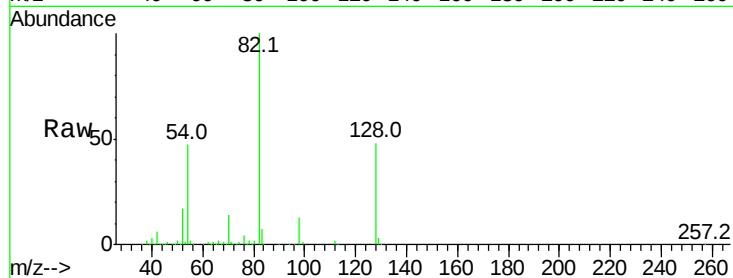

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.76 min Scan# 1952
Delta R.T. -0.02 min
Lab File: BG031309.D
Acq: 1 Dec 2017 4:36

Tgt Ion:164 Resp: 176073
Ion Ratio Lower Upper
164 100
162 105.9 78.8 118.2
160 45.4 35.4 53.0

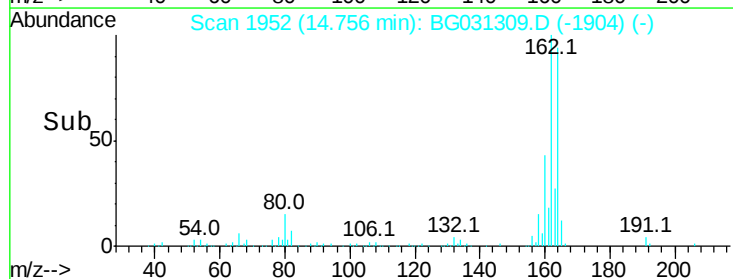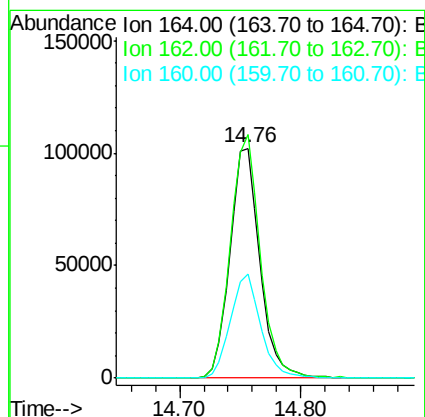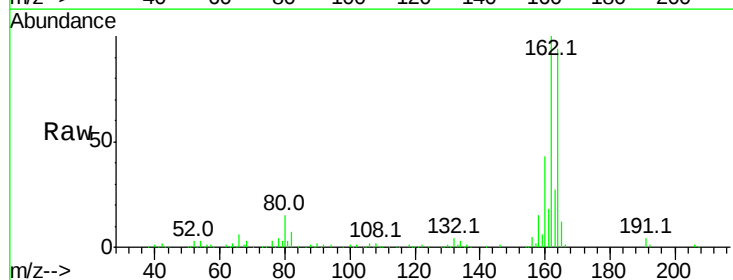







#41
 2,4,6-Tribromophenol
 Concen: 79.724 ng
 RT: 16.24 min Scan# 2205
 Delta R.T. -0.01 min
 Lab File: BG031309.D
 Acq: 1 Dec 2017 4:36

Instrument :
 BNA_G
 ClientSampleId :
 112817-TIDO-E-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.0	115.6
141	34.5	25.2	37.8

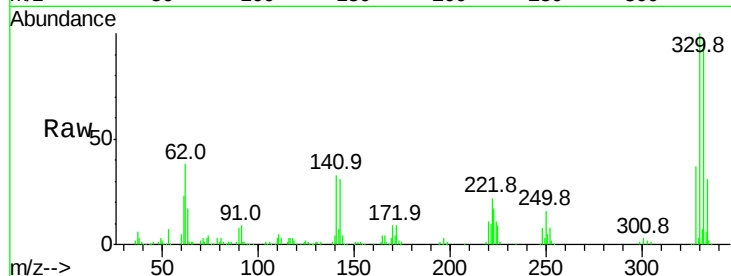


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

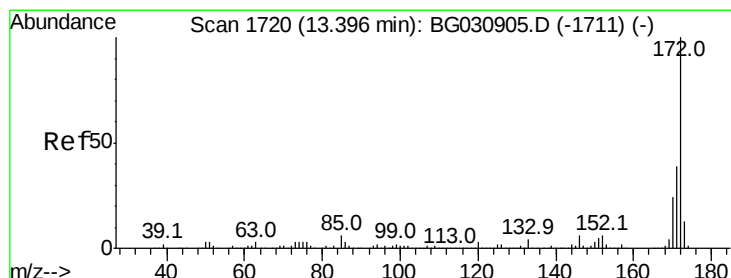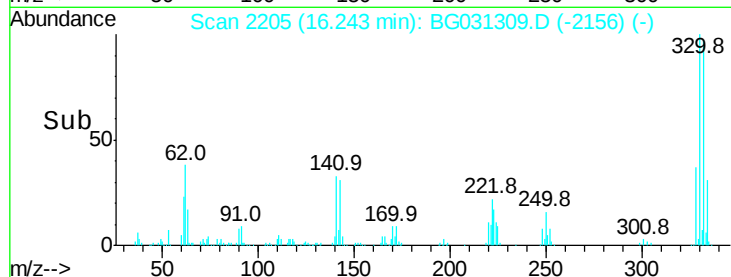
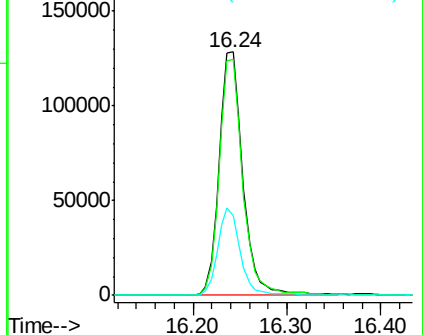


#44
 2-Fluorobiphenyl
 Concen: 93.849 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.02 min
 Lab File: BG031309.D
 Acq: 1 Dec 2017 4:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	30.0	45.0
170	24.1	19.5	29.3

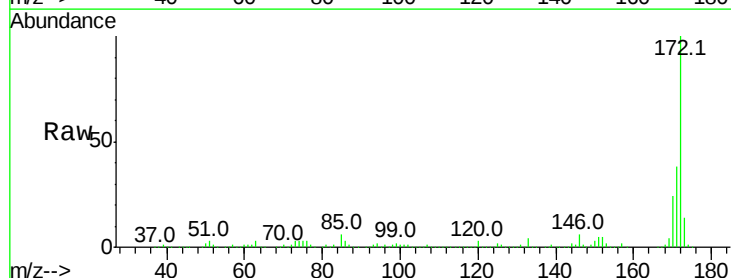

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

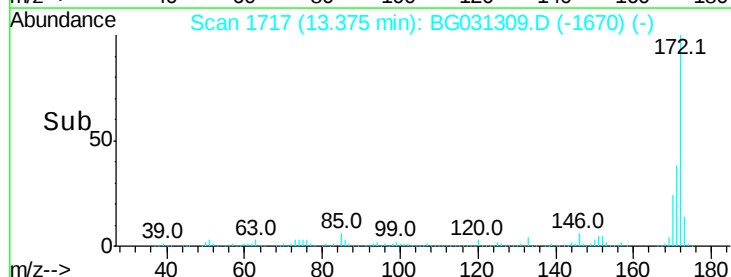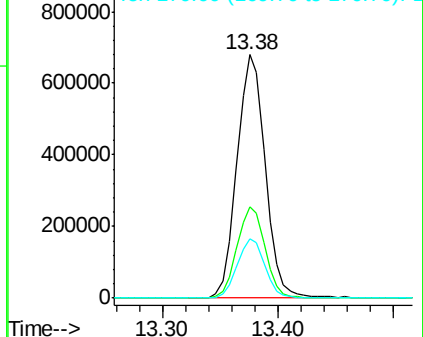



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.49 min Scan# 2418

Delta R.T. -0.02 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36

Instrument :

BNA_G

ClientSampleId :

112817-TIDO-E-U-B


Tot Ion:188 Resp: 479400

Ion Ratio Lower Upper

188 100

94 7.0 6.9 10.3




80 7.3 7.7 11.5#

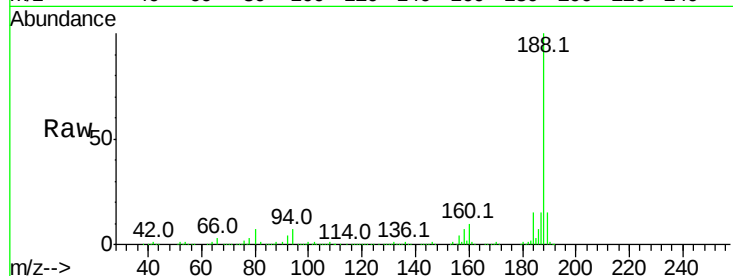

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

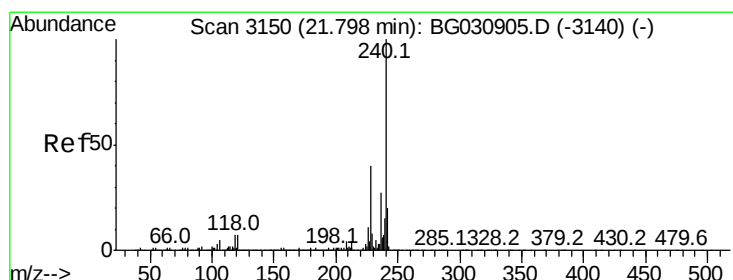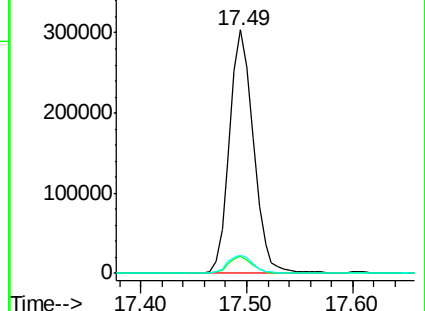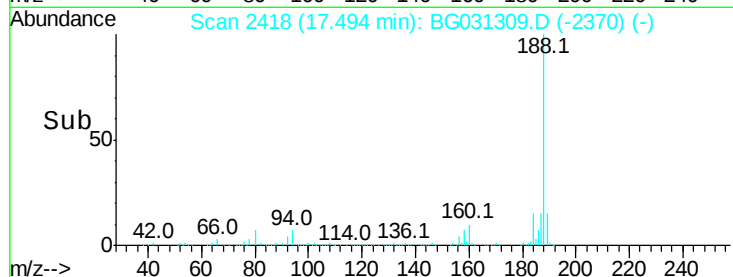

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.02 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36


Tgt Ion:240 Resp: 567086

Ion Ratio Lower Upper

240 100

120 7.5 6.8 10.2



236 26.4 20.9 31.3

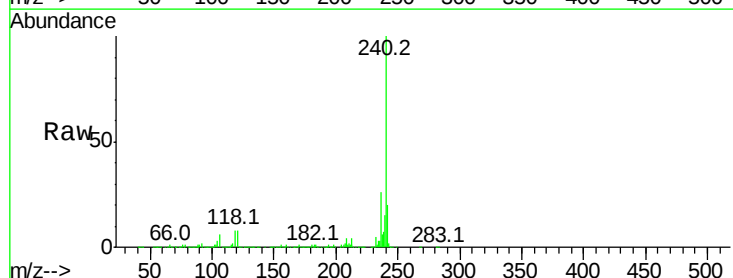

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

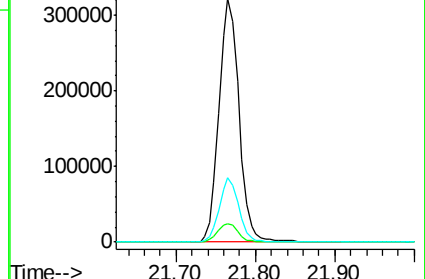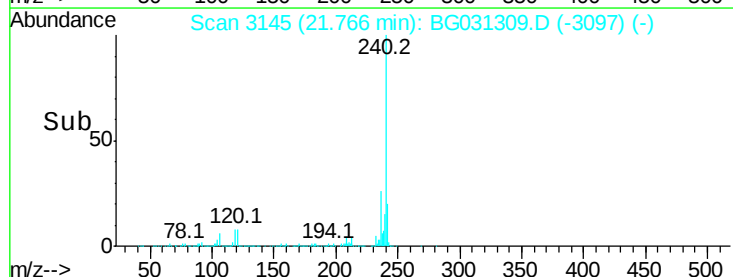



#78

Terphenyl-d14

Concen: 78.071 ng

RT: 20.09 min Scan# 2859

Delta R.T. -0.01 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36

Instrument :


BNA_G

ClientSampleId :

112817-TIDO-E-U-B

Tot Ion:244 Resp: 2005025



Ion	Ratio	Lower	Upper
244	100		
212	8.7	5.8	8.8
122	9.3	7.0	10.4

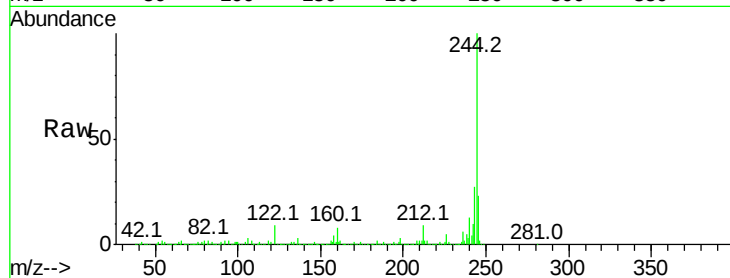

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

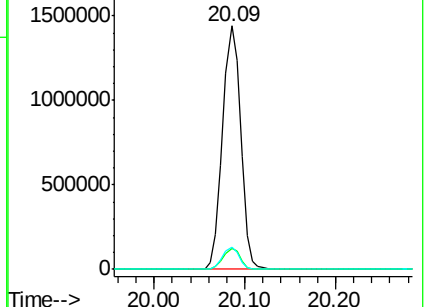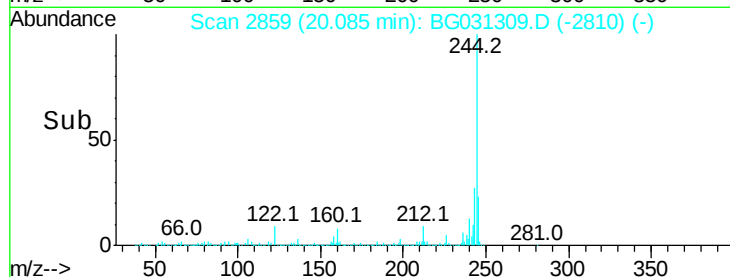

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.07 min Scan# 3707


Delta R.T. -0.02 min

Lab File: BG031309.D

Acq: 1 Dec 2017 4:36

Tgt Ion:264 Resp: 543461

Ion	Ratio	Lower	Upper
264	100		
260	24.5	17.4	26.0
265	22.7	17.7	26.5

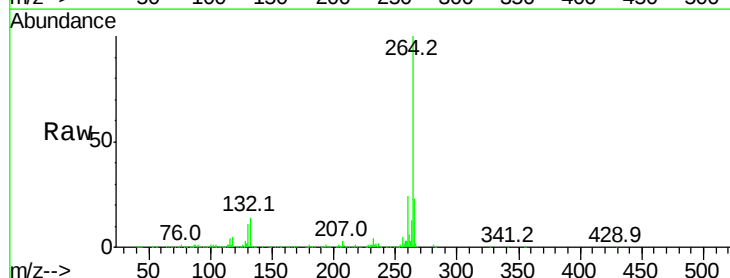

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

