
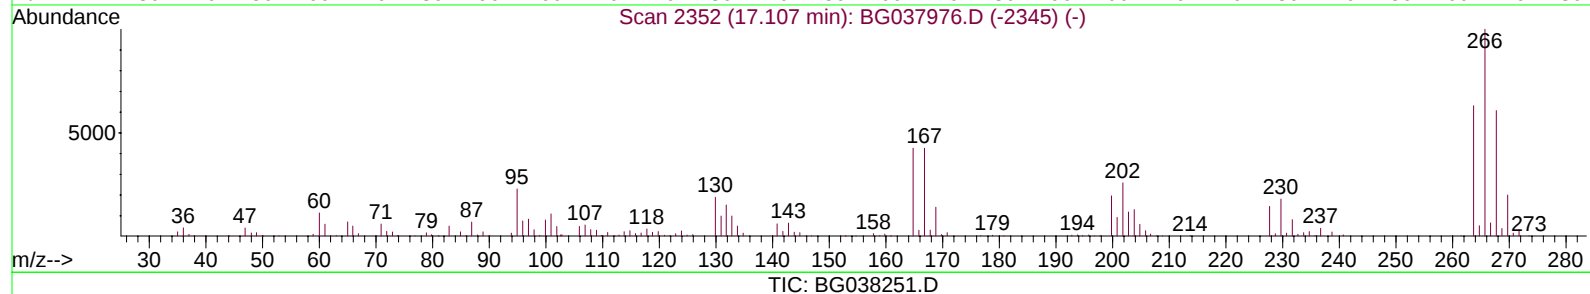
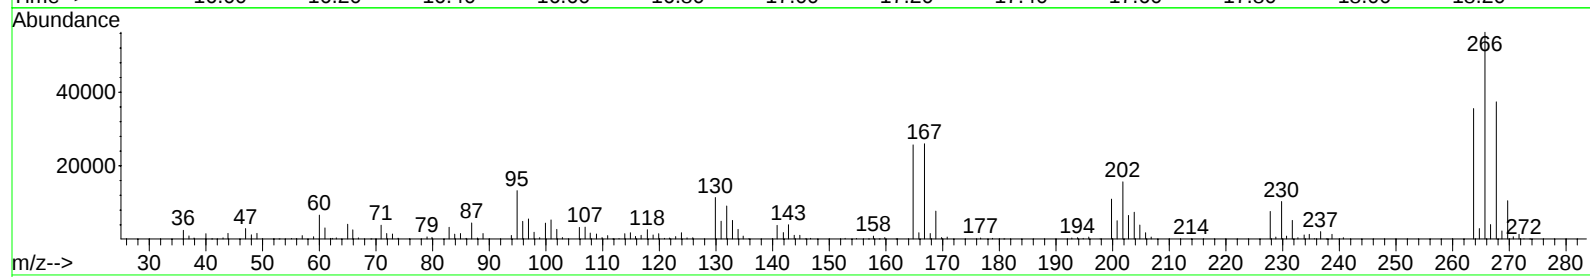


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG113018\  
Data File : BG038251.D  
Acq On : 30 Nov 2018 10:47  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:11:43 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 13 16:39:28 2018  
Response via : Initial Calibration

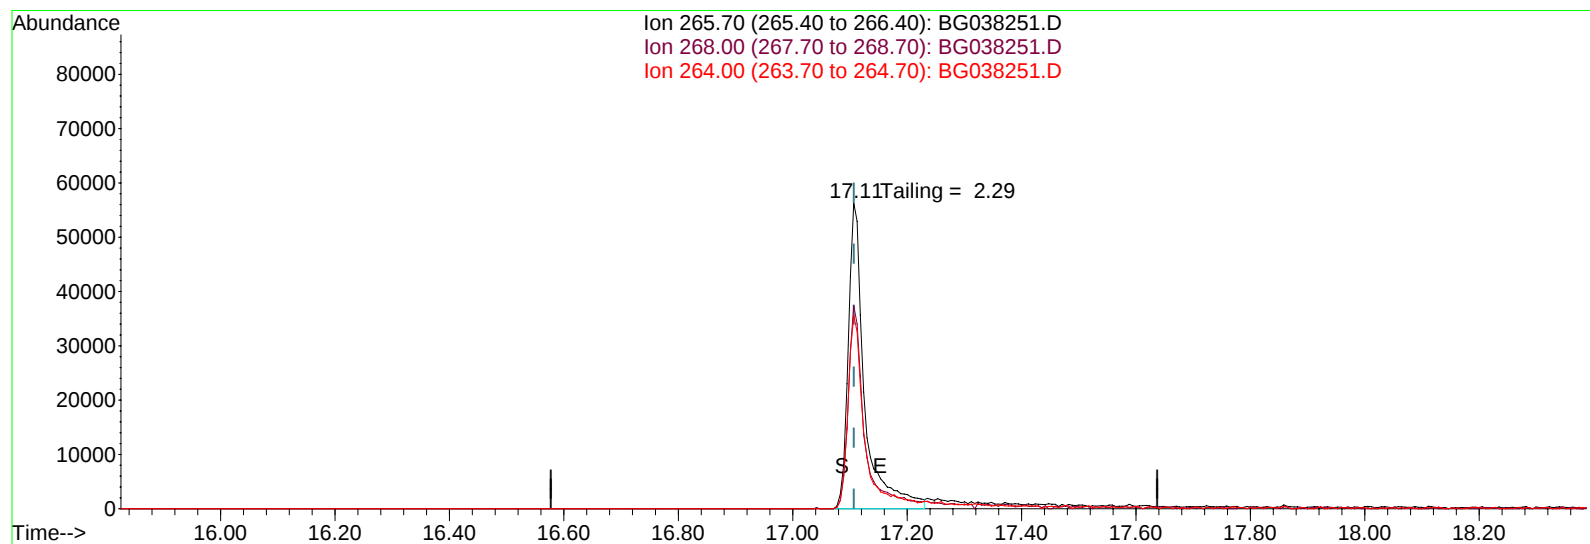

(70) Pentachlorophenol (C)




17.107min (-0.001) 83514.62ng

response 113740

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 70.59 |
| 264.00 | 73.60 | 68.50 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG113018\  
Data File : BG038251.D  
Acq On : 30 Nov 2018 10:47  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 11:11:43 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 13 16:39:28 2018  
Response via : Initial Calibration

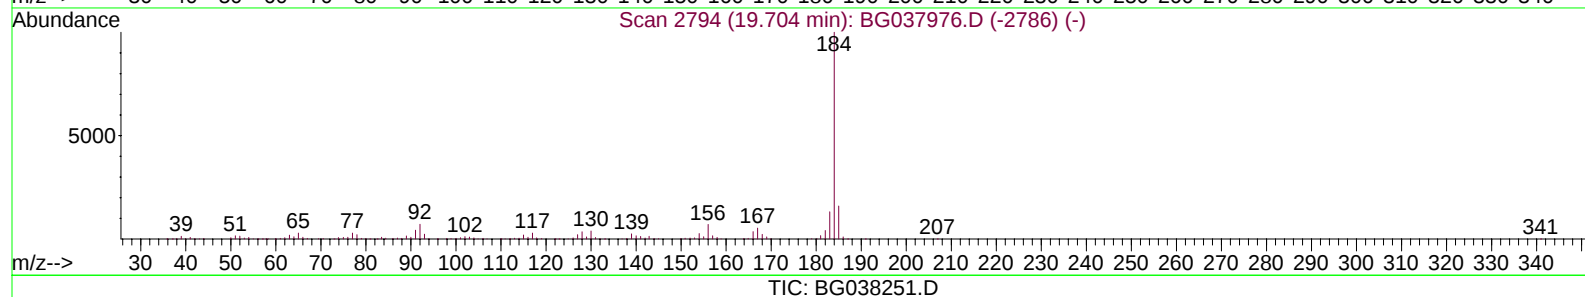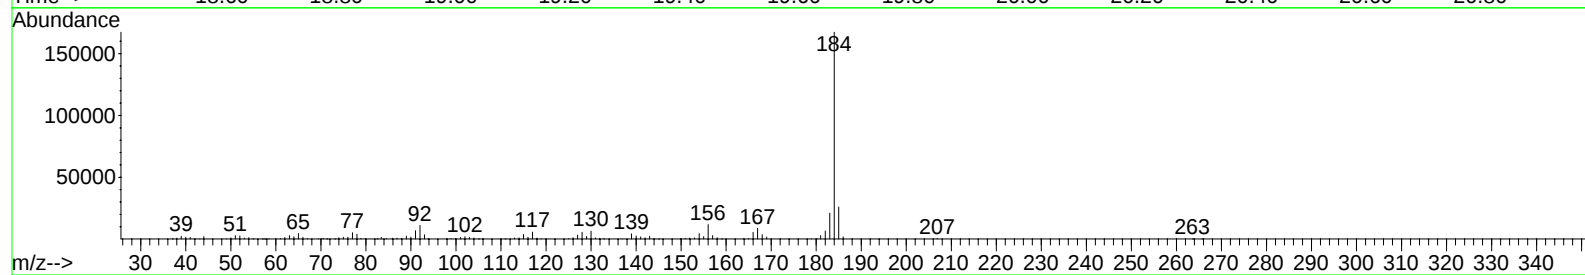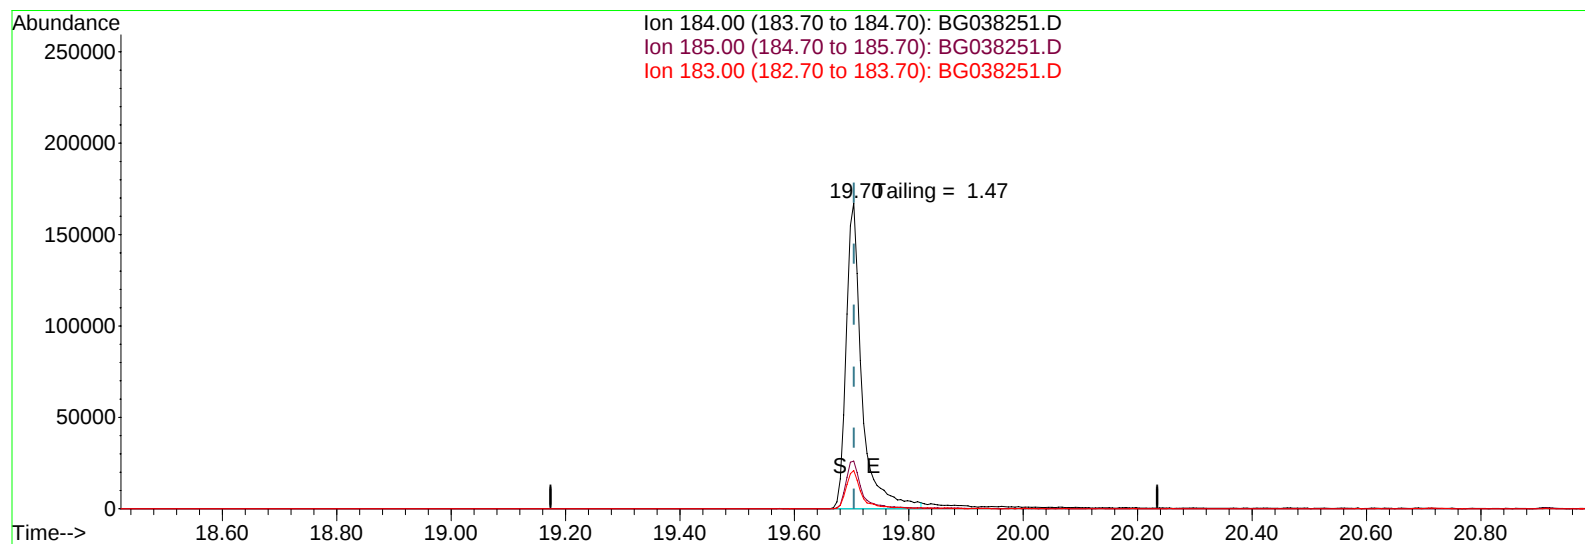

(77) Benzidine

19.704min (-0.001) 0.00ng

response 323657

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 15.58 |
| 183.00 | 12.70 | 12.51 |
| 0.00   | 0.00  | 0.00  |