
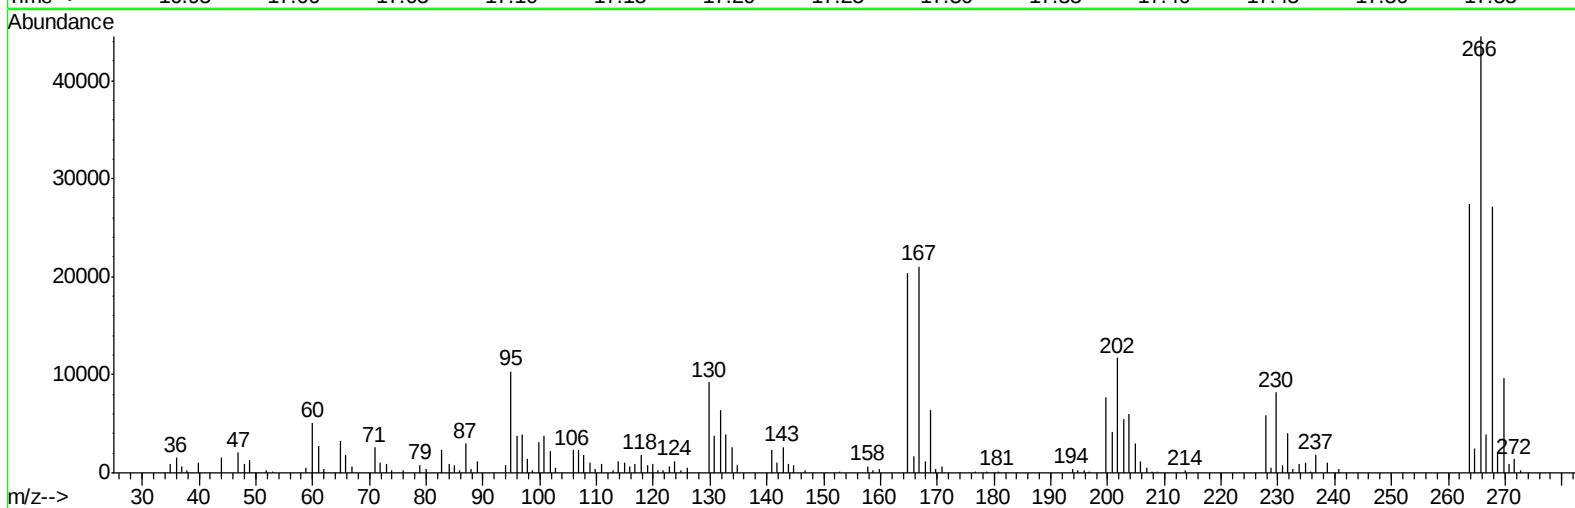


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113018\
Data File : BG038270.D
Acq On : 30 Nov 2018 23:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 00:38:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

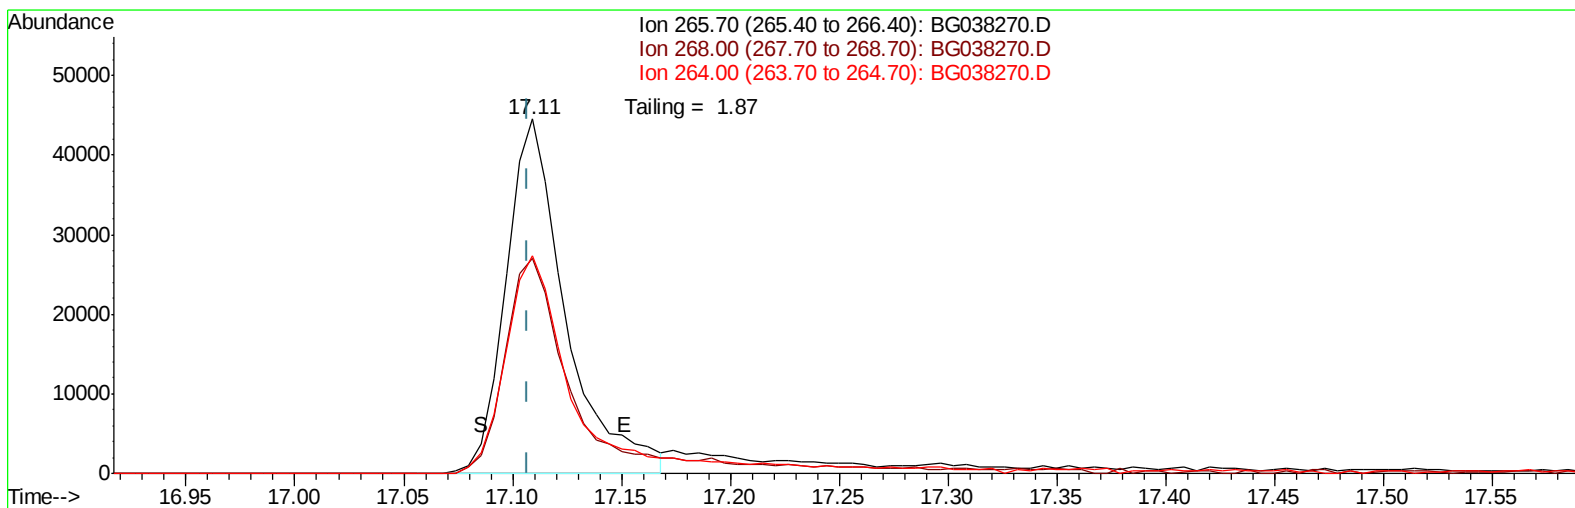

TIC: BG038270.D

(70) Pentachlorophenol (C)



17.109min (+0.002) 37032.67ng

response 94887

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.63
264.00	73.60	67.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113018\
Data File : BG038270.D
Acq On : 30 Nov 2018 23:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 00:38:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

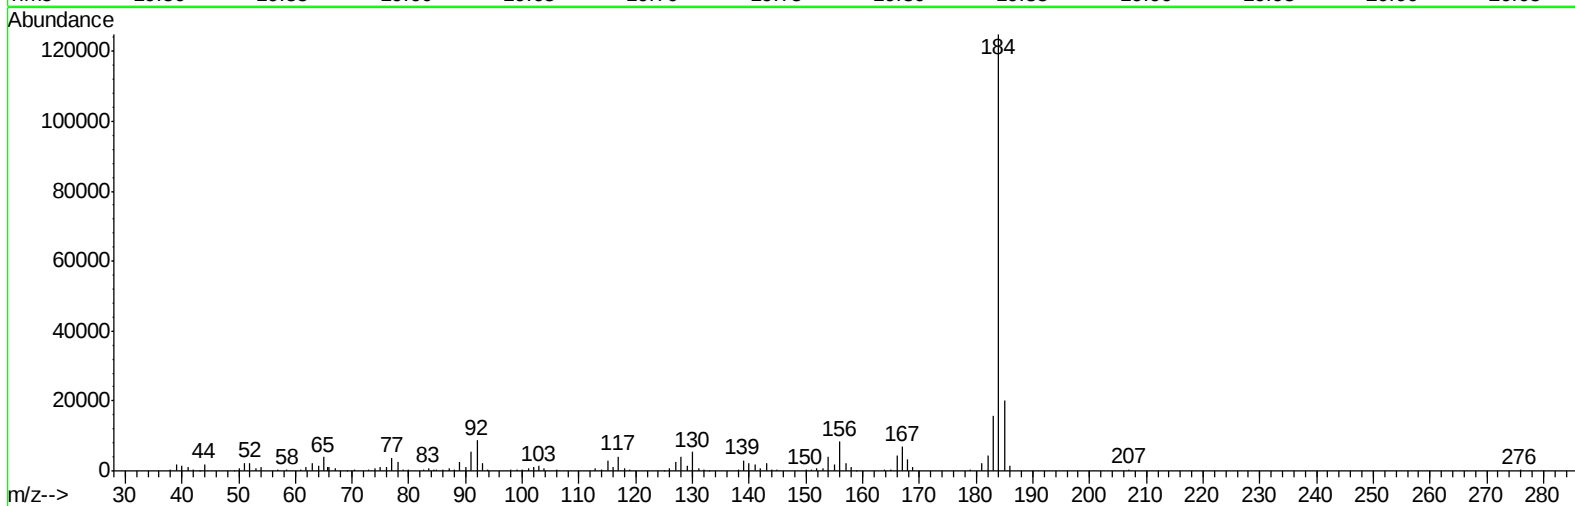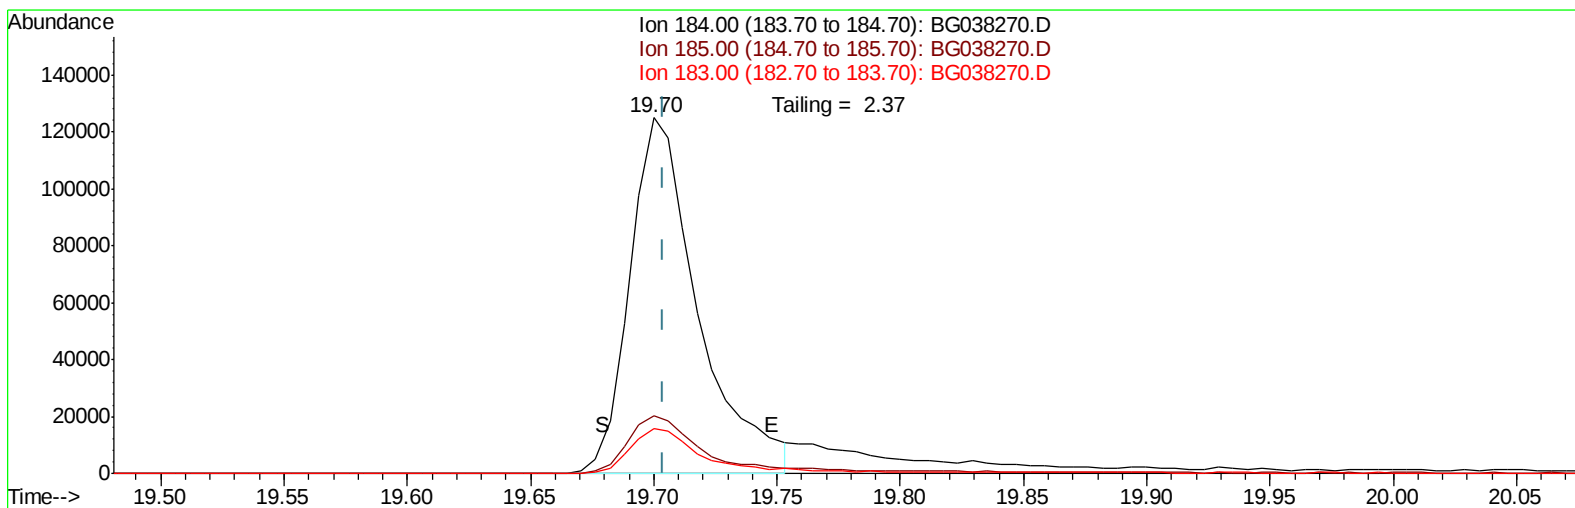

TIC: BG038270.D

(77) Benzidine

19.700min (-0.004) 0.00ng

response 278617

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.21
183.00	12.70	12.54
0.00	0.00	0.00