

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113018\
 Data File : BG038284.D
 Acq On : 1 Dec 2018 9:08
 Operator : JU/SJ
 Sample : J6129-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 112818-CHDE-F-U-S

Quant Time: Dec 03 00:16:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	34963	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	160822	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	104573	20.00	ng	0.00
64) Phenanthrene-d10	17.46	188	232386	20.00	ng	-0.01
76) Chrysene-d12	21.74	240	214080	20.00	ng	-0.01
87) Perylene-d12	25.06	264	200611	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	89209	44.05	ng	0.00
7) Phenol-d6	7.23	99	78987	27.33	ng	0.00
23) Nitrobenzene-d5	9.26	82	293303	97.63	ng	0.00
42) 2,4,6-Tribromophenol	16.20	330	96350	80.79	ng	-0.01
45) 2-Fluorobiphenyl	13.34	172	670791	93.45	ng	-0.01
79) Terphenyl-d14	20.06	244	953520	104.80	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113018\
Data File : BG038284.D
Acq On : 1 Dec 2018 9:08
Operator : JU/SJ
Sample : J6129-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
112818-CHDE-F-U-S

Quant Time: Dec 03 00:16:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

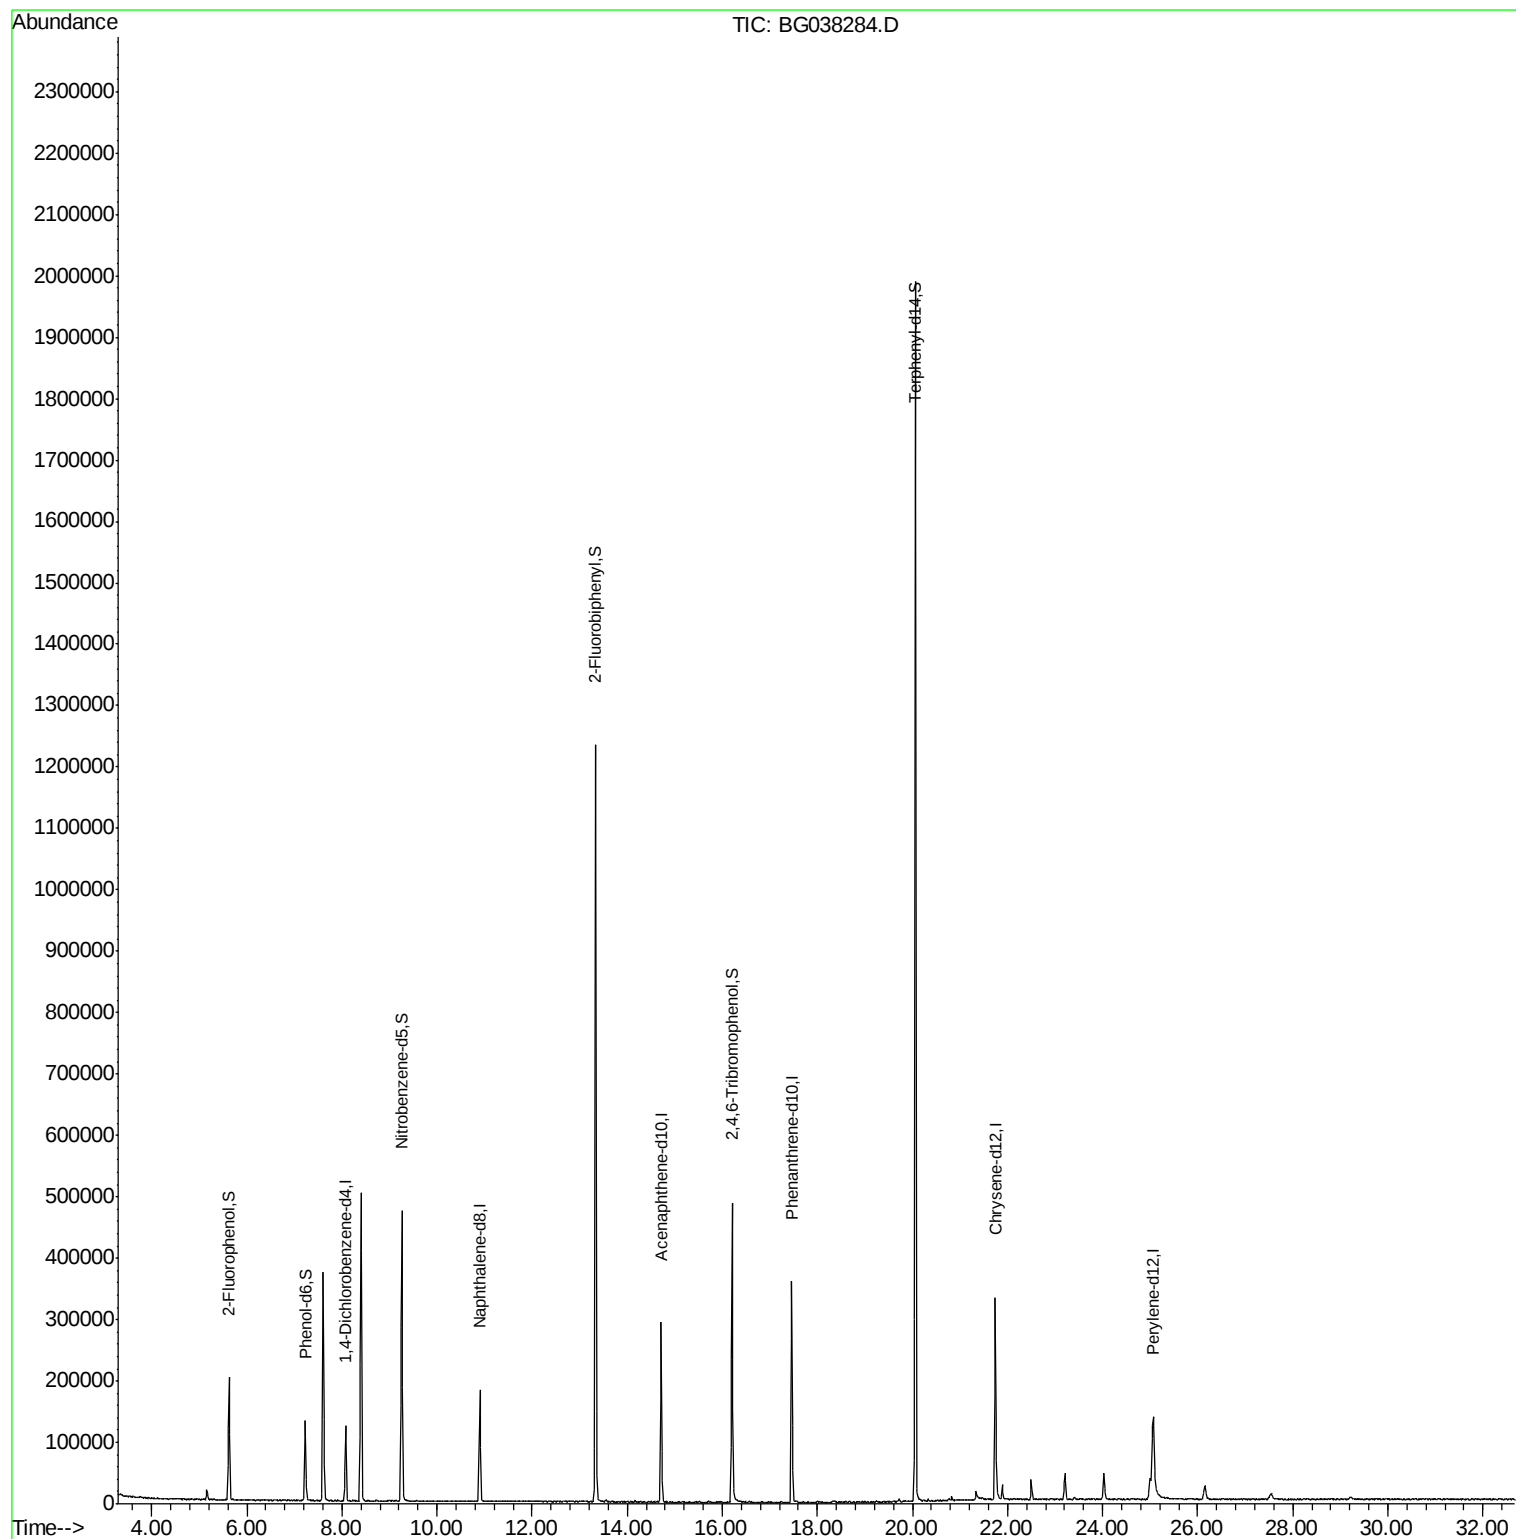

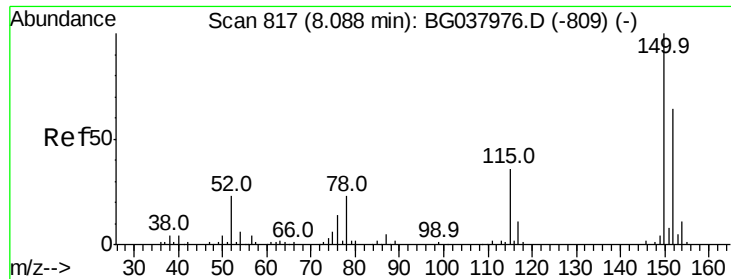


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.08 min Scan# 816
 Delta R.T. -0.01 min
 Lab File: BG038284.D
 Acq: 1 Dec 2018 9:08

Instrument :
 BNA_G
 ClientSampleId :
 112818-CHDE-F-U-S

Tot Ion:152 Resp: 34963
 Ion Ratio Lower Upper
 152 100
 150 157.7 126.0 189.0
 115 58.3 45.5 68.3

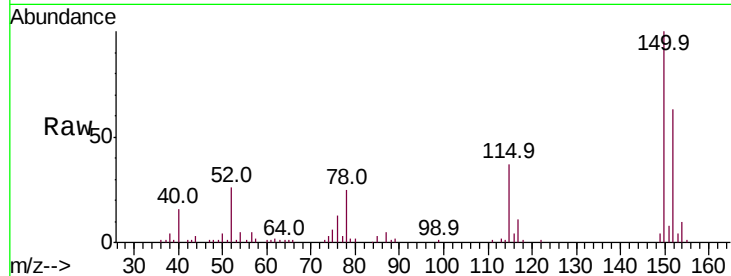


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

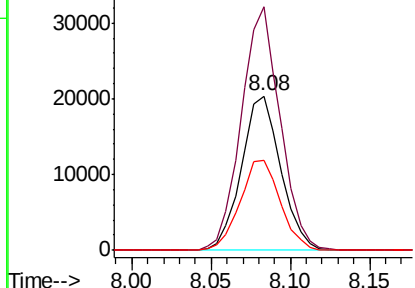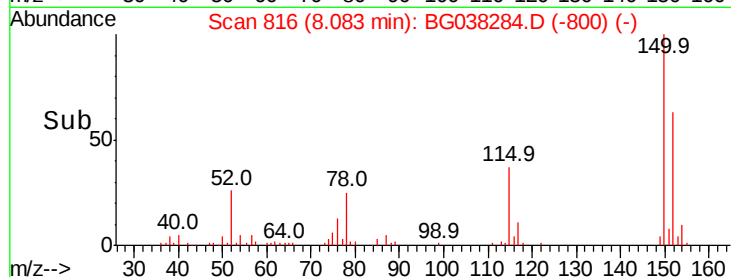



#5

2-Fluorophenol
 Concen: 44.054 ng
 RT: 5.63 min Scan# 398
 Delta R.T. -0.01 min
 Lab File: BG038284.D
 Acq: 1 Dec 2018 9:08

Tgt Ion:112 Resp: 89209
 Ion Ratio Lower Upper
 112 100
 64 67.3 53.1 79.7
 63 35.4 27.3 40.9

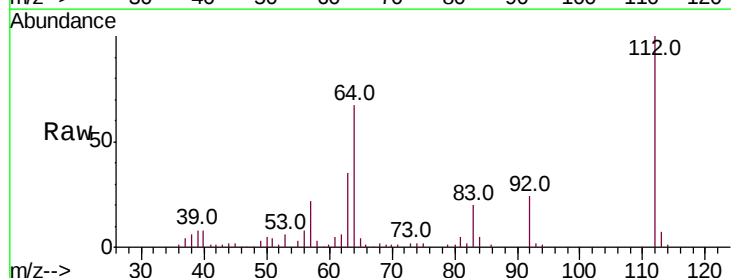

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

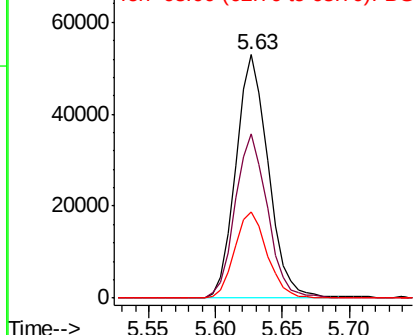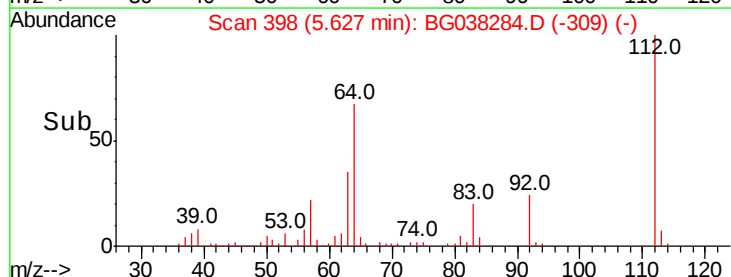



#7

Phenol-d6

Concen: 27.326 ng

RT: 7.23 min Scan# 670

Delta R.T. -0.01 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08

Instrument :

BNA_G

ClientSampleId :

112818-CHDE-F-U-S


Tot Ion: 99 Resp: 78987

Ion Ratio Lower Upper

99 100

42 22.5 15.0 22.4#

71 32.6 25.5 38.3



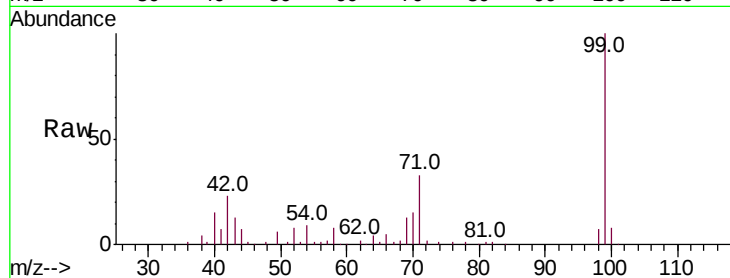


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

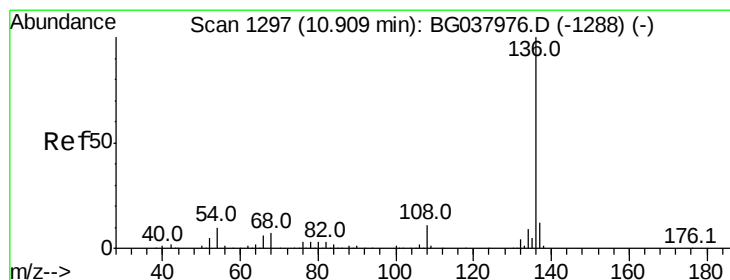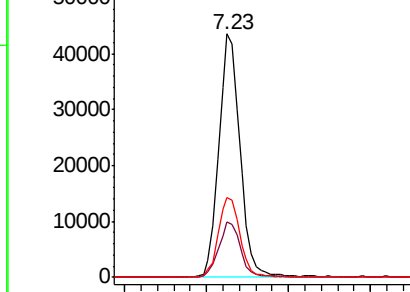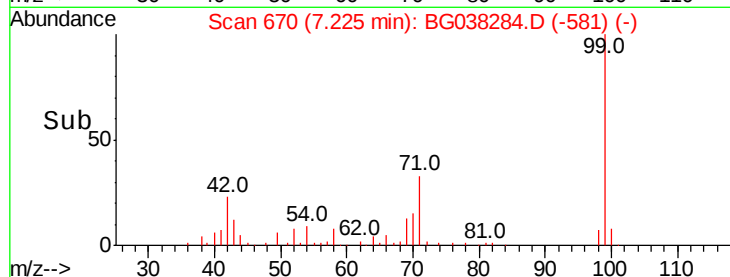

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08

Tgt Ion: 136 Resp: 160822


Ion Ratio Lower Upper

136 100

137 11.5 9.6 14.4

54 11.0 7.9 11.9

68 7.0 4.8 7.2

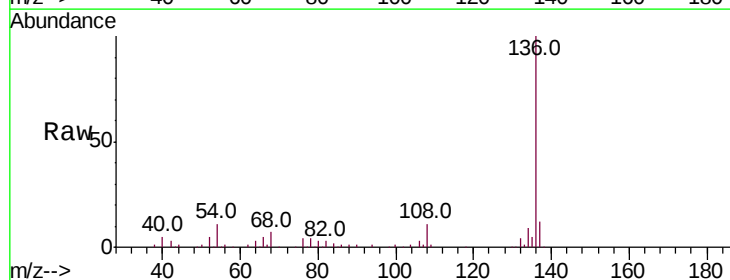



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

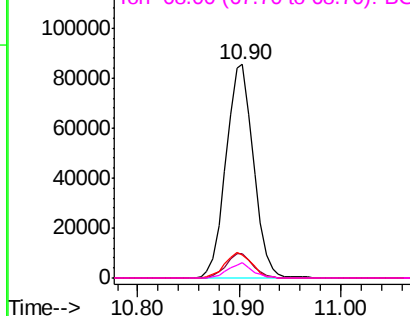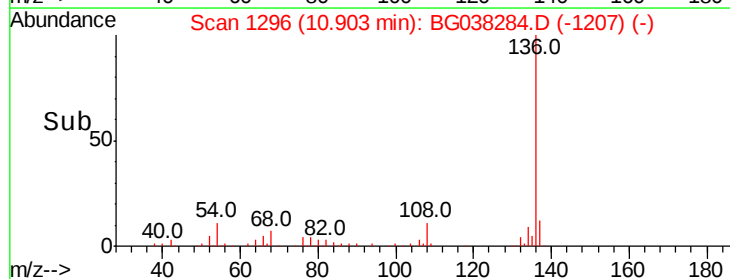


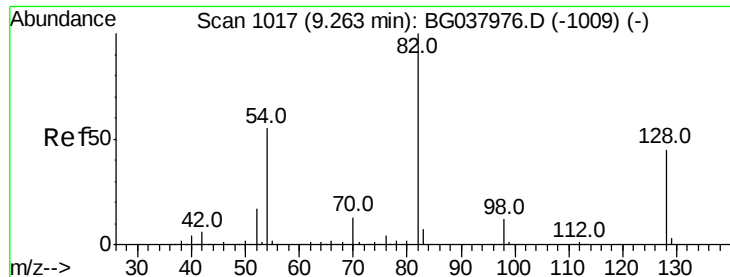




#23
Nitrobenzene-d5
Concen: 97.627 ng
RT: 9.26 min Scan# 1016
Delta R.T. -0.01 min
Lab File: BG038284.D
Acq: 1 Dec 2018 9:08

Instrument :
BNA_G
ClientSampleId :
112818-CHDE-F-U-S

Tot Ion: 82 Resp: 293303
Ion Ratio Lower Upper
82 100
128 42.1 34.6 51.8
54 59.7 45.3 67.9

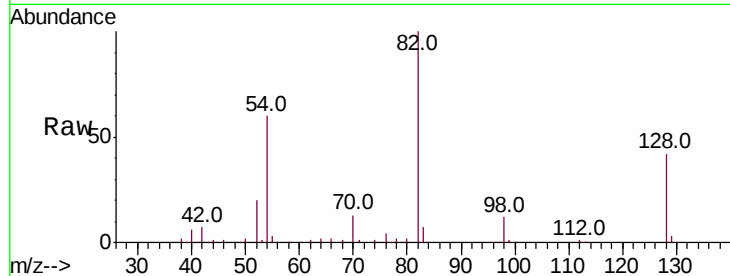


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

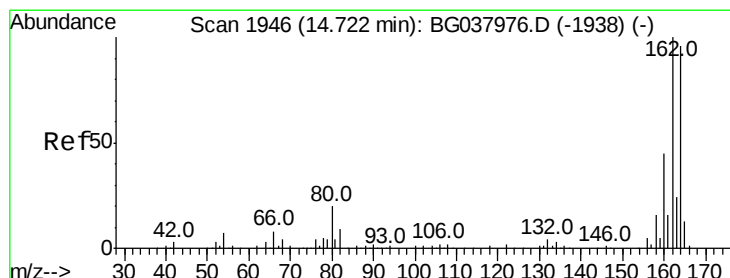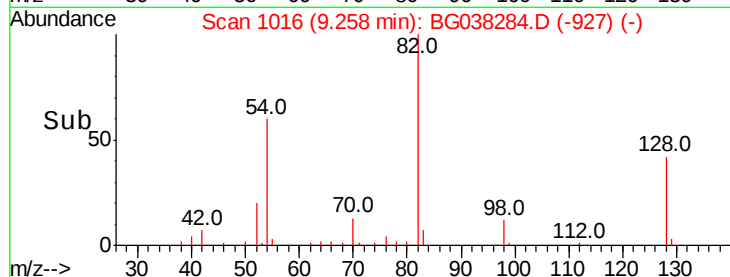
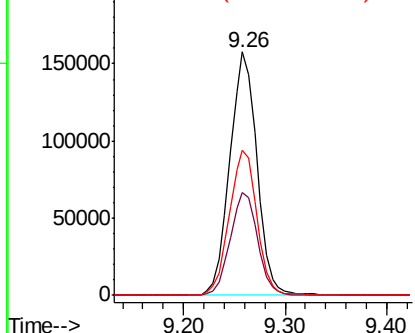


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.72 min Scan# 1945
Delta R.T. -0.01 min
Lab File: BG038284.D
Acq: 1 Dec 2018 9:08

Tgt Ion: 164 Resp: 104573
Ion Ratio Lower Upper
164 100
162 107.5 81.3 121.9
160 45.3 36.3 54.5

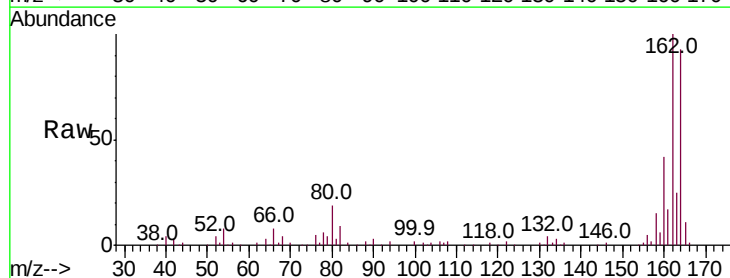

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

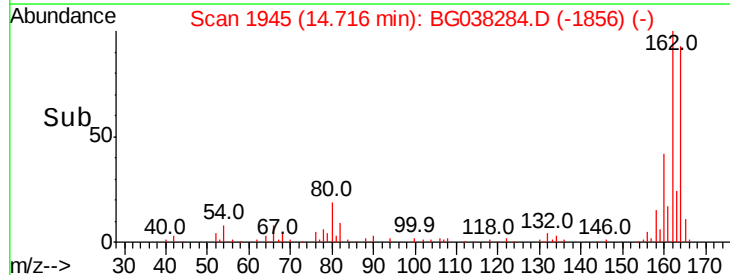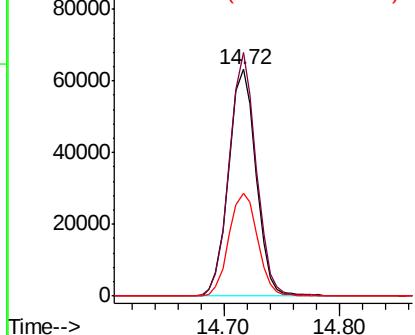






#42
 2,4,6-Tribromophenol
 Concen: 80.788 ng
 RT: 16.20 min Scan# 2198
 Delta R.T. -0.01 min
 Lab File: BG038284.D
 Acq: 1 Dec 2018 9:08

Instrument :
 BNA_G
 ClientSampleId :
 112818-CHDE-F-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.7	78.4	117.6
141	40.4	32.2	48.2

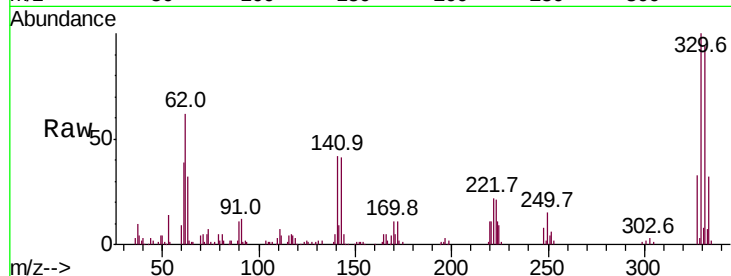


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

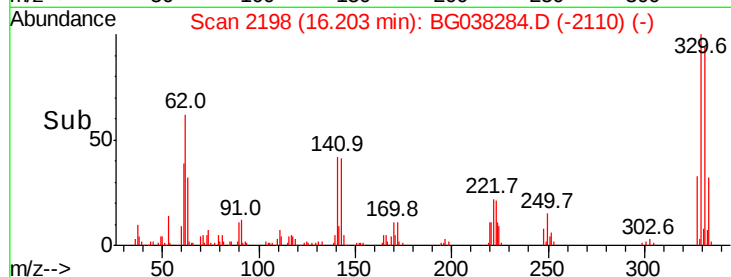
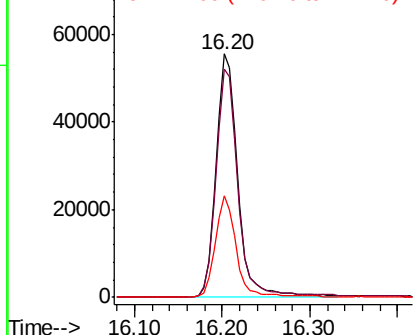



#45
 2-Fluorobiphenyl
 Concen: 93.451 ng
 RT: 13.34 min Scan# 1710
 Delta R.T. -0.01 min
 Lab File: BG038284.D
 Acq: 1 Dec 2018 9:08

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	31.0	46.4
170	25.1	20.2	30.2

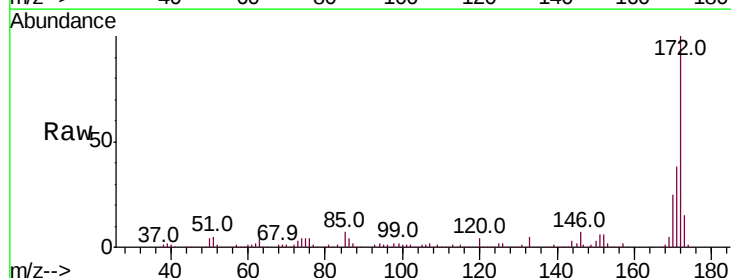

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

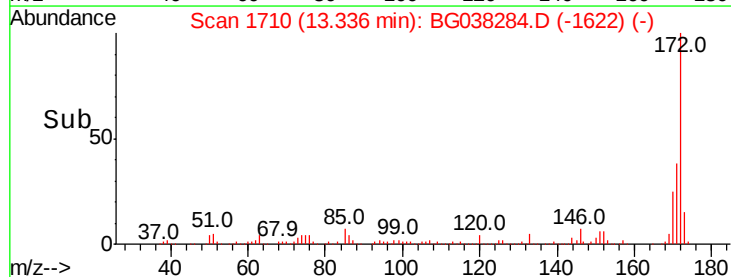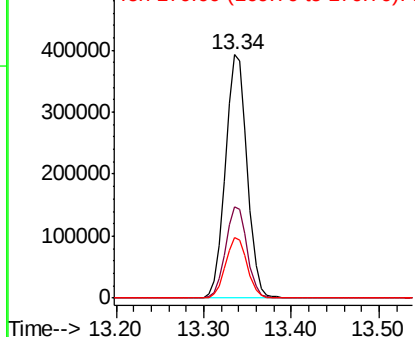

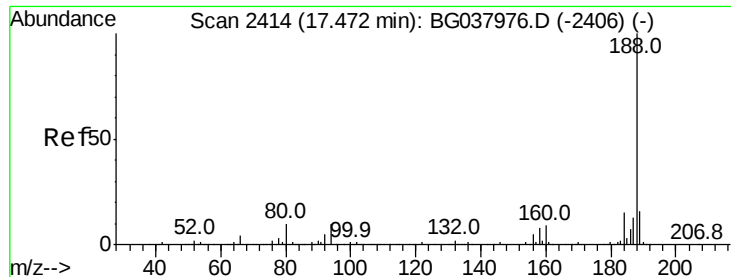

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.46 min Scan# 2412

Delta R.T. -0.01 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08

Instrument :

BNA_G

ClientSampleId :

112818-CHDE-F-U-S


Tot Ion:188 Resp: 232386

Ion Ratio Lower Upper

188 100

94 8.2 7.2 10.8




80 9.1 7.7 11.5

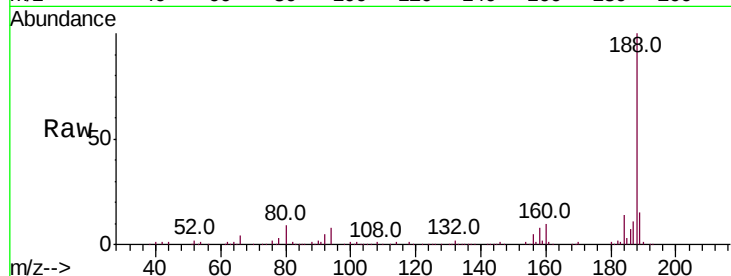

Abundance Ion 188.00 (187.70 to 188.70): E

200000 Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

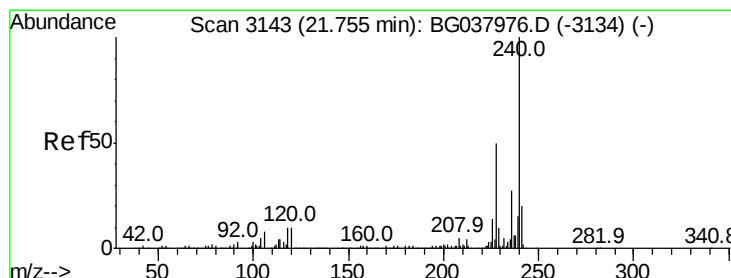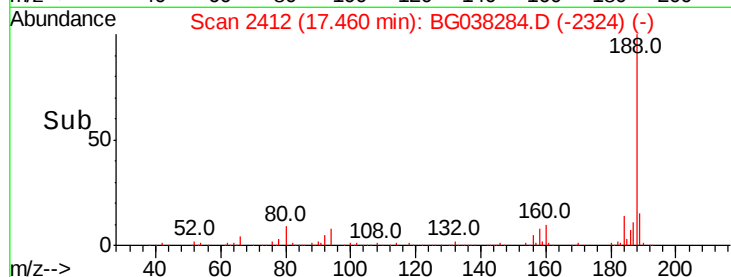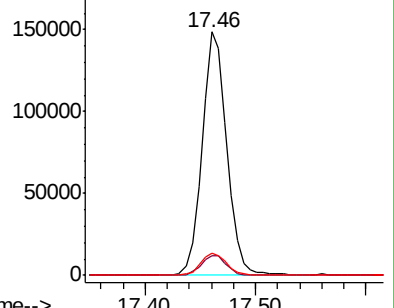

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.74 min Scan# 3141

Delta R.T. -0.01 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08


Tgt Ion:240 Resp: 214080

Ion Ratio Lower Upper

240 100

120 9.9 8.1 12.1



236 27.6 21.4 32.0

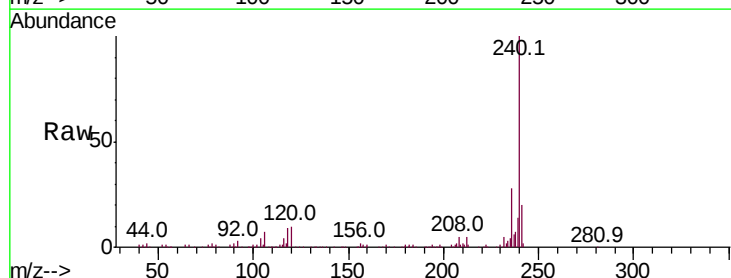

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

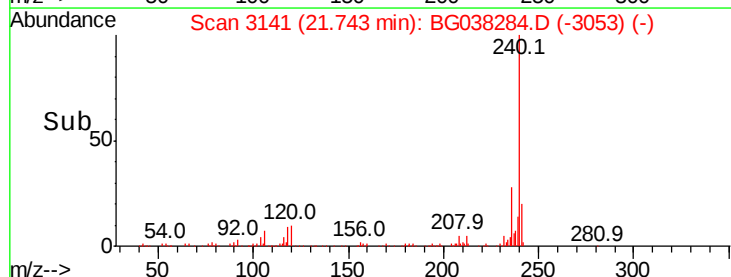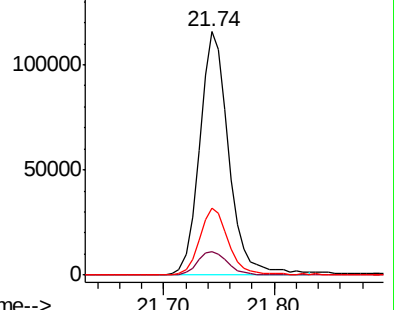



#79

Terphenyl-d14

Concen: 104.804 ng

RT: 20.06 min Scan# 2855

Delta R.T. -0.01 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08

Instrument :

BNA_G

ClientSampleId :

112818-CHDE-F-U-S


Tot Ion:244 Resp: 953520

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7




122 9.7 9.0 13.4

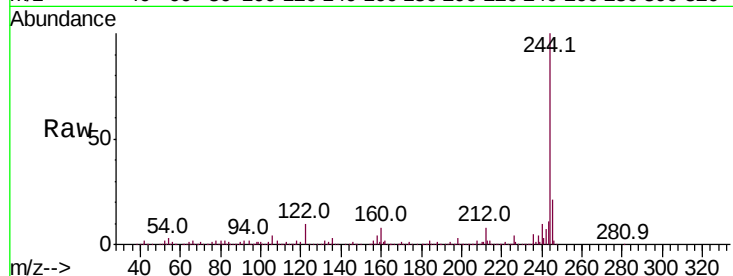

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

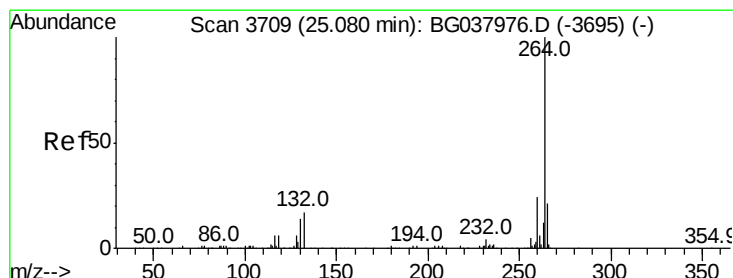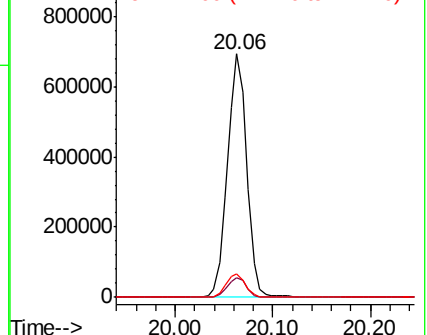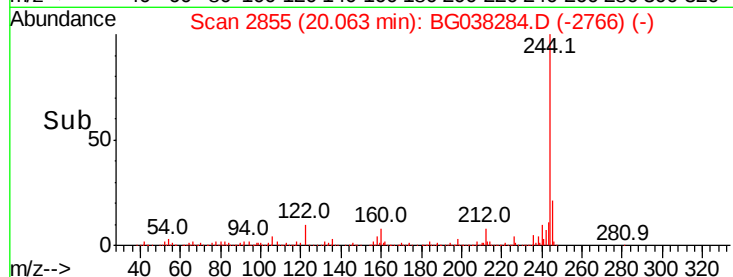

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.02 min

Lab File: BG038284.D

Acq: 1 Dec 2018 9:08


Tgt Ion:264 Resp: 200611

Ion Ratio Lower Upper

264 100

260 24.9 18.2 27.4

265 22.0 17.9 26.9

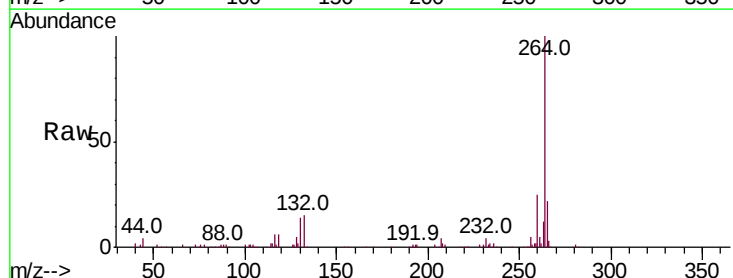

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

