

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113020\
 Data File : BG047483.D
 Acq On : 30 Nov 2020 10:46
 Operator : CG/JU
 Sample : PB133258BL
 Misc : MDL-WATER-BL-06
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.491	25	26	30	rBV	2673	2543	0.18%	0.019%
2	3.550	30	36	37	rBV3	3326	3818	0.27%	0.028%
3	3.608	42	46	52	rVV3	10719	16210	1.15%	0.119%
4	3.650	52	53	57	rVB	2282	2773	0.20%	0.020%
5	4.031	115	118	129	rBV	132542	238290	16.94%	1.750%
6	4.349	170	172	174	rBV2	2731	2721	0.19%	0.020%
7	4.390	175	179	181	rVV2	4733	5763	0.41%	0.042%
8	4.831	250	254	256	rVB	2457	3652	0.26%	0.027%
9	4.854	256	258	259	rBV	2359	2000	0.14%	0.015%
10	5.459	357	361	364	rVB	2501	3963	0.28%	0.029%
11	5.559	376	378	381	rBV2	1887	2831	0.20%	0.021%
12	5.876	430	432	433	rBV2	3354	2217	0.16%	0.016%
13	6.105	468	471	475	rBV2	2381	3288	0.23%	0.024%
14	6.158	478	480	482	rBV2	2548	2078	0.15%	0.015%
15	6.288	499	502	506	rVB2	2577	2648	0.19%	0.019%
16	6.517	538	541	544	rBV2	1320	1958	0.14%	0.014%
17	7.292	669	673	676	rBV	1857	2022	0.14%	0.015%
18	7.398	684	691	701	rBV	213443	365389	25.98%	2.683%
19	7.580	714	722	730	rBV	120409	210149	14.94%	1.543%
20	7.709	741	744	746	rBV	2006	1918	0.14%	0.014%
21	7.792	748	758	768	rBV	200175	363482	25.85%	2.669%
22	7.874	768	772	774	rVB	1717	2383	0.17%	0.018%
23	8.068	803	805	807	rBV	3038	2072	0.15%	0.015%
24	8.268	832	839	845	rBV2	140092	237728	16.90%	1.746%
25	8.420	860	865	867	rBV2	1236	2350	0.17%	0.017%
26	8.673	903	908	910	rVB2	1594	2234	0.16%	0.016%
27	8.720	912	916	919	rVV	2392	2350	0.17%	0.017%
28	8.955	949	956	964	rBV	241937	427404	30.39%	3.139%
29	9.431	1029	1037	1046	rBV	194271	360420	25.63%	2.647%
30	9.525	1051	1053	1056	rBV	1723	2057	0.15%	0.015%
31	9.889	1112	1115	1117	rBV	2452	2138	0.15%	0.016%
32	9.948	1122	1125	1127	rBV	1626	1979	0.14%	0.015%
33	10.007	1133	1135	1137	rBV	2518	1950	0.14%	0.014%
34	10.089	1145	1149	1152	rBV	1402	2047	0.15%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113020\
 Data File : BG047483.D
 Acq On : 30 Nov 2020 10:46
 Operator : CG/JU
 Sample : PB133258BL
 Misc : MDL-WATER-BL-06
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	10.165	1155	1162	1169	rVV	184722	334480	23.78%	2.456%
36	10.700	1245	1253	1263	rBV2	255532	481682	34.25%	3.537%
37	11.094	1311	1320	1329	rVB	161645	305999	21.76%	2.247%
38	11.217	1332	1341	1350	rBV	240299	440735	31.34%	3.237%
39	11.294	1350	1354	1356	rVV	2237	2246	0.16%	0.016%
40	11.540	1393	1396	1399	rVB	1832	2417	0.17%	0.018%
41	11.576	1399	1402	1404	rBV	1902	1971	0.14%	0.014%
42	11.687	1418	1421	1423	rBV	1563	2194	0.16%	0.016%
43	11.805	1439	1441	1444	rBV	2097	2192	0.16%	0.016%
44	11.858	1449	1450	1454	rBV	1559	1907	0.14%	0.014%
45	12.051	1480	1483	1485	rBV	2192	2396	0.17%	0.018%
46	12.398	1538	1542	1545	rBV	1382	1908	0.14%	0.014%
47	12.651	1584	1585	1587	rBV	2314	1983	0.14%	0.015%
48	13.027	1647	1649	1655	rVB	1547	2295	0.16%	0.017%
49	13.168	1671	1673	1676	rVB	2170	1925	0.14%	0.014%
50	14.272	1853	1861	1868	rBV	537941	764699	54.37%	5.616%
51	14.325	1868	1870	1873	rVV	3096	3120	0.22%	0.023%
52	14.361	1875	1876	1881	rVV	2063	2967	0.21%	0.022%
53	14.578	1907	1913	1922	rVB	503167	783158	55.69%	5.751%
54	14.748	1939	1942	1945	rVB	1568	1934	0.14%	0.014%
55	14.883	1955	1965	1971	rVB	289945	451937	32.14%	3.319%
56	15.042	1985	1992	2003	rBV	257943	413687	29.42%	3.038%
57	15.113	2003	2004	2007	rVB3	3312	2450	0.17%	0.018%
58	15.218	2019	2022	2024	rBV	2013	2028	0.14%	0.015%
59	15.277	2027	2032	2034	rVB3	3207	3853	0.27%	0.028%
60	15.865	2126	2132	2139	rBV	645904	969218	68.92%	7.118%
61	15.965	2144	2149	2160	rVV	196511	299191	21.27%	2.197%
62	16.070	2163	2167	2168	rBV	1753	2109	0.15%	0.015%
63	16.106	2168	2173	2178	rVB3	10819	15004	1.07%	0.110%
64	16.252	2195	2198	2201	rBV	1454	2159	0.15%	0.016%
65	16.605	2255	2258	2261	rVB2	1964	1945	0.14%	0.014%
66	16.646	2261	2265	2271	rBV	4867	7449	0.53%	0.055%
67	16.722	2276	2278	2281	rBV	1783	2113	0.15%	0.016%
68	16.863	2300	2302	2305	rVB	1948	1982	0.14%	0.015%
69	16.963	2317	2319	2323	rVB	1711	2532	0.18%	0.019%
70	17.046	2330	2333	2336	rBV	1894	2131	0.15%	0.016%
71	17.234	2362	2365	2367	rBV	1244	1918	0.14%	0.014%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113020\
 Data File : BG047483.D
 Acq On : 30 Nov 2020 10:46
 Operator : CG/JU
 Sample : PB133258BL
 Misc : MDL-WATER-BL-06
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

72	17.363	2384	2387	2390	rBV2	2903	2875	0.20%	0.021%
73	17.404	2390	2394	2395	rBV	2470	2405	0.17%	0.018%
74	17.522	2413	2414	2417	rVB	2446	2217	0.16%	0.016%
75	17.616	2423	2430	2440	rBV	407360	619320	44.04%	4.548%
76	17.715	2440	2447	2455	rBV2	735076	1152627	81.96%	8.465%
77	17.868	2472	2473	2476	rBV	2078	2144	0.15%	0.016%
78	18.050	2502	2504	2506	rBV	1982	1917	0.14%	0.014%
79	18.109	2511	2514	2520	rVB3	1816	2672	0.19%	0.020%
80	18.561	2584	2591	2592	rBV3	3976	5437	0.39%	0.040%
81	18.826	2635	2636	2640	rVB2	2939	2223	0.16%	0.016%
82	18.967	2655	2660	2661	rBV2	3277	3972	0.28%	0.029%
83	19.008	2665	2667	2670	rBV3	2035	2556	0.18%	0.019%
84	19.220	2702	2703	2705	rBV2	2949	2185	0.16%	0.016%
85	19.384	2730	2731	2734	rBV	2018	2020	0.14%	0.015%
86	19.554	2758	2760	2763	rVB3	3072	2452	0.17%	0.018%
87	19.584	2763	2765	2767	rBV2	3279	2926	0.21%	0.021%
88	19.619	2767	2771	2776	rVB2	10439	12623	0.90%	0.093%
89	19.872	2810	2814	2819	rBV3	9651	10761	0.77%	0.079%
90	19.983	2826	2833	2842	rBV	964920	1406349	100.00%	10.328%
91	20.118	2854	2856	2859	rBV3	3620	5213	0.37%	0.038%
92	20.295	2884	2886	2888	rBV3	3322	2635	0.19%	0.019%
93	20.536	2925	2927	2928	rBV	5129	2445	0.17%	0.018%
94	20.553	2928	2930	2933	rVB4	4188	3557	0.25%	0.026%
95	20.929	2993	2994	2999	rVB4	6358	6275	0.45%	0.046%
96	21.899	3152	3159	3167	rVB2	423776	722662	51.39%	5.307%
97	23.109	3363	3365	3366	rBV2	9124	5845	0.42%	0.043%
98	25.072	3688	3699	3710	rVB	442837	1312401	93.32%	9.638%
99	25.307	3729	3739	3752	rVB2	216055	701732	49.90%	5.153%
100	28.985	4363	4365	4366	rBV2	7567	3744	0.27%	0.027%


Sum of corrected areas: 13616929

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG113020\
Data File : BG047483.D
Acq On : 30 Nov 2020 10:46
Operator : CG/JU
Sample : PB133258BL
Misc : MDL-WATER-BL-06
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK258

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

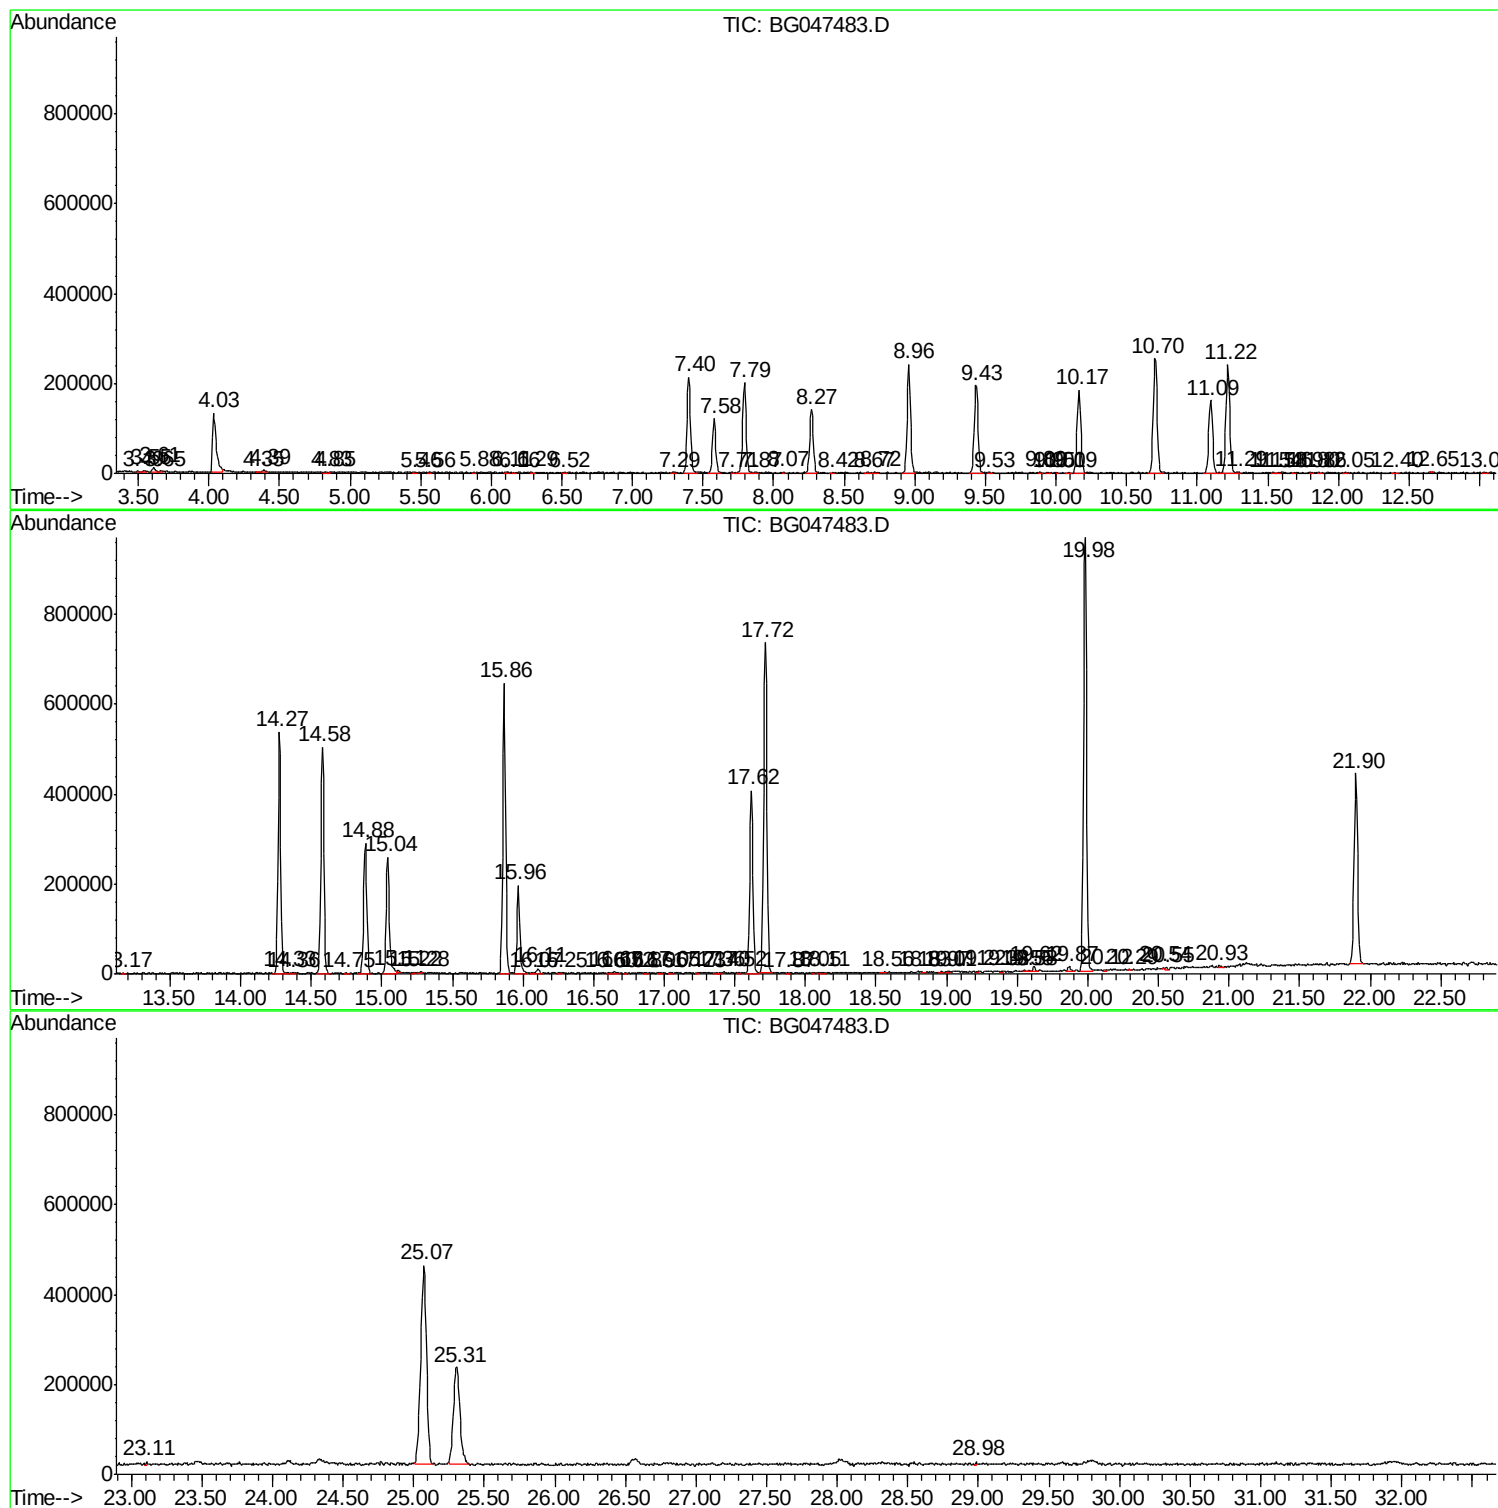

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG113020\
Data_File : BG047483.D
Acq_On : 30 Nov 2020 10:466
Operator : CG/JUU
Sample : PB133258BLL
Misc : MDL-WATER-BL-066
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK258

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
