

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051279.D
 Acq On : 30 Nov 2021 14:17
 Operator : CG/JU
 Sample : M4839-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQP2

Quant Time: Nov 30 14:52:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.191	152	23512	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.023	136	106571	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.830	164	74092	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.574	188	165538	20.000	ng/ul	0.00
79) Chrysene-d12	21.875	240	153166	20.000	ng/ul	0.00
88) Perylene-d12	25.271	264	153948	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	2637	3.897	ng/uL	-0.01
4) Pyridine-d5	3.966	84	13269	6.683	ng/ul	-0.01
7) Phenol-d5	7.356	99	38504	16.570	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.509	67	30490	20.892	ng/ul	0.00
11) 2-Chlorophenol-d4	7.721	132	30889	18.459	ng/ul	-0.01
15) 4-Methylphenol-d8	8.908	113	29491	15.727	ng/ul	0.00
21) Nitrobenzene-d5	9.372	128	18583	20.657	ng/ul	0.00
24) 2-Nitrophenol-d4	10.094	143	20163	19.869	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.647	165	31030	18.022	ng/ul	0.00
31) 4-Chloroaniline-d4	11.164	131	30373	12.056	ng/ul	0.00
46) Dimethylphthalate-d6	14.219	166	120014	21.052	ng/ul	0.00
49) Acenaphthylene-d8	14.524	160	143747	19.996	ng/ul	0.00
54) 4-Nitrophenol-d4	15.053	143	11732	12.714	ng/ul	0.00
60) Fluorene-d10	15.817	176	105574	20.565	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.952	200	12299	12.040	ng/ul	0.00
73) Anthracene-d10	17.674	188	174699	22.066	ng/ul	0.00
81) Pyrene-d10	19.953	212	201205	21.710	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.036	264	164923	20.059	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.386	94	2913	1.210	ng/ul	93
78) Di-n-butylphthalate	18.508	149	19375	1.886	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051279.D
Acq On : 30 Nov 2021 14:17
Operator : CG/JU
Sample : M4839-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQP2

Quant Time: Nov 30 14:52:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




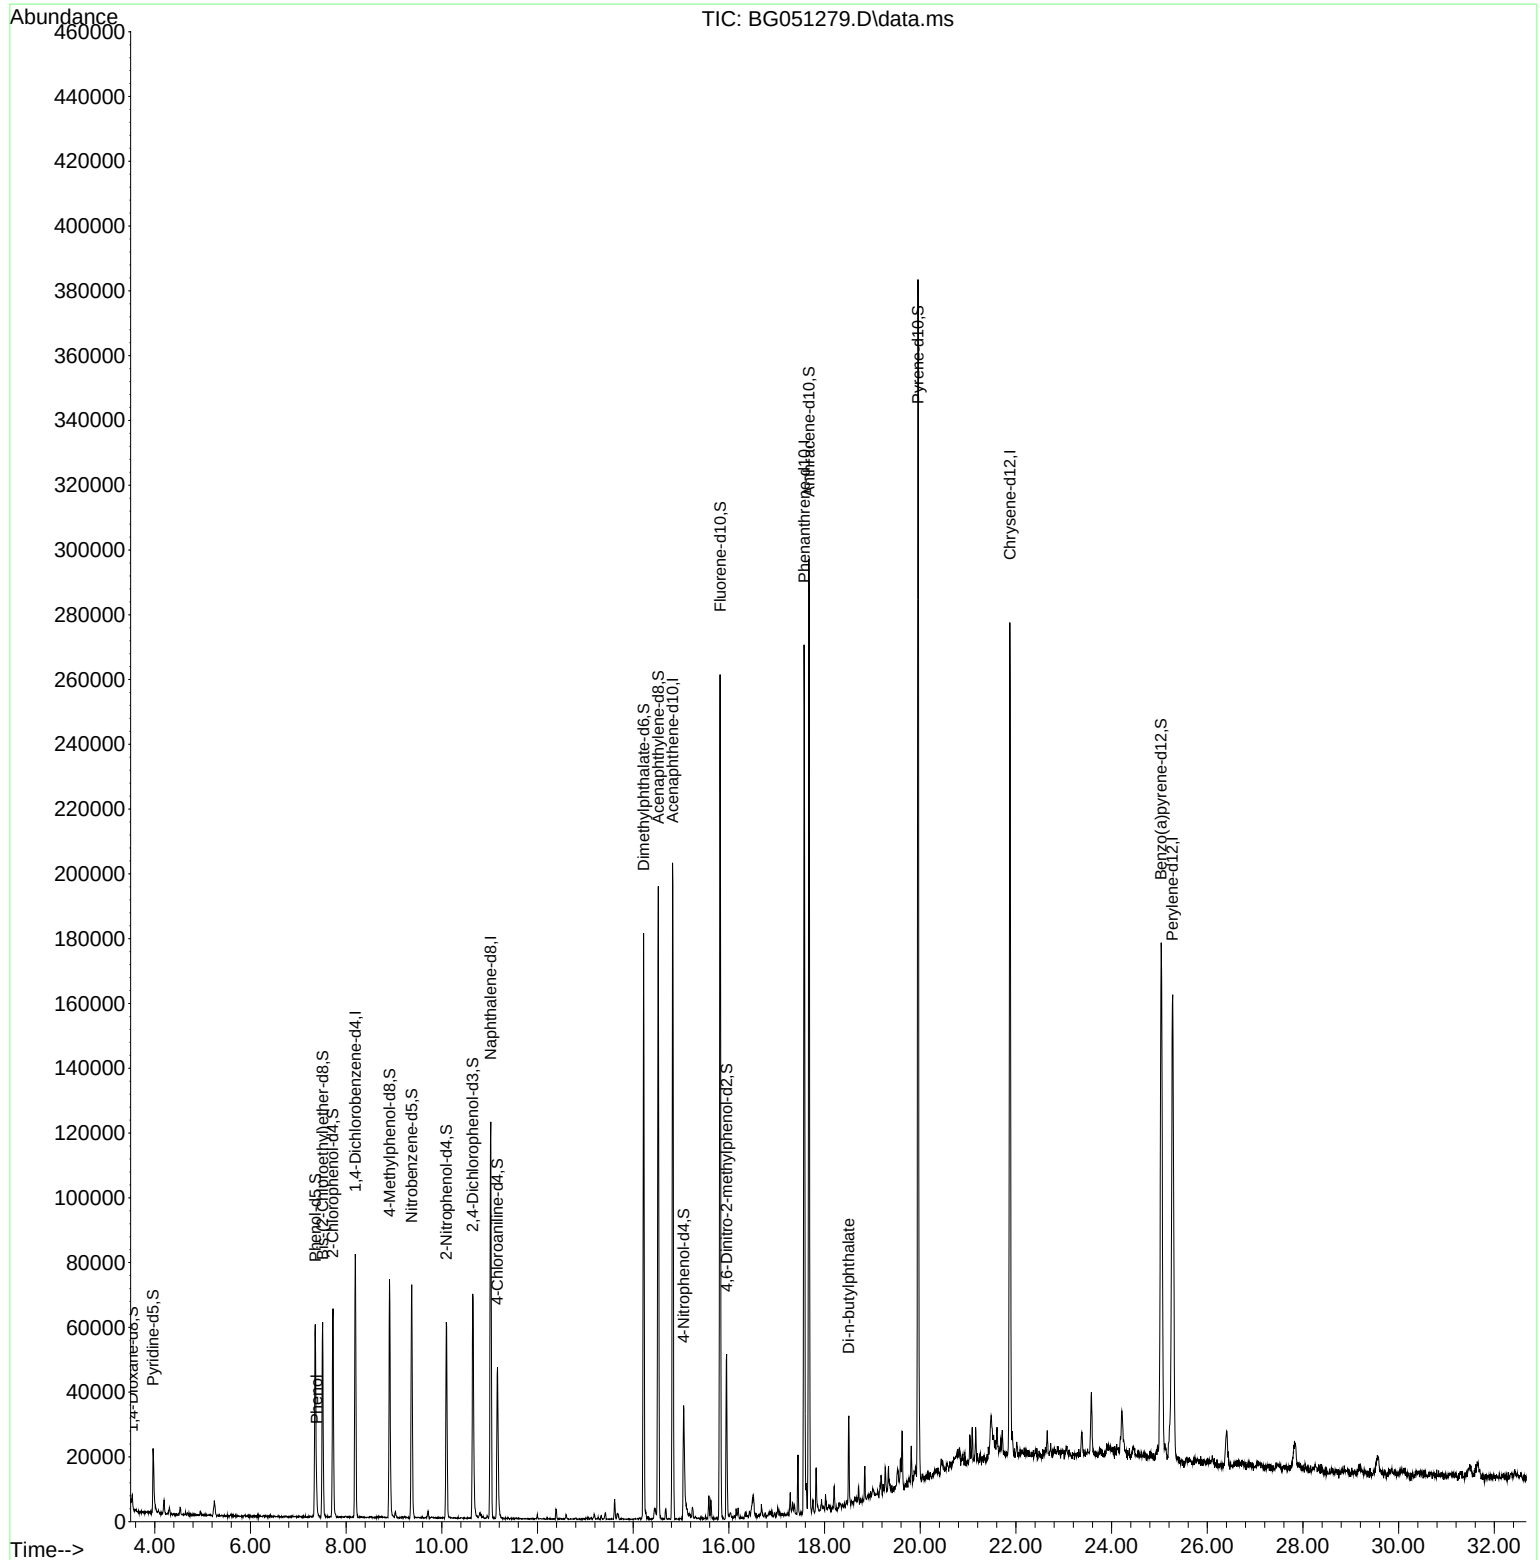


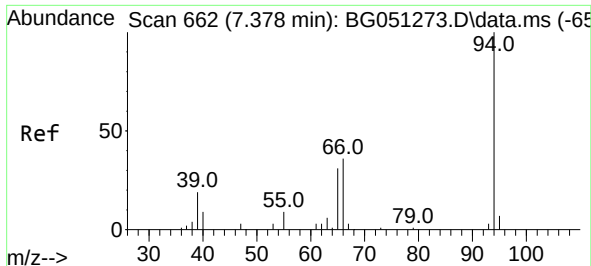

#8
Phenol
Concen: 1.210 ng/ul
RT: 7.386 min Scan# 60
Delta R.T. -0.001 min
Lab File: BG051279.D
Acq: 30 Nov 2021 14:17

Instrument :
BNA_G
ClientSampleId :
ESQP2

Tgt Ion: 94 Resp: 2913
Ion Ratio Lower Upper
94 100
65 37.3 25.1 37.7
66 42.3 31.6 47.4

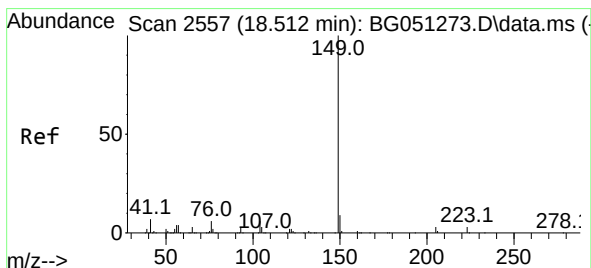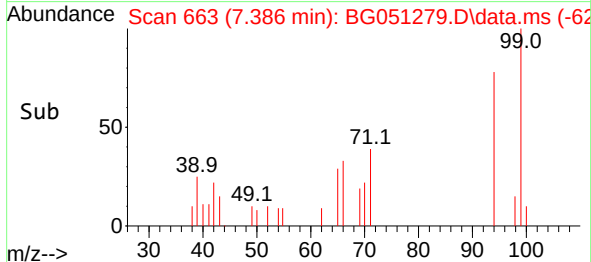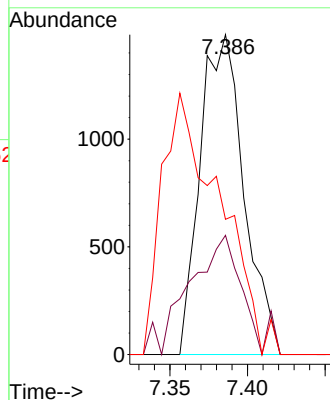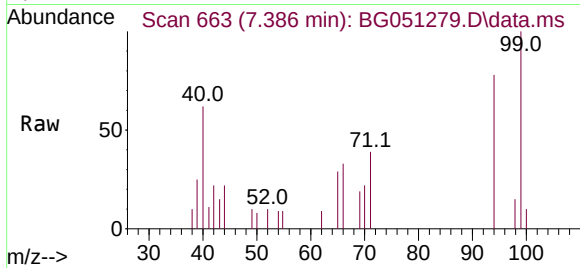

#78
Di-n-butylphthalate
Concen: 1.886 ng/ul
RT: 18.508 min Scan# 2556
Delta R.T. -0.006 min
Lab File: BG051279.D
Acq: 30 Nov 2021 14:17

Tgt Ion: 149 Resp: 19375
Ion Ratio Lower Upper
149 100
150 8.6 7.5 11.3
104 6.4 5.0 7.6

