

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051282.D
 Acq On : 30 Nov 2021 16:20
 Operator : CG/JU
 Sample : M4839-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQP1

Quant Time: Nov 30 16:52:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.194	152	25953	20.000	ng/ul	0.00
20) Naphthalene-d8	11.021	136	116917	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.828	164	82340	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.578	188	183924	20.000	ng/ul	0.00
79) Chrysene-d12	21.878	240	166785	20.000	ng/ul	0.00
88) Perylene-d12	25.274	264	162065	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.529	96	2616	3.503	ng/uL	-0.01
4) Pyridine-d5	3.964	84	23532	10.738	ng/ul	-0.01
7) Phenol-d5	7.354	99	47263	18.426	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.507	67	34376	21.339	ng/ul	0.00
11) 2-Chlorophenol-d4	7.724	132	36216	19.607	ng/ul	0.00
15) 4-Methylphenol-d8	8.905	113	39083	18.882	ng/ul	0.00
21) Nitrobenzene-d5	9.375	128	20140	20.406	ng/ul	0.00
24) 2-Nitrophenol-d4	10.098	143	22983	20.644	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.650	165	35390	18.735	ng/ul	0.00
31) 4-Chloroaniline-d4	11.162	131	38426	13.903	ng/ul	0.00
46) Dimethylphthalate-d6	14.217	166	133677	21.099	ng/ul	0.00
49) Acenaphthylene-d8	14.522	160	159473	19.961	ng/ul	0.00
54) 4-Nitrophenol-d4	15.051	143	15356	14.974	ng/ul	0.00
60) Fluorene-d10	15.815	176	115850	20.306	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.950	200	13509	11.903	ng/ul	0.00
73) Anthracene-d10	17.677	188	190194	21.622	ng/ul	0.00
81) Pyrene-d10	19.957	212	217826	21.585	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.039	264	175029	20.222	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.384	94	4279	1.610	ng/ul	97
78) Di-n-butylphthalate	18.506	149	12596	1.103	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051282.D
Acq On : 30 Nov 2021 16:20
Operator : CG/JU
Sample : M4839-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQP1

Quant Time: Nov 30 16:52:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




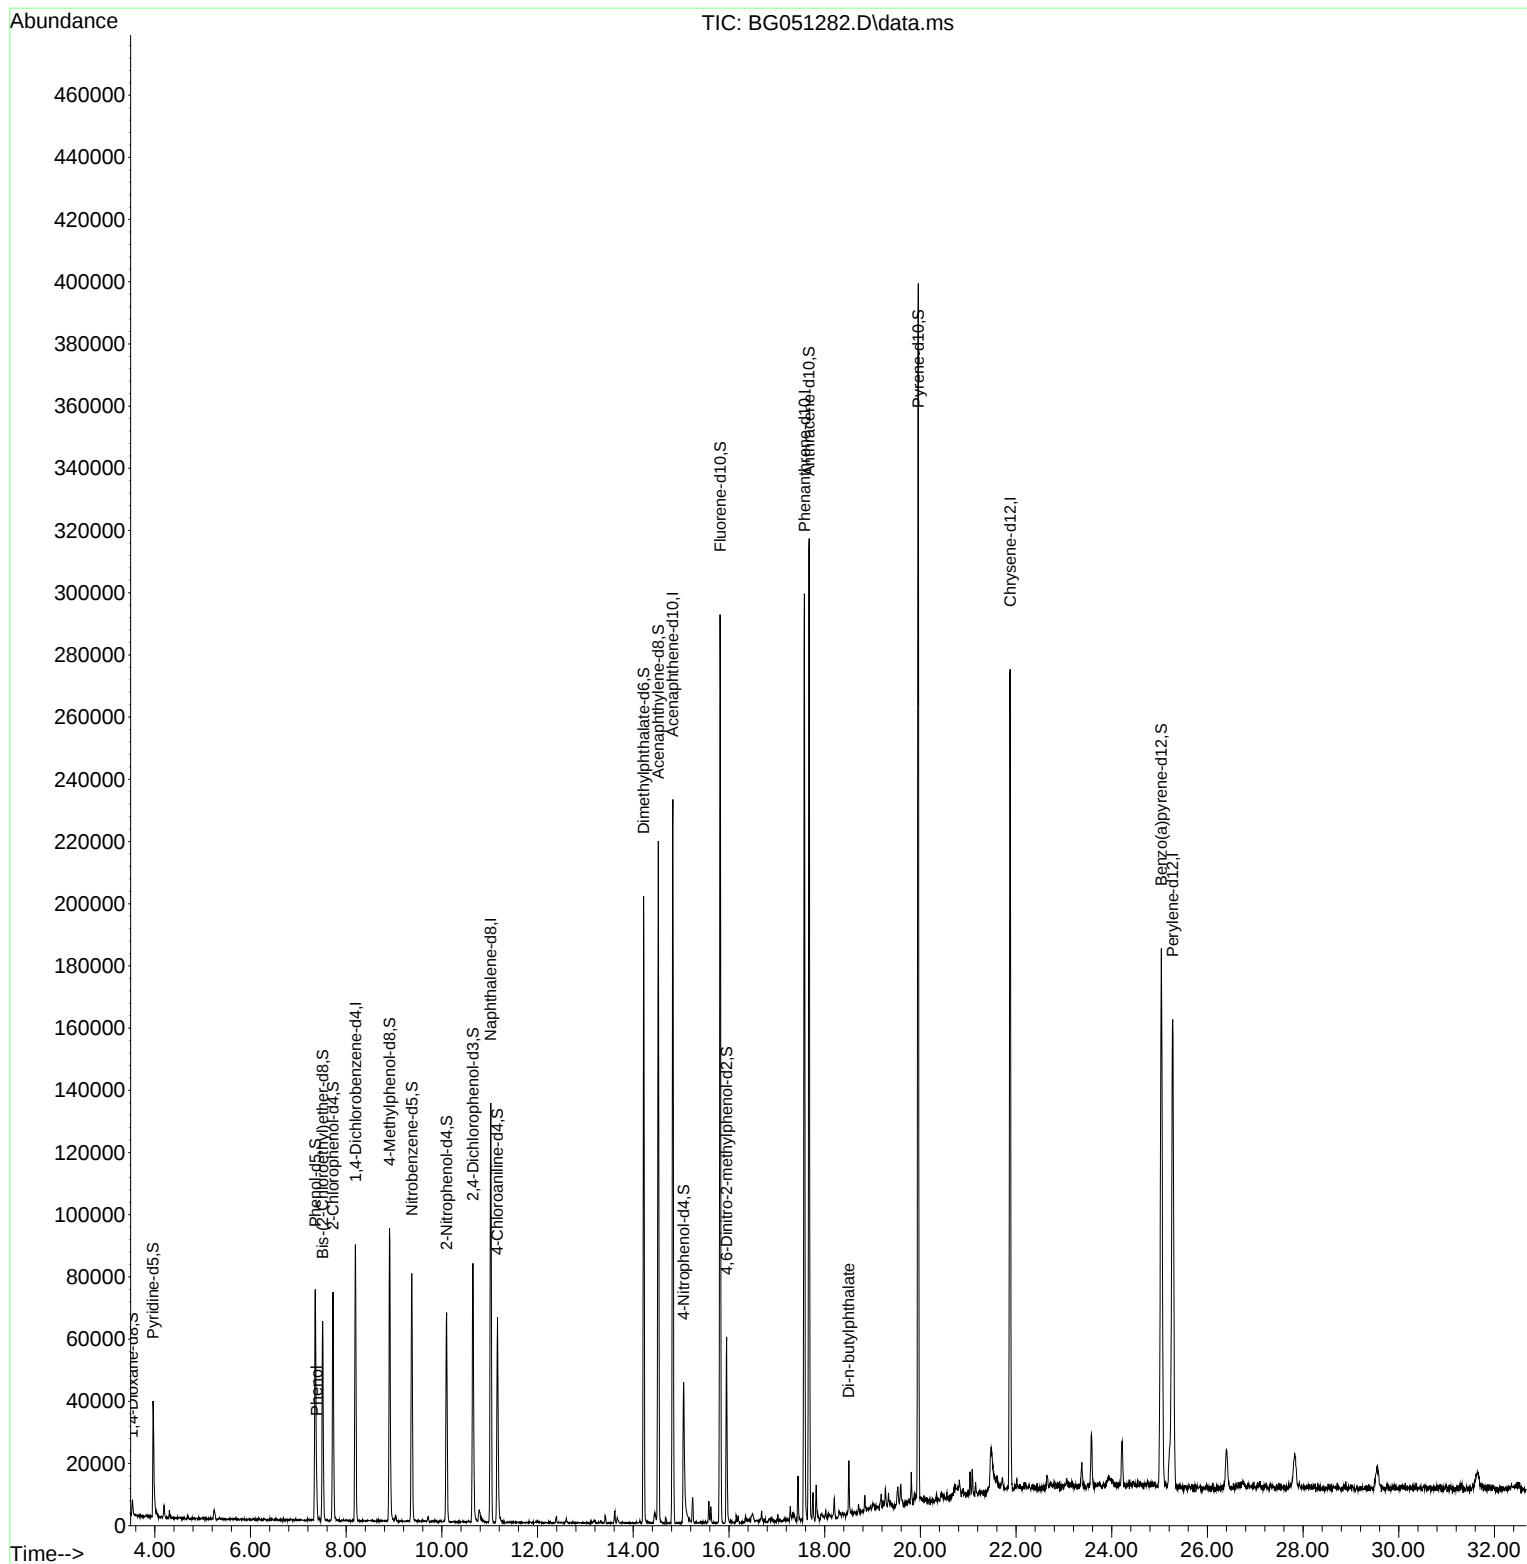


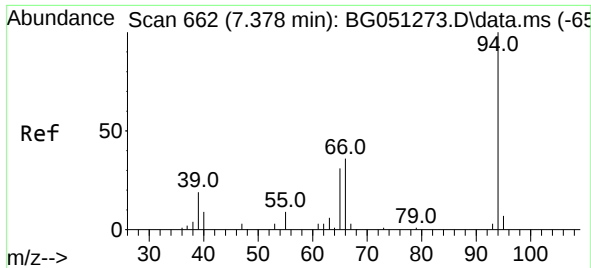

#8
Phenol
Concen: 1.610 ng/ul
RT: 7.384 min Scan# 663
Delta R.T. -0.003 min
Lab File: BG051282.D
Acq: 30 Nov 2021 16:20

Instrument :
BNA_G
ClientSampleId :
ESQP1

Tgt Ion: 94	Resp: 4279
Ion Ratio	Lower Upper
94 100	
65 32.8	25.1 37.7
66 41.6	31.6 47.4

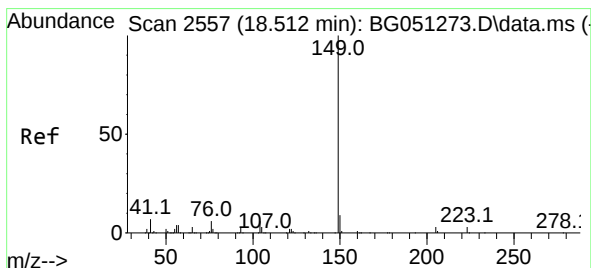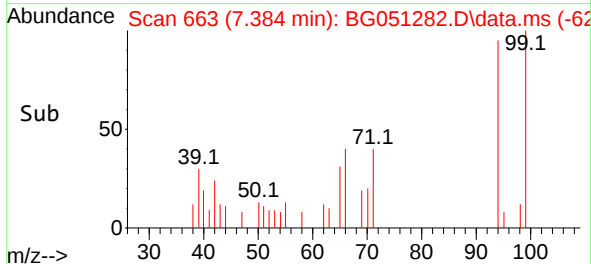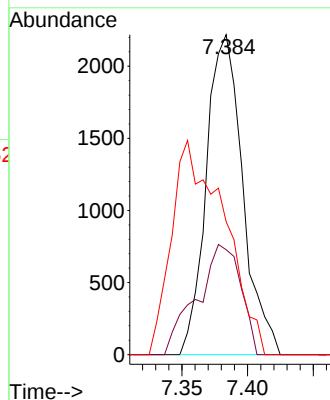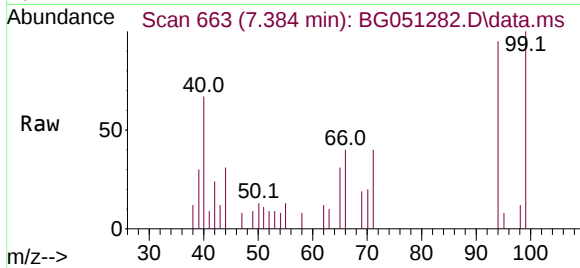

#78
Di-n-butylphthalate
Concen: 1.103 ng/ul
RT: 18.506 min Scan# 2556
Delta R.T. -0.009 min
Lab File: BG051282.D
Acq: 30 Nov 2021 16:20

Tgt Ion: 149	Resp: 12596
Ion Ratio	Lower Upper
149 100	
150 10.7	7.5 11.3
104 5.6	5.0 7.6

