

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051277.D
 Acq On : 30 Nov 2021 12:52
 Operator : CG/JU
 Sample : M4847-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.707	35	37	43	rBV3	691	900	0.18%	0.041%
2	3.760	43	46	49	rVB3	777	856	0.17%	0.039%
3	3.860	62	63	70	rVB4	829	1157	0.23%	0.053%
4	3.966	79	81	86	rBV5	749	851	0.17%	0.039%
5	4.254	129	130	133	rVB2	1308	850	0.17%	0.039%
6	4.301	133	138	143	rBV4	1589	3853	0.78%	0.176%
7	4.459	162	165	170	rBV4	697	1250	0.25%	0.057%
8	4.606	186	190	192	rVB4	698	639	0.13%	0.029%
9	4.941	243	247	249	rVB2	575	689	0.14%	0.031%
10	4.994	255	256	261	rVB2	711	940	0.19%	0.043%
11	5.211	291	293	296	rVB3	640	557	0.11%	0.025%
12	5.282	302	305	309	rVB2	572	803	0.16%	0.037%
13	5.429	327	330	333	rBV	650	738	0.15%	0.034%
14	5.629	362	364	367	rVV3	643	768	0.15%	0.035%
15	5.693	371	375	378	rVB4	469	907	0.18%	0.041%
16	5.764	384	387	390	rBV4	622	899	0.18%	0.041%
17	6.034	431	433	438	rVB3	421	688	0.14%	0.031%
18	6.404	493	496	499	rBV2	594	938	0.19%	0.043%
19	6.833	566	569	572	rBV2	357	581	0.12%	0.027%
20	8.196	794	801	812	rBV	77988	142639	28.69%	6.518%
21	11.022	1275	1282	1296	rBV	109018	206945	41.63%	9.457%
22	12.015	1448	1451	1455	rBV	518	817	0.16%	0.037%
23	13.813	1754	1757	1761	rVB2	468	696	0.14%	0.032%
24	14.830	1922	1930	1941	rBV	187835	318615	64.09%	14.559%
25	14.900	1941	1942	1947	rVB2	748	733	0.15%	0.033%
26	16.216	2162	2166	2170	rBV2	403	607	0.12%	0.028%
27	17.573	2391	2397	2407	rVV	258798	422059	84.90%	19.286%
28	17.638	2407	2408	2412	rVB3	845	886	0.18%	0.040%
29	17.685	2412	2416	2419	rBV3	535	677	0.14%	0.031%
30	18.355	2529	2530	2537	rVB2	404	651	0.13%	0.030%
31	18.461	2542	2548	2550	rBV2	566	882	0.18%	0.040%
32	18.513	2555	2557	2560	rBV	540	604	0.12%	0.028%
33	18.754	2597	2598	2602	rVB2	543	593	0.12%	0.027%
34	18.801	2602	2606	2608	rBV3	631	866	0.17%	0.040%
35	19.442	2714	2715	2720	rVB2	610	600	0.12%	0.027%
36	19.671	2750	2754	2755	rBV3	462	604	0.12%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051277.D
 Acq On : 30 Nov 2021 12:52
 Operator : CG/JU
 Sample : M4847-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	19.759	2766	2769	2773	rBV3	625	888	0.18%	0.041%
38	19.900	2792	2793	2795	rBV2	648	536	0.11%	0.024%
39	19.941	2798	2800	2802	rBV2	1016	790	0.16%	0.036%
40	19.965	2802	2804	2805	rBV	914	777	0.16%	0.036%
41	20.135	2830	2833	2836	rBV2	797	896	0.18%	0.041%
42	20.164	2836	2838	2839	rVB2	1117	690	0.14%	0.032%
43	20.188	2839	2842	2843	rBV2	1070	1116	0.22%	0.051%
44	20.235	2848	2850	2854	rVB2	737	905	0.18%	0.041%
45	20.276	2854	2857	2858	rBV2	873	1088	0.22%	0.050%
46	20.411	2878	2880	2882	rBV3	640	785	0.16%	0.036%
47	20.505	2895	2896	2899	rBV3	1097	1139	0.23%	0.052%
48	20.535	2899	2901	2905	rVB4	1742	2055	0.41%	0.094%
49	20.582	2905	2909	2910	rBV4	1148	1440	0.29%	0.066%
50	20.623	2914	2916	2921	rVB4	789	1080	0.22%	0.049%
51	20.664	2921	2923	2925	rBV3	989	1138	0.23%	0.052%
52	20.687	2925	2927	2929	rBV3	1476	1014	0.20%	0.046%
53	20.711	2929	2931	2932	rBV2	1512	821	0.17%	0.038%
54	20.764	2938	2940	2941	rBV2	1939	1569	0.32%	0.072%
55	20.787	2941	2944	2947	rVV4	1337	1951	0.39%	0.089%
56	20.811	2947	2948	2952	rVB4	1651	1212	0.24%	0.055%
57	20.905	2962	2964	2966	rBV3	1040	1319	0.27%	0.060%
58	21.040	2986	2987	2990	rBV3	1434	1229	0.25%	0.056%
59	21.146	3003	3005	3006	rBV2	1329	670	0.13%	0.031%
60	21.381	3043	3045	3049	rBV5	1948	2408	0.48%	0.110%
61	21.410	3049	3050	3051	rBV	1389	578	0.12%	0.026%
62	21.428	3051	3053	3054	rVV2	1527	692	0.14%	0.032%
63	21.445	3054	3056	3059	rVV3	1276	1168	0.23%	0.053%
64	21.575	3077	3078	3079	rBV	1560	939	0.19%	0.043%
65	21.680	3094	3096	3097	rBV	2027	1204	0.24%	0.055%
66	21.874	3122	3129	3137	rBV2	286440	497137	100.00%	22.717%
67	22.450	3226	3227	3229	rBV2	1825	1065	0.21%	0.049%
68	22.591	3249	3251	3254	rVB4	1930	1332	0.27%	0.061%
69	22.644	3257	3260	3263	rBV5	3056	5351	1.08%	0.245%
70	23.314	3372	3374	3379	rVB6	1836	2502	0.50%	0.114%
71	23.466	3399	3400	3402	rBV2	1563	1628	0.33%	0.074%
72	23.508	3405	3407	3409	rBV3	1916	1641	0.33%	0.075%
73	23.531	3409	3411	3414	rVB4	1662	1496	0.30%	0.068%
74	23.801	3456	3457	3458	rBV	1660	814	0.16%	0.037%
75	24.307	3541	3543	3547	rBV4	1633	1471	0.30%	0.067%
76	24.389	3555	3557	3558	rBV2	2782	1976	0.40%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051277.D
 Acq On : 30 Nov 2021 12:52
 Operator : CG/JU
 Sample : M4847-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	24.407	3558	3560	3563	rVB3	2180	1775	0.36%	0.081%
78	24.495	3574	3575	3576	rVB	1597	563	0.11%	0.026%
79	24.553	3583	3585	3588	rVB3	2273	2240	0.45%	0.102%
80	24.612	3593	3595	3597	rBV3	1810	1636	0.33%	0.075%
81	24.683	3605	3607	3609	rBV3	1849	1167	0.23%	0.053%
82	25.194	3692	3694	3696	rBV2	2611	3406	0.69%	0.156%
83	25.276	3697	3708	3719	rVB2	157981	483601	97.28%	22.099%
84	25.805	3797	3798	3803	rBV4	2288	2137	0.43%	0.098%
85	26.304	3881	3883	3884	rBV2	1519	789	0.16%	0.036%
86	27.180	4030	4032	4033	rBV3	1566	1103	0.22%	0.050%
87	27.532	4091	4092	4094	rBV2	2183	1827	0.37%	0.083%
88	27.826	4140	4142	4144	rBV2	2663	2265	0.46%	0.104%
89	28.273	4216	4218	4221	rBV3	2185	2053	0.41%	0.094%
90	28.314	4221	4225	4227	rVV5	2411	2920	0.59%	0.133%
91	28.796	4305	4307	4309	rBV2	1750	1427	0.29%	0.065%
92	29.042	4347	4349	4351	rBV3	1802	1613	0.32%	0.074%
93	29.213	4376	4378	4379	rVB2	2106	1054	0.21%	0.048%
94	29.230	4379	4381	4382	rBV2	1458	1131	0.23%	0.052%
95	29.348	4397	4401	4402	rBV4	1689	1872	0.38%	0.086%
96	30.429	4583	4585	4586	rBV2	2014	1379	0.28%	0.063%
97	31.152	4707	4708	4710	rBV2	2097	1659	0.33%	0.076%
98	31.610	4784	4786	4787	rBV2	1982	1253	0.25%	0.057%
99	31.627	4787	4789	4791	rVV3	2482	1850	0.37%	0.085%
100	32.227	4890	4891	4892	rBV	1672	811	0.16%	0.037%




Sum of corrected areas: 2188379

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051277.D
Acq On : 30 Nov 2021 12:52
Operator : CG/JU
Sample : M4847-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

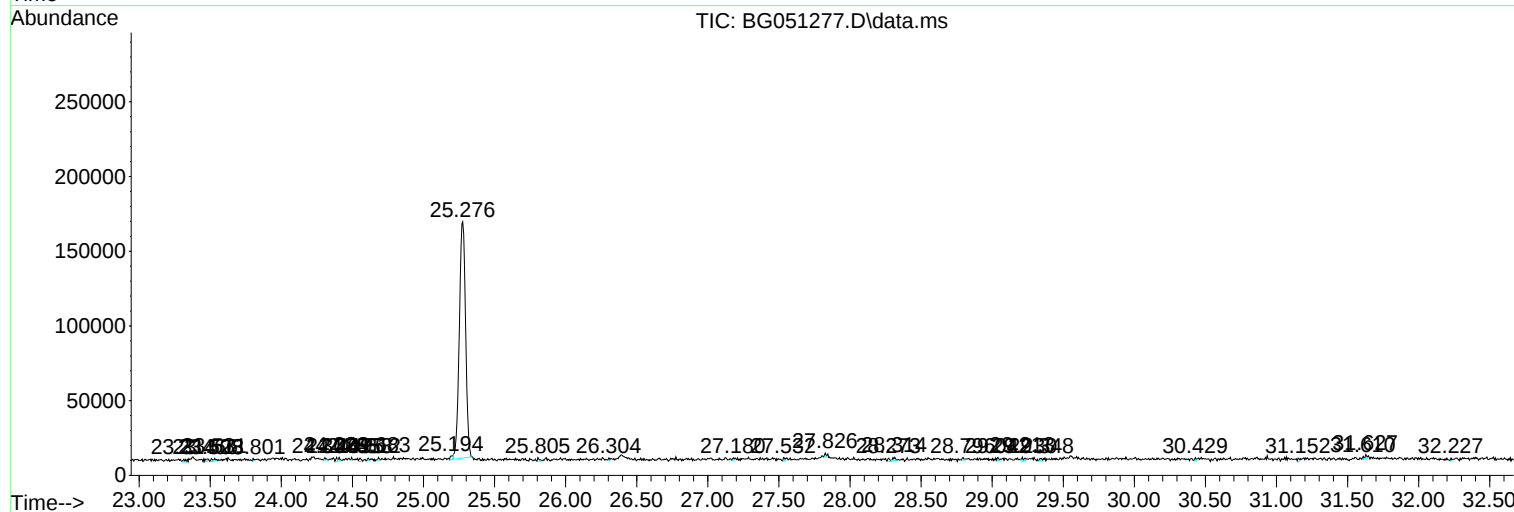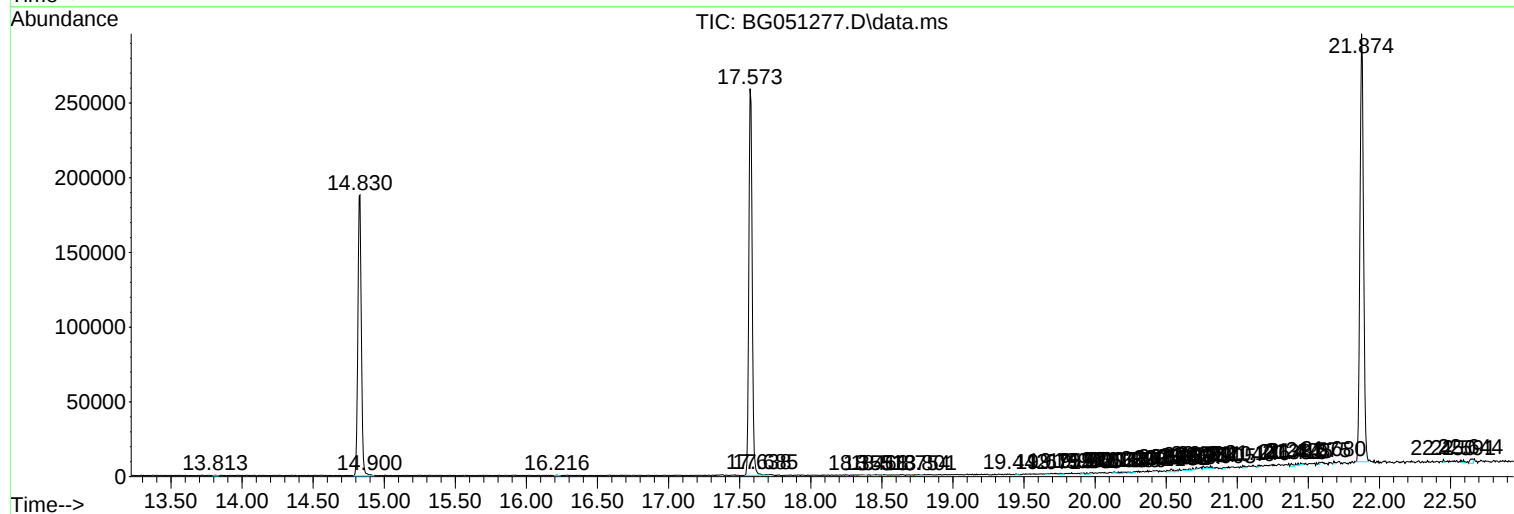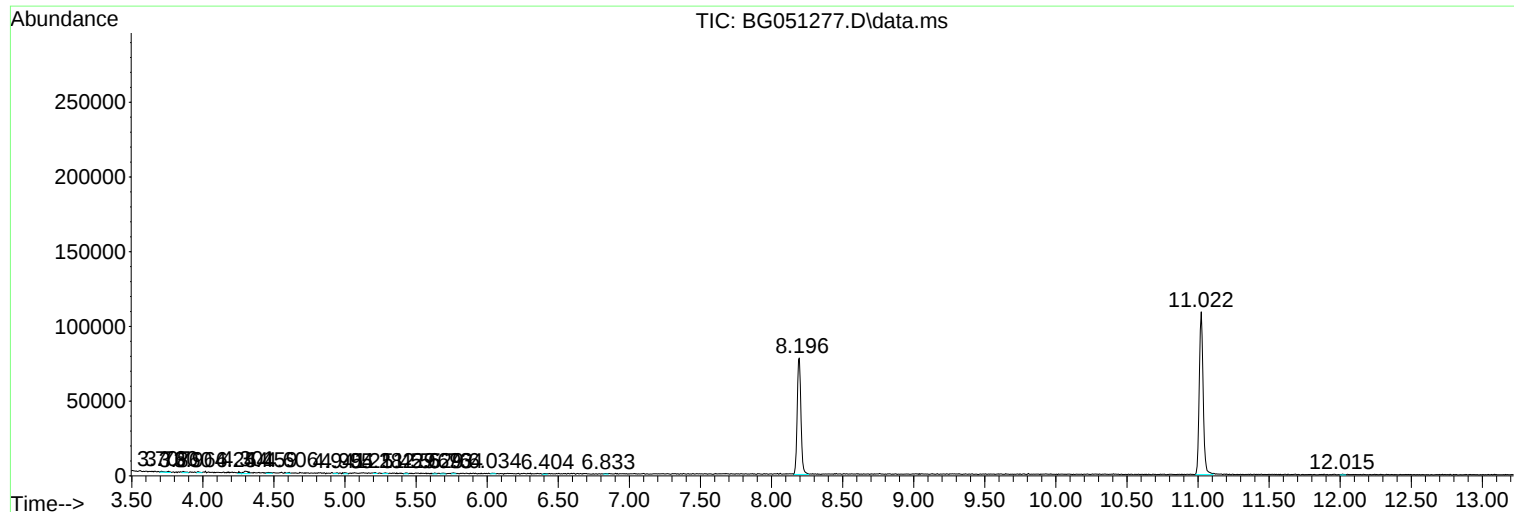

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051277.D
Acq On : 30 Nov 2021 12:52
Operator : CG/JU
Sample : M4847-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051277.D
Acq On : 30 Nov 2021 12:52
Operator : CG/JU
Sample : M4847-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc