

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051282.D
 Acq On : 30 Nov 2021 16:20
 Operator : CG/JU
 Sample : M4839-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.535	4	8	15	rVB2	4799	7231	1.28%	0.110%
2	3.964	78	81	91	rBV	37108	64661	11.48%	0.982%
3	4.193	115	120	128	rVB2	4299	7223	1.28%	0.110%
4	4.305	134	139	141	rBV4	2839	3137	0.56%	0.048%
5	4.681	201	203	205	rBV2	1125	809	0.14%	0.012%
6	5.239	294	298	305	rVB4	3164	6642	1.18%	0.101%
7	6.690	542	545	546	rBV	1048	873	0.15%	0.013%
8	6.837	566	570	572	rBV3	622	788	0.14%	0.012%
9	7.049	603	606	610	rBV3	565	898	0.16%	0.014%
10	7.354	652	658	668	rBV	74263	148303	26.33%	2.252%
11	7.507	677	684	693	rBV	64607	115695	20.54%	1.757%
12	7.724	714	721	728	rBV	73365	131774	23.39%	2.001%
13	7.907	749	752	755	rBV3	548	767	0.14%	0.012%
14	8.194	795	801	809	rVB	88852	157846	28.02%	2.397%
15	8.905	916	922	934	rBV	94067	170896	30.34%	2.596%
16	9.035	939	944	947	rBV3	1855	2694	0.48%	0.041%
17	9.370	993	1001	1011	rBV	79853	151527	26.90%	2.301%
18	9.716	1054	1060	1065	rVB2	1895	3431	0.61%	0.052%
19	10.098	1118	1125	1134	rVB2	67237	125933	22.35%	1.913%
20	10.650	1212	1219	1230	rBV	83215	164868	29.27%	2.504%
21	10.780	1236	1241	1245	rBV6	3605	7868	1.40%	0.119%
22	11.021	1275	1282	1291	rVB	134878	249671	44.32%	3.792%
23	11.162	1298	1306	1317	rBV	66048	128650	22.84%	1.954%
24	12.395	1511	1516	1520	rVB2	2074	2849	0.51%	0.043%
25	12.601	1546	1551	1554	rBV3	1536	1902	0.34%	0.029%
26	12.795	1582	1584	1589	rBV2	493	770	0.14%	0.012%
27	13.189	1648	1651	1655	rVB4	1105	1802	0.32%	0.027%
28	13.324	1671	1674	1678	rBV2	854	1078	0.19%	0.016%
29	13.412	1683	1689	1695	rVB3	2622	3938	0.70%	0.060%
30	13.618	1719	1724	1728	rBV2	4007	5467	0.97%	0.083%
31	13.665	1728	1732	1740	rBV3	1778	3330	0.59%	0.051%
32	14.217	1820	1826	1837	rVB	201502	298445	52.98%	4.533%
33	14.452	1861	1866	1871	rBV5	3481	7888	1.40%	0.120%
34	14.522	1872	1878	1886	rVV	219399	345891	61.40%	5.253%
35	14.593	1888	1890	1895	rVB2	667	918	0.16%	0.014%
36	14.675	1902	1904	1908	rBV3	1995	2545	0.45%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051282.D
 Acq On : 30 Nov 2021 16:20
 Operator : CG/JU
 Sample : M4839-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	14.828	1923	1930	1938	rVB	232841	371950	66.03%	5.649%
38	15.051	1962	1968	1986	rBV2	45285	104429	18.54%	1.586%
39	15.239	1996	2000	2008	rVB5	8315	12192	2.16%	0.185%
40	15.580	2051	2058	2062	rBV	7062	9580	1.70%	0.146%
41	15.621	2062	2065	2070	rVB4	5343	6415	1.14%	0.097%
42	15.815	2092	2098	2108	rVB	292187	445659	79.11%	6.769%
43	15.950	2114	2121	2131	rBV	59971	91780	16.29%	1.394%
44	16.032	2133	2135	2137	rVV	1200	967	0.17%	0.015%
45	16.062	2137	2140	2144	rVV2	849	774	0.14%	0.012%
46	16.150	2151	2155	2158	rBV3	2714	3136	0.56%	0.048%
47	16.191	2158	2162	2167	rVB4	2517	3512	0.62%	0.053%
48	16.350	2184	2189	2191	rBV3	2019	2590	0.46%	0.039%
49	16.438	2201	2204	2206	rVB2	1116	1123	0.20%	0.017%
50	16.579	2223	2228	2231	rVB2	515	895	0.16%	0.014%
51	16.632	2235	2237	2239	rBV2	1076	947	0.17%	0.014%
52	16.661	2239	2242	2243	rBV	882	842	0.15%	0.013%
53	16.685	2243	2246	2252	rVB3	3875	5313	0.94%	0.081%
54	16.749	2254	2257	2258	rBV2	961	914	0.16%	0.014%
55	16.837	2268	2272	2274	rBV4	1182	1657	0.29%	0.025%
56	16.890	2279	2281	2285	rVB2	1141	1189	0.21%	0.018%
57	17.019	2301	2303	2307	rVB4	2354	2870	0.51%	0.044%
58	17.066	2309	2311	2313	rVB2	836	853	0.15%	0.013%
59	17.155	2320	2326	2329	rBV4	1127	1579	0.28%	0.024%
60	17.284	2344	2348	2353	rBV4	5047	7468	1.33%	0.113%
61	17.331	2353	2356	2360	rVV4	2824	4209	0.75%	0.064%
62	17.366	2360	2362	2367	rVB3	2200	2633	0.47%	0.040%
63	17.442	2371	2375	2379	rBV3	14521	18307	3.25%	0.278%
64	17.531	2385	2390	2391	rVB3	1181	1380	0.24%	0.021%
65	17.578	2391	2398	2408	rBV	298472	464202	82.40%	7.050%
66	17.677	2408	2415	2424	rBV	315630	492222	87.38%	7.476%
67	17.760	2424	2429	2435	rVB5	9137	13915	2.47%	0.211%
68	17.824	2435	2440	2444	rBV	11662	16020	2.84%	0.243%
69	17.901	2451	2453	2454	rBV2	996	801	0.14%	0.012%
70	17.924	2454	2457	2458	rBV2	1682	1758	0.31%	0.027%
71	18.024	2471	2474	2478	rVB4	2616	2922	0.52%	0.044%
72	18.071	2480	2482	2483	rBV	1415	1110	0.20%	0.017%
73	18.200	2500	2504	2508	rVB5	6688	9658	1.71%	0.147%
74	18.300	2519	2521	2525	rBV4	1381	1623	0.29%	0.025%
75	18.506	2552	2556	2562	rVB	16948	20497	3.64%	0.311%
76	18.712	2588	2591	2595	rVB5	2731	3262	0.58%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
 Data File : BG051282.D
 Acq On : 30 Nov 2021 16:20
 Operator : CG/JU
 Sample : M4839-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	18.841	2610	2613	2616	rBV3	4556	5454	0.97%	0.083%
78	19.270	2683	2686	2693	rVB4	6047	8672	1.54%	0.132%
79	19.528	2725	2730	2736	rBV7	5763	10334	1.83%	0.157%
80	19.810	2774	2778	2783	rVB2	10698	13739	2.44%	0.209%
81	19.957	2797	2803	2809	rVB	390705	563339	100.00%	8.556%
82	21.038	2984	2987	2991	rVB2	7202	8794	1.56%	0.134%
83	21.085	2992	2995	3000	rVB3	8191	10050	1.78%	0.153%
84	21.156	3004	3007	3012	rBV7	4574	6915	1.23%	0.105%
85	21.479	3057	3062	3072	rBV10	9882	29528	5.24%	0.448%
86	21.878	3123	3130	3138	rVB	264353	462990	82.19%	7.032%
87	23.576	3416	3419	3427	rVB2	17509	31329	5.56%	0.476%
88	24.217	3523	3528	3534	rVB6	14817	31135	5.53%	0.473%
89	25.039	3658	3668	3679	rVB2	173243	488880	86.78%	7.425%
90	25.274	3700	3708	3719	rVB3	150554	450844	80.03%	6.847%




Sum of corrected areas: 6584164

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051282.D
Acq On : 30 Nov 2021 16:20
Operator : CG/JU
Sample : M4839-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

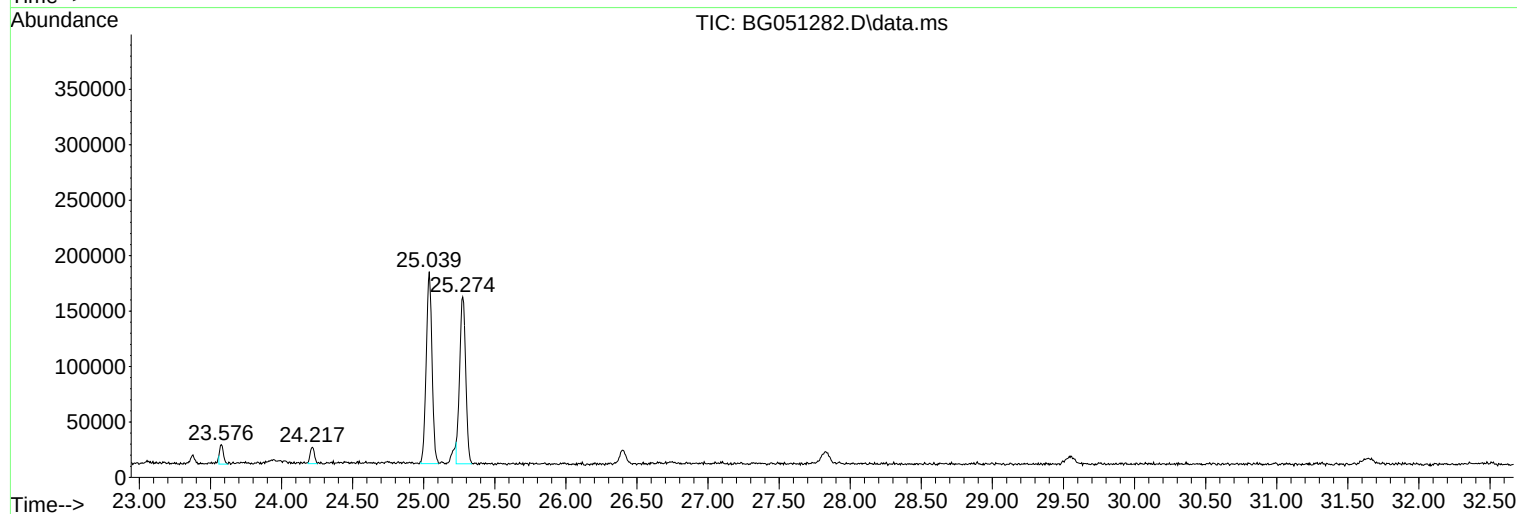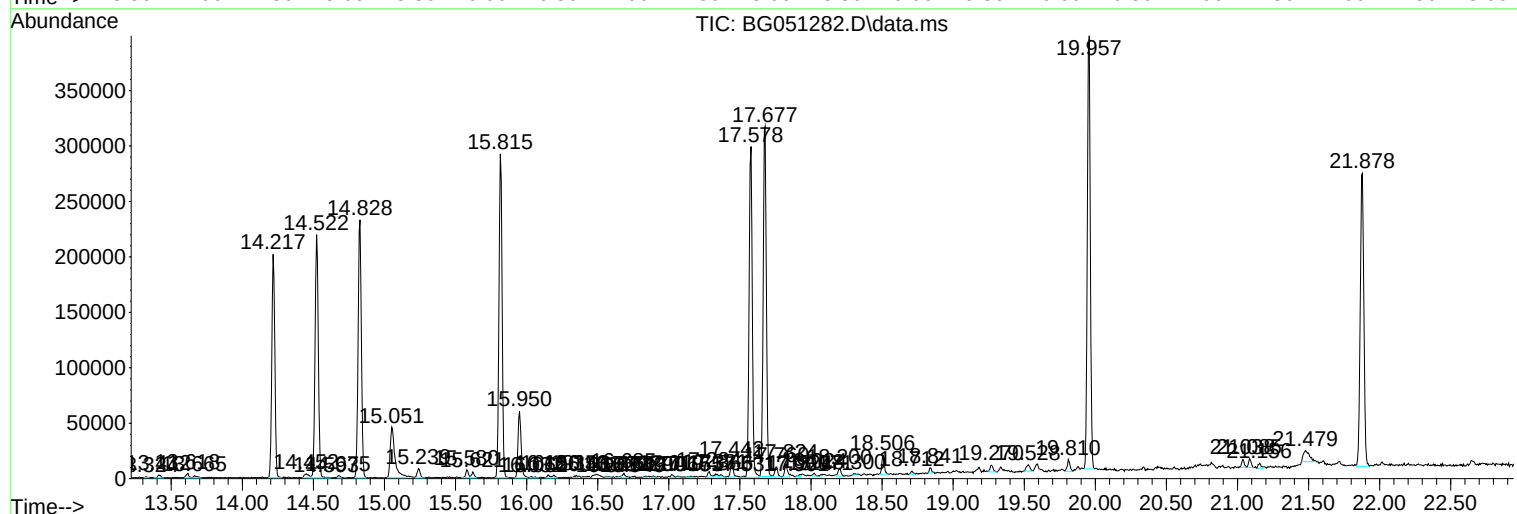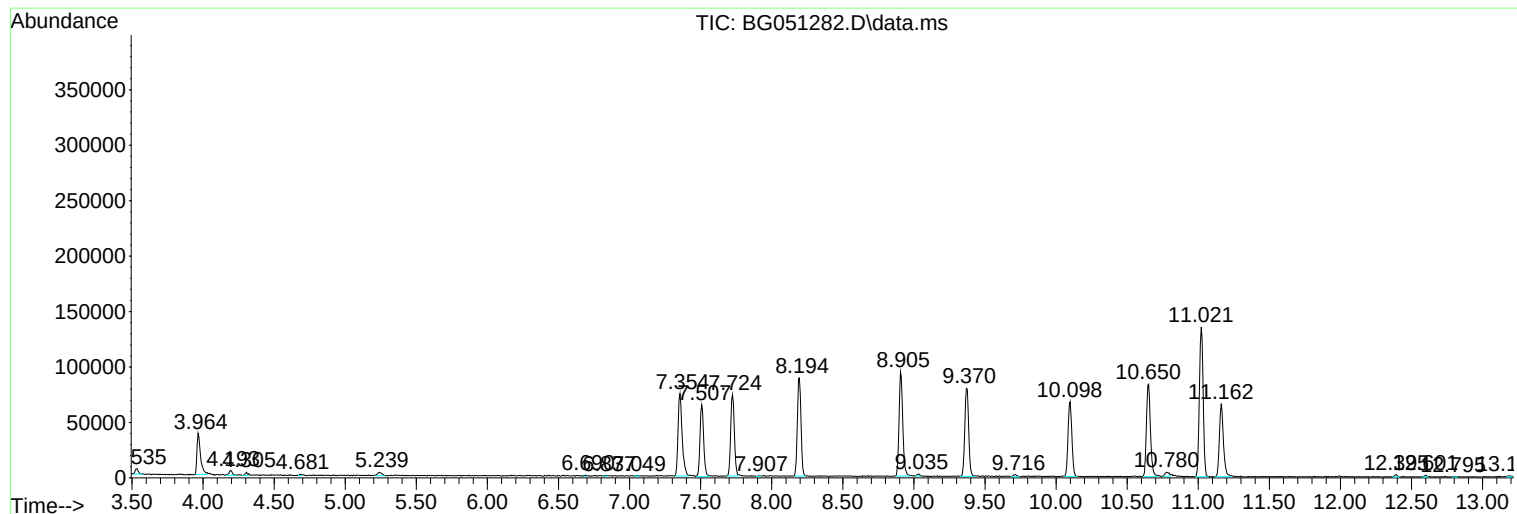

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051282.D
Acq On : 30 Nov 2021 16:20
Operator : CG/JU
Sample : M4839-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113021\
Data File : BG051282.D
Acq On : 30 Nov 2021 16:20
Operator : CG/JU
Sample : M4839-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc