
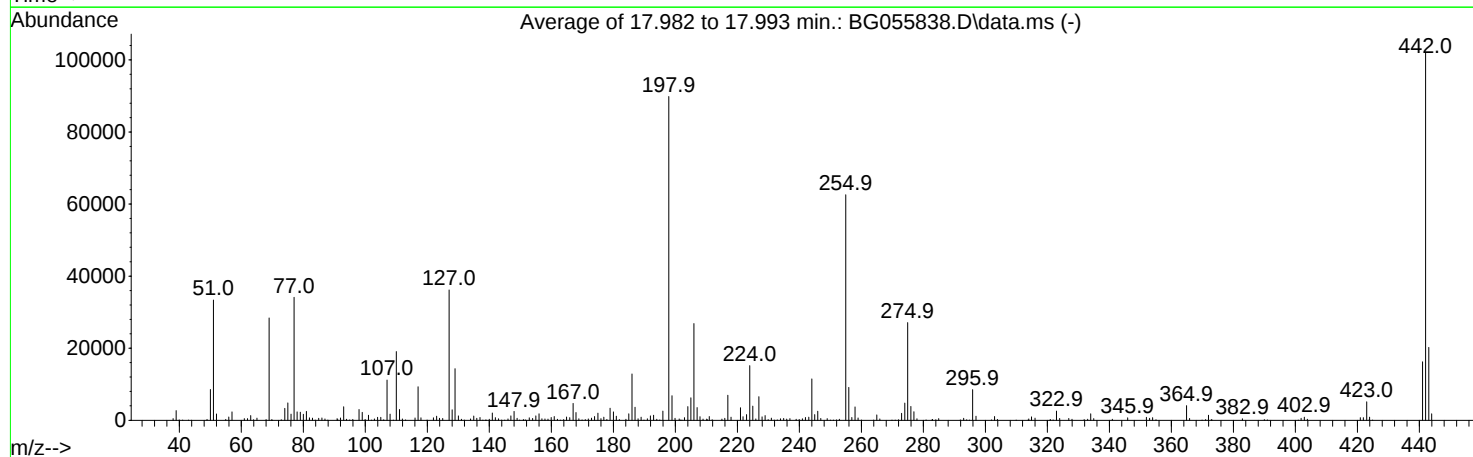


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113022\
 Data File : BG055838.D
 Acq On : 30 Nov 2022 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 02:10:33 2022

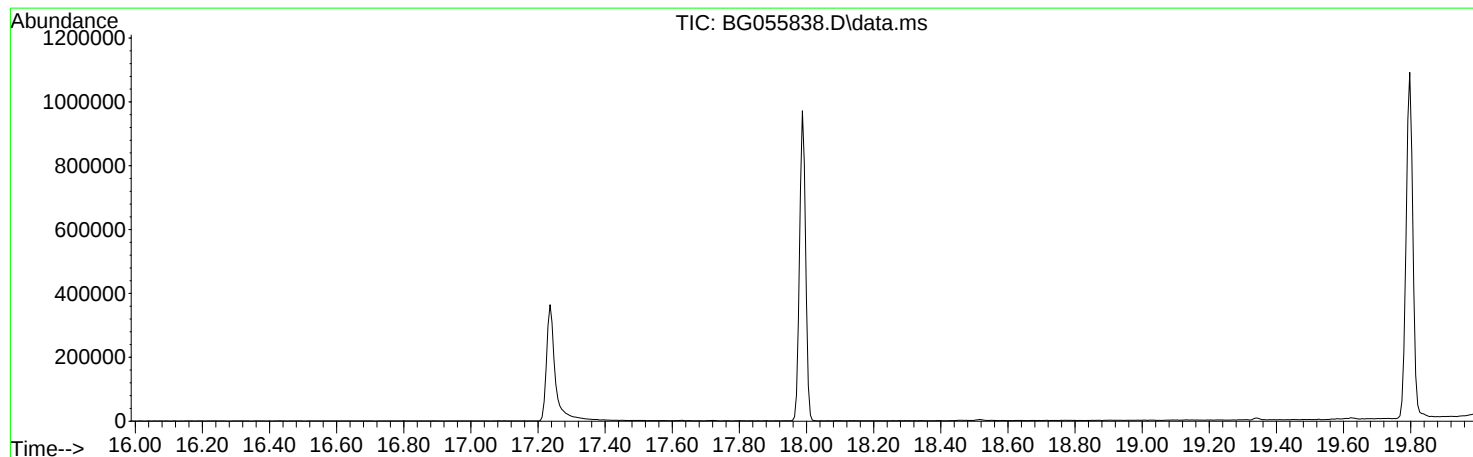




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	33384	PASS
68	69	0.00	2	0.6	180	PASS
69	198	0.00	100	31.6	28413	PASS
70	69	0.00	2	0.5	147	PASS
127	198	10	80	40.3	36179	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89845	PASS
199	198	5	9	7.6	6809	PASS
275	198	10	60	30.2	27107	PASS
365	198	1	100	4.5	4059	PASS
441	198	0.01	100	18.1	16219	PASS
442	442	50	100	100.0	102080	PASS
443	442	15	24	19.8	20204	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG113022\
Data File : BG055838.D
Acq On : 30 Nov 2022 11:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 01 04:25:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 02:10:33 2022
Response via : Initial Calibration

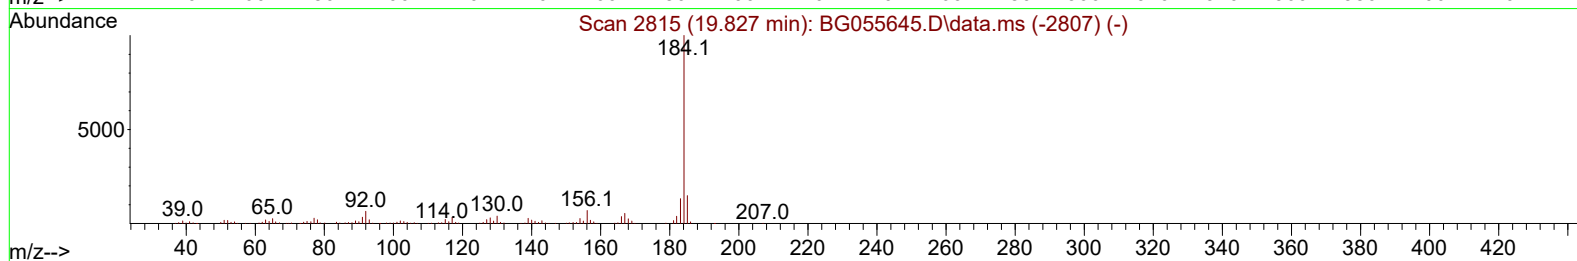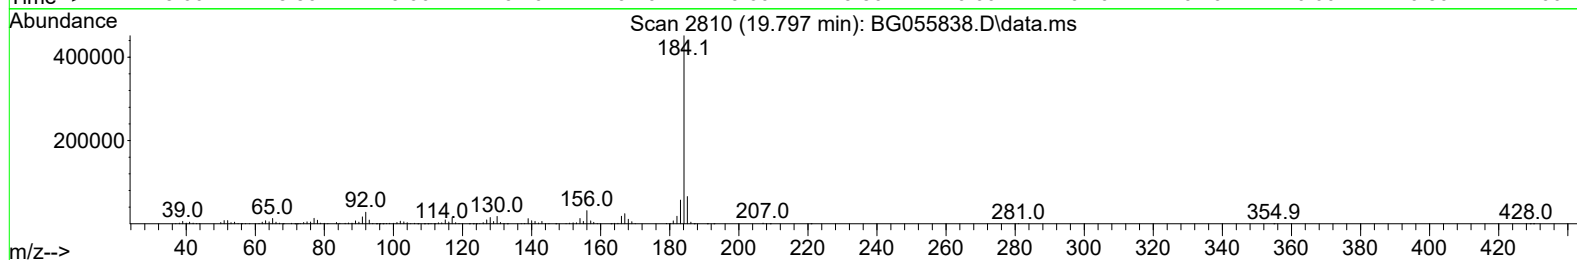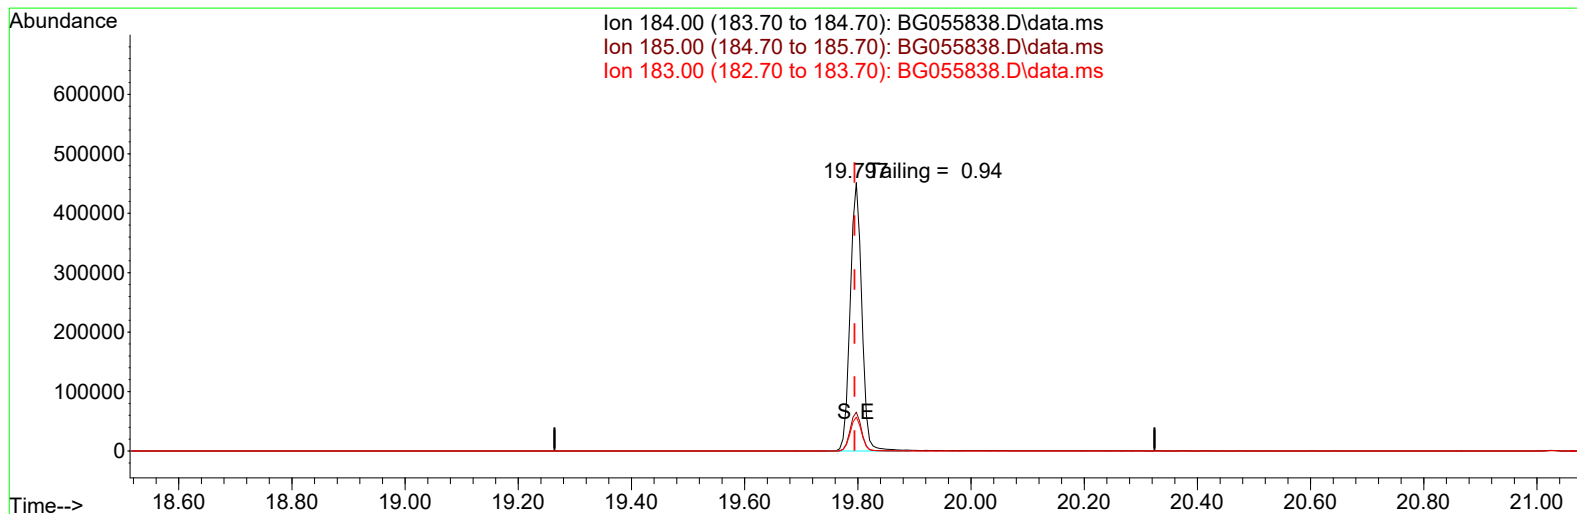

TIC: BG055838.D\data.ms

(77) Benzidine

19.797min (+ 0.003) 0.00 ng

response 642635

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.53
183.00	13.20	12.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2022	BNA_G	BG055838.D
Compound Name	Response	Retention Time
DDT	305505	21.025
DDD	6284	20.632
DDE	325	20.073
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6609	312114	2.12

Instrument :
BNA_G
ClientSampleId :
DFTPP