

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120114\
 Data File : BG015561.D
 Acq On : 1 Dec 2014 14:26
 Operator : TP/JJ
 Sample : F4757-13DL2 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F3W22DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG112514.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.935	37	42	51	rVB4	77322	155562	6.82%	1.597%
2	3.382	115	118	121	rBV4	6645	7834	0.34%	0.080%
3	3.434	125	127	130	rVV3	6103	7331	0.32%	0.075%
4	3.481	134	135	139	rVB4	7949	6860	0.30%	0.070%
5	4.263	265	268	270	rBV3	5615	6960	0.31%	0.071%
6	4.292	270	273	277	rVB2	6742	7852	0.34%	0.081%
7	4.521	310	312	315	rVV4	5694	8066	0.35%	0.083%
8	4.568	318	320	323	rVB2	5866	7028	0.31%	0.072%
9	4.774	353	355	359	rVB3	5459	6953	0.30%	0.071%
10	4.903	376	377	381	rVB4	5848	7192	0.32%	0.074%
11	4.980	387	390	395	rVB5	4463	7279	0.32%	0.075%
12	5.015	395	396	398	rBV2	6509	5292	0.23%	0.054%
13	6.008	562	565	569	rBV3	6958	9670	0.42%	0.099%
14	6.313	612	617	620	rVB2	6359	12463	0.55%	0.128%
15	6.807	699	701	704	rBV2	5923	5994	0.26%	0.062%
16	6.901	716	717	722	rVB2	6654	6058	0.27%	0.062%
17	7.365	795	796	800	rVB2	5768	5651	0.25%	0.058%
18	7.770	858	865	873	rVB	422895	679533	29.79%	6.975%
19	8.047	911	912	915	rVB	6203	5652	0.25%	0.058%
20	8.076	915	917	920	rBV2	4065	5110	0.22%	0.052%
21	8.241	944	945	949	rBV3	5063	6353	0.28%	0.065%
22	8.305	954	956	959	rVV3	9609	7429	0.33%	0.076%
23	8.758	1030	1033	1035	rVB	4198	5032	0.22%	0.052%
24	9.016	1074	1077	1079	rBV	5584	5678	0.25%	0.058%
25	9.339	1129	1132	1134	rBV	6145	7372	0.32%	0.076%
26	9.380	1137	1139	1143	rBV2	7891	9050	0.40%	0.093%
27	9.457	1150	1152	1155	rBV2	5634	5219	0.23%	0.054%
28	9.521	1160	1163	1166	rVB3	5590	6203	0.27%	0.064%
29	9.680	1186	1190	1192	rBV2	5264	5664	0.25%	0.058%
30	10.121	1264	1265	1270	rVB	4489	6136	0.27%	0.063%
31	10.168	1270	1273	1275	rBV2	5559	6820	0.30%	0.070%
32	10.338	1298	1302	1304	rBV2	5703	5207	0.23%	0.053%
33	10.497	1326	1329	1330	rBV2	5192	5040	0.22%	0.052%
34	10.555	1333	1339	1347	rVB	511909	907296	39.78%	9.313%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120114\
 Data File : BG015561.D
 Acq On : 1 Dec 2014 14:26
 Operator : TP/JJ
 Sample : F4757-13DL2 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F3W22DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG112514.M
 Title : SVOA CALIBRATION

35	10.855	1388	1390	1395	rBV3	2973	5362	0.24%	0.055%
36	10.937	1401	1404	1409	rBV3	4701	5721	0.25%	0.059%
37	10.990	1409	1413	1414	rVB2	5733	7182	0.31%	0.074%
38	11.390	1479	1481	1485	rVB2	4243	5854	0.26%	0.060%
39	12.571	1680	1682	1686	rVV2	6815	7307	0.32%	0.075%
40	12.618	1689	1690	1693	rVB2	6584	5193	0.23%	0.053%
41	12.935	1742	1744	1747	rBV2	5292	7378	0.32%	0.076%
42	13.094	1768	1771	1774	rBV3	4416	6124	0.27%	0.063%
43	13.176	1780	1785	1786	rBV2	6313	7573	0.33%	0.078%
44	13.305	1805	1807	1809	rVB	6160	5653	0.25%	0.058%
45	13.329	1809	1811	1814	rBV2	6070	8503	0.37%	0.087%
46	13.405	1821	1824	1826	rVB	4958	5300	0.23%	0.054%
47	13.622	1859	1861	1864	rVB	6576	5900	0.26%	0.061%
48	13.869	1899	1903	1905	rBV2	5500	6781	0.30%	0.070%
49	13.899	1905	1908	1910	rVB2	5860	6279	0.28%	0.064%
50	14.134	1947	1948	1952	rVB3	8319	8706	0.38%	0.089%
51	14.169	1952	1954	1955	rBV	7755	6308	0.28%	0.065%
52	14.404	1987	1994	2000	rBV	839267	1243347	54.51%	12.762%
53	14.486	2005	2008	2010	rVV3	5552	6437	0.28%	0.066%
54	14.533	2014	2016	2019	rVV	6045	6323	0.28%	0.065%
55	14.574	2019	2023	2025	rVV	6194	9831	0.43%	0.101%
56	14.604	2025	2028	2029	rVB2	8155	5714	0.25%	0.059%
57	14.786	2057	2059	2064	rBV	3391	6158	0.27%	0.063%
58	14.933	2081	2084	2086	rBV	4208	4891	0.21%	0.050%
59	15.191	2127	2128	2134	rBV2	5586	8221	0.36%	0.084%
60	15.397	2161	2163	2165	rVV2	9052	6433	0.28%	0.066%
61	15.503	2177	2181	2184	rVB3	5727	6729	0.30%	0.069%
62	15.526	2184	2185	2191	rBV3	4374	7046	0.31%	0.072%
63	15.632	2201	2203	2205	rBV2	6249	6216	0.27%	0.064%
64	15.755	2222	2224	2229	rVB3	5372	5863	0.26%	0.060%
65	15.820	2232	2235	2236	rBV2	4671	5177	0.23%	0.053%
66	16.043	2271	2273	2276	rBV2	5409	6318	0.28%	0.065%
67	16.319	2319	2320	2323	rBV2	5999	7444	0.33%	0.076%
68	16.360	2326	2327	2329	rVB	9393	4943	0.22%	0.051%
69	16.519	2352	2354	2358	rVB2	5950	7371	0.32%	0.076%
70	16.889	2415	2417	2420	rVB2	6353	6195	0.27%	0.064%
71	16.930	2420	2424	2430	rBV6	14294	24051	1.05%	0.247%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120114\
 Data File : BG015561.D
 Acq On : 1 Dec 2014 14:26
 Operator : TP/JJ
 Sample : F4757-13DL2 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F3W22DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG112514.M
 Title : SVOA CALIBRATION

72	16.971	2430	2431	2436	rBV4	4049	5612	0.25%	0.058%
73	17.083	2449	2450	2454	rBV3	5930	5486	0.24%	0.056%
74	17.148	2454	2461	2468	rVV2	1247018	1760982	77.20%	18.075%
75	17.295	2482	2486	2487	rBV2	4788	5173	0.23%	0.053%
76	17.453	2510	2513	2514	rVB2	7021	5190	0.23%	0.053%
77	17.565	2531	2532	2535	rBV2	7820	6991	0.31%	0.072%
78	17.706	2552	2556	2557	rBV2	5632	5853	0.26%	0.060%
79	17.800	2570	2572	2575	rVV2	5605	5181	0.23%	0.053%
80	17.917	2587	2592	2595	rBV4	5495	9421	0.41%	0.097%
81	18.141	2629	2630	2633	rBV3	7109	5200	0.23%	0.053%
82	18.170	2633	2635	2638	rVB2	5983	6437	0.28%	0.066%
83	18.205	2638	2641	2644	rBV3	3902	6106	0.27%	0.063%
84	18.323	2660	2661	2664	rVB3	5760	4956	0.22%	0.051%
85	18.358	2666	2667	2671	rVB4	5562	4890	0.21%	0.050%
86	18.481	2684	2688	2689	rBV3	6869	9361	0.41%	0.096%
87	18.693	2721	2724	2728	rBV3	4140	6583	0.29%	0.068%
88	18.793	2739	2741	2745	rVB4	5814	7745	0.34%	0.079%
89	18.822	2745	2746	2750	rBV3	4802	6266	0.27%	0.064%
90	19.251	2817	2819	2823	rVB3	6643	6528	0.29%	0.067%
91	19.621	2880	2882	2886	rVB4	7791	8267	0.36%	0.085%
92	19.709	2896	2897	2901	rVB2	6131	5722	0.25%	0.059%
93	19.745	2901	2903	2906	rBV3	6719	8345	0.37%	0.086%
94	19.850	2919	2921	2924	rBV	5790	6791	0.30%	0.070%
95	19.933	2932	2935	2937	rBV4	4915	6135	0.27%	0.063%
96	20.256	2987	2990	2992	rBV2	6323	6937	0.30%	0.071%
97	20.538	3036	3038	3041	rBV3	9331	10651	0.47%	0.109%
98	21.120	3135	3137	3143	rBV7	17842	26549	1.16%	0.273%
99	21.325	3167	3172	3177	rBV	1848054	2280994	100.00%	23.413%
100	23.611	3554	3561	3571	rBV	1054412	2059481	90.29%	21.139%


Sum of corrected areas: 9742504

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120114\
Data File : BG015561.D
Acq On : 1 Dec 2014 14:26
Operator : TP/JJ
Sample : F4757-13DL2 100X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F3W22DL2

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG112514.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

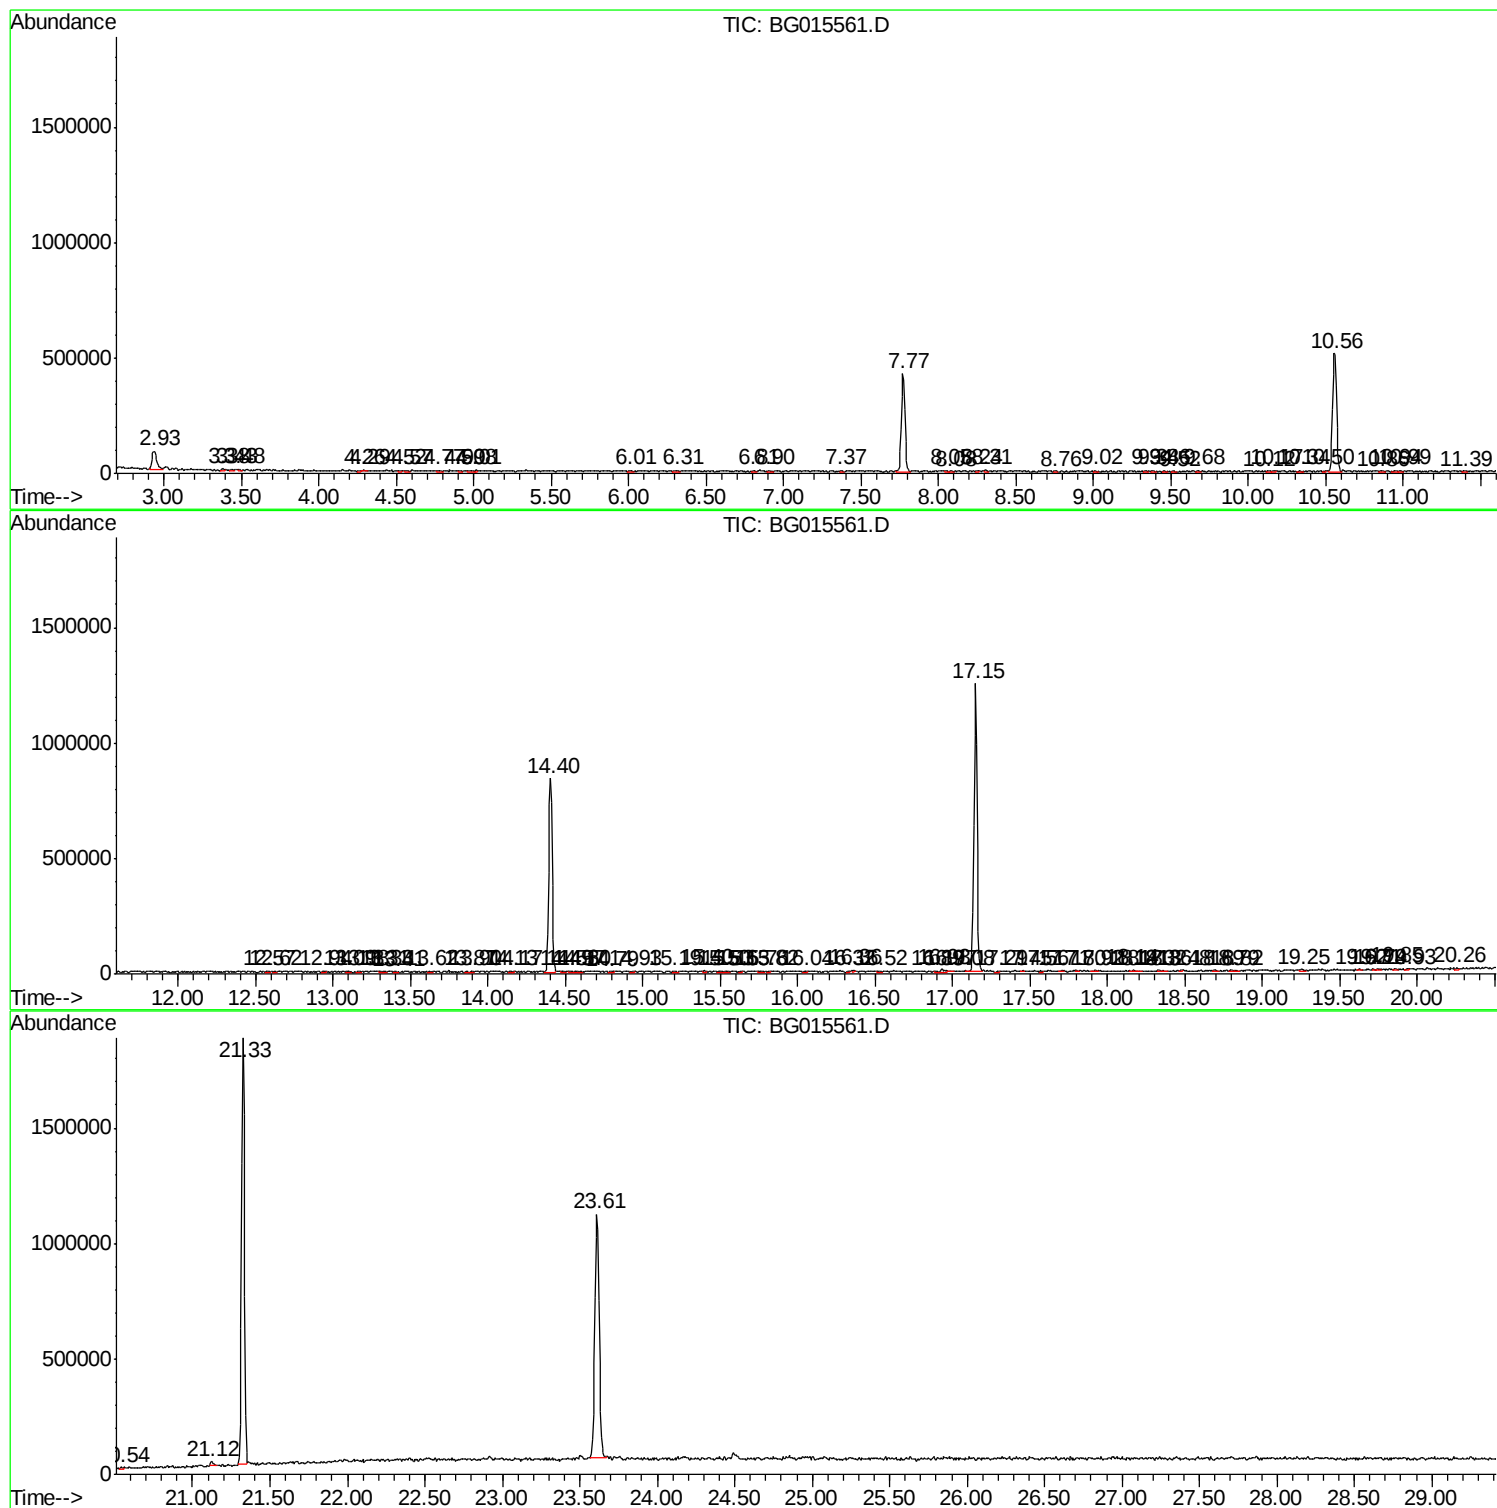

DbaaaPathh::ZZ\NRPBHHM1BBAAGCDBAAABBG20014\
 DbaaaFile::BB0055661DD
 Aeqq00n :: 11Dec2004 144206
 Opeaaor ::TPPJ
 Sample ::F#757130D22100X
 Misc ::
 AASSVal ::88 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampled :
 F3W22DL2

QqaabMebdd::ZZ\NRPBHHM1BBAAGCMEEH00SS0000122EPABBG12514MM
 QqaabTitle ::S00ACALIBRATION

TICLibrary ::CC\DATA\BASSEN05002LL
 TICIntegratíonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
