

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
 Data File : BG031332.D
 Acq On : 2 Dec 2017 00:01
 Operator : SJ/JU
 Sample : I6653-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.685	402	408	427	rBV	499510	889153	13.49%	3.477%
2	7.295	675	682	702	rVB	319790	600652	9.11%	2.349%
3	7.659	737	744	756	rBV	942563	1710924	25.95%	6.691%
4	8.129	817	824	834	rBV	216483	385710	5.85%	1.508%
5	8.453	870	879	893	rBV	901136	1629393	24.71%	6.372%
6	9.299	1015	1023	1035	rBV	651574	1286247	19.51%	5.030%
7	10.944	1295	1303	1322	rBV	276880	581424	8.82%	2.274%
8	13.370	1709	1716	1737	rBV	2196239	3692401	56.00%	14.441%
9	14.751	1942	1951	1970	rVB2	542790	903612	13.70%	3.534%
10	16.238	2197	2204	2223	rBV	1875390	3019046	45.79%	11.807%
11	17.489	2410	2417	2433	rBV2	783229	1274916	19.34%	4.986%
12	20.080	2852	2858	2869	rBV	4690336	6593577	100.00%	25.787%
13	21.760	3137	3144	3159	rVB	864075	1542335	23.39%	6.032%
14	25.057	3694	3705	3725	rVB2	494683	1460180	22.15%	5.711%


Sum of corrected areas: 25569570

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
Data File : BG031332.D
Acq On : 2 Dec 2017 00:01
Operator : SJ/JU
Sample : I6653-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-7

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

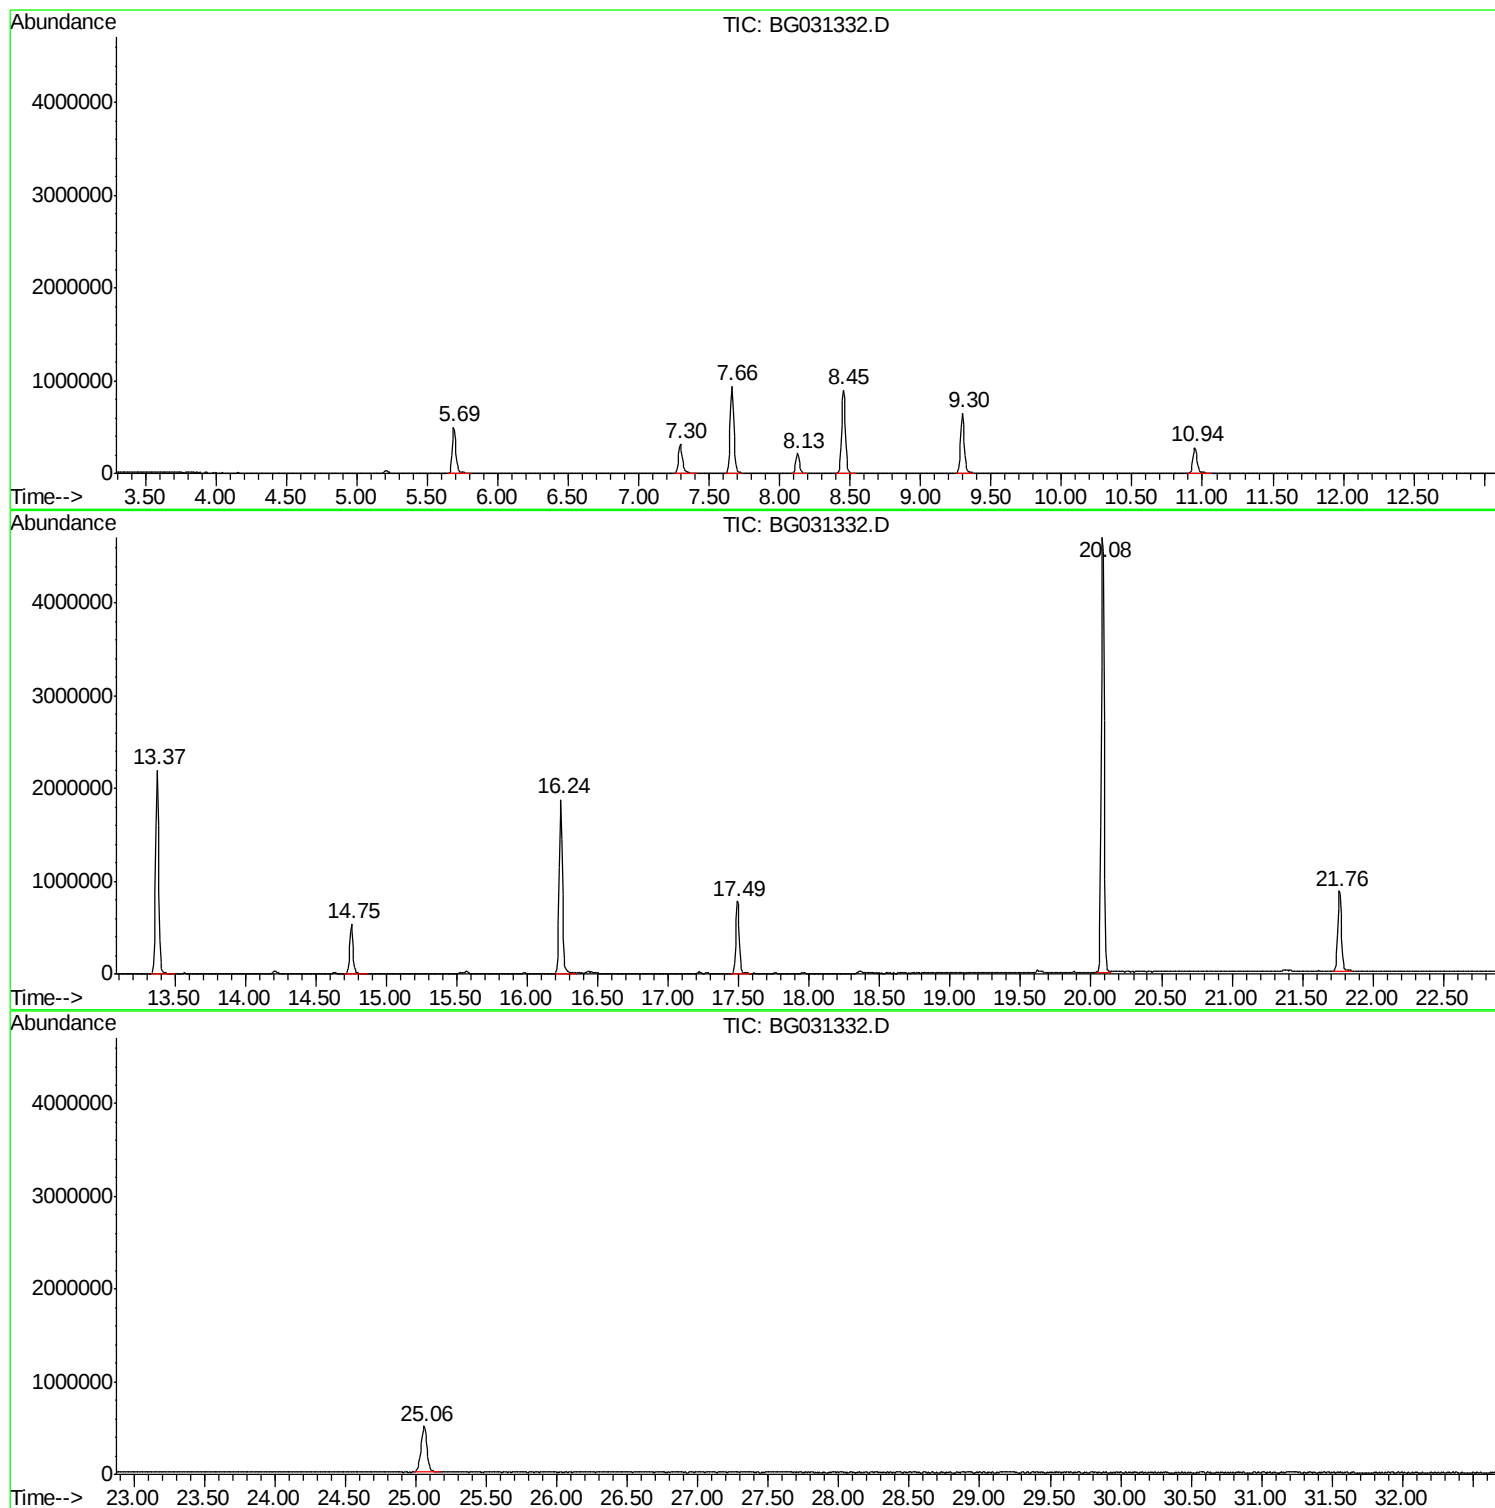

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
Data File : BG031332.D
Acq On : 2 Dec 2017 00:01
Operator : SJ/JU
Sample : I6653-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-7









Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.66	88.72 ng	1710920	1,4-Dichlorobenzene-d4	8.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

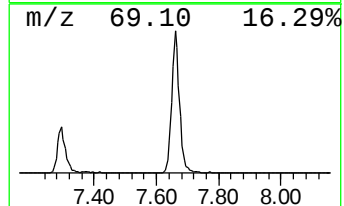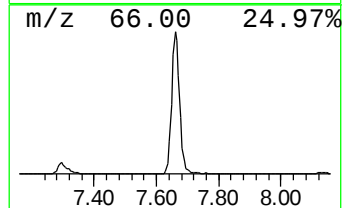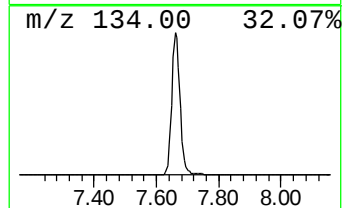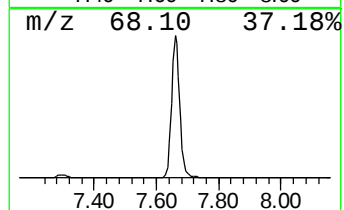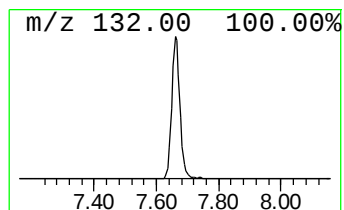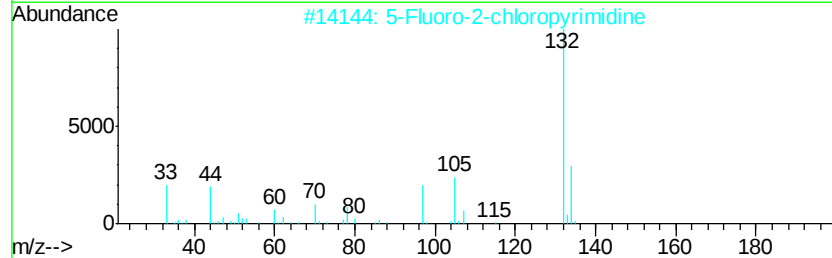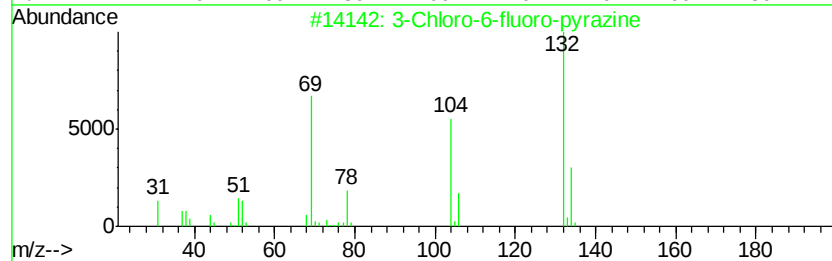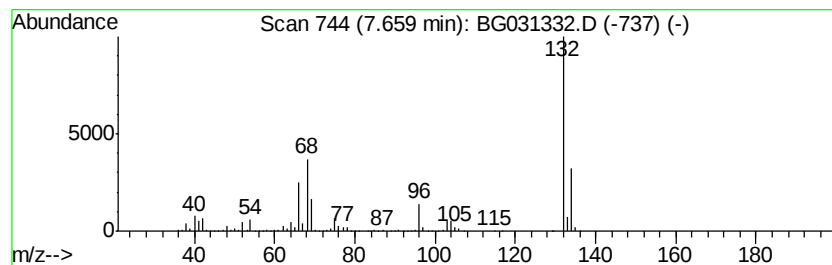

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120117\
Data File : BG031332.D
Acq On : 2 Dec 2017 00:01
Operator : SJ/JU
Sample : I6653-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.66	7.66	88.7	ng	1710920	1	8.13	385710	20.0