

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
 Data File : BG031346.D
 Acq On : 2 Dec 2017 9:29
 Operator : SJ/JU
 Sample : I6653-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.692	402	409	422	rBV	428882	769591	12.76%	3.207%
2	7.296	675	682	695	rBV	257210	513497	8.51%	2.140%
3	7.660	737	744	756	rBV	860114	1568040	26.00%	6.535%
4	8.130	817	824	832	rBV	214154	377099	6.25%	1.572%
5	8.453	870	879	892	rBV	864763	1599788	26.52%	6.667%
6	9.299	1014	1023	1037	rBV	638302	1263885	20.95%	5.267%
7	10.944	1295	1303	1322	rBV	268229	571310	9.47%	2.381%
8	13.371	1709	1716	1728	rBV	2134967	3512630	58.24%	14.639%
9	14.752	1944	1951	1962	rBV2	478746	860604	14.27%	3.587%
10	16.238	2197	2204	2223	rBV	1685740	2699325	44.75%	11.249%
11	17.490	2409	2417	2430	rBV2	712949	1189913	19.73%	4.959%
12	18.359	2559	2565	2571	rBV3	39479	73470	1.22%	0.306%
13	19.616	2775	2779	2785	rBV7	43567	74977	1.24%	0.312%
14	20.081	2852	2858	2867	rBV	4522921	6031745	100.00%	25.137%
15	21.373	3074	3078	3085	rBV3	52171	98946	1.64%	0.412%
16	21.761	3137	3144	3155	rBV2	846452	1425898	23.64%	5.942%
17	25.057	3694	3705	3719	rVB2	460569	1364725	22.63%	5.687%


Sum of corrected areas: 23995443

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
Data File : BG031346.D
Acq On : 2 Dec 2017 9:29
Operator : SJ/JU
Sample : I6653-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

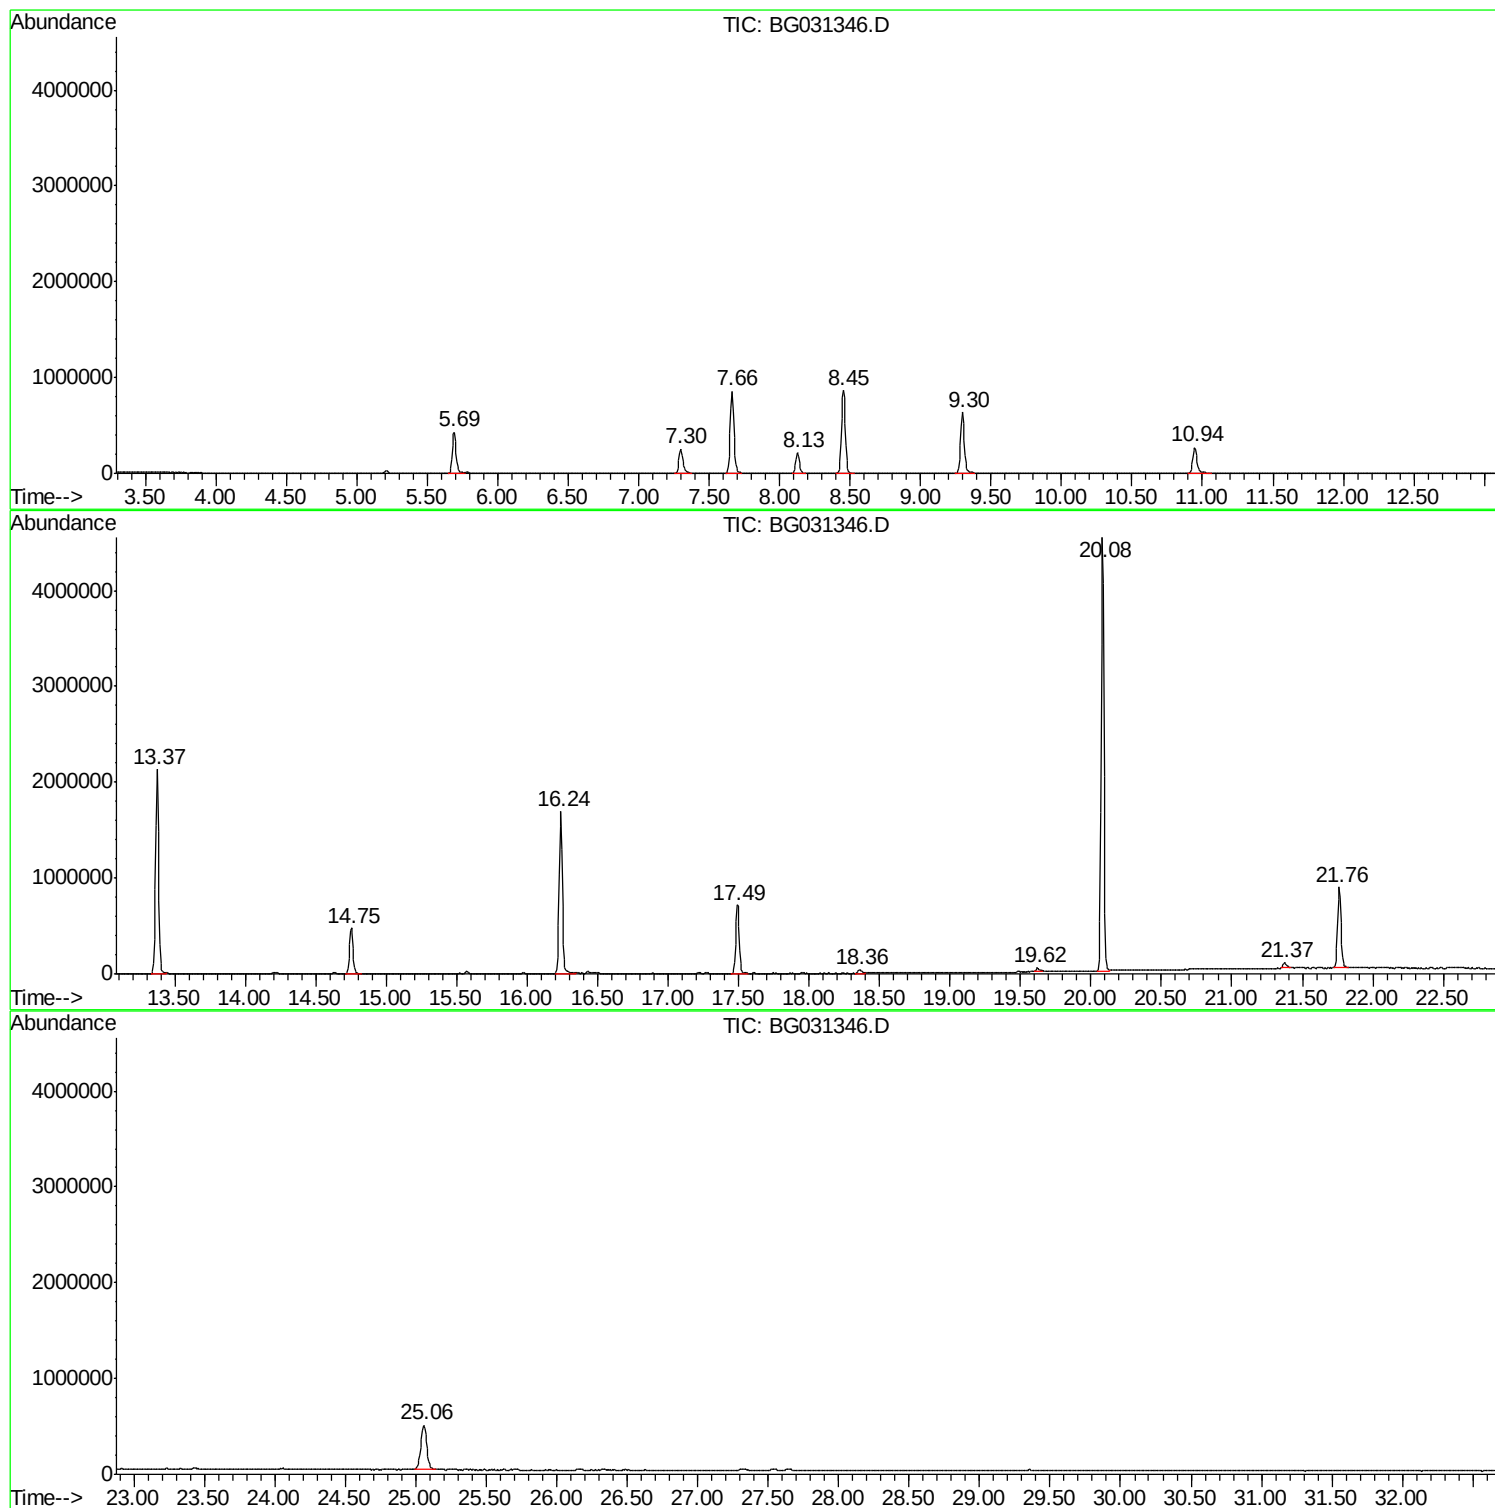

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120117\
Data File : BG031346.D
Acq On : 2 Dec 2017 9:29
Operator : SJ/JU
Sample : I6653-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-6










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.66 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.66	83.16 ng	1568040	1,4-Dichlorobenzene-d4	8.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

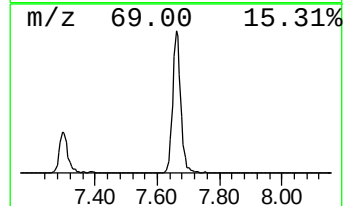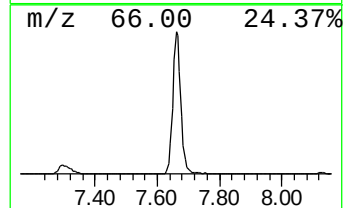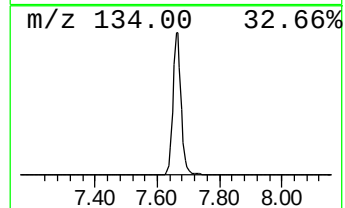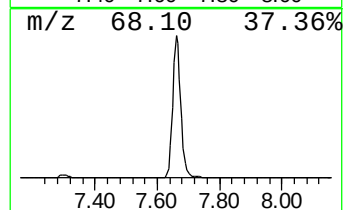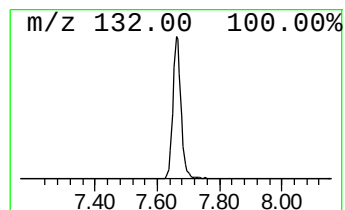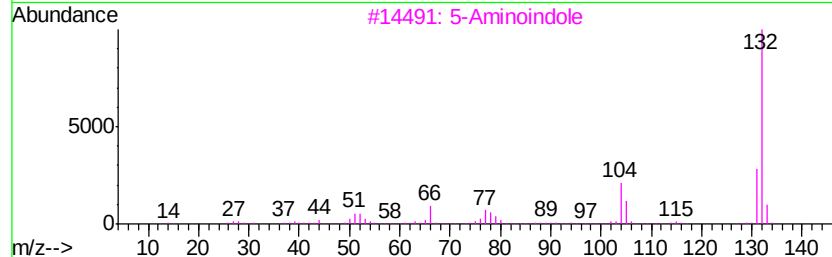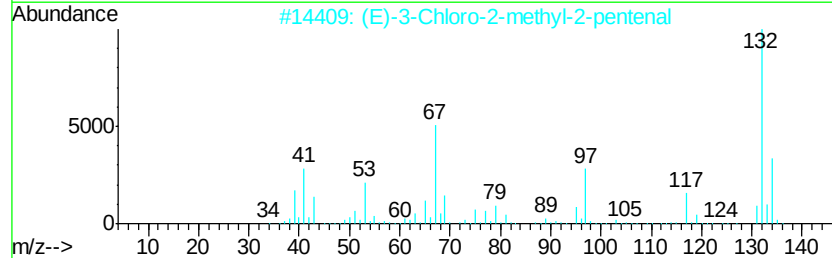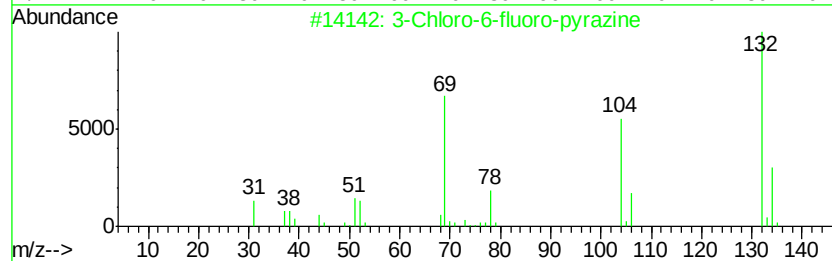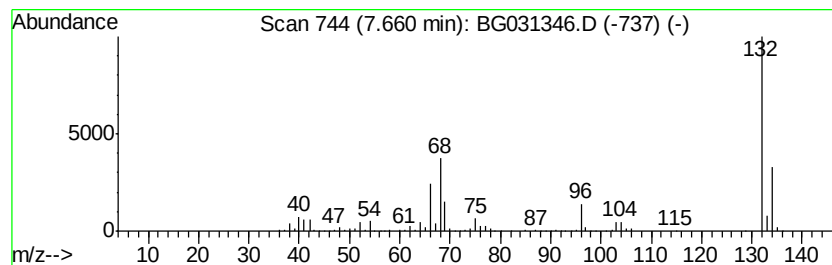

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120117\
Data File : BG031346.D
Acq On : 2 Dec 2017 9:29
Operator : SJ/JU
Sample : I6653-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-6

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.66	7.66	83.2	ng	1568040	1	8.13	377099	20.0