


Data Path : Z:\HPCHEM1\BNA G\Data\BG120117\
 Data File : BG031334.D
 Acq On : 2 Dec 2017 1:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

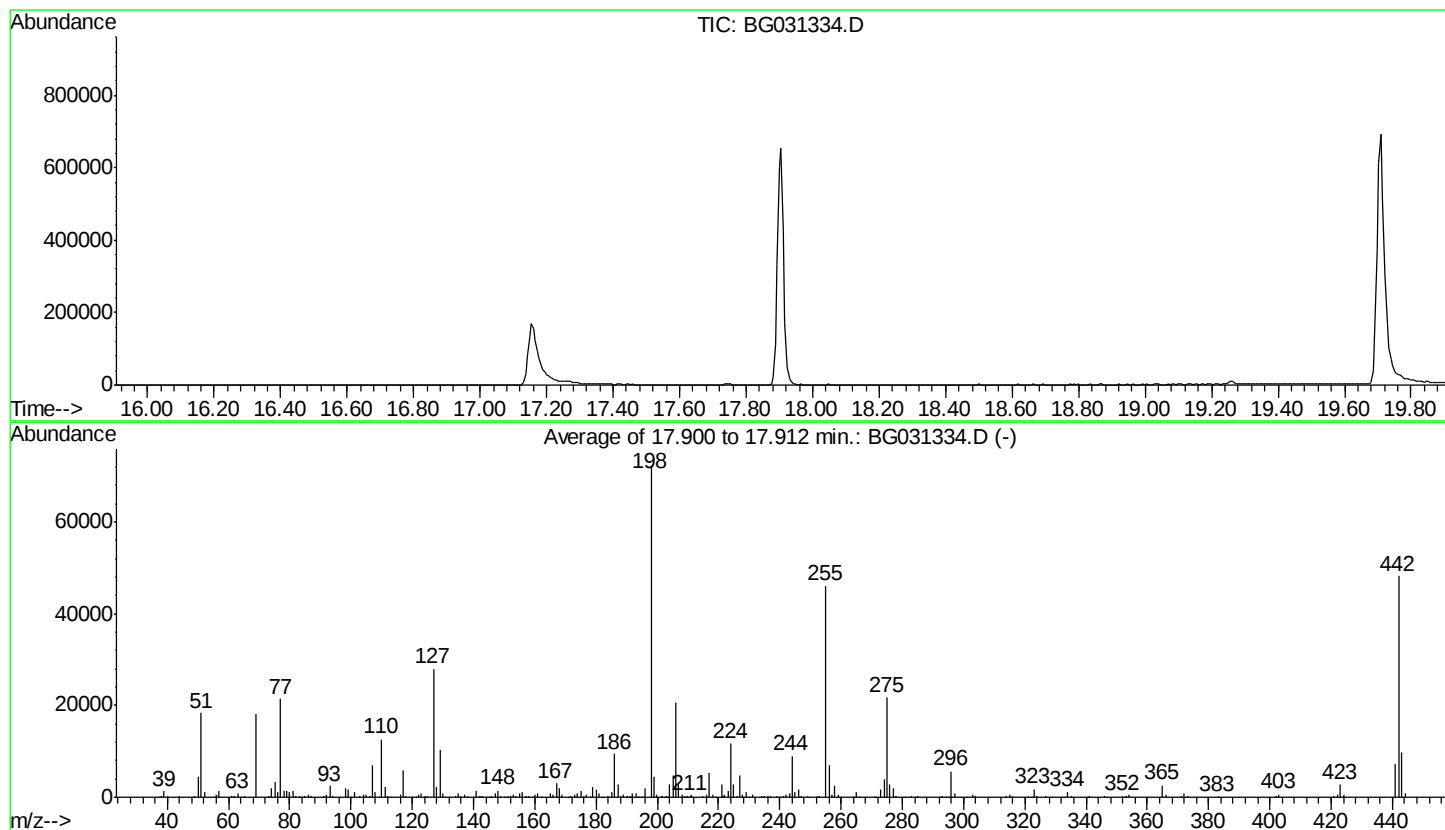

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	18401	PASS
68	69	0.00	2	0.4	79	PASS
69	198	0.00	100	25.2	18202	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.7	27968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72245	PASS
199	198	5	9	6.3	4528	PASS
275	198	10	60	30.0	21696	PASS
365	198	1	100	3.6	2613	PASS
441	442	0.01	24	15.3	7383	PASS
442	198	50	100	66.6	48122	PASS
443	442	15	24	20.0	9644	PASS