
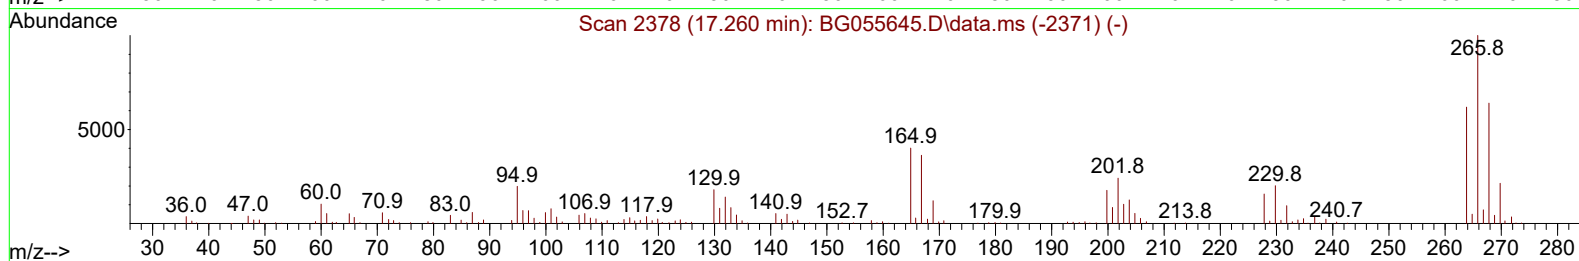
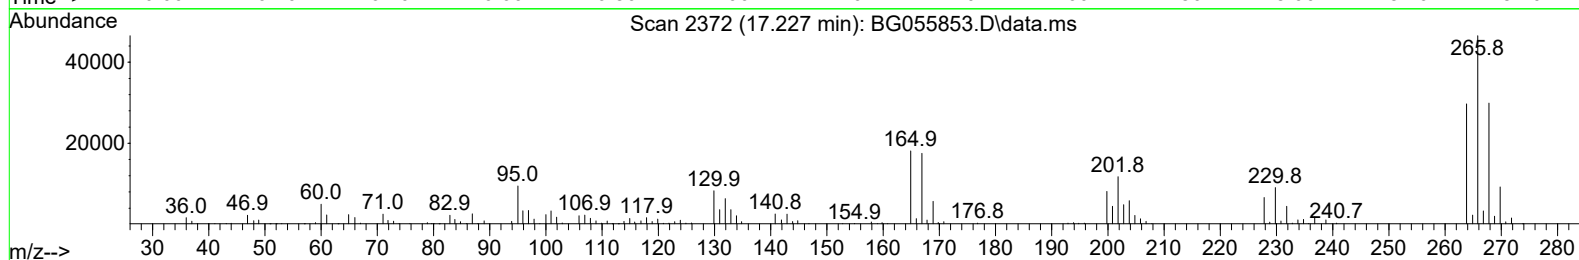


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120122\
Data File : BG055853.D
Acq On : 1 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 05:50:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

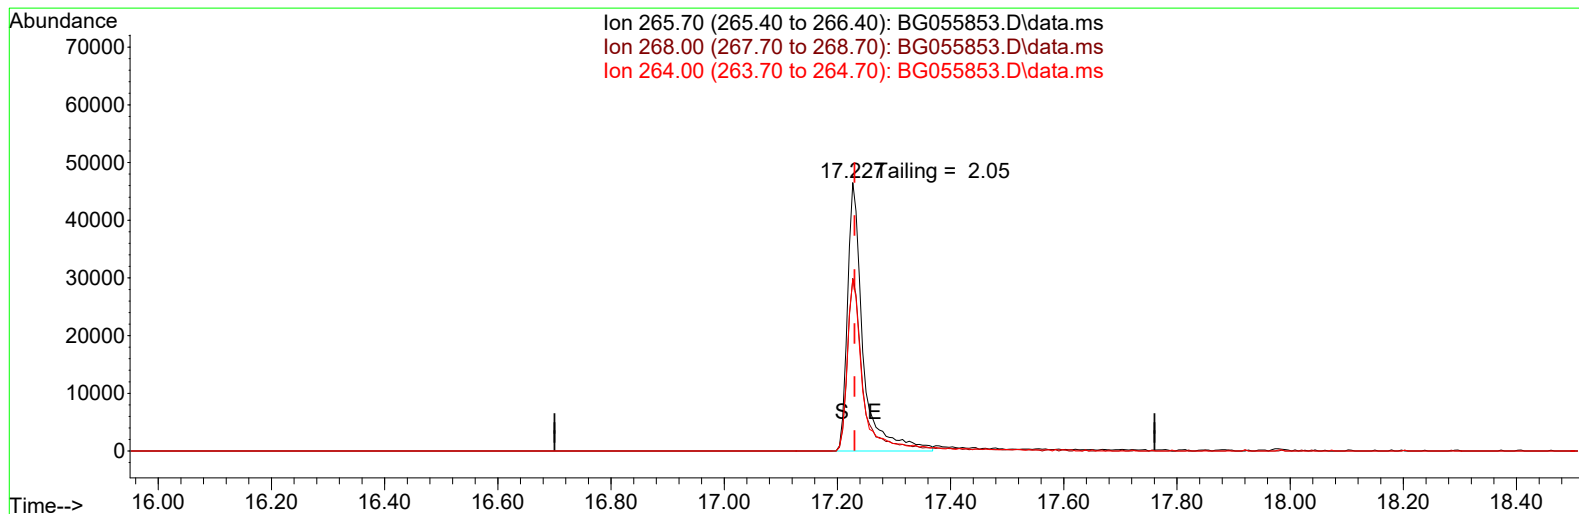

TIC: BG055853.D\data.ms

(70) Pentachlorophenol (C)




17.227min (-0.003) 18899.25 ng

response 89391

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.30
264.00	61.90	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120122\
Data File : BG055853.D
Acq On : 1 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 05:50:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

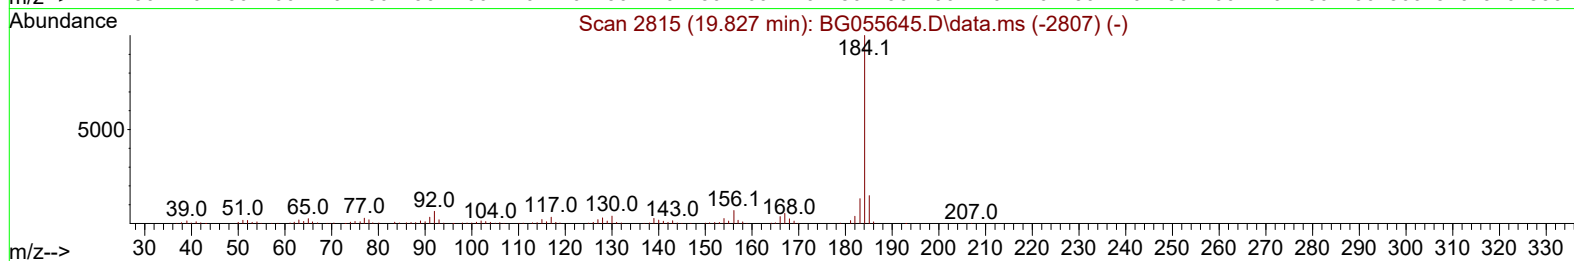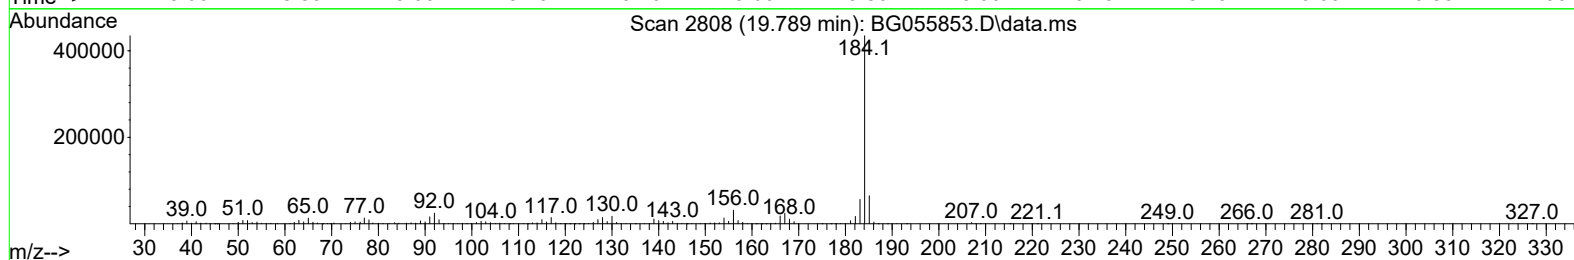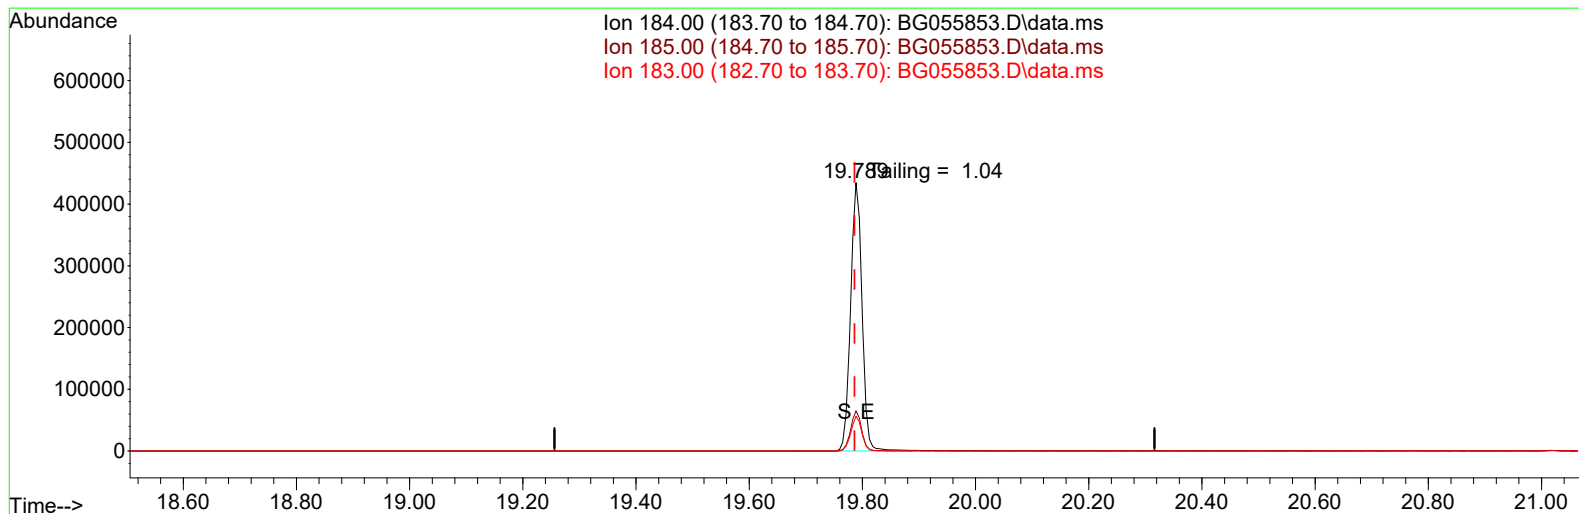

TIC: BG055853.D\data.ms

(77) Benzidine**19.789min (+ 0.003) 498913.87 ng****response 611732**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.97
183.00	13.20	12.98
0.00	0.00	0.00