


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120122\
 Data File : BG055853.D
 Acq On : 1 Dec 2022 11:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 02 04:07:17 2022

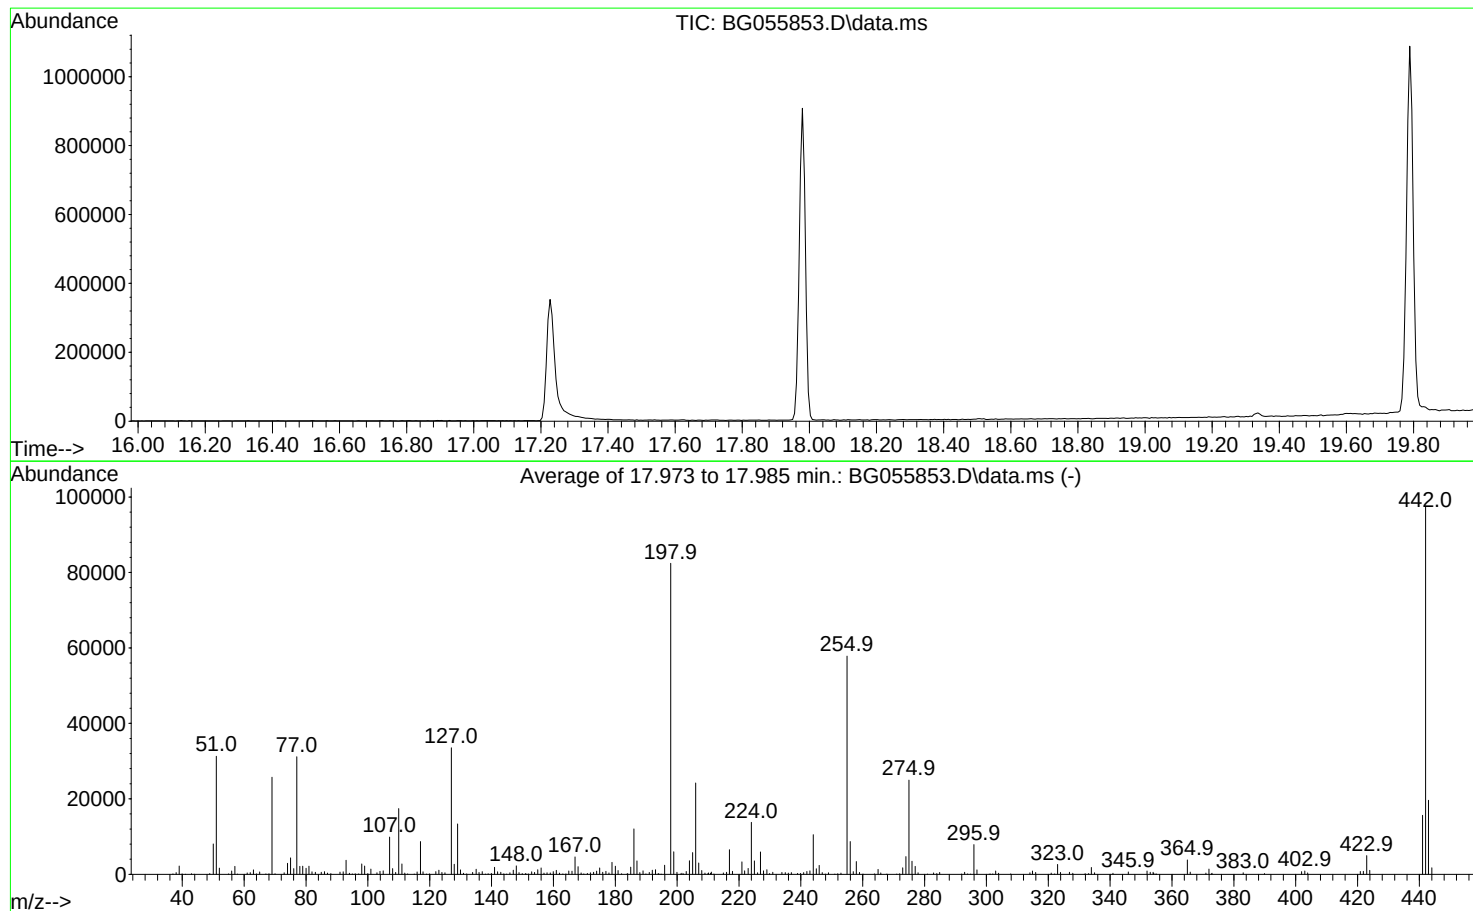




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	31293	PASS
68	69	0.00	2	0.6	165	PASS
69	198	0.00	100	31.2	25744	PASS
70	69	0.00	2	0.5	139	PASS
127	198	10	80	40.7	33547	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82432	PASS
199	198	5	9	7.2	5943	PASS
275	198	10	60	30.3	24957	PASS
365	198	1	100	4.6	3799	PASS
441	198	0.01	100	19.0	15654	PASS
442	442	50	100	100.0	97515	PASS
443	442	15	24	20.1	19600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120122\
Data File : BG055853.D
Acq On : 1 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 02 05:50:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

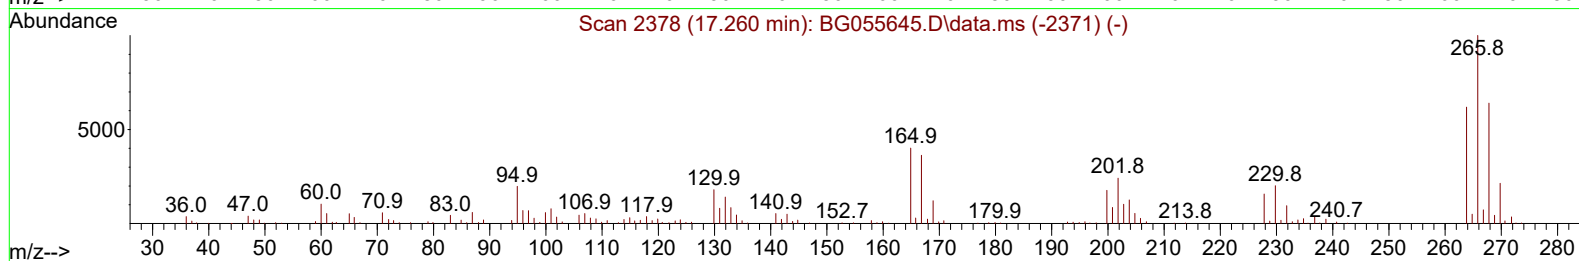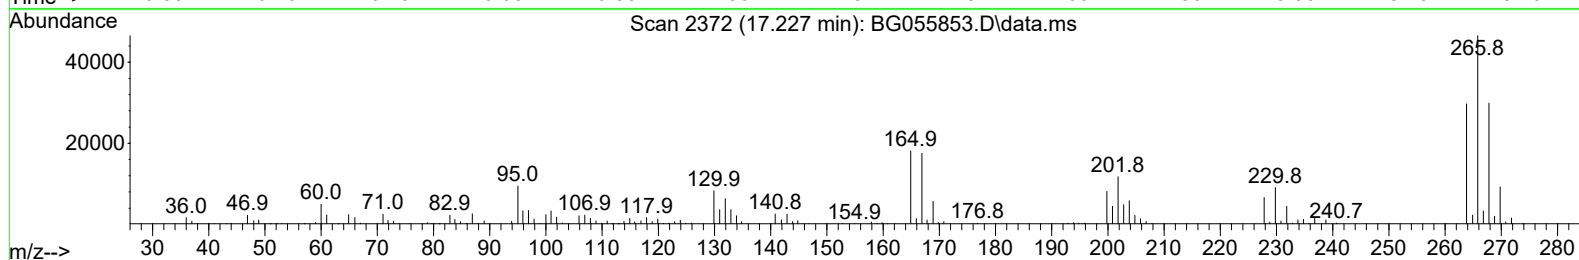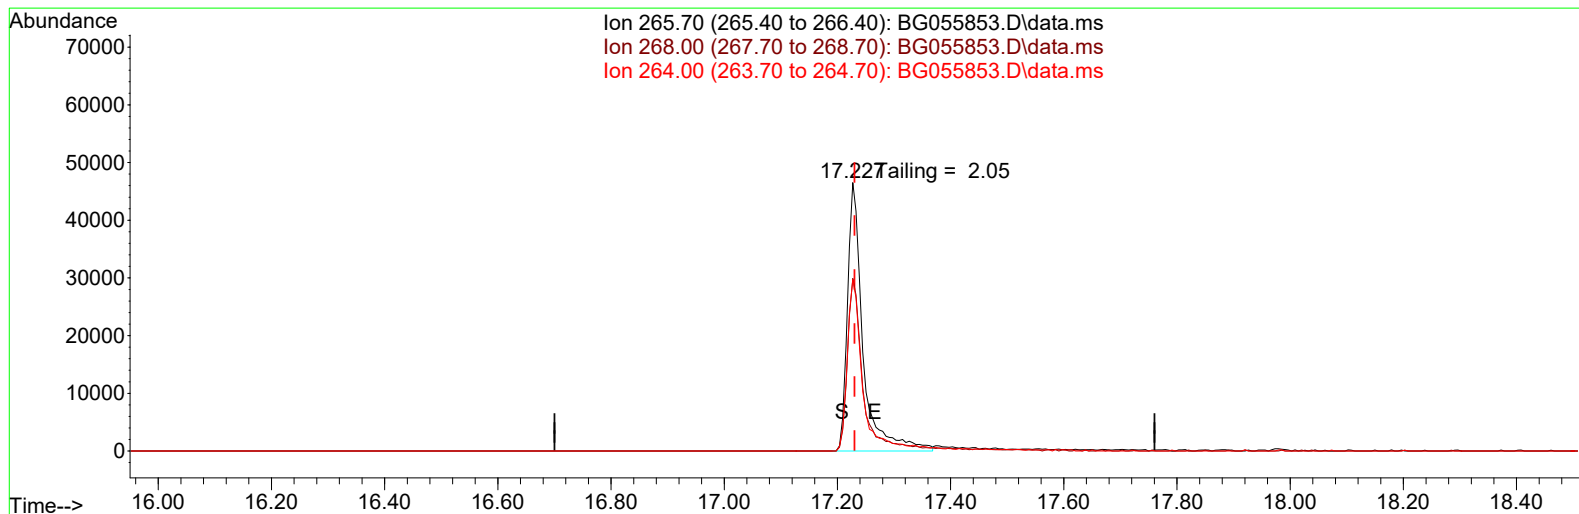

TIC: BG055853.D\data.ms

(70) Pentachlorophenol (C)

17.227min (-0.003) 18899.25 ng




response 89391

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.30
264.00	61.90	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120122\
Data File : BG055853.D
Acq On : 1 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 02 05:50:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

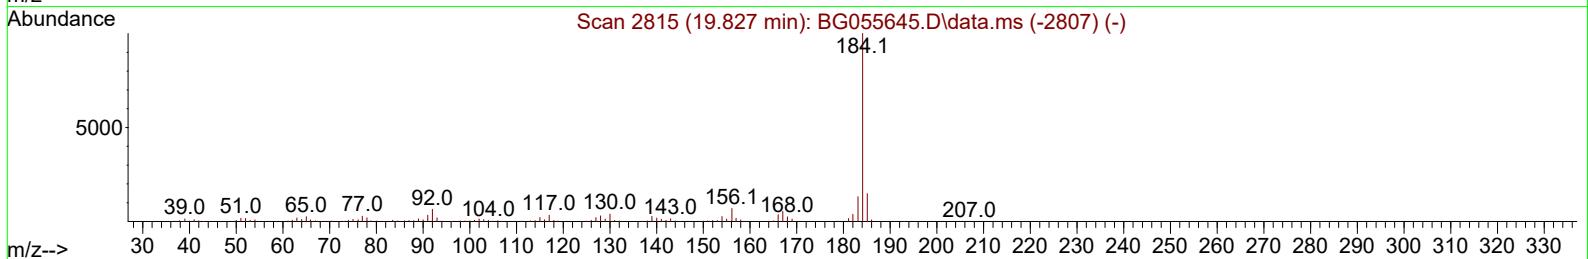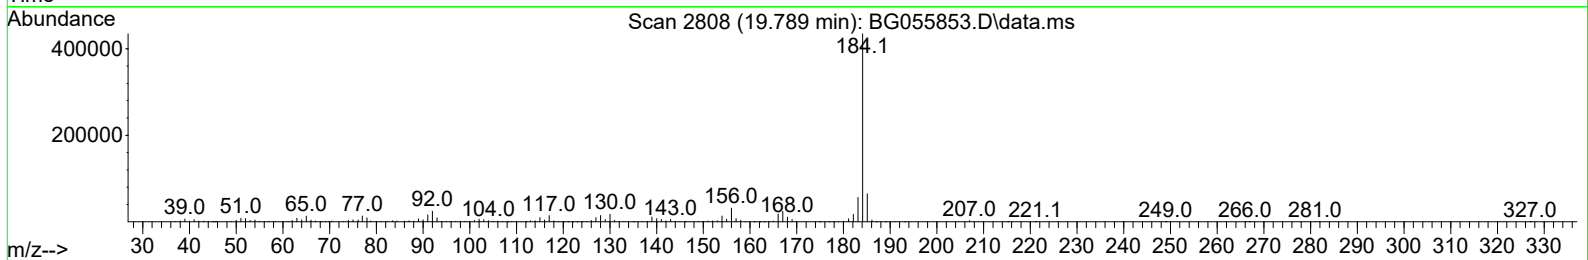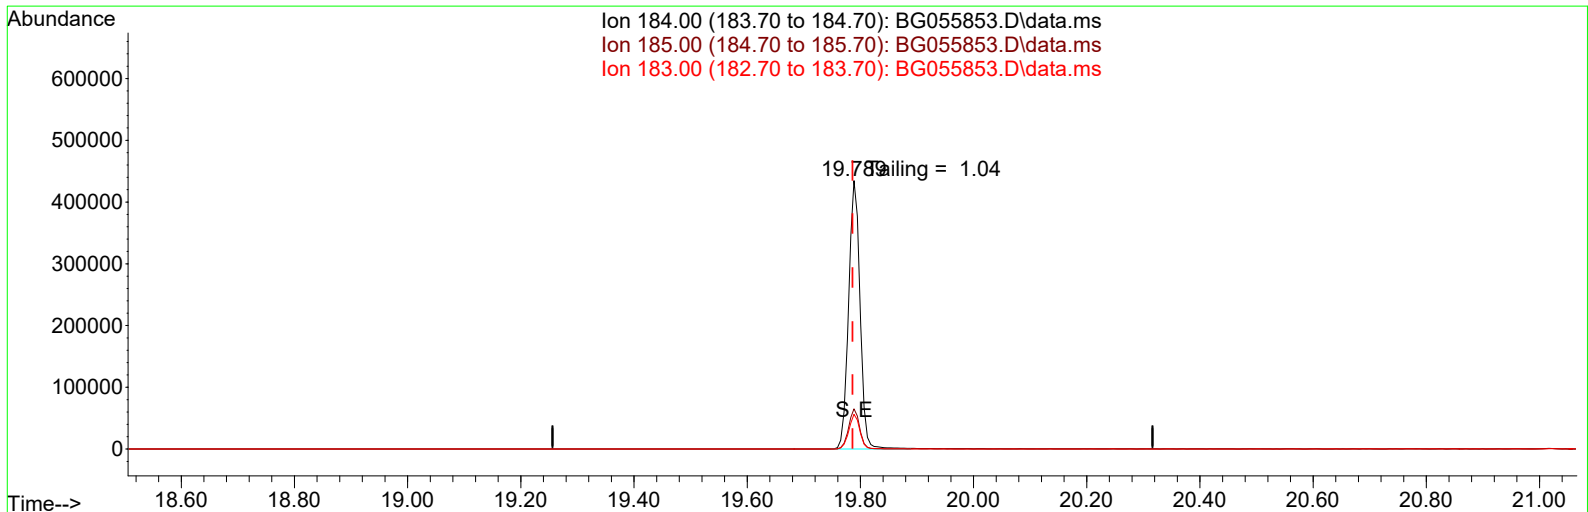

TIC: BG055853.D\data.ms

(77) Benzidine

19.789min (+ 0.003) 498913.87 ng

response 611732

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.97
183.00	13.20	12.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2022	BNA_G	<u>BG055853.D</u>
Compound Name	Response	Retention Time
DDT	281344	21.017
DDD	7552	20.57
DDE	666	20.071
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8218	289562	2.84

Instrument :
BNA_G
ClientSampleId :
DFTPP