
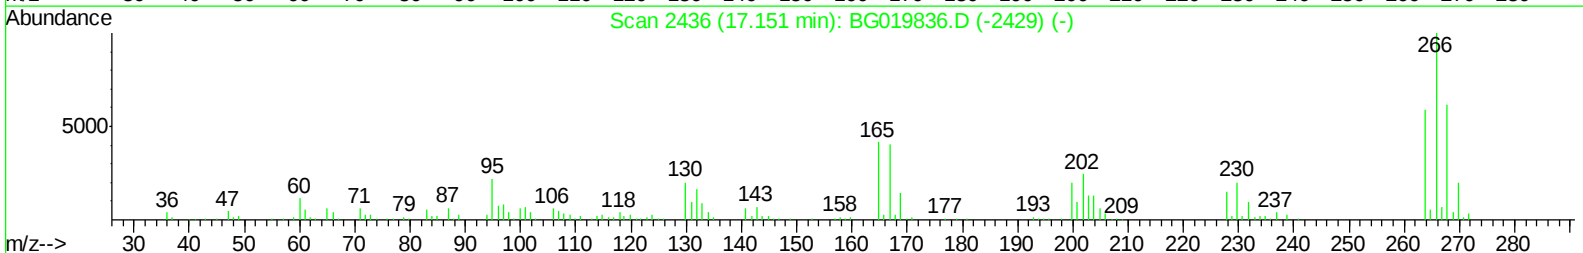
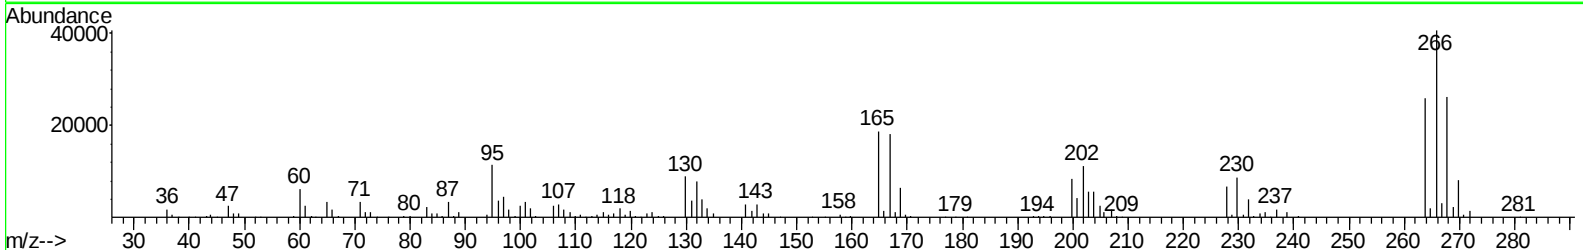


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120215\
Data File : BG019841.D
Acq On : 2 Dec 2015 19:20
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 08:13:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

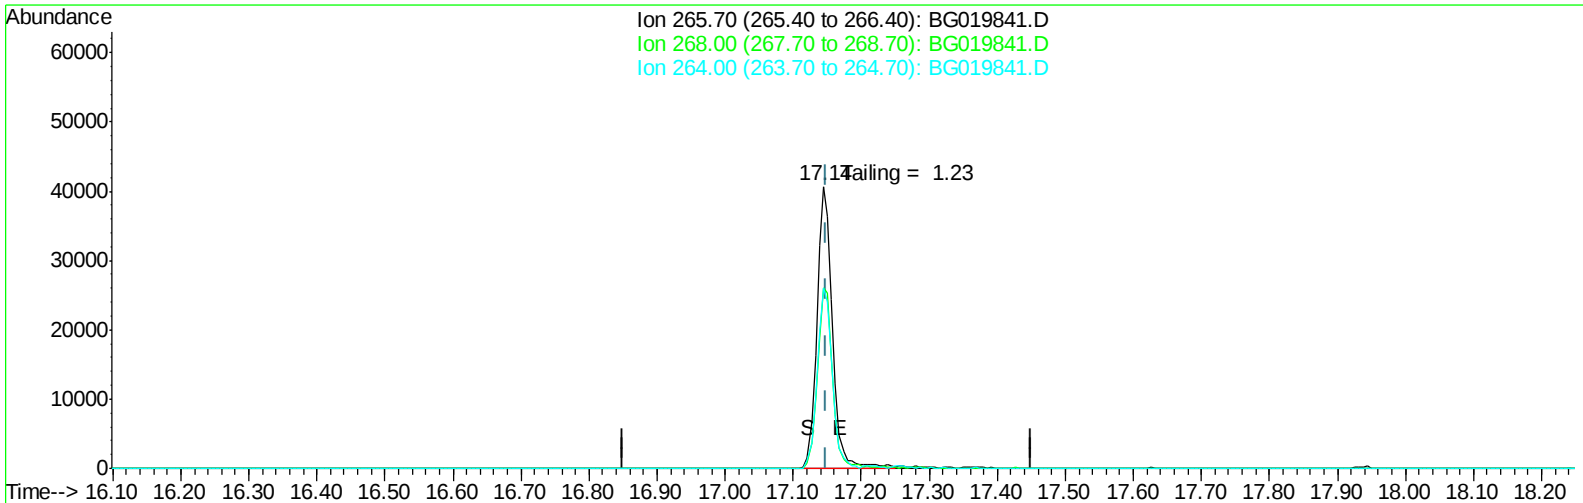

TIC: BG019841.D

(69) Pentachlorophenol (C)




17.144min (-0.006) 0.00ng

response 65493

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	64.22
264.00	60.10	69.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120215\
 Data File : BG019841.D
 Acq On : 2 Dec 2015 19:20
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 08:13:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

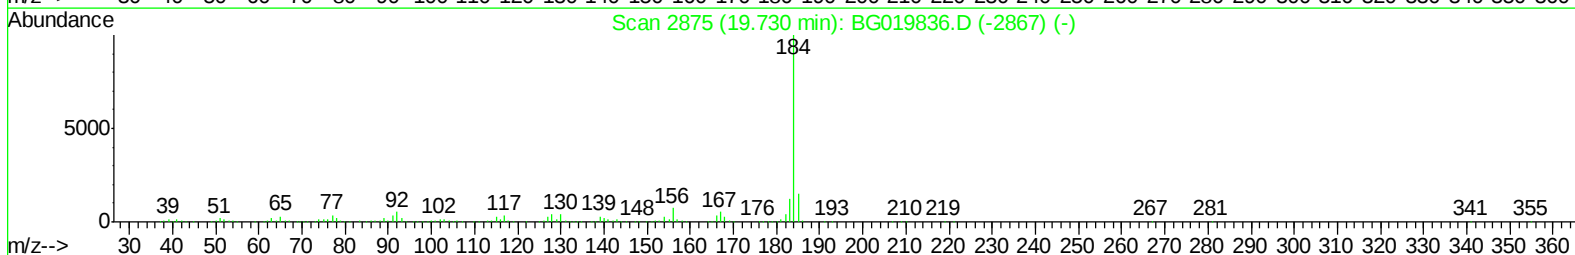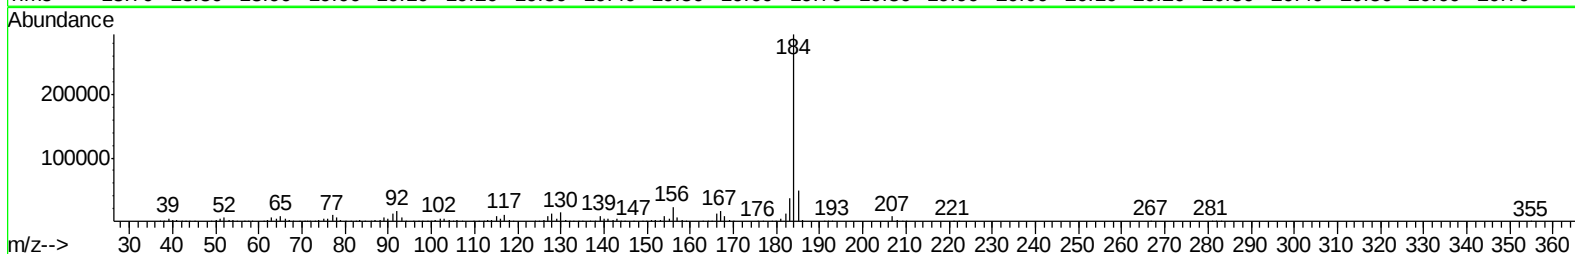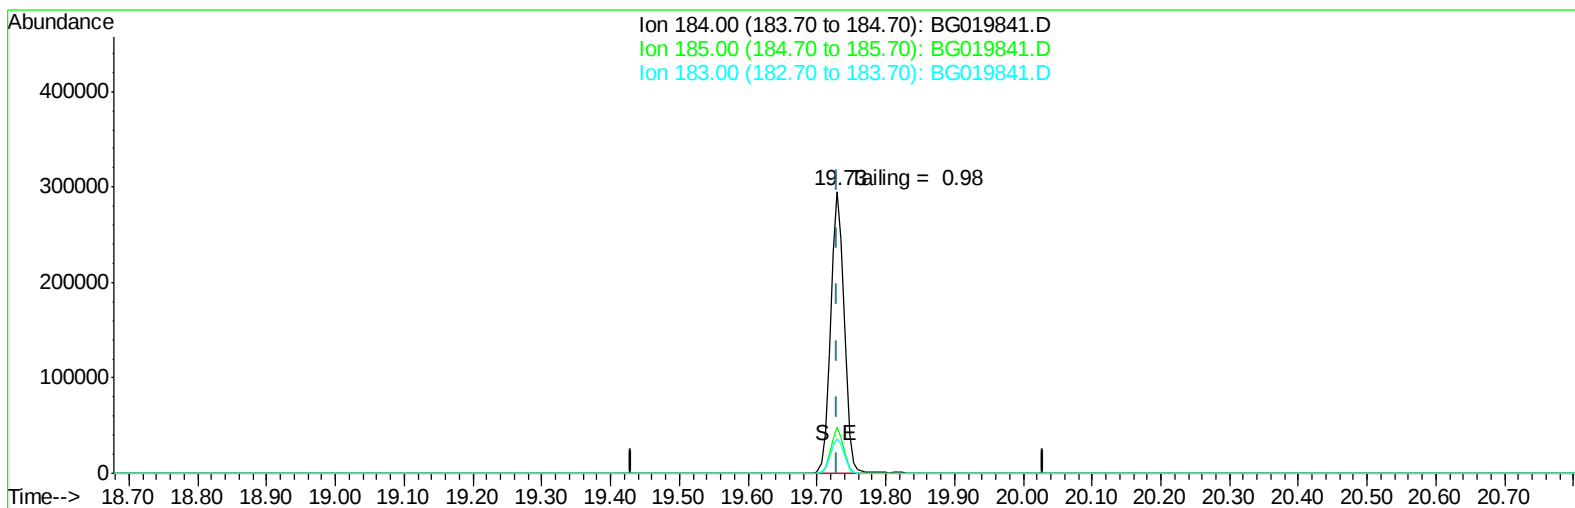

TIC: BG019841.D

(76) Benzidine

19.730min (-0.000) 218913.96ng

response 402686

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.21
183.00	12.60	12.51
0.00	0.00	0.00