
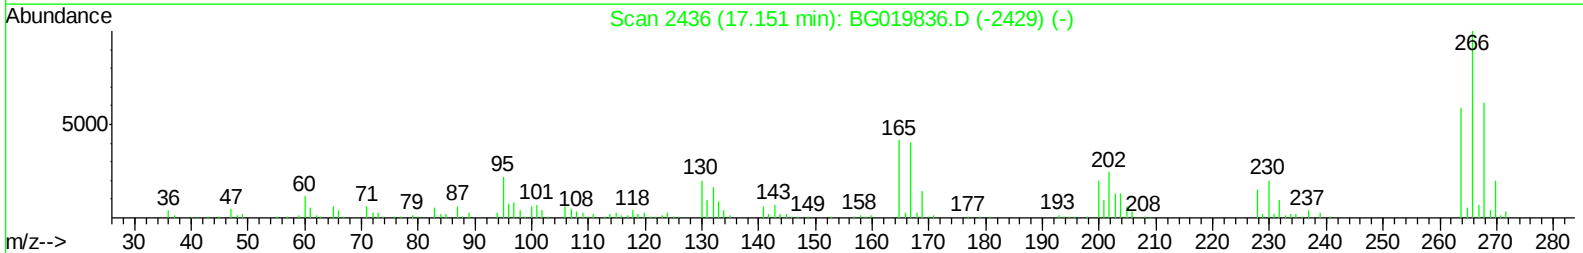
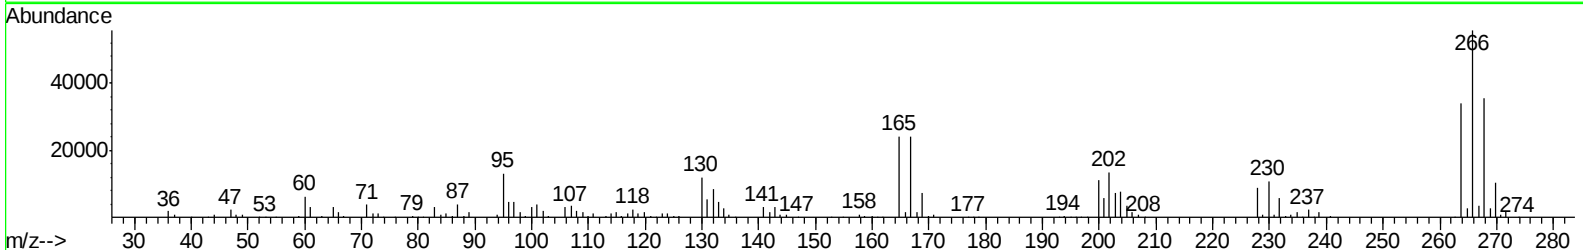


```
Data Path : Z:\HPCHEM1\BNA_G\Data\BG120215\  
Data File : BG019856.D  
Acq On    : 3 Dec 2015    5:02  
Operator  : UM/NP  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 03 08:14:51 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

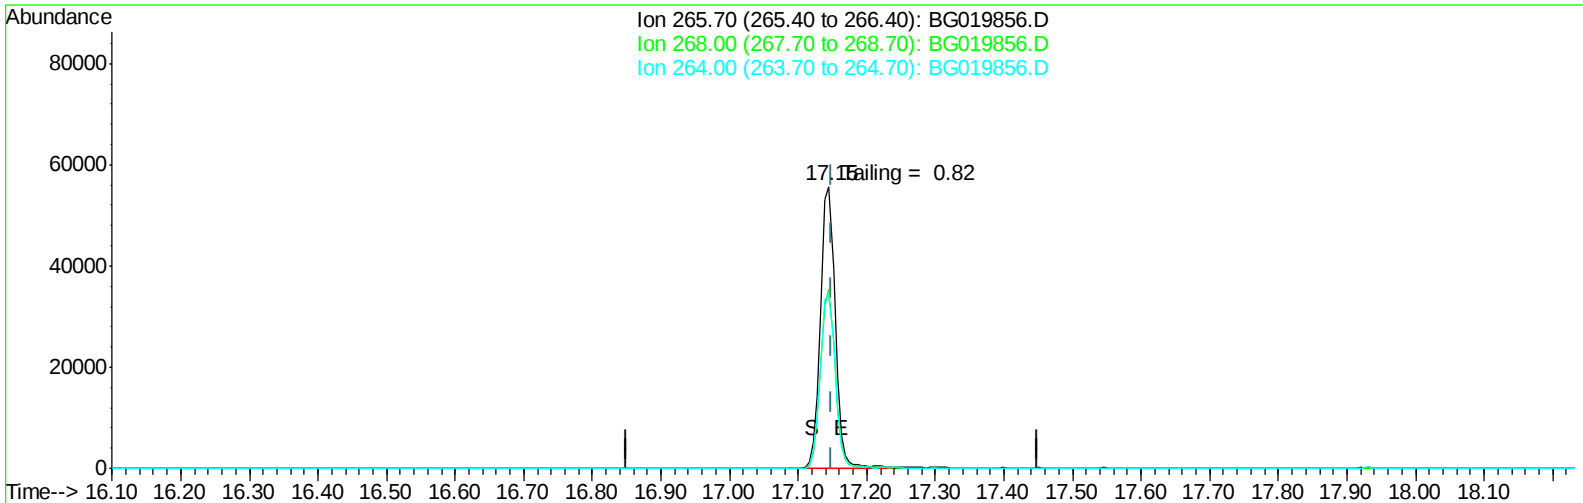

TIC: BG019856.D




(69) Pentachlorophenol (C)

17.145min (-0.005) 0.00ng

response 82841

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120215\
 Data File : BG019856.D
 Acq On : 3 Dec 2015 5:02
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 08:14:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

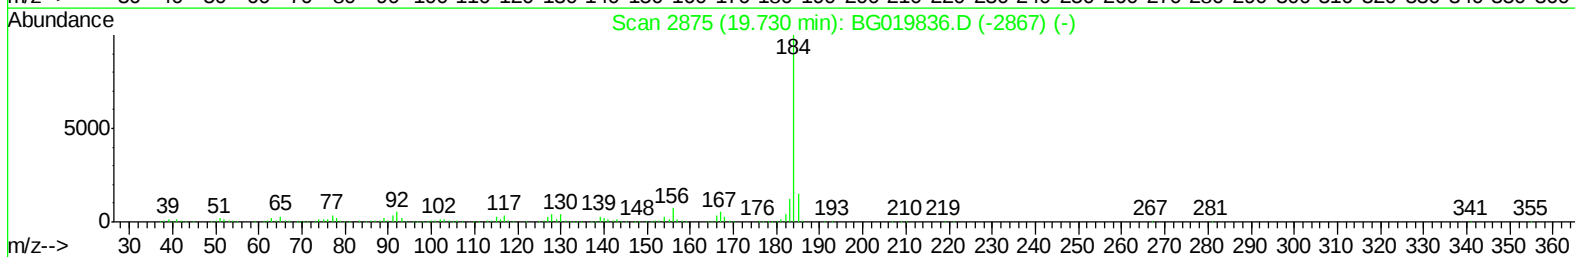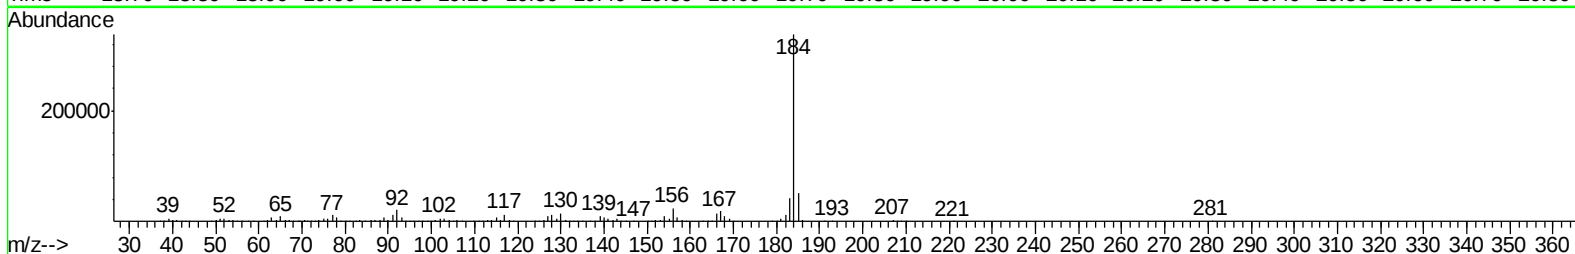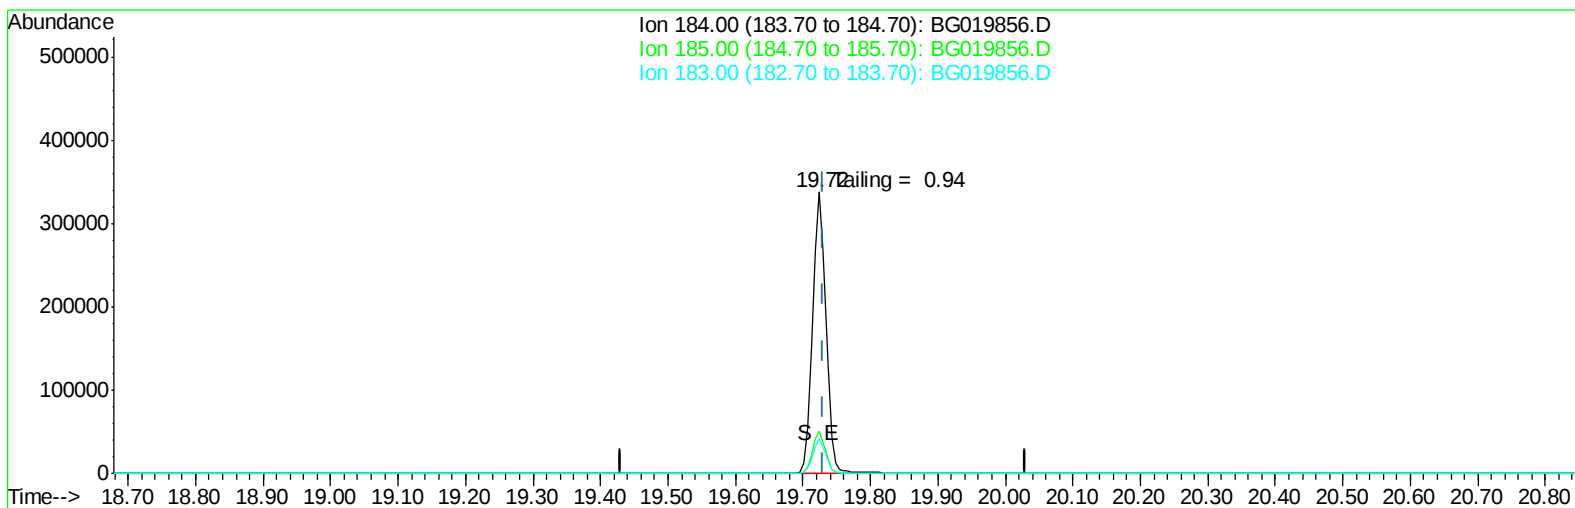

TIC: BG019856.D

(76) Benzidine

19.725min (-0.005) 258300.35ng

response 458167

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.06
183.00	12.60	12.43
0.00	0.00	0.00