


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120215\
 Data File : BG019856.D
 Acq On : 3 Dec 2015 5:02
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

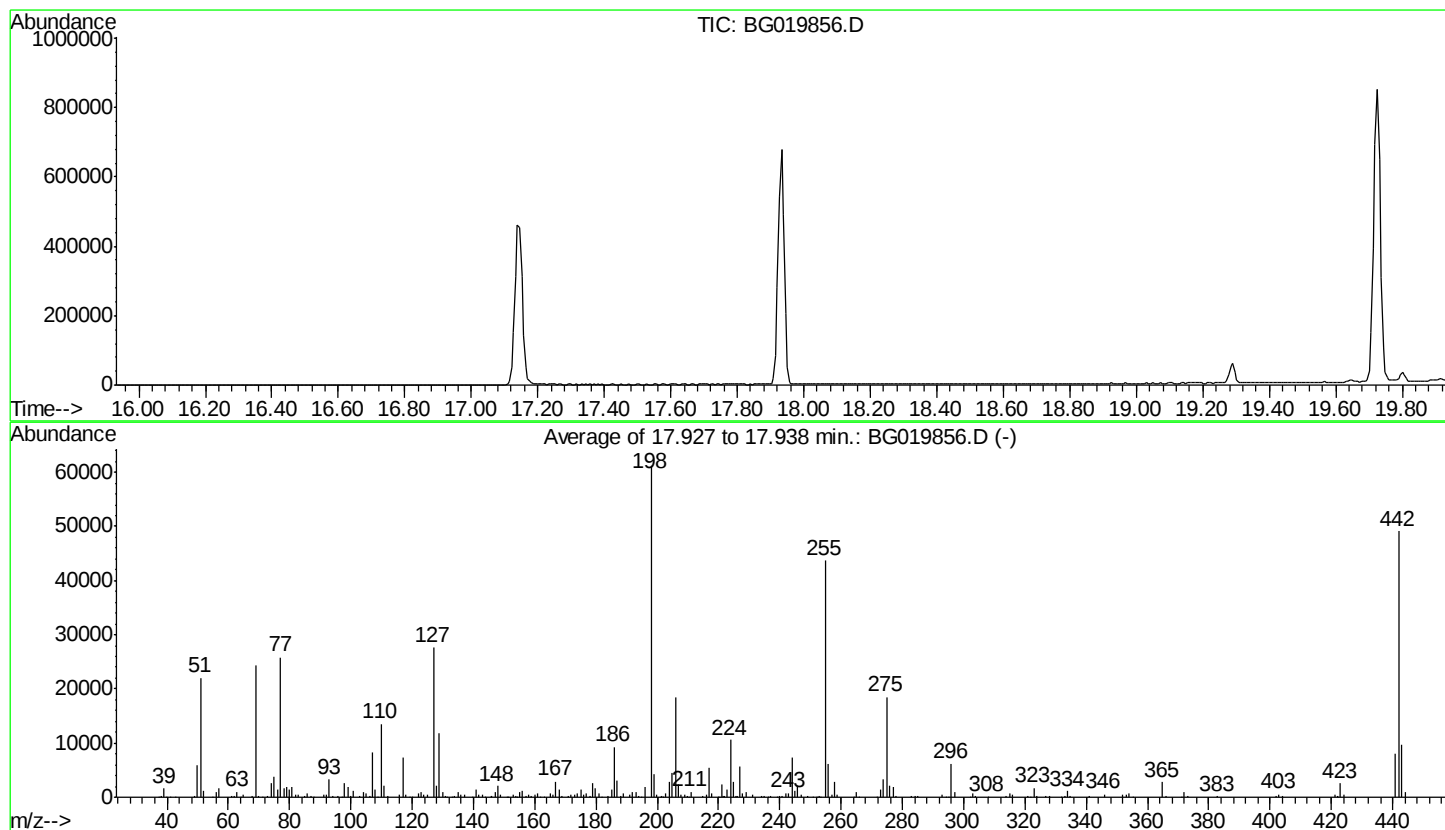

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	22090	PASS
68	69	0.00	2	0.6	139	PASS
69	198	0.00	100	39.9	24426	PASS
70	69	0.00	2	0.9	215	PASS
127	198	10	80	45.1	27624	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61218	PASS
199	198	5	9	7.1	4331	PASS
275	198	10	60	30.3	18549	PASS
365	198	1	100	4.6	2813	PASS
441	442	0.01	24	16.5	8091	PASS
442	198	50	100	80.1	49045	PASS
443	442	15	24	19.9	9757	PASS