
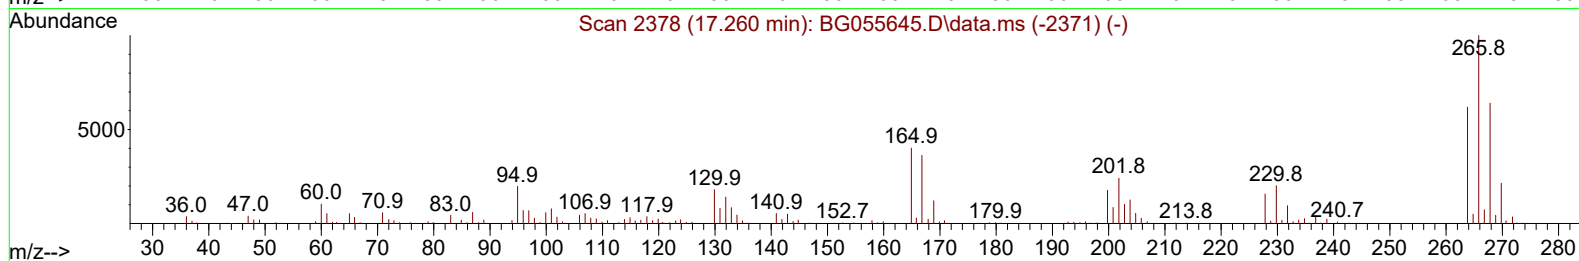
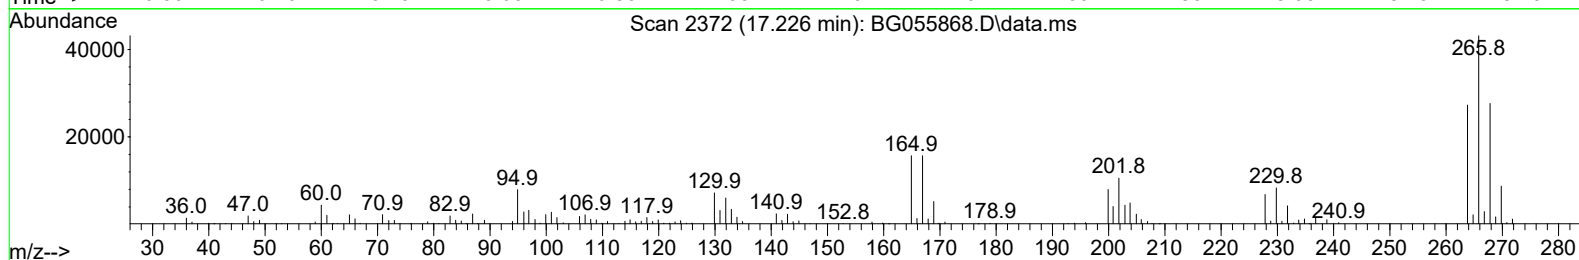


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120222\
Data File : BG055868.D
Acq On : 2 Dec 2022 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 06:01:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

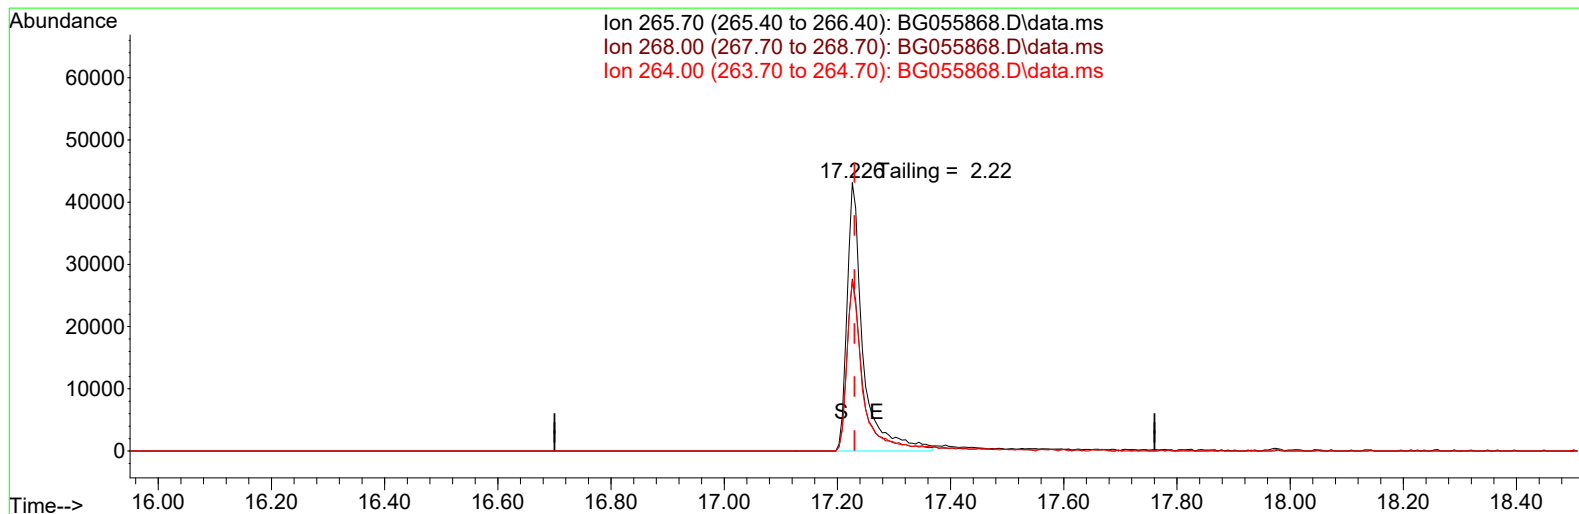

TIC: BG055868.D\data.ms

(70) Pentachlorophenol (C)




17.226min (-0.004) 54365.55 ng

response 83193

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.09
264.00	61.90	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120222\
 Data File : BG055868.D
 Acq On : 2 Dec 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 06:01:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 04:07:17 2022
 Response via : Initial Calibration

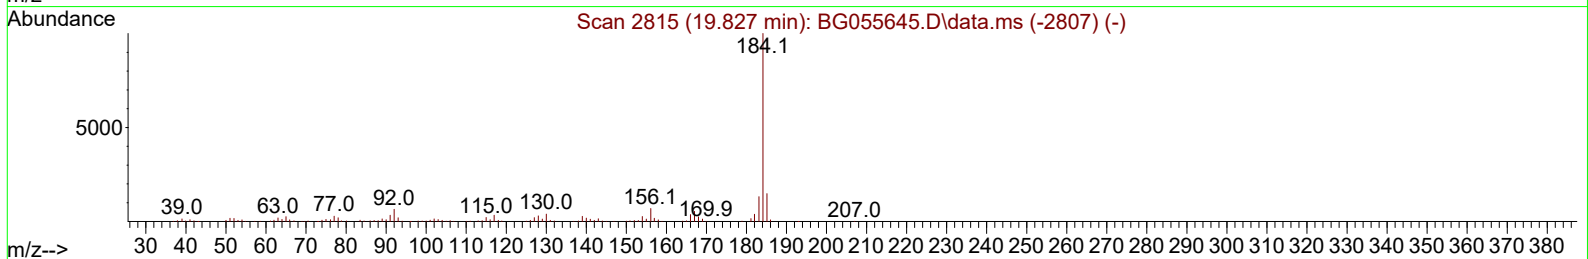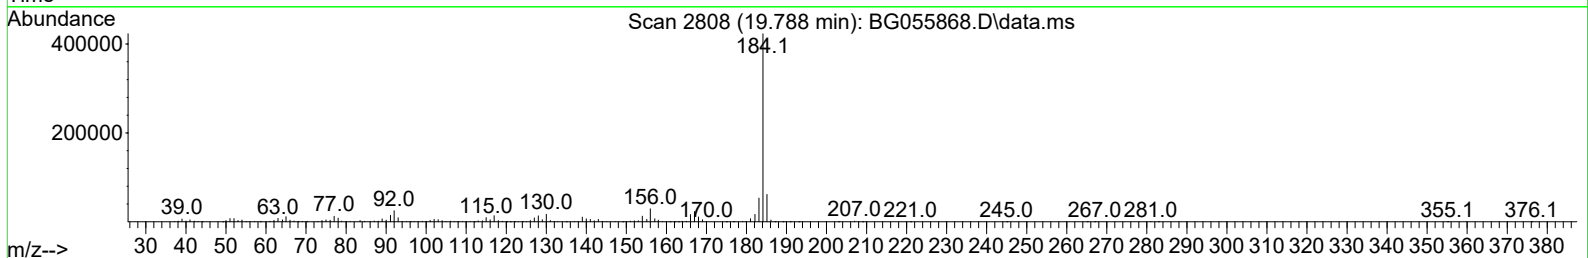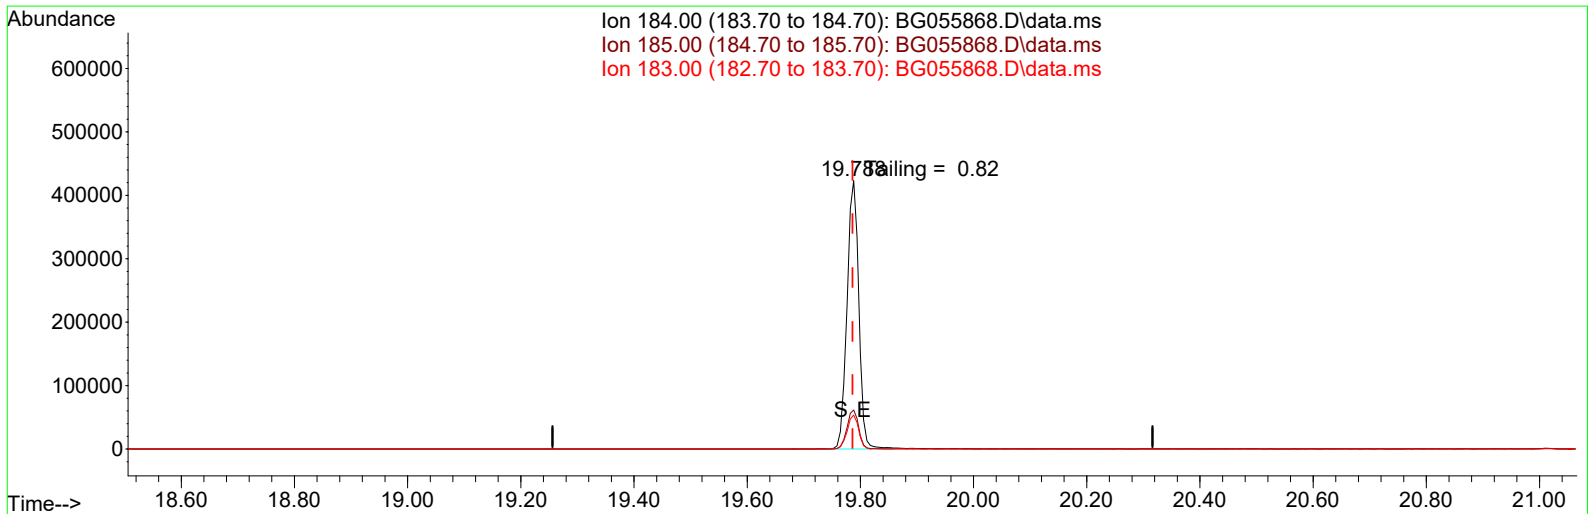

TIC: BG055868.D\data.ms

(77) Benzidine**19.788min (+ 0.002) 433132.49 ng****response 611238**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.55
183.00	13.20	12.67
0.00	0.00	0.00