


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120222\
 Data File : BG055868.D
 Acq On : 2 Dec 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 02 04:07:17 2022

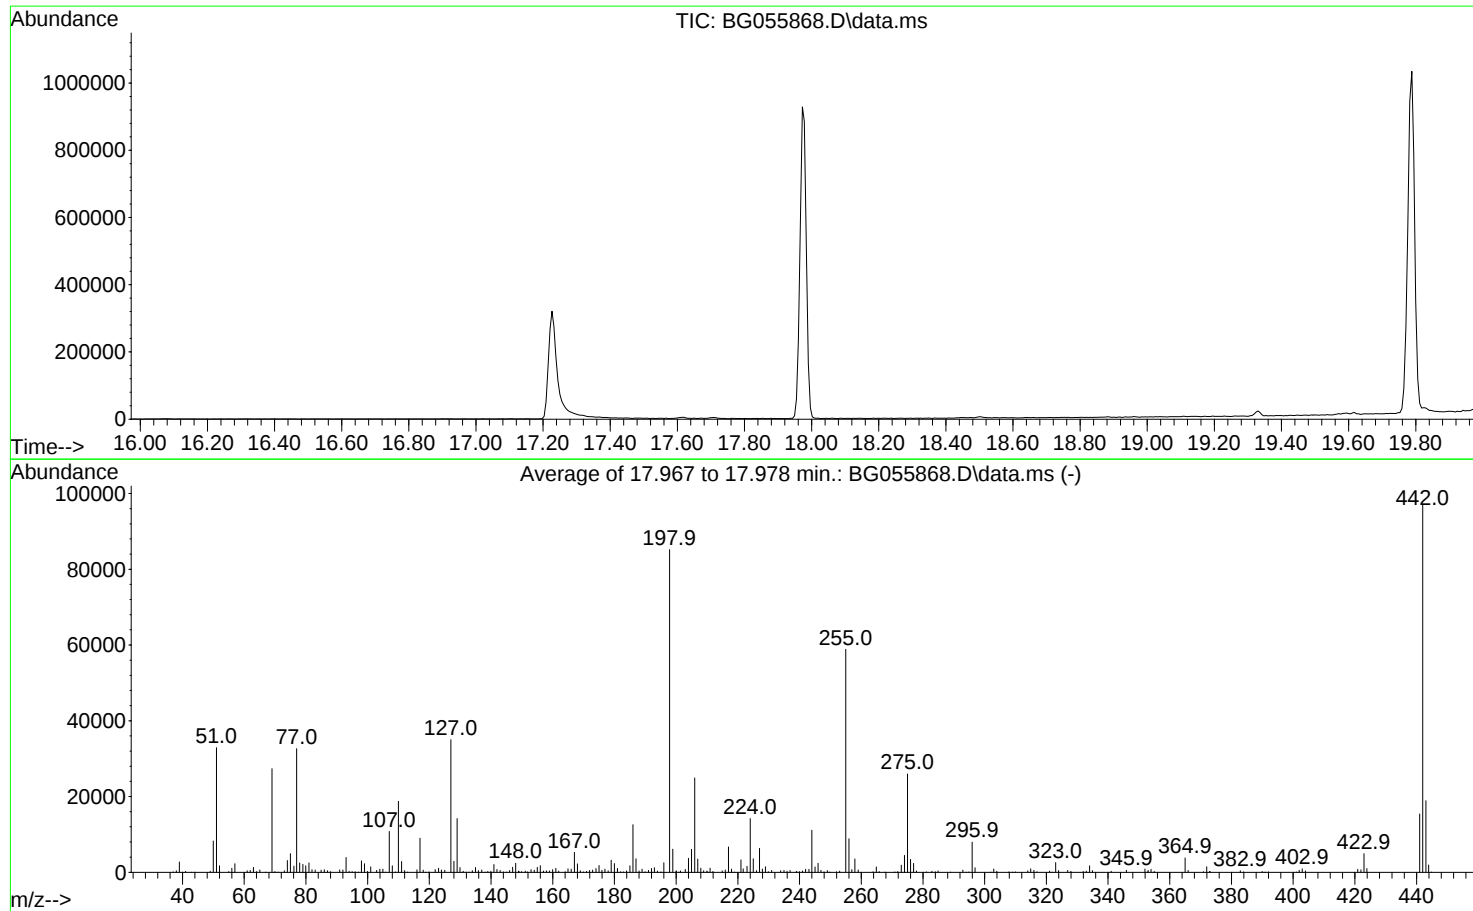




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	32880	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	27365	PASS
70	69	0.00	2	0.6	161	PASS
127	198	10	80	41.1	34987	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85179	PASS
199	198	5	9	7.2	6103	PASS
275	198	10	60	30.5	25941	PASS
365	198	1	100	4.4	3766	PASS
441	198	0.01	100	18.1	15381	PASS
442	442	50	100	100.0	97117	PASS
443	442	15	24	19.5	18922	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120222\
Data File : BG055868.D
Acq On : 2 Dec 2022 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 03 06:01:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 04:07:17 2022
Response via : Initial Calibration

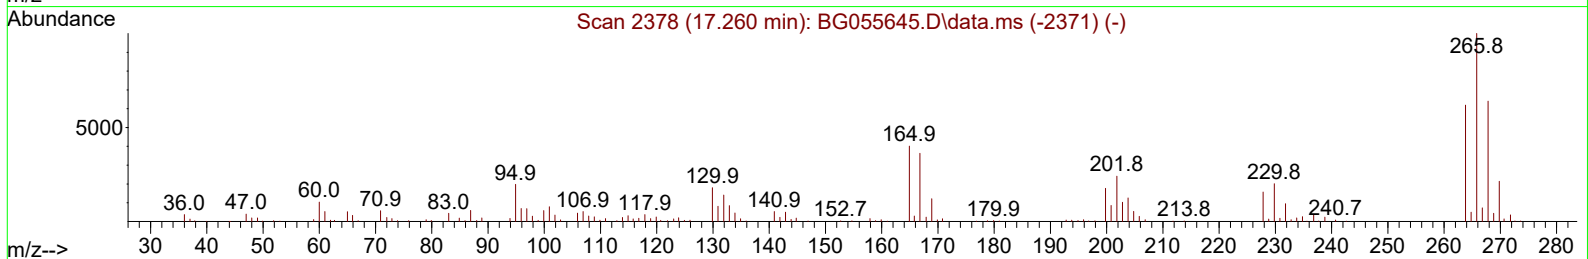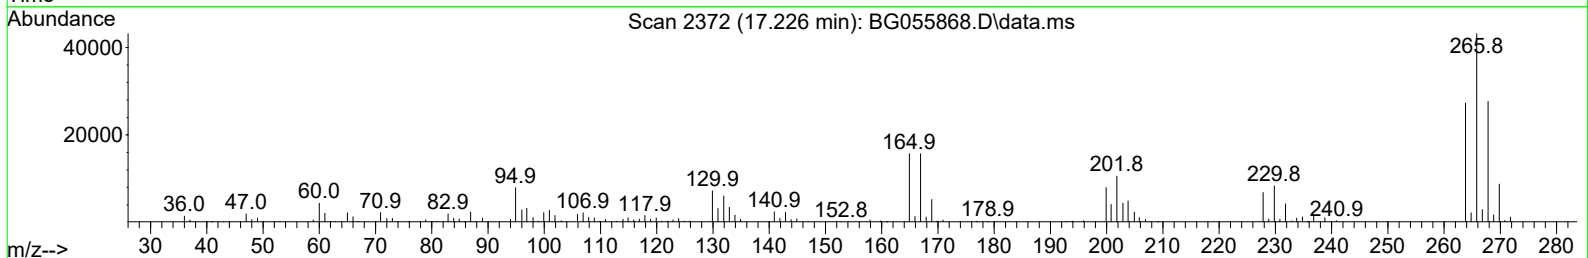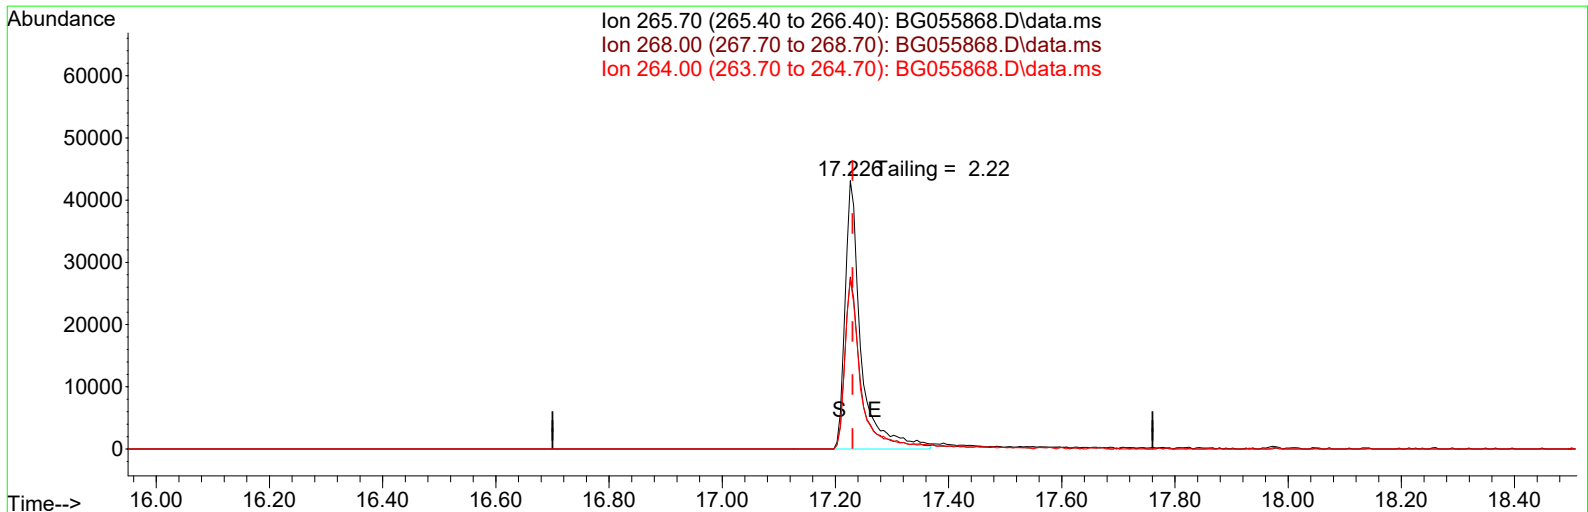

TIC: BG055868.D\data.ms

(70) Pentachlorophenol (C)

17.226min (-0.004) 54365.55 ng




response 83193

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.09
264.00	61.90	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120222\
 Data File : BG055868.D
 Acq On : 2 Dec 2022 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 03 06:01:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 04:07:17 2022
 Response via : Initial Calibration

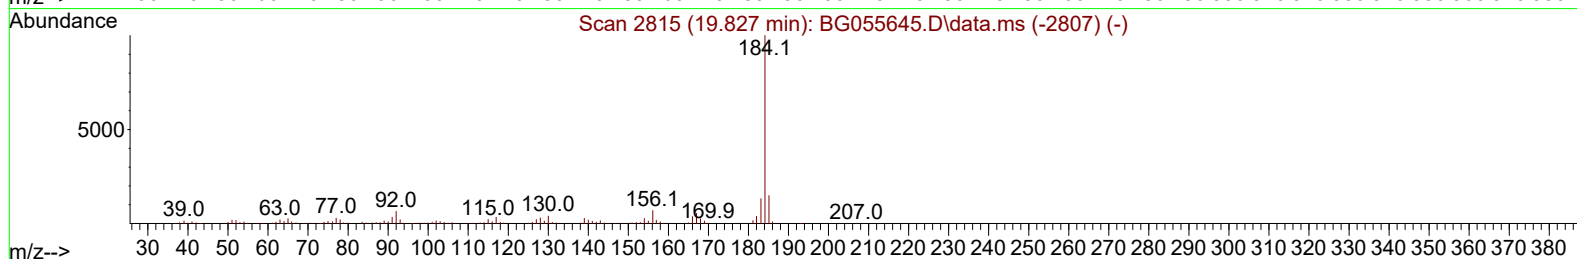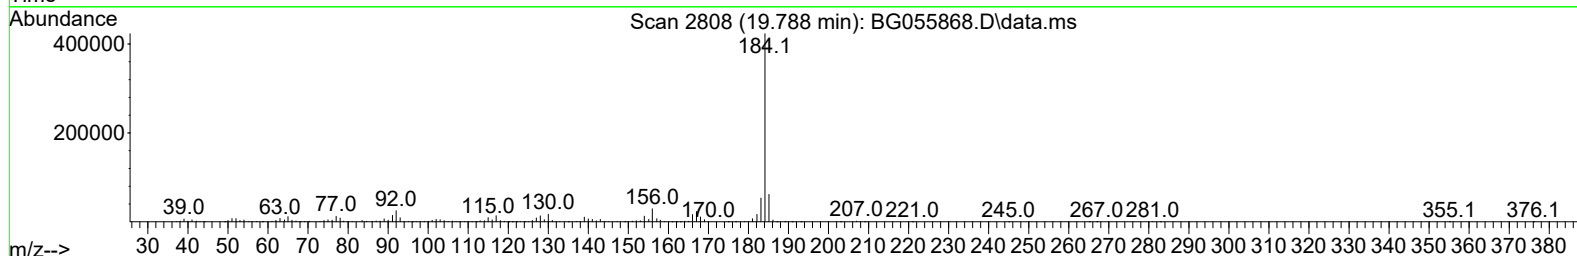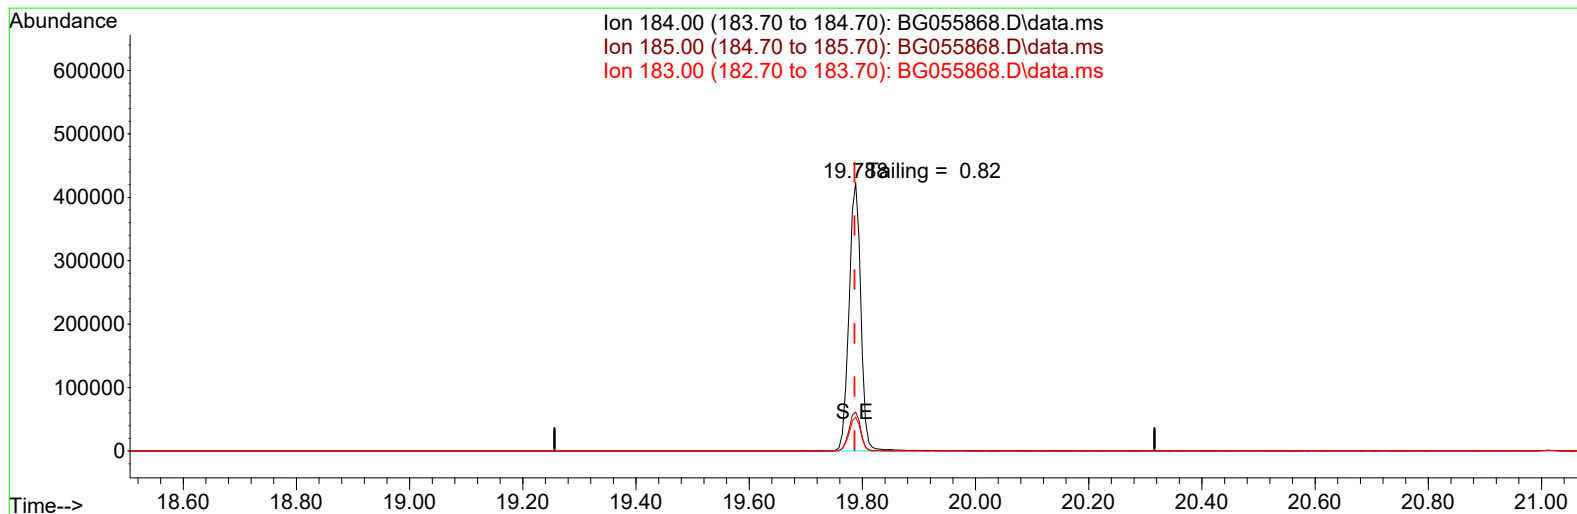

TIC: BG055868.D\data.ms

(77) Benzidine**19.788min (+ 0.002) 433132.49 ng****response 611238**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.55
183.00	13.20	12.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2022	BNA_G	BG055868.D
Compound Name	Response	Retention Time
DDT	287576	21.016
DDD	8114	20.564
DDE	766	20.064
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8880	296456	3.00

Instrument :
BNA_G
ClientSampleId :
DFTPP