
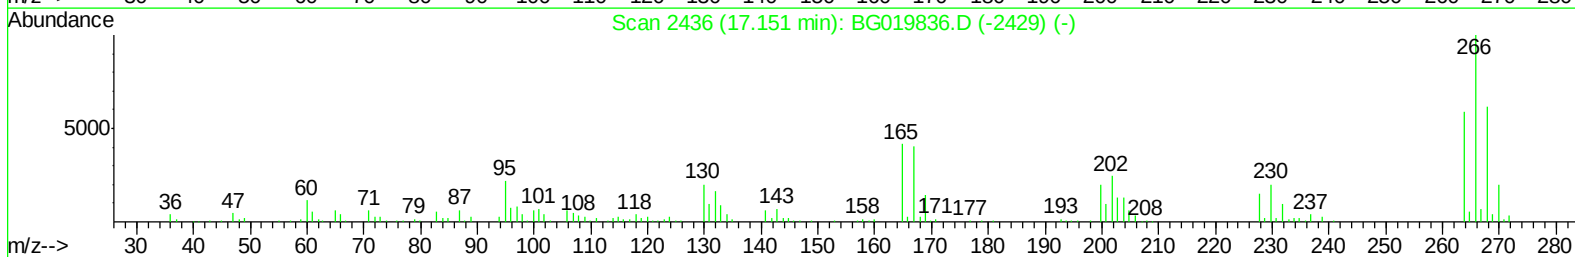
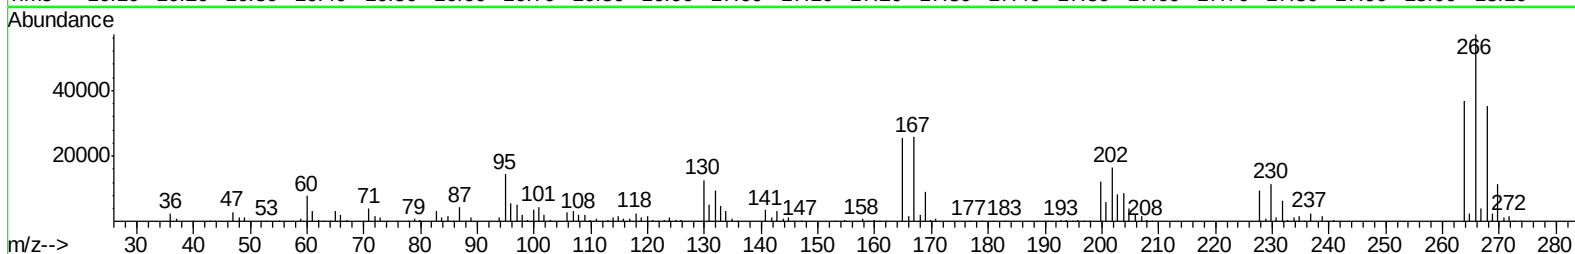


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120315\
Data File : BG019872.D
Acq On : 3 Dec 2015 16:08
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:28:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

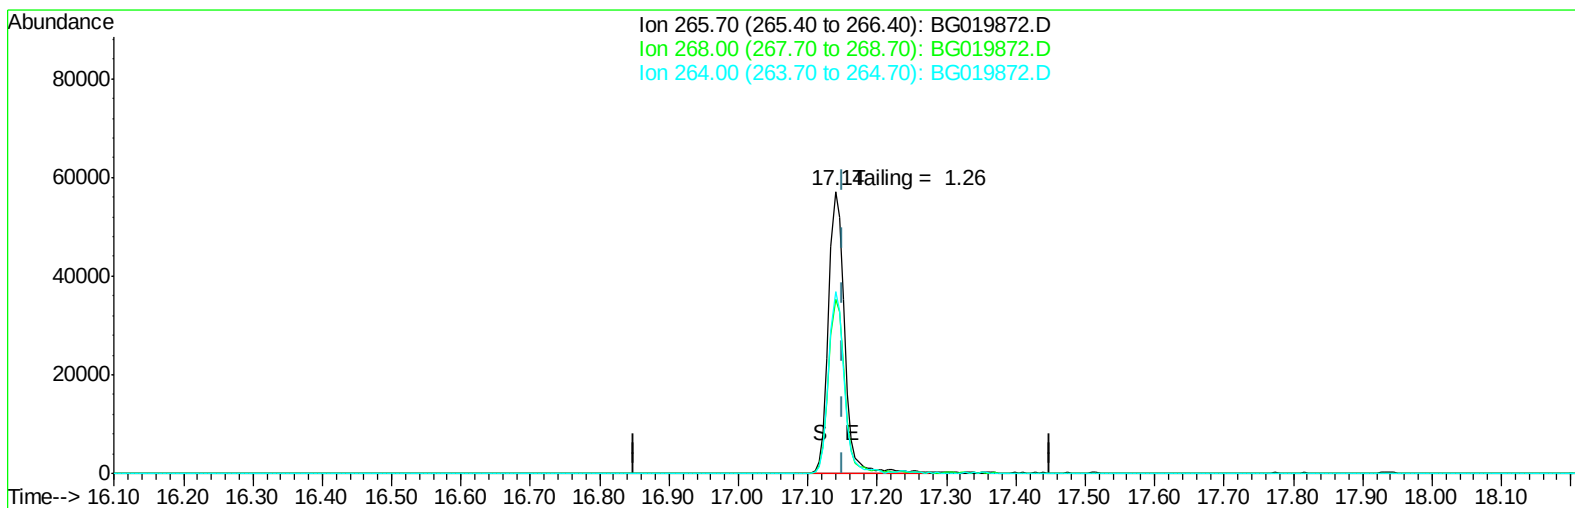

TIC: BG019872.D

(69) Pentachlorophenol (C)




17.139min (-0.011) 0.00ng

response 90883

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.73
264.00	60.10	64.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120315\
Data File : BG019872.D
Acq On : 3 Dec 2015 16:08
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:28:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

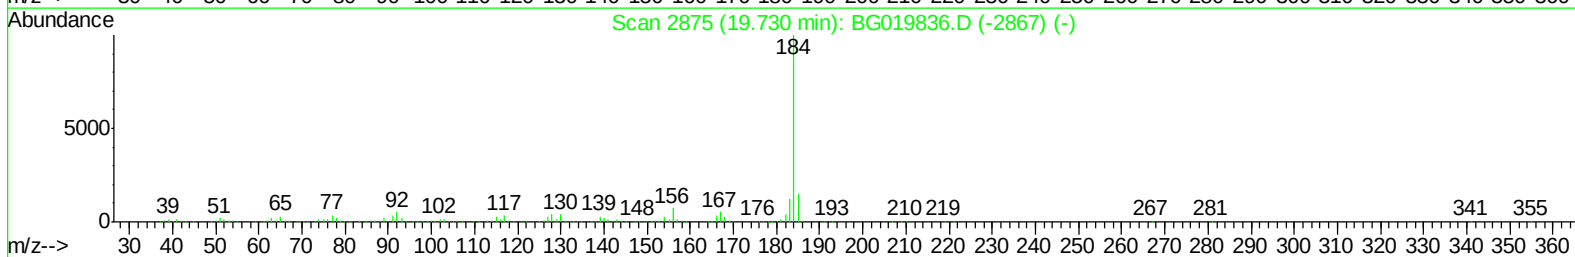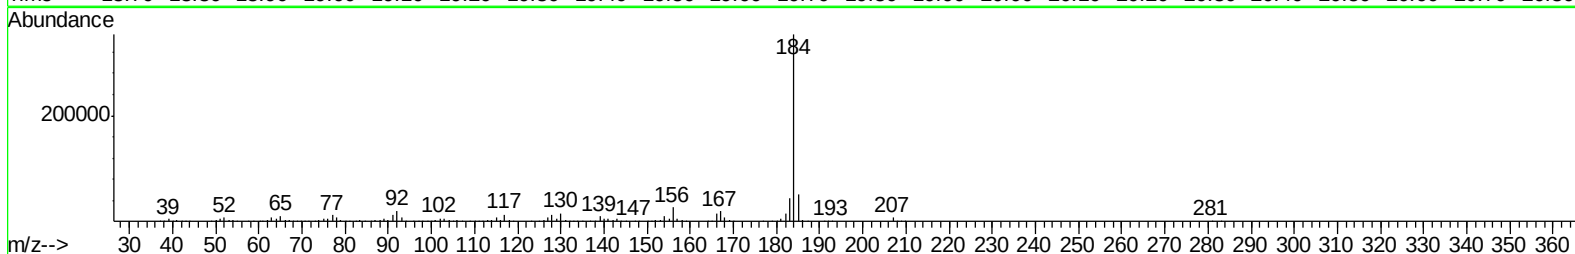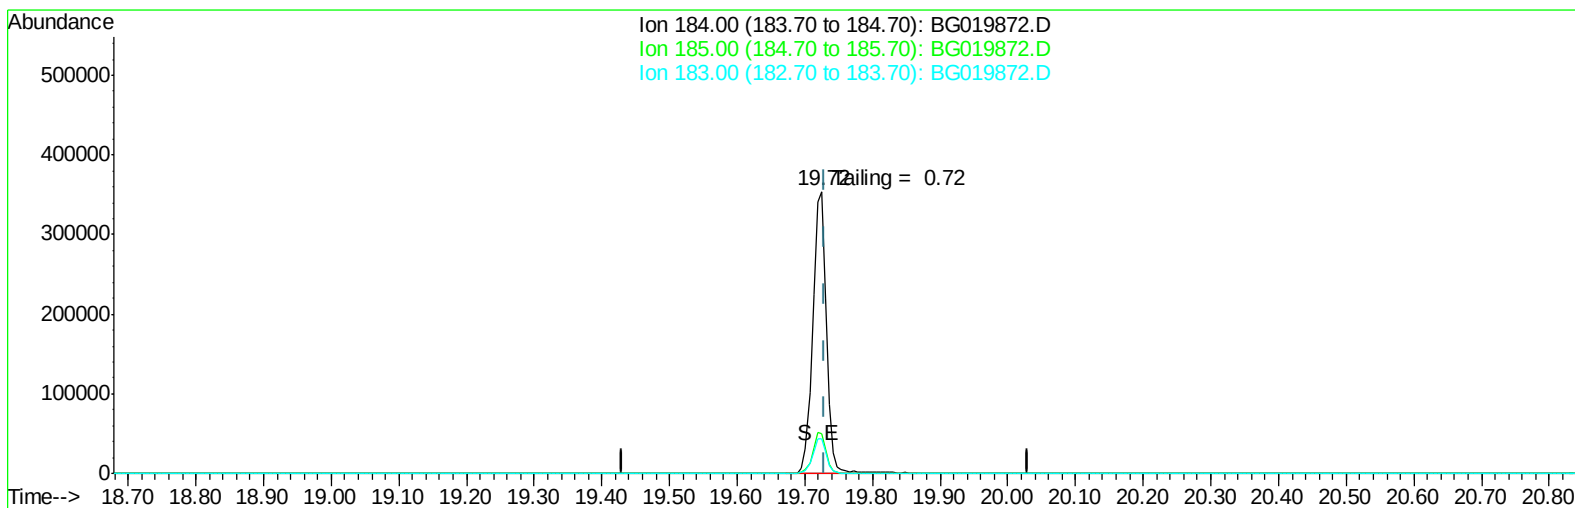

TIC: BG019872.D

(76) Benzidine

19.725min (-0.005) 0.00ng

response 502176

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.25
183.00	12.60	12.14
0.00	0.00	0.00