
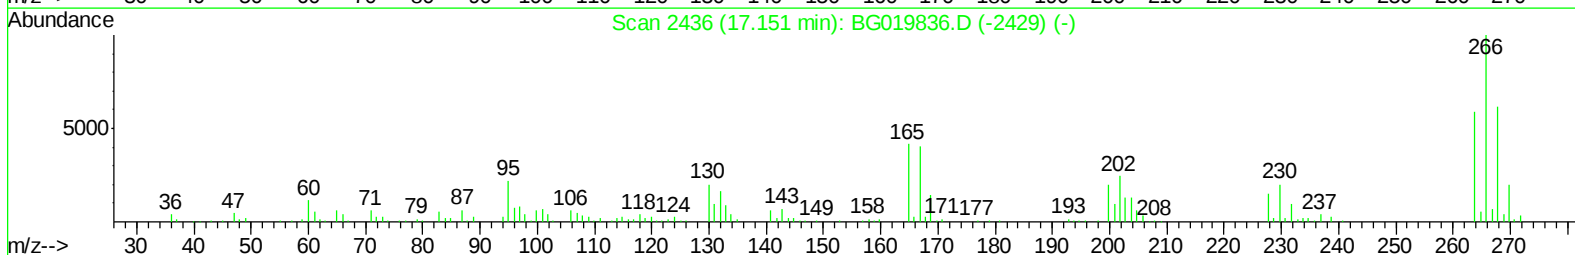
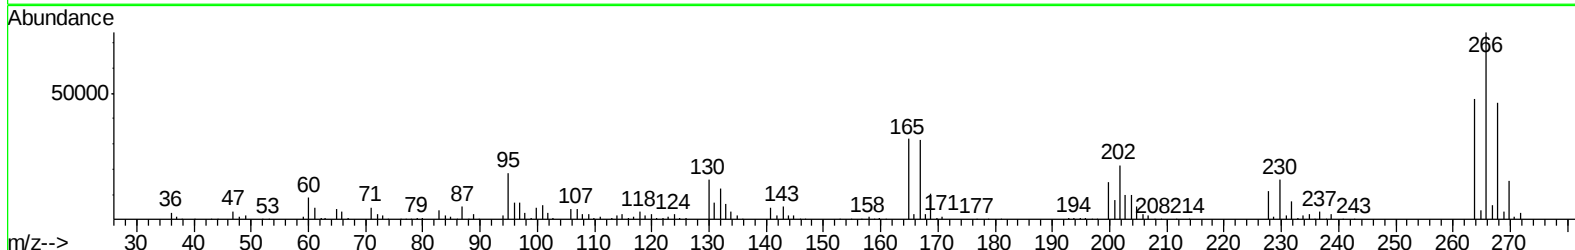


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120315\
Data File : BG019890.D
Acq On : 4 Dec 2015 3:47
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:30:09 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

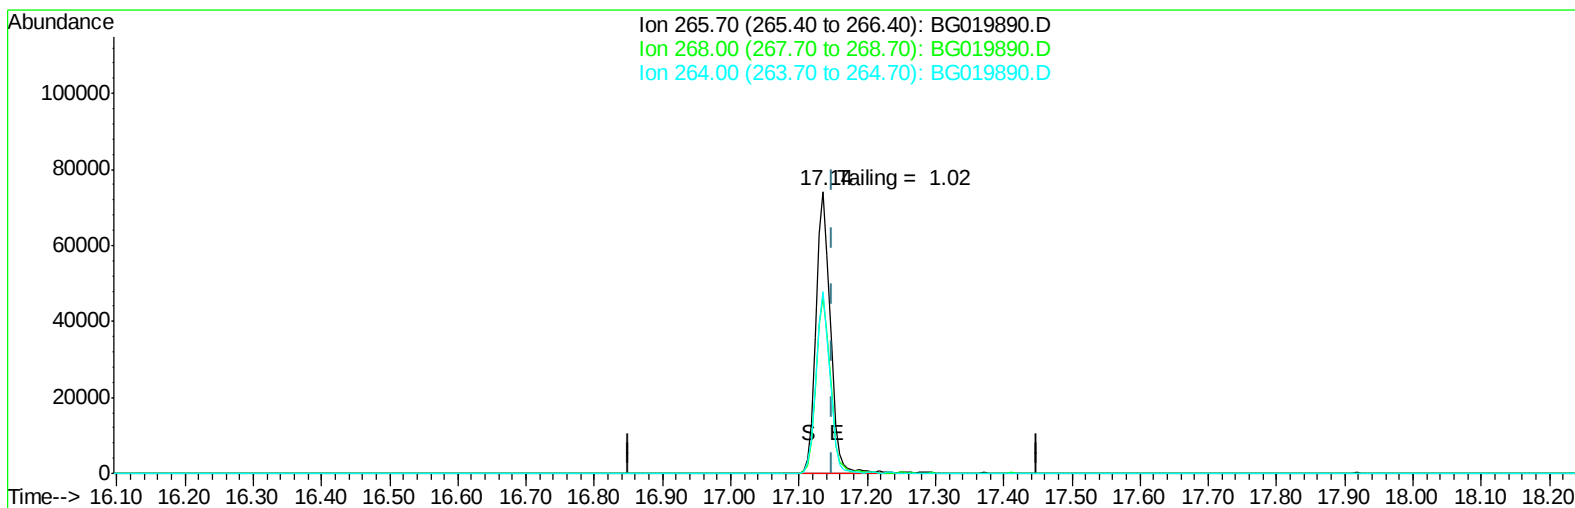

TIC: BG019890.D

(69) Pentachlorophenol (C)




17.136min (-0.014) 0.00ng

response 108189

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	62.68
264.00	60.10	64.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120315\
Data File : BG019890.D
Acq On : 4 Dec 2015 3:47
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:30:09 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

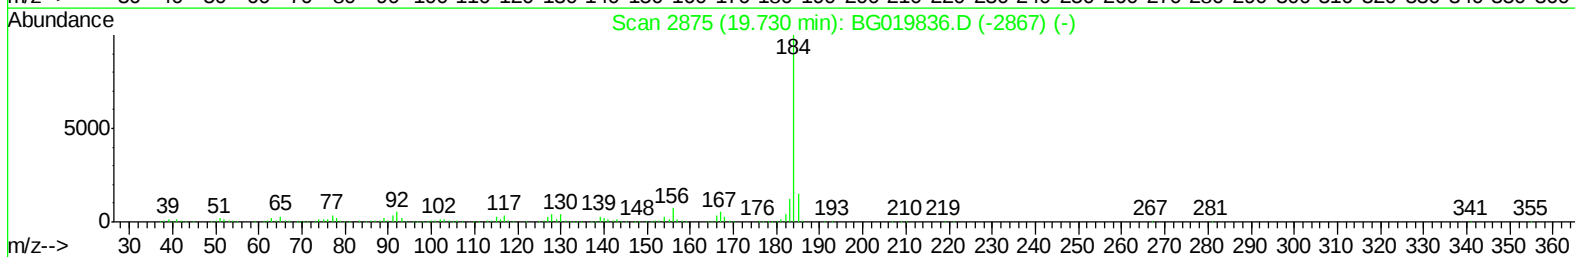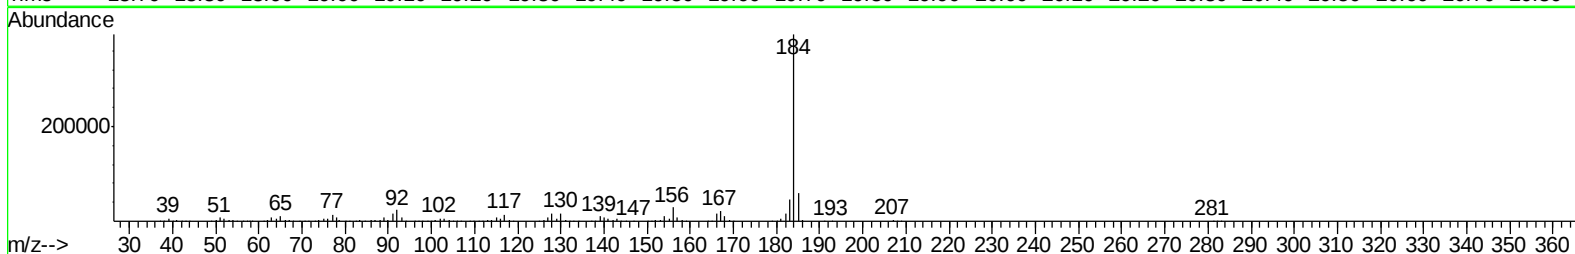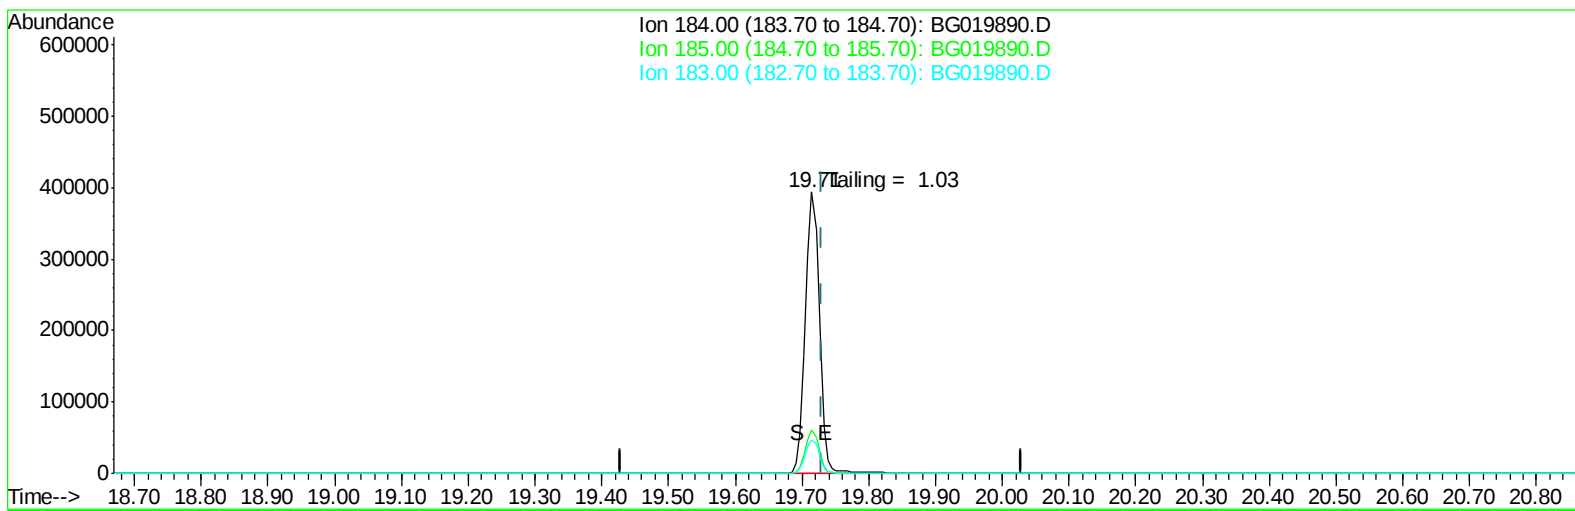

TIC: BG019890.D

(76) Benzidine

19.715min (-0.015) 0.00ng

response 561236

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.44
183.00	12.60	11.79
0.00	0.00	0.00