


Data Path : Z:\HPCHEM1\BNA G\DATA\BG120315\
 Data File : BG019890.D
 Acq On : 4 Dec 2015 3:47
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

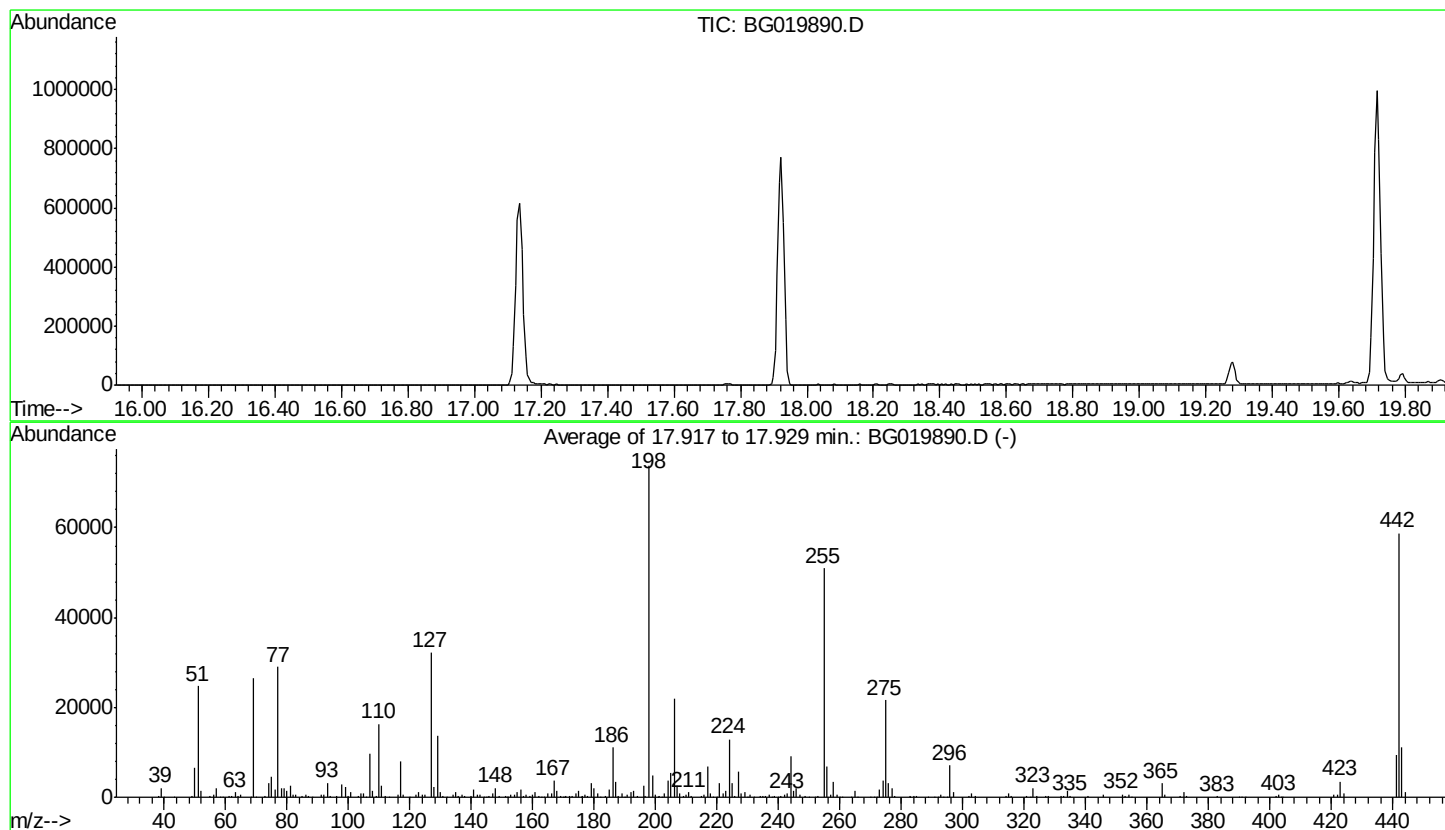

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	24786	PASS
68	69	0.00	2	0.5	142	PASS
69	198	0.00	100	36.1	26650	PASS
70	69	0.00	2	0.5	134	PASS
127	198	10	80	43.6	32152	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73824	PASS
199	198	5	9	6.7	4942	PASS
275	198	10	60	29.3	21602	PASS
365	198	1	100	4.2	3124	PASS
441	442	0.01	24	16.1	9463	PASS
442	198	50	100	79.6	58794	PASS
443	442	15	24	19.1	11236	PASS