

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120318\
 Data File : BG038322.D
 Acq On : 4 Dec 2018 5:32
 Operator : JU/SJ
 Sample : J5764-26
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-113018-C

Quant Time: Dec 04 06:38:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	11014	20.00	ng	-0.02
21) Naphthalene-d8	10.90	136	54887	20.00	ng	-0.01
39) Acenaphthene-d10	14.71	164	43346	20.00	ng	-0.01
64) Phenanthrene-d10	17.46	188	153948	20.00	ng	-0.01
76) Chrysene-d12	21.74	240	172556	20.00	ng	-0.01
87) Perylene-d12	25.06	264	176569	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	74719	117.13	ng	0.00
7) Phenol-d6	7.22	99	100133	109.97	ng	-0.01
23) Nitrobenzene-d5	9.25	82	106056	103.43	ng	-0.01
42) 2,4,6-Tribromophenol	16.20	330	88869	179.77	ng	-0.01
45) 2-Fluorobiphenyl	13.33	172	217173	72.99	ng	-0.02
79) Terphenyl-d14	20.06	244	868165	118.38	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.25	70	13171	19.990	ng	# 79
51) 2,6-Dinitrotoluene	14.71	165	5654	7.270	ng	# 23
57) 2,4-Dinitrotoluene	14.71	165	5654	5.343	ng	# 23
67) 4-Bromophenyl-phenylether	16.20	248	6013	3.559	ng	# 1
77) Benzidine	20.06	184	14528	2.399	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120318\
Data File : BG038322.D
Acq On : 4 Dec 2018 5:32
Operator : JU/SJ
Sample : J5764-26
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-02-113018-C

Quant Time: Dec 04 06:38:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

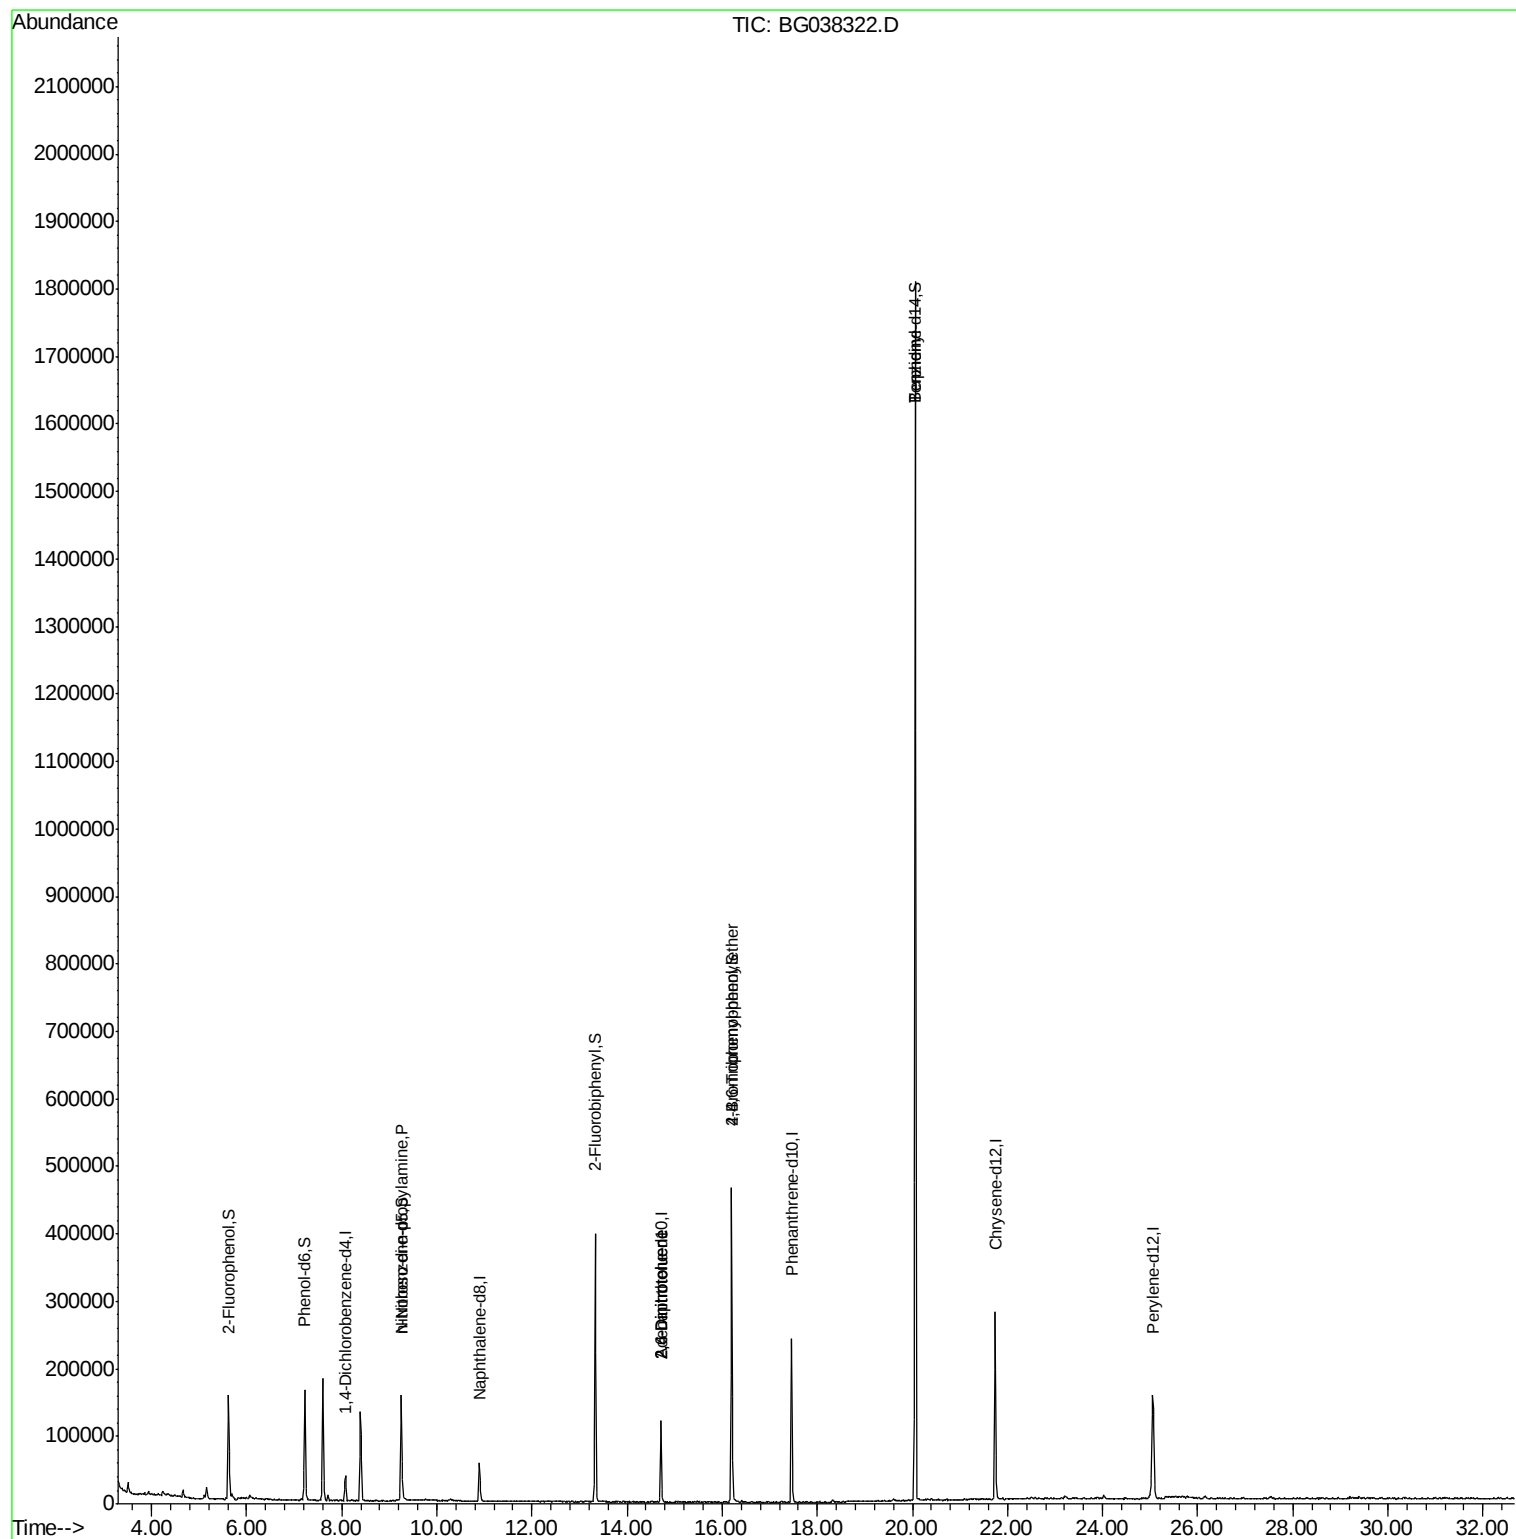




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. -0.02 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Instrument :
BNA_G
ClientSampleId :
JC-02-113018-C

Tgt Ion:152 Resp: 11014
Ion Ratio Lower Upper
152 100
150 148.8 126.0 189.0
115 57.0 45.5 68.3

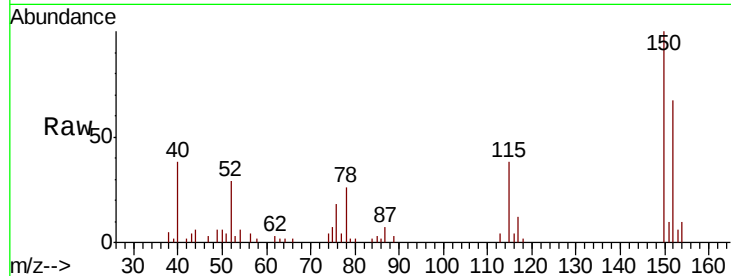


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

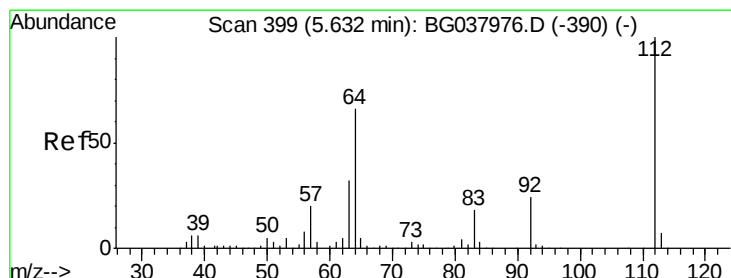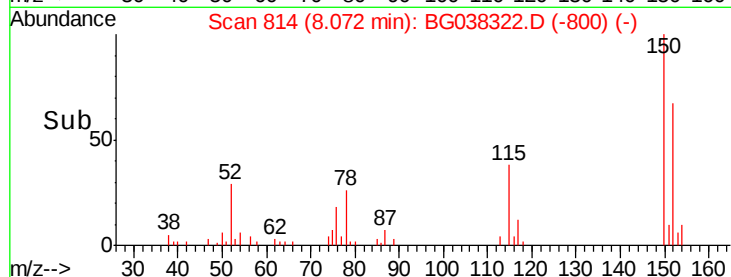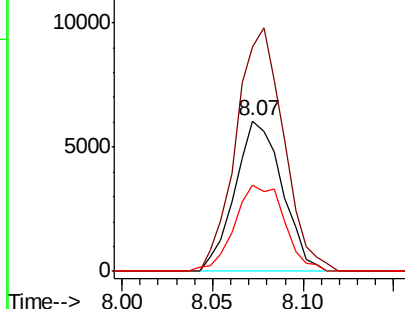



#5

2-Fluorophenol
Concen: 117.130 ng
RT: 5.62 min Scan# 397
Delta R.T. -0.01 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Tgt Ion:112 Resp: 74719
Ion Ratio Lower Upper
112 100
64 59.3 53.1 79.7
63 36.2 27.3 40.9

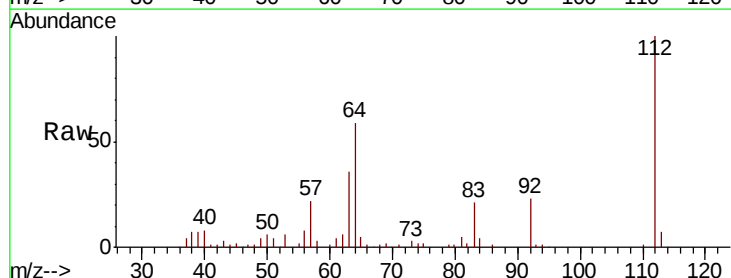

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

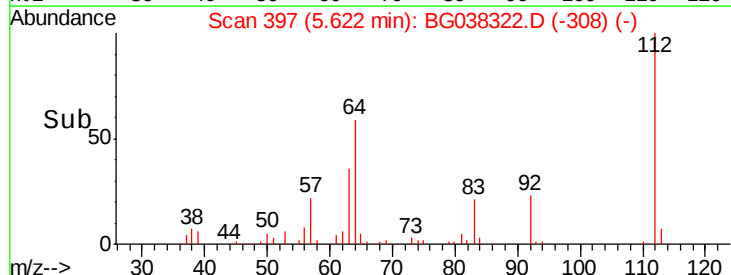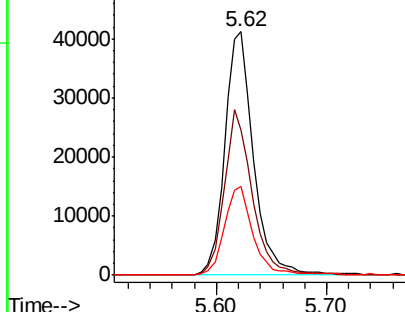



#7

Phenol-d6

Concen: 109.966 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32

Instrument :

BNA_G

ClientSampleId :

JC-02-113018-C


Tgt Ion: 99 Resp: 100133

Ion Ratio Lower Upper




99 100

42 21.8 15.0 22.4

71 33.4 25.5 38.3

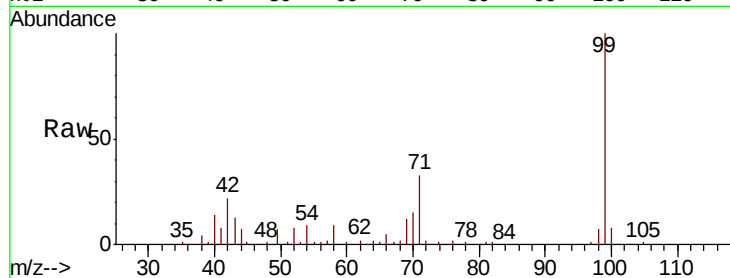

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

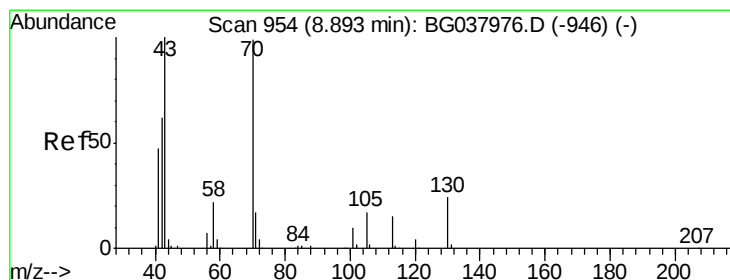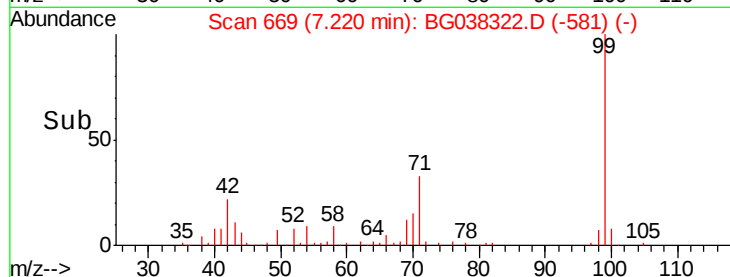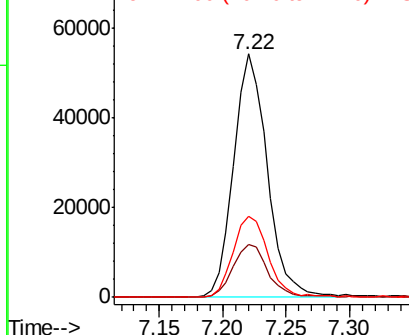

#19

n-Nitroso-di-n-propylamine

Concen: 19.990 ng

RT: 9.25 min Scan# 1015

Delta R.T. 0.36 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32

Tgt Ion: 70 Resp: 13171


Ion Ratio Lower Upper

70 100



42 58.8 53.9 80.9


101 0.0 8.2 12.2#

130 0.0 18.2 27.4#

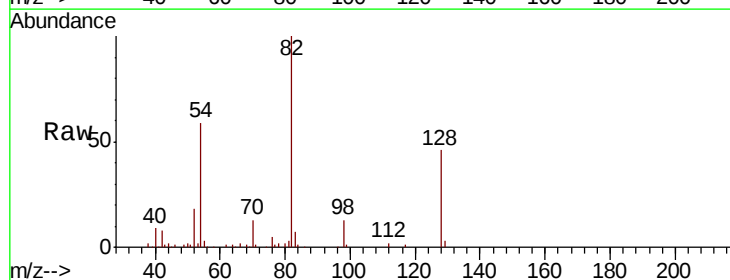

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

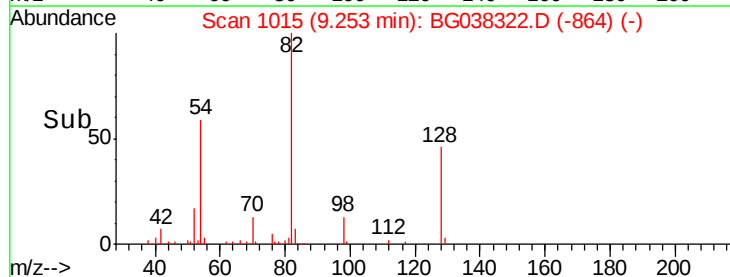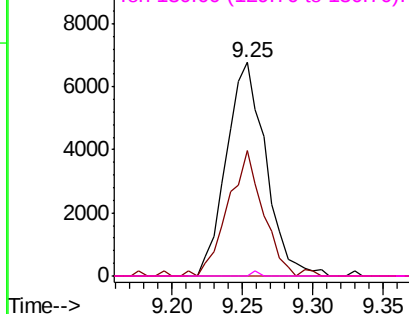


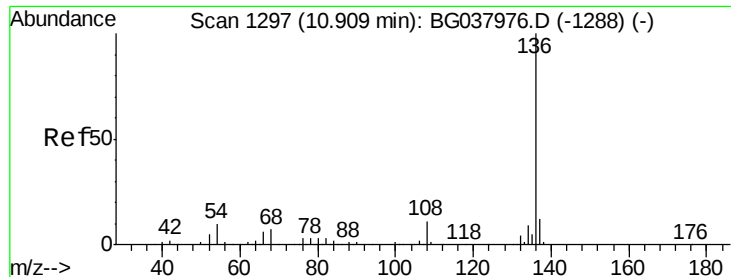




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.90 min Scan# 1295
Delta R.T. -0.01 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Instrument :
BNA_G
ClientSampleId :
JC-02-113018-C

Tgt Ion:	136	Resp:	54887
Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.6	14.4
54	11.9	7.9	11.9#
68	4.9	4.8	7.2

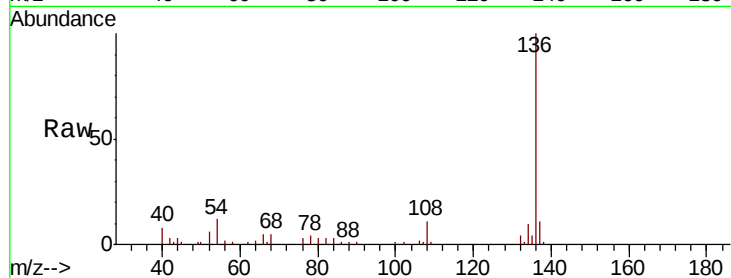


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

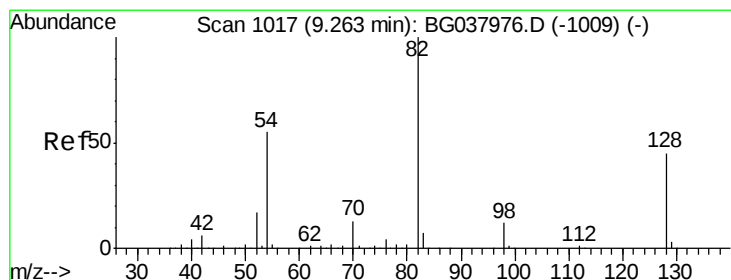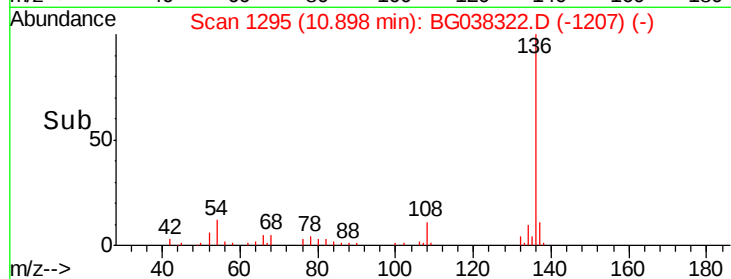
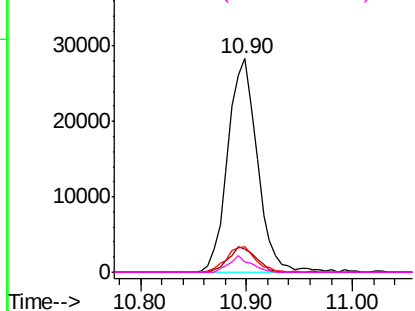



#23
Nitrobenzene-d5
Concen: 103.435 ng
RT: 9.25 min Scan# 1015
Delta R.T. -0.01 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Tgt Ion:	82	Resp:	106056
Ion	Ratio	Lower	Upper
82	100		
128	45.8	34.6	51.8
54	59.0	45.3	67.9

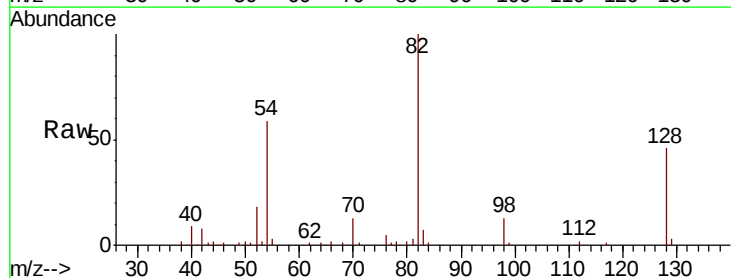

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

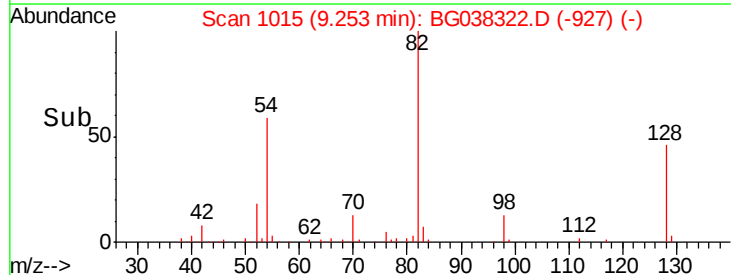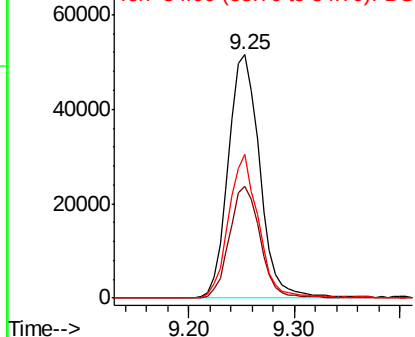

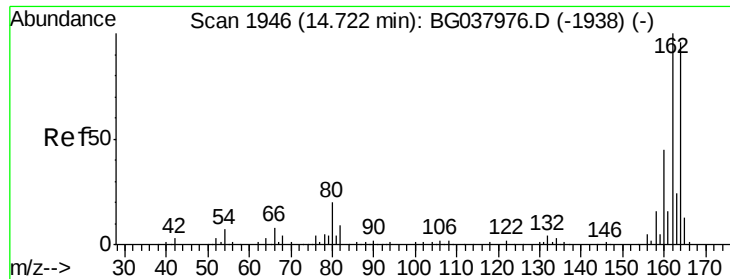

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.71 min Scan# 1944

Delta R.T. -0.01 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32

Instrument :

BNA_G

ClientSampleId :

JC-02-113018-C


Tgt Ion:164 Resp: 43346

Ion Ratio Lower Upper

164 100

162 106.0 81.3 121.9




160 43.2 36.3 54.5

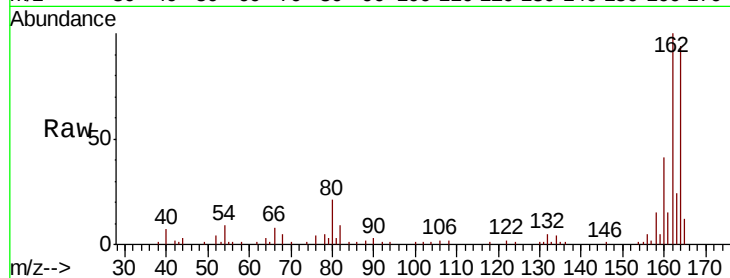

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

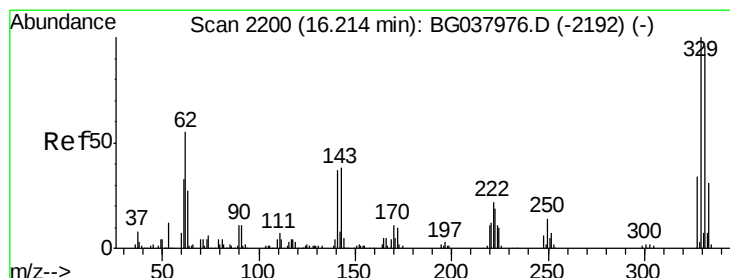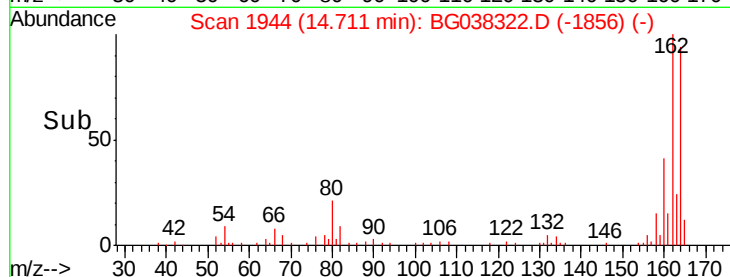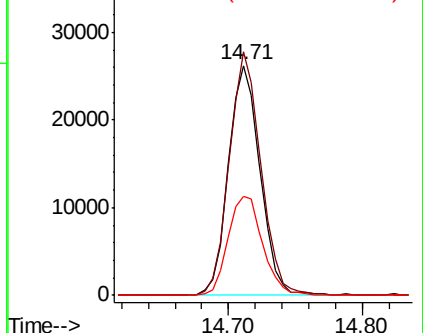

#42

2,4,6-Tribromophenol

Concen: 179.769 ng

RT: 16.20 min Scan# 2198

Delta R.T. -0.01 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32


Tgt Ion:330 Resp: 88869

Ion Ratio Lower Upper

330 100

332 94.9 78.4 117.6



141 39.7 32.2 48.2

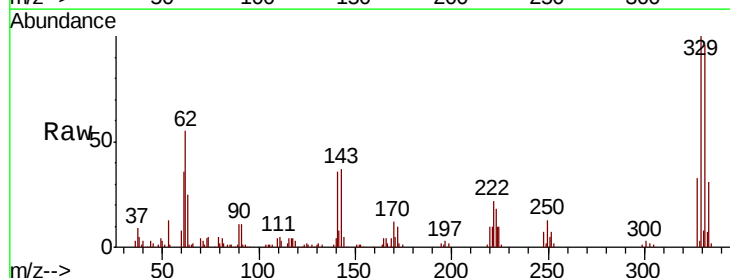

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



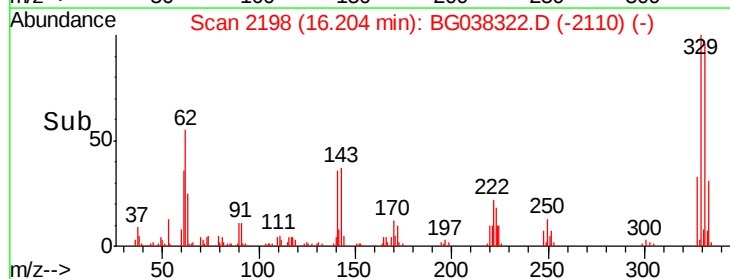
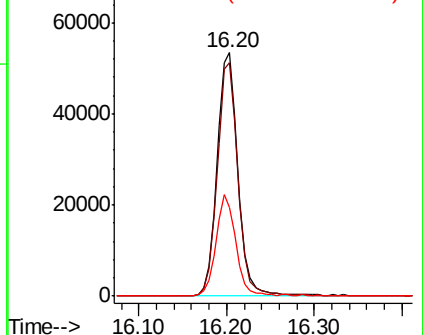




#45
 2-Fluorobiphenyl
 Concen: 72.991 ng
 RT: 13.33 min Scan# 1709
 Delta R.T. -0.02 min
 Lab File: BG038322.D
 Acq: 4 Dec 2018 5:32




Instrument :
 BNA_G
 ClientSampleId :
 JC-02-113018-C


Tgt Ion:172 Resp: 217173
 Ion Ratio Lower Upper
 172 100
 171 36.8 31.0 46.4
 170 23.6 20.2 30.2

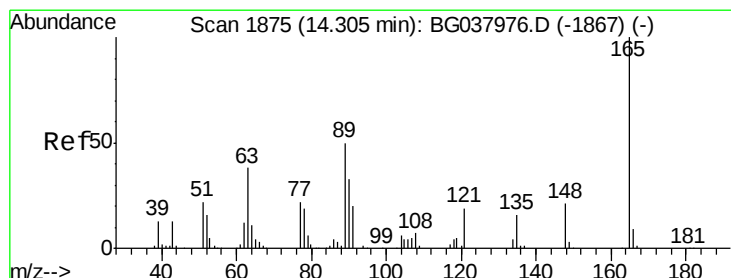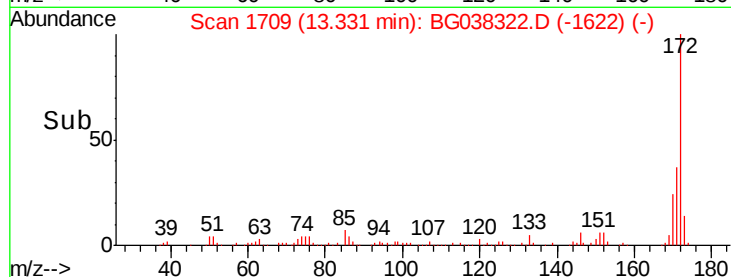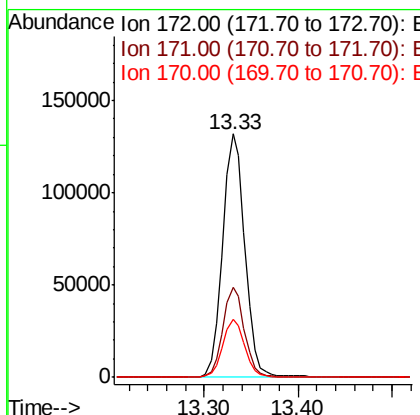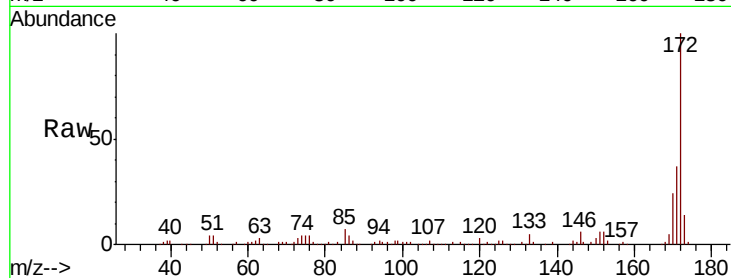

#51
 2,6-Dinitrotoluene
 Concen: 7.270 ng
 RT: 14.71 min Scan# 1944
 Delta R.T. 0.41 min
 Lab File: BG038322.D
 Acq: 4 Dec 2018 5:32

Tgt Ion:165 Resp: 5654
 Ion Ratio Lower Upper
 165 100
 63 0.0 43.4 65.2#
 89 0.0 45.8 68.6#

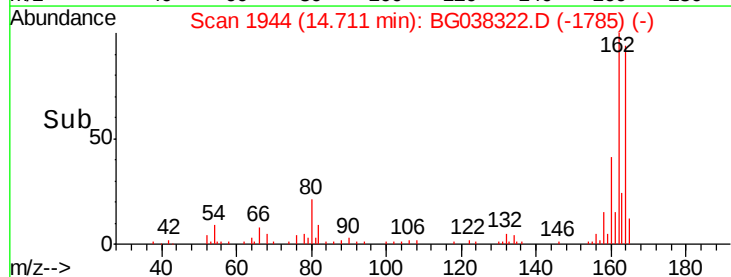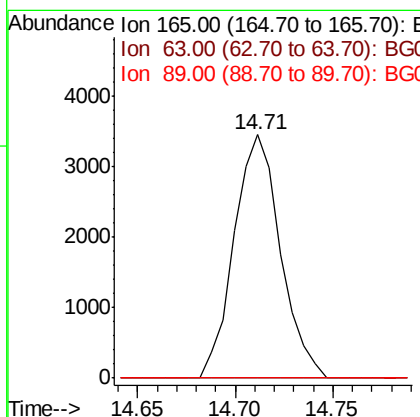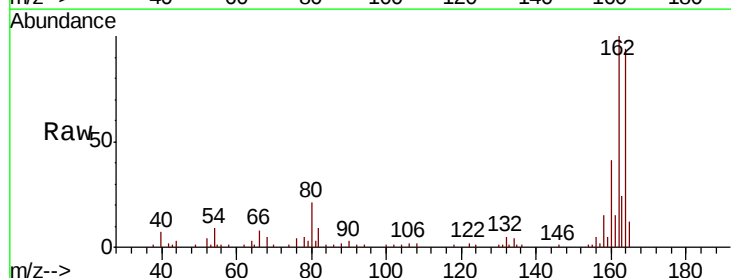


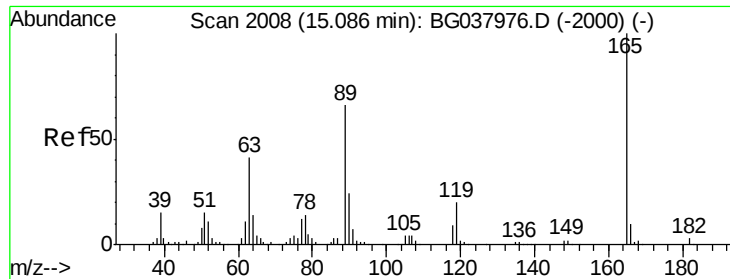

#57
 2,4-Dinitrotoluene
 Concen: 5.343 ng
 RT: 14.71 min Scan# 1944
 Delta R.T. -0.37 min
 Lab File: BG038322.D
 Acq: 4 Dec 2018 5:32

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-113018-C

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.4	50.0#
89	0.0	57.2	85.8#
182	0.0	2.6	4.0#

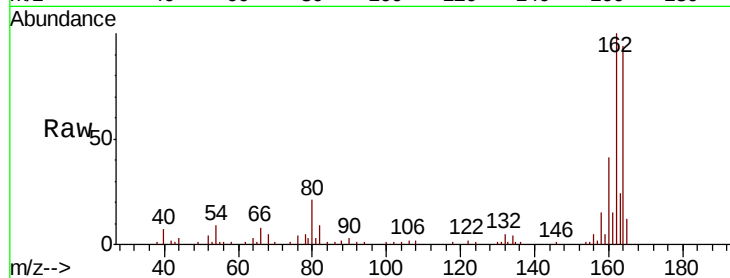




Abundance

Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

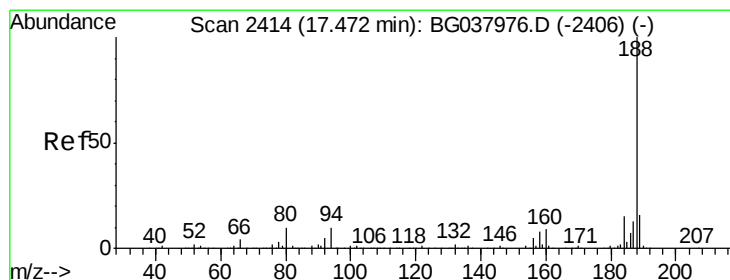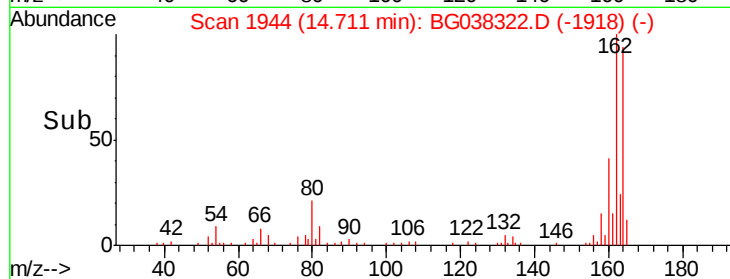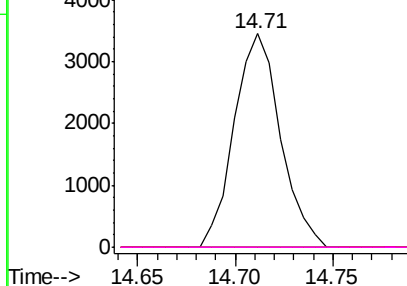

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.46 min Scan# 2412
 Delta R.T. -0.01 min
 Lab File: BG038322.D
 Acq: 4 Dec 2018 5:32




Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.3	7.2	10.8
80	9.0	7.7	11.5

Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

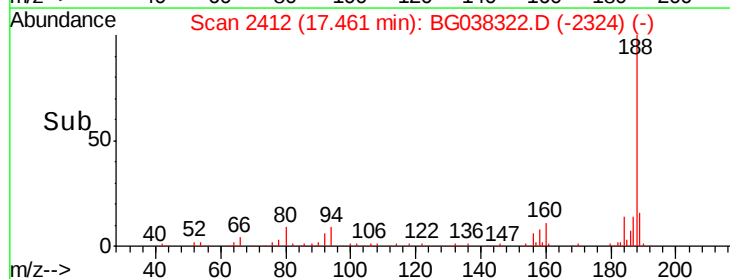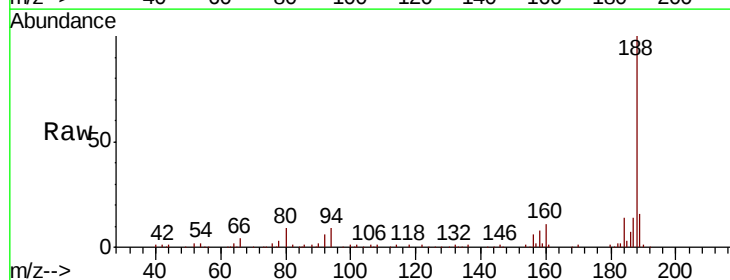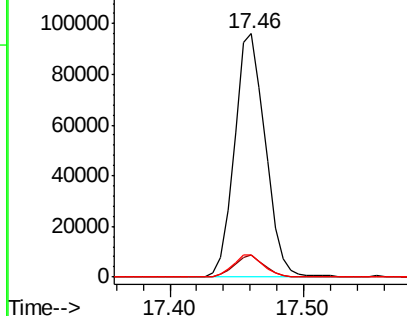







#67
4-Bromophenyl-phenylether
Concen: 3.559 ng
RT: 16.20 min Scan# 2197
Delta R.T. -0.46 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Instrument :
BNA_G
ClientSampleId :
JC-02-113018-C

Tgt Ion:248 Resp: 6013
Ion Ratio Lower Upper
248 100
250 169.2 77.0 115.6#
141 431.3 55.5 83.3#

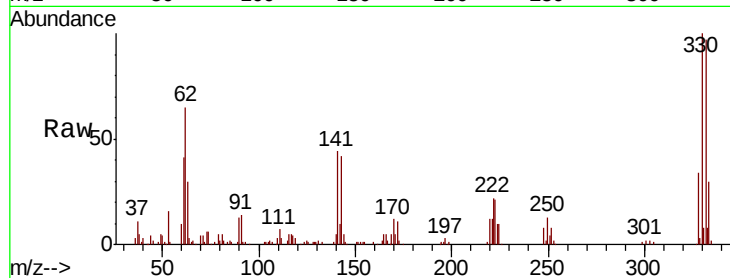


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

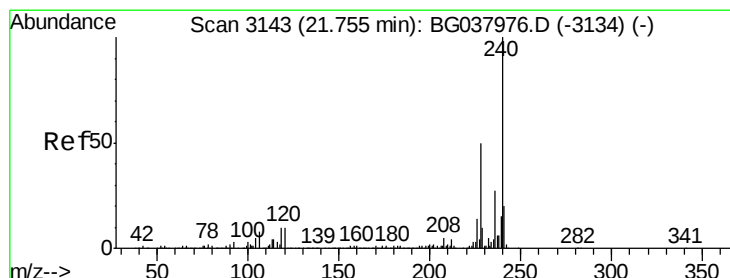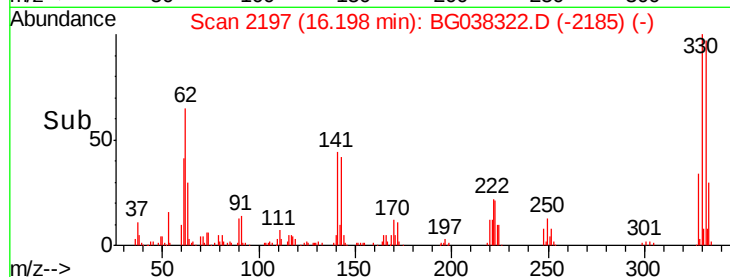
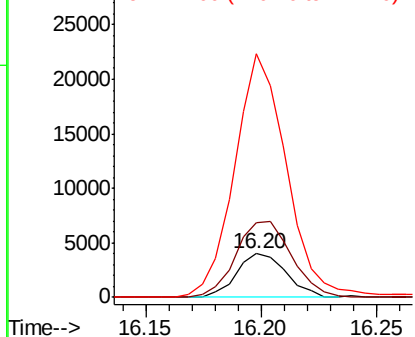



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.74 min Scan# 3141
Delta R.T. -0.01 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Tgt Ion:240 Resp: 172556
Ion Ratio Lower Upper
240 100
120 9.7 8.1 12.1
236 27.1 21.4 32.0

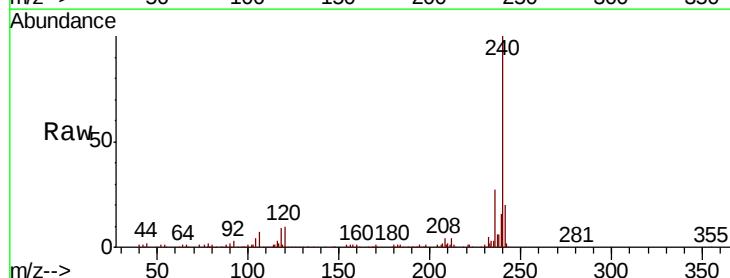

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

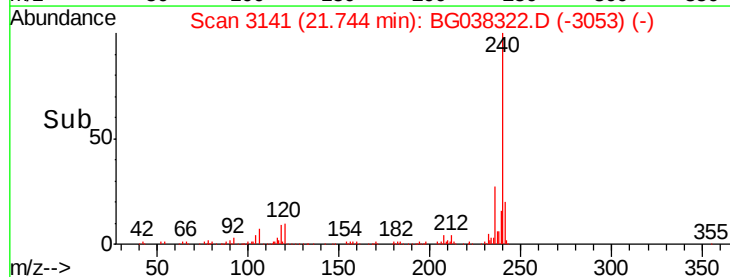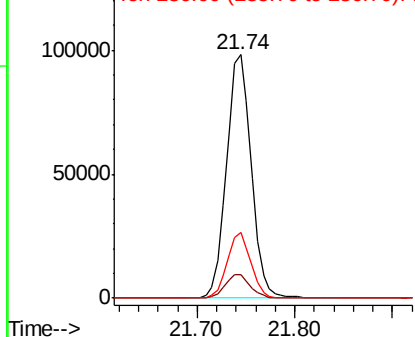

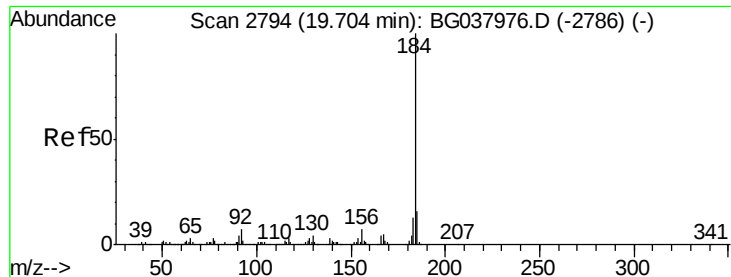

#77

Benzidine

Concen: 2.399 ng

RT: 20.06 min Scan# 2855

Delta R.T. 0.36 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32

Instrument :

BNA_G

ClientSampleId :

JC-02-113018-C


Tgt Ion:184 Resp: 14528

Ion Ratio Lower Upper

184 100

185 16.6 12.6 18.8




183 12.4 10.2 15.2

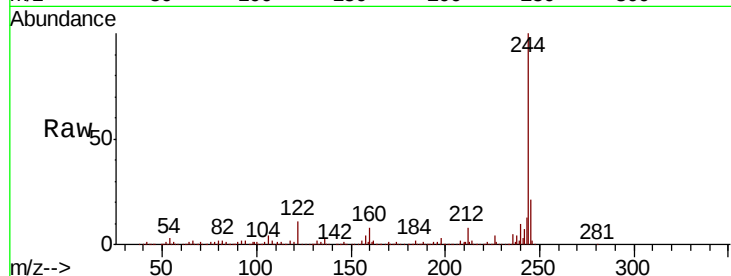

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

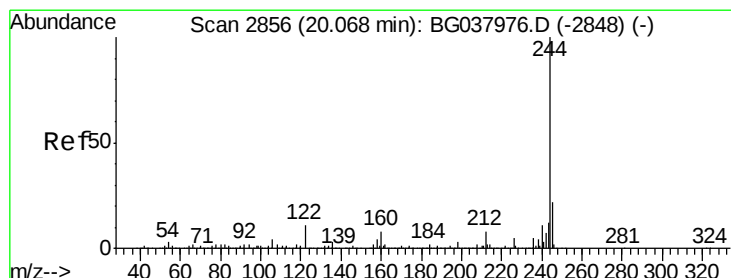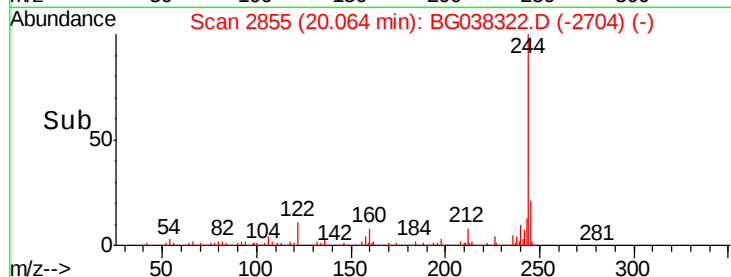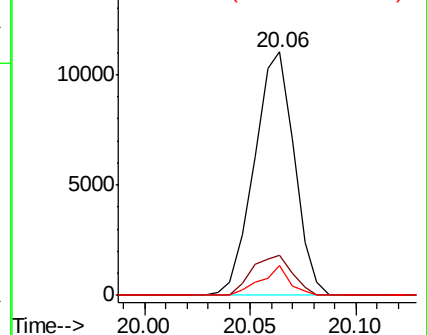

#79

Terphenyl-d14

Concen: 118.385 ng

RT: 20.06 min Scan# 2855

Delta R.T. -0.00 min

Lab File: BG038322.D

Acq: 4 Dec 2018 5:32


Tgt Ion:244 Resp: 868165

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7



122 10.8 9.0 13.4

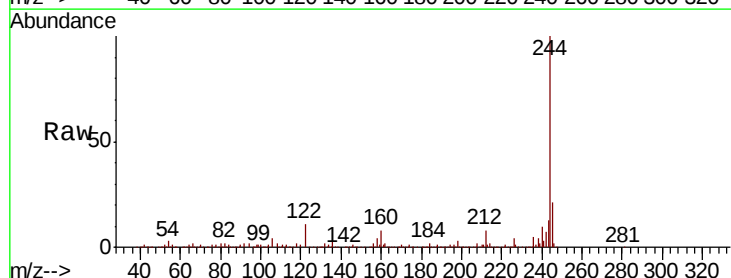


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

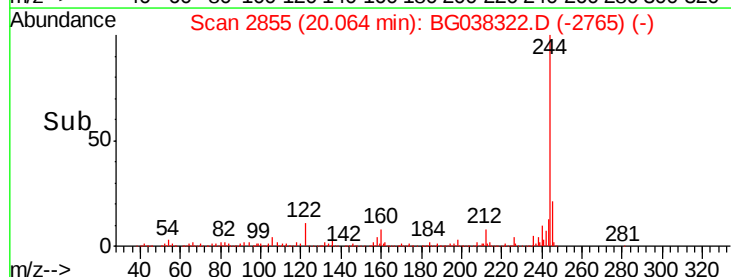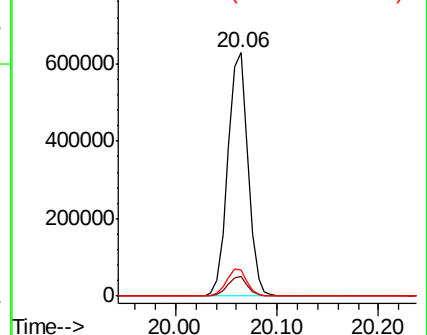

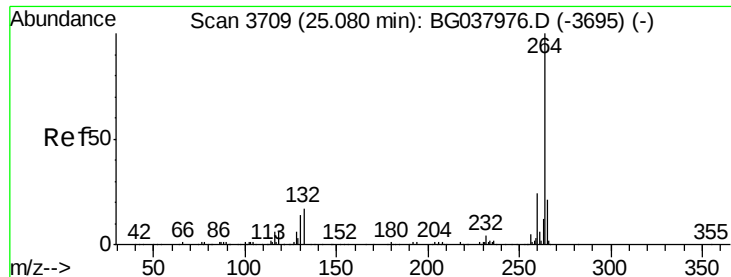

#87
Perylene-d12
Concen: 20.000 ng
RT: 25.06 min Scan# 3705
Delta R.T. -0.02 min
Lab File: BG038322.D
Acq: 4 Dec 2018 5:32

Instrument :
BNA_G
ClientSampleId :
JC-02-113018-C

Tgt Ion:	264	Resp:	176569
Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.2	27.4
265	21.3	17.9	26.9

