
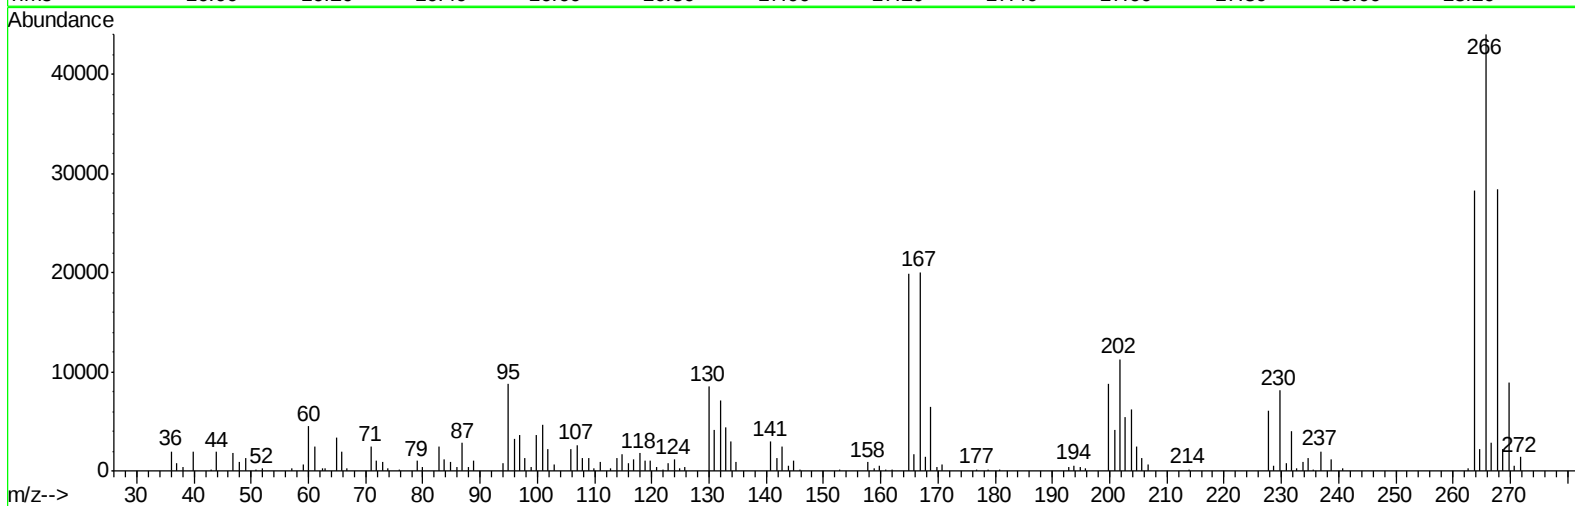


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120318\
Data File : BG038304.D
Acq On : 3 Dec 2018 17:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:20:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

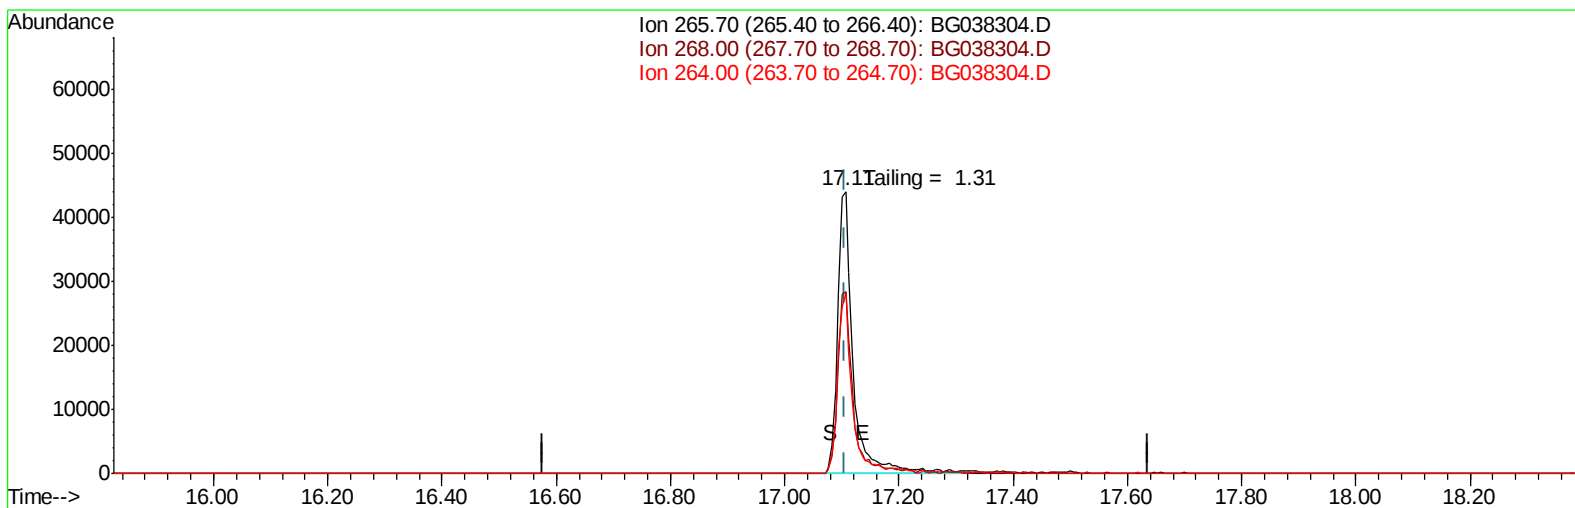

TIC: BG038304.D

(70) Pentachlorophenol (C)



17.106min (-0.001) 111710.84ng

response 80798

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.44
264.00	73.60	69.36
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120318\
Data File : BG038304.D
Acq On : 3 Dec 2018 17:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 07:20:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

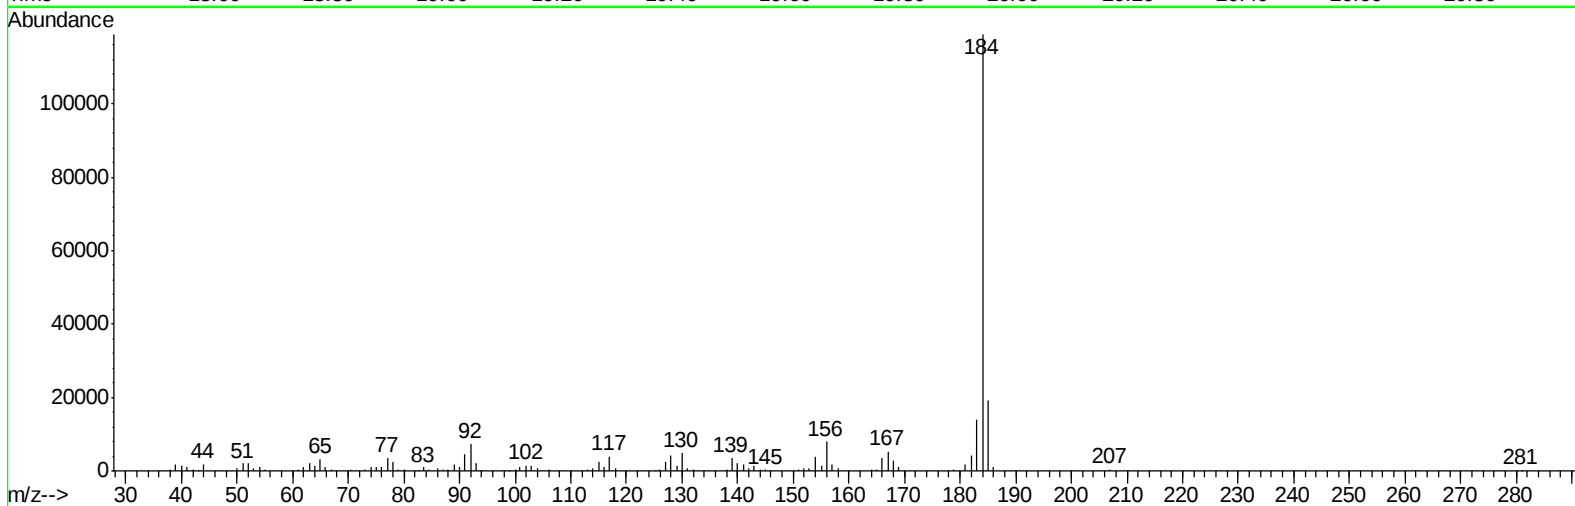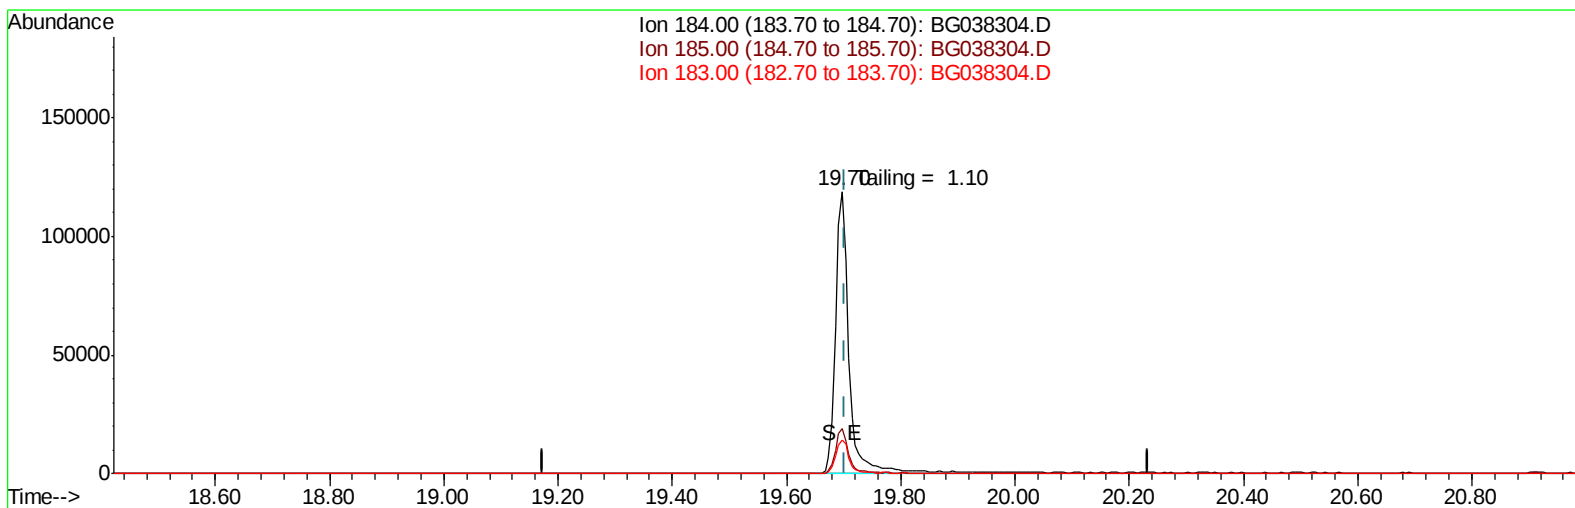

TIC: BG038304.D

(77) Benzidine

19.697min (-0.007) 11473.31ng

response 189217

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.02
183.00	12.70	11.81
0.00	0.00	0.00