


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120318\
Data File : BG038304.D
Acq On : 3 Dec 2018 17:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 13 16:39:28 2018

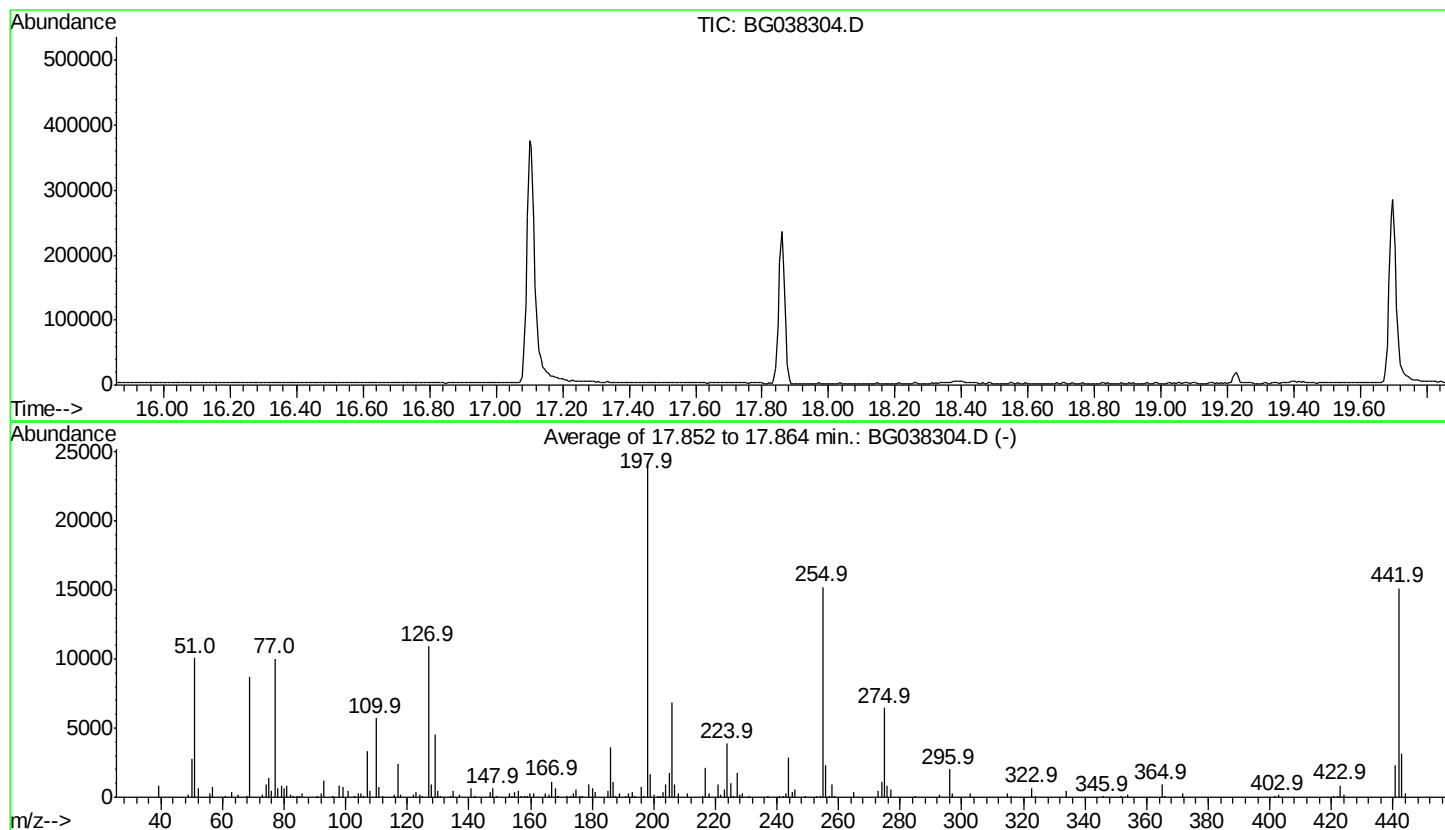

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	10076	PASS
68	69	0.00	2	0.8	71	PASS
69	198	0.00	100	36.4	8736	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	10903	PASS
197	198	0.00	2	0.4	94	PASS
198	198	100	100	100.0	24008	PASS
199	198	5	9	7.1	1712	PASS
275	198	10	60	26.9	6469	PASS
365	198	1	100	3.7	894	PASS
441	198	0.01	100	9.7	2334	PASS
442	198	50	100	63.0	15129	PASS
443	442	15	24	20.8	3140	PASS