

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120415\
 Data File : BG019921.D
 Acq On : 5 Dec 2015 1:35
 Operator : UM/NP
 Sample : G4630-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-23

Quant Time: Dec 05 04:24:08 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	29652	20.00	ng	-0.02
21) Naphthalene-d8	10.93	136	128806	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	93210	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	229289	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	278748	20.00	ng	-0.03
86) Perylene-d12	25.04	264	267496	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	114758	69.95	ng	-0.01
7) Phenol-d6	7.26	99	107878	43.55	ng	-0.01
23) Nitrobenzene-d5	9.28	82	257936	102.20	ng	-0.02
41) 2,4,6-Tribromophenol	16.23	330	211478	148.28	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	645342	94.53	ng	-0.02
78) Terphenyl-d14	20.09	244	1093217	95.66	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120415\
Data File : BG019921.D
Acq On : 5 Dec 2015 1:35
Operator : UM/NP
Sample : G4630-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-23

Quant Time: Dec 05 04:24:08 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

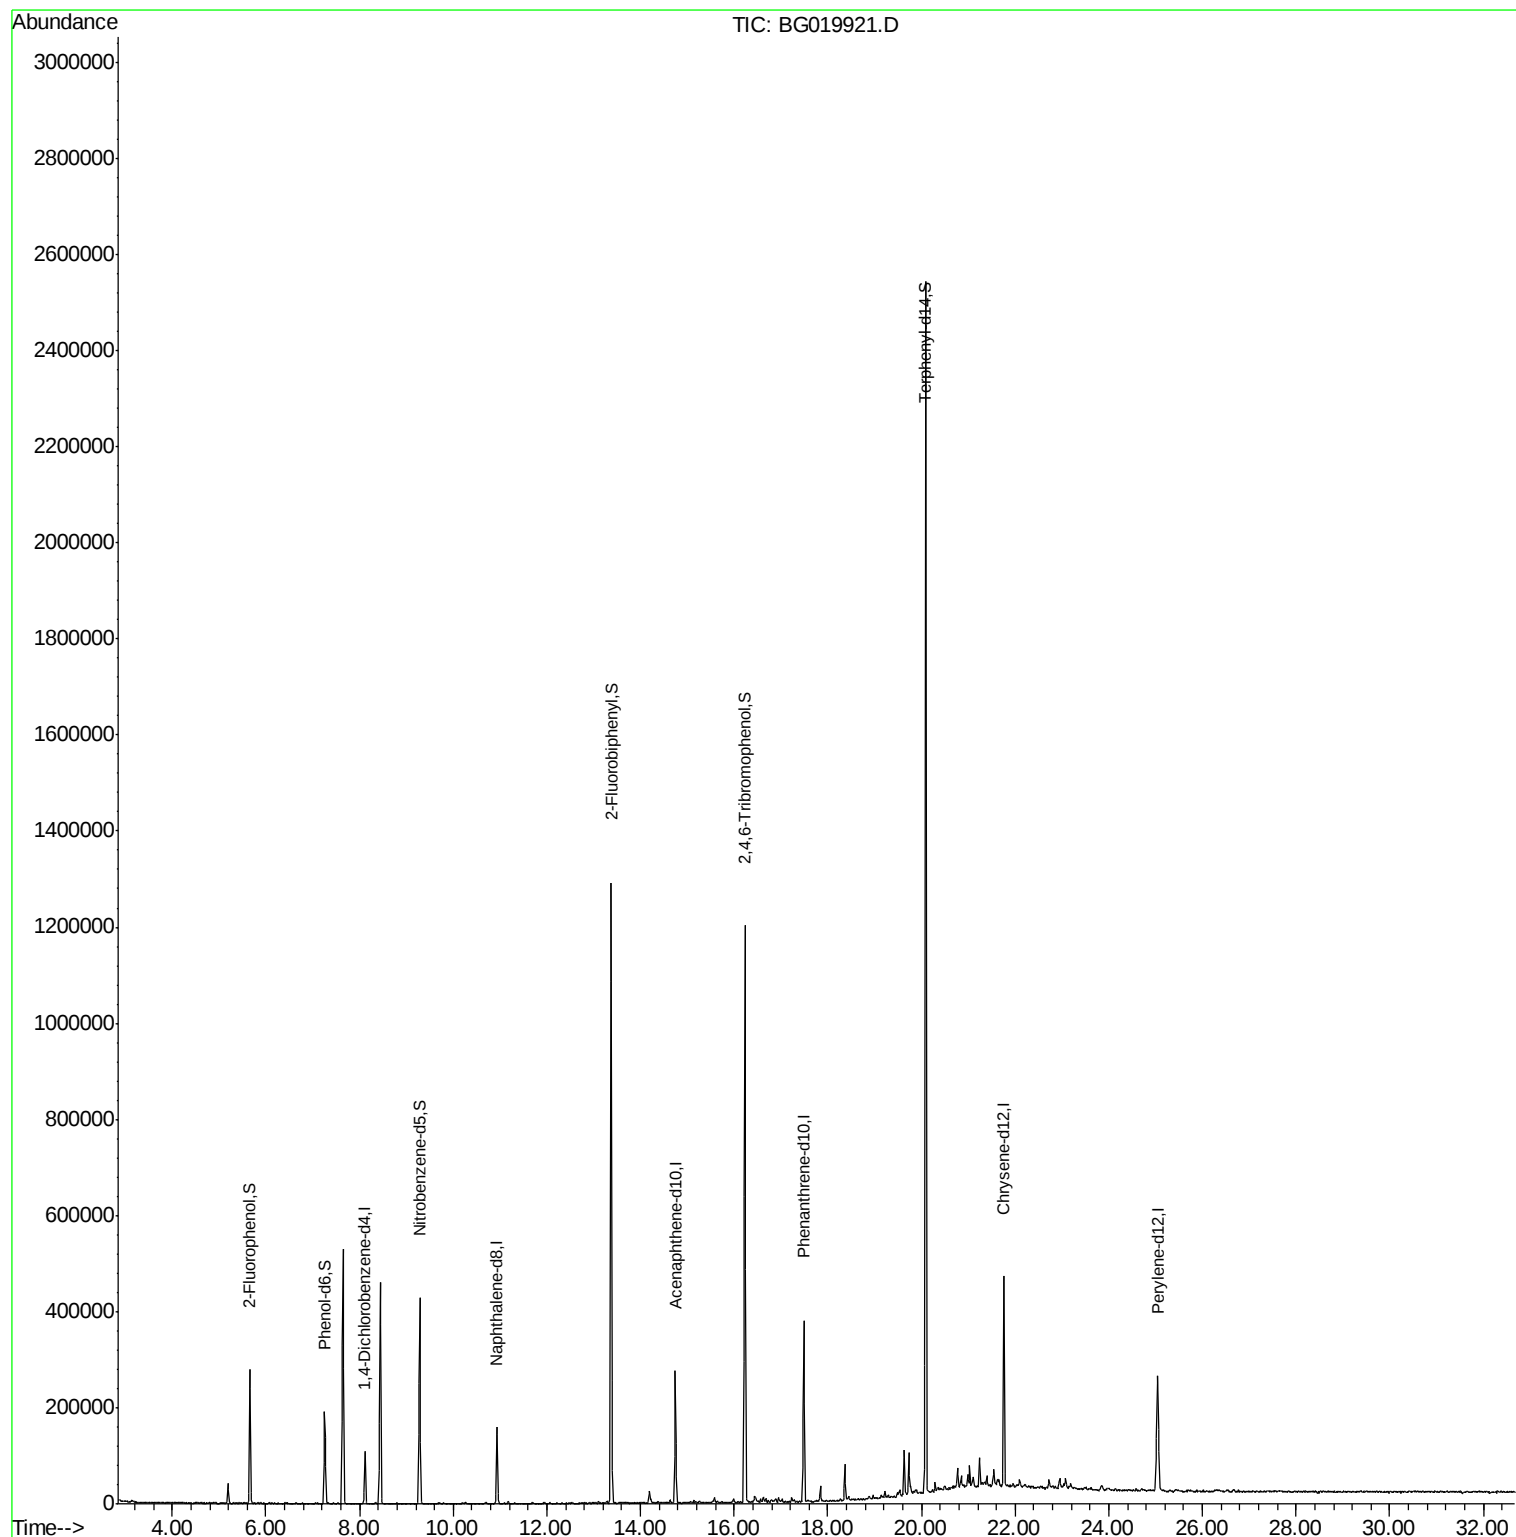

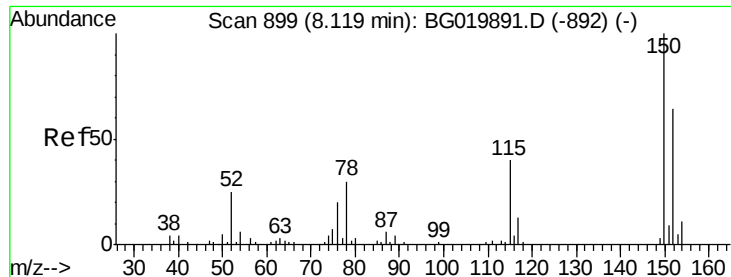

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.11 min Scan# 898

Delta R.T. -0.02 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35

Instrument :

BNA_G

ClientSampleId :

MW-23


Tgt Ion:152 Resp: 29652

Ion Ratio Lower Upper

152 100

150 148.9 115.0 172.4




115 56.2 43.9 65.9

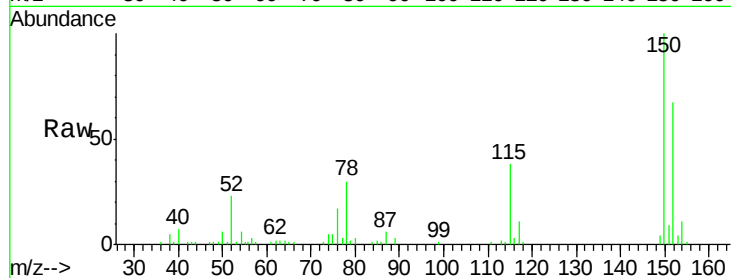

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

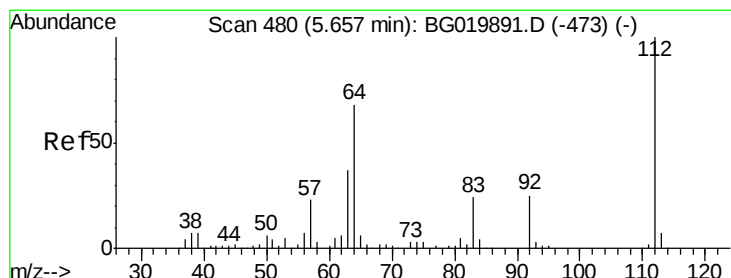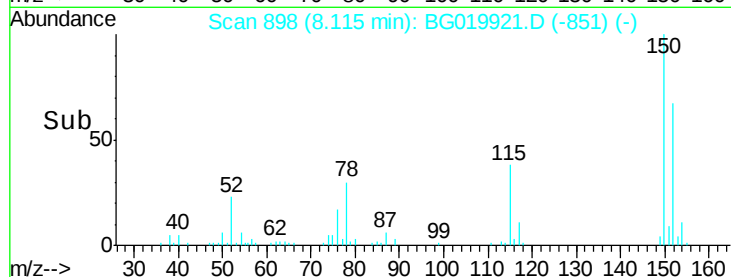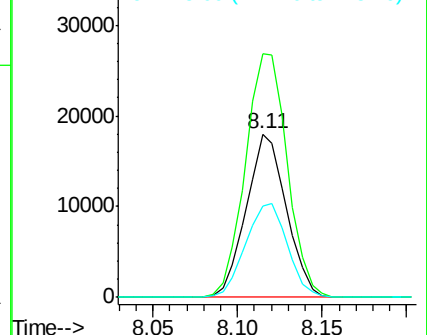

#5

2-Fluorophenol

Concen: 69.95 ng

RT: 5.66 min Scan# 480

Delta R.T. -0.01 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35


Tgt Ion:112 Resp: 114758

Ion Ratio Lower Upper

112 100

64 67.6 43.7 65.5#



63 36.9 24.0 36.0#

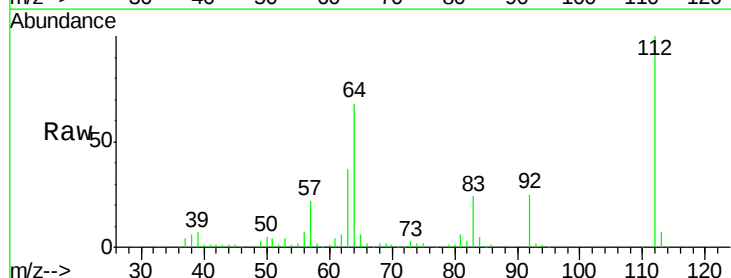


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

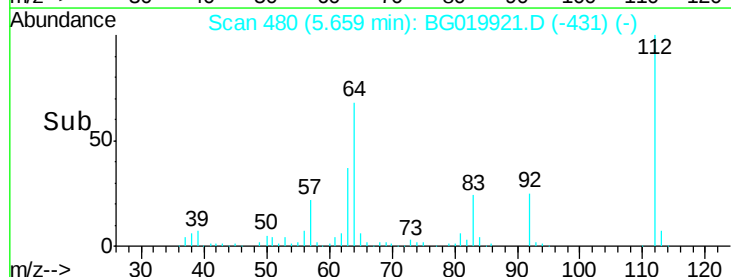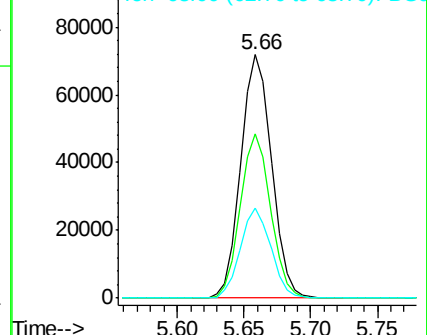

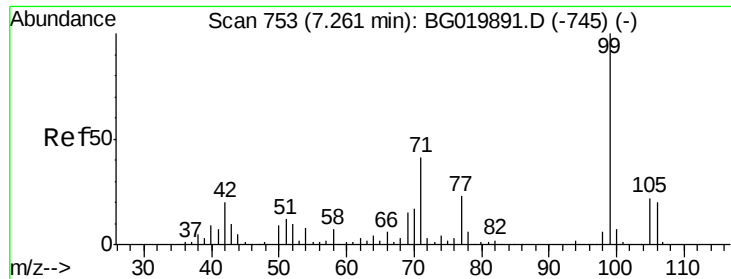

#7

Phenol-d6

Concen: 43.55 ng

RT: 7.26 min Scan# 753

Delta R.T. -0.01 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35

Instrument :

BNA_G

ClientSampleId :

MW-23


Tgt Ion: 99 Resp: 107878

Ion Ratio Lower Upper




99 100

42 20.7 11.5 17.3#

71 39.7 22.6 34.0#

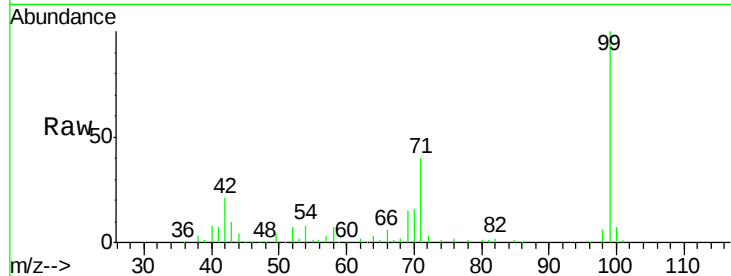

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

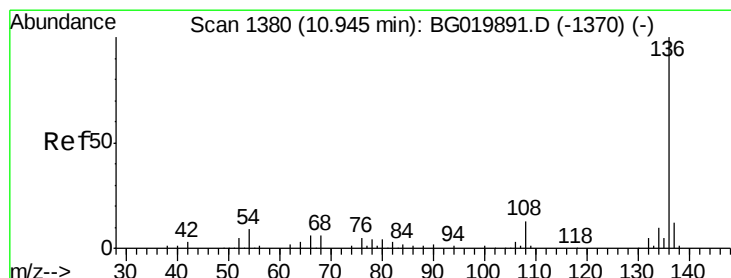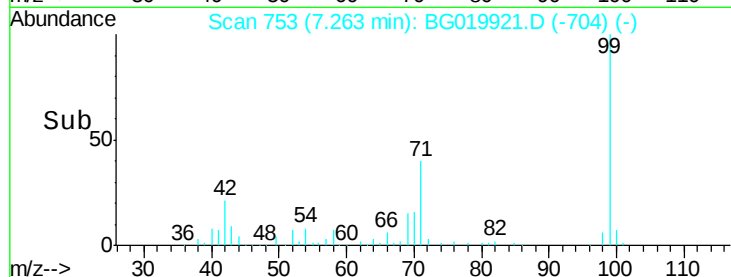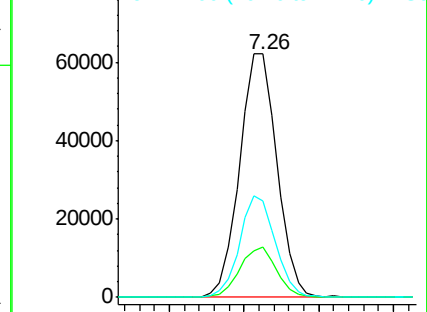

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1378

Delta R.T. -0.02 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35

Tgt Ion: 136 Resp: 128806


Ion Ratio Lower Upper

136 100



137 11.7 8.6 12.8


54 8.5 5.4 8.2#

68 6.3 5.3 7.9

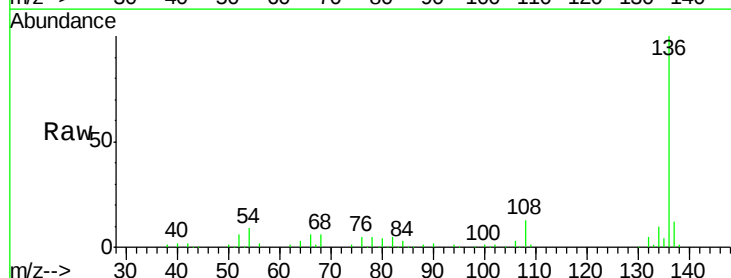

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

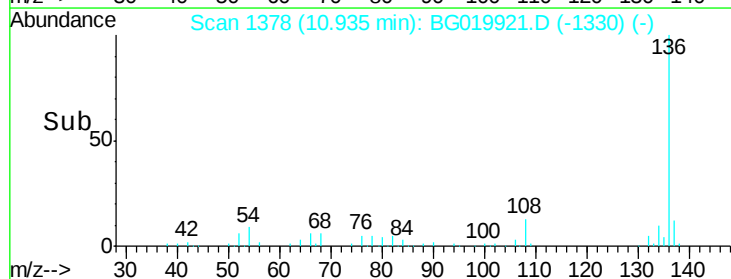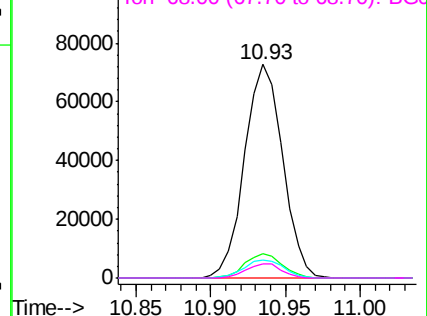


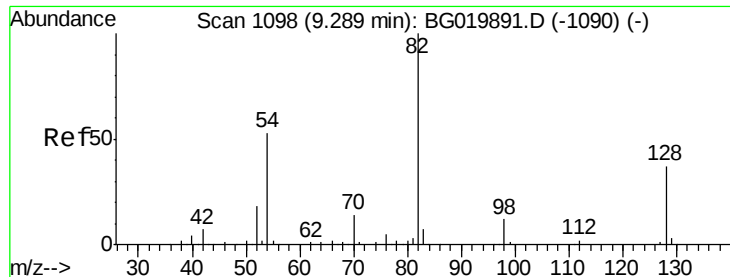




#23
 Nitrobenzene-d5
 Concen: 102.20 ng
 RT: 9.28 min Scan# 1097
 Delta R.T. -0.02 min
 Lab File: BG019921.D
 Acq: 5 Dec 2015 1:35

Instrument :
 BNA_G
 ClientSampled :
 MW-23

Tgt Ion	Ratio	Lower	Upper
82	100		
128	40.5	36.7	55.1
54	50.7	33.8	50.8

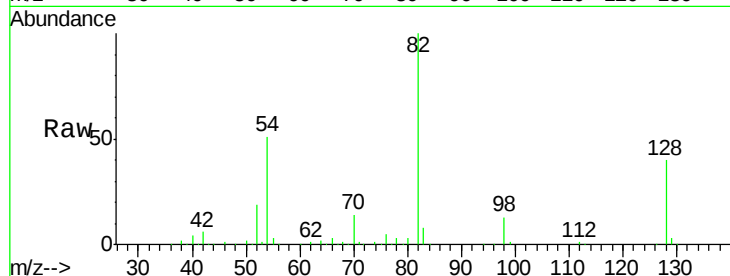


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

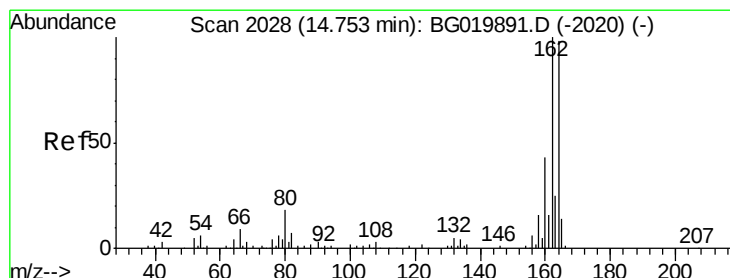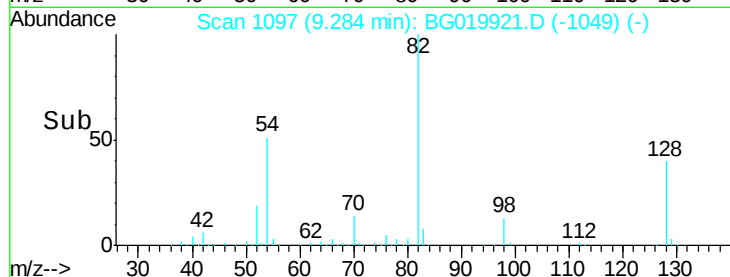
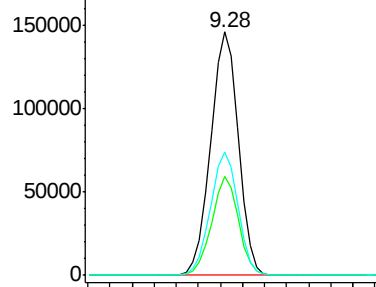



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.74 min Scan# 2026
 Delta R.T. -0.02 min
 Lab File: BG019921.D
 Acq: 5 Dec 2015 1:35

Tgt Ion	Ratio	Lower	Upper
164	100		
162	100.4	78.8	118.2
160	43.1	36.4	54.6

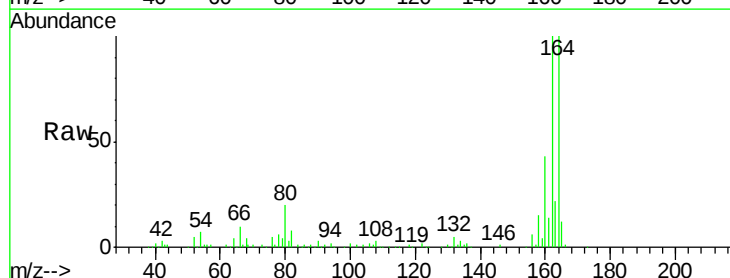

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



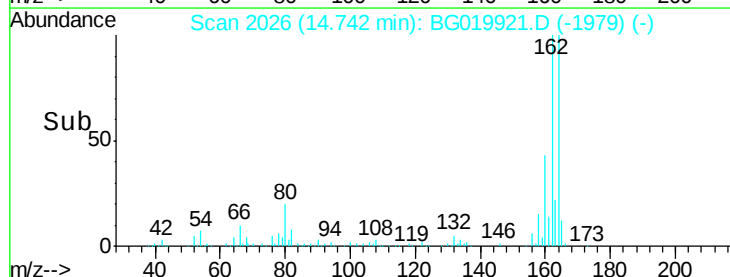
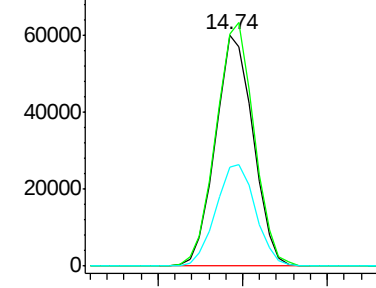


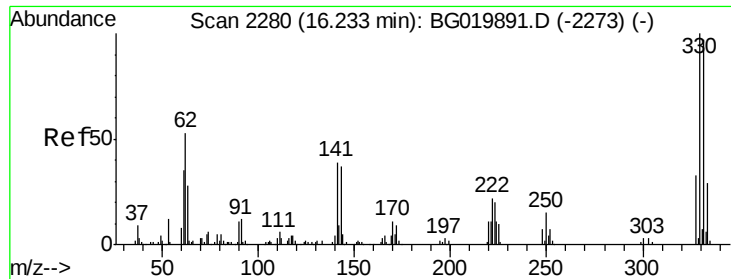

#41
 2,4,6-Tribromophenol
 Concen: 148.28 ng
 RT: 16.23 min Scan# 2279
 Delta R.T. -0.02 min
 Lab File: BG019921.D
 Acq: 5 Dec 2015 1:35




Instrument :
 BNA_G
 ClientSampleId :
 MW-23


Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.6	78.1	117.1
141	37.4	28.2	42.2

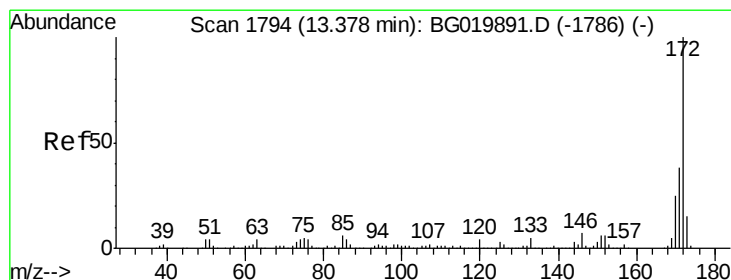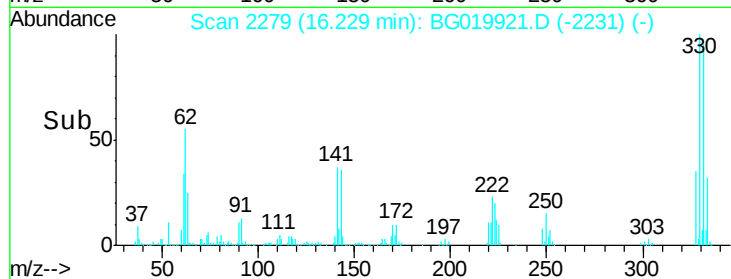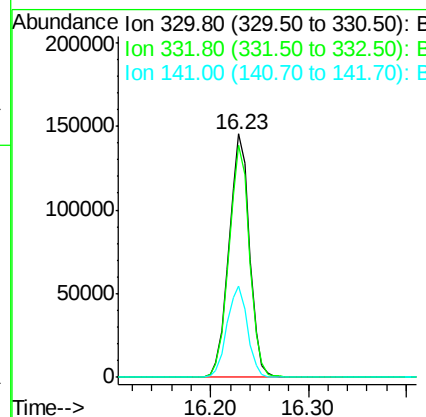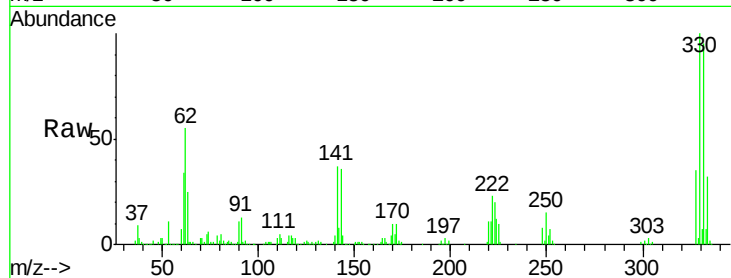

#44
 2-Fluorobiphenyl
 Concen: 94.53 ng
 RT: 13.37 min Scan# 1793
 Delta R.T. -0.02 min
 Lab File: BG019921.D
 Acq: 5 Dec 2015 1:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	29.0	43.6
170	25.1	19.9	29.9

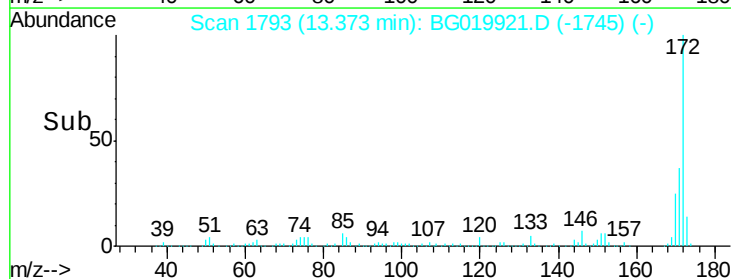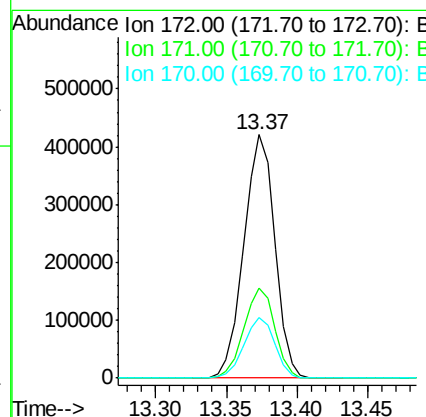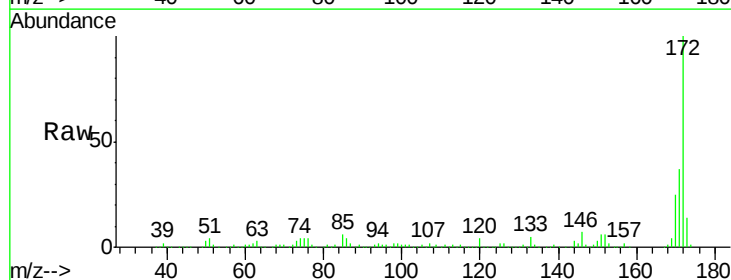


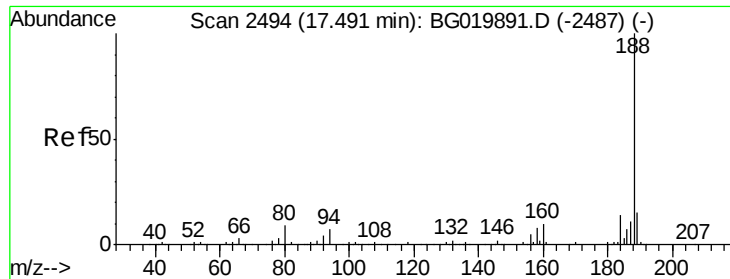




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2493
Delta R.T. -0.02 min
Lab File: BG019921.D
Acq: 5 Dec 2015 1:35

Instrument :
BNA_G
ClientSampleId :
MW-23

Tgt Ion:188 Resp: 229289
Ion Ratio Lower Upper
188 100
94 7.5 7.7 11.5#
80 8.8 7.8 11.8

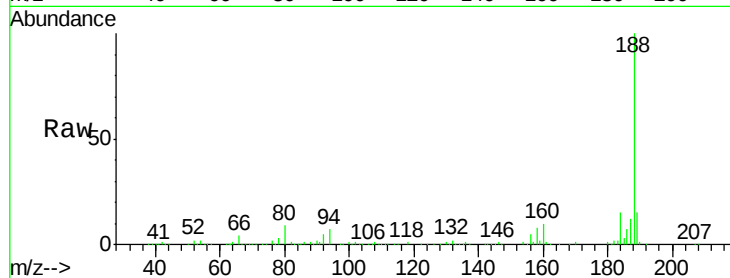


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

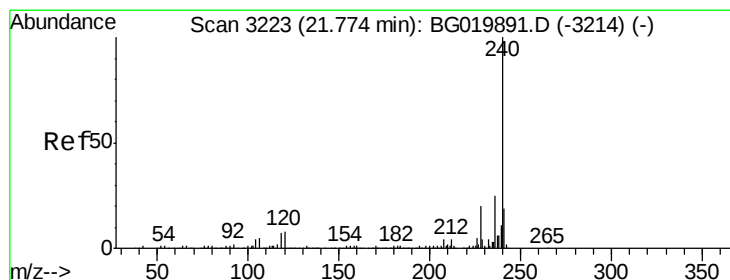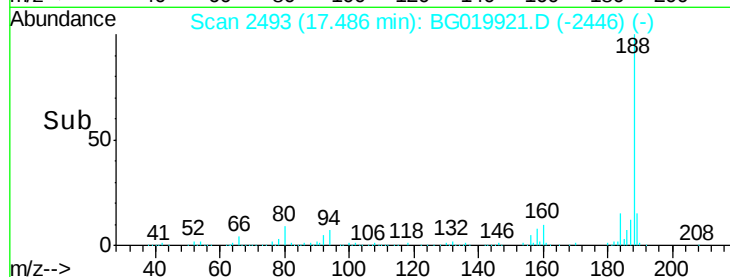
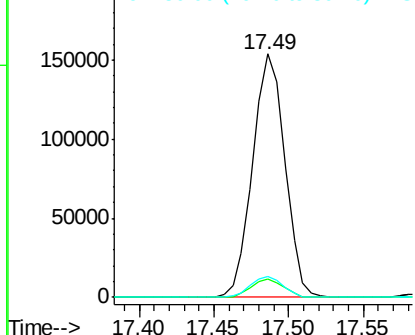



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.76 min Scan# 3220
Delta R.T. -0.03 min
Lab File: BG019921.D
Acq: 5 Dec 2015 1:35

Tgt Ion:240 Resp: 278748
Ion Ratio Lower Upper
240 100
120 7.8 7.4 11.0
236 24.9 20.7 31.1

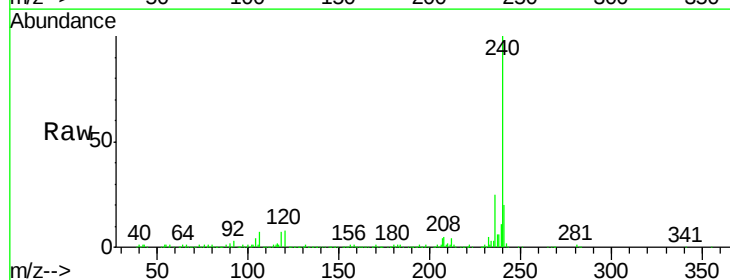

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

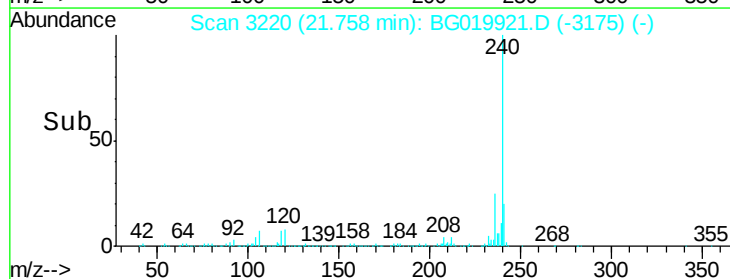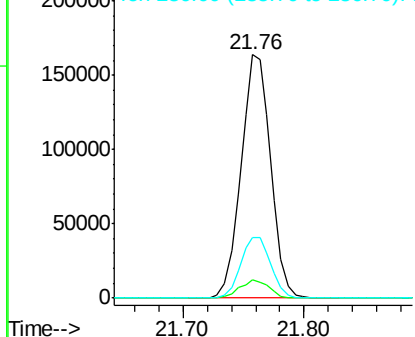

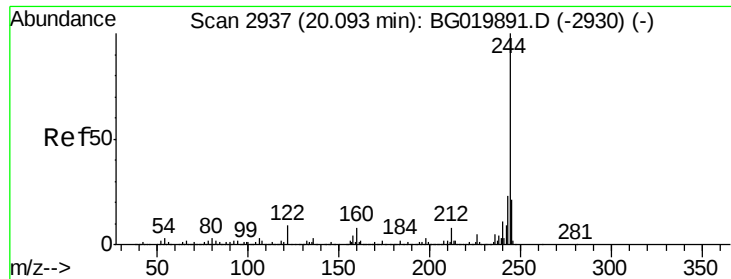

#78

Terphenyl-d14

Concen: 95.66 ng

RT: 20.09 min Scan# 2936

Delta R.T. -0.02 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35

Instrument :

BNA_G

ClientSampleId :

MW-23


Tgt Ion:244 Resp: 1093217

Ion Ratio Lower Upper

244 100

212 8.8 6.9 10.3




122 9.1 10.2 15.2#

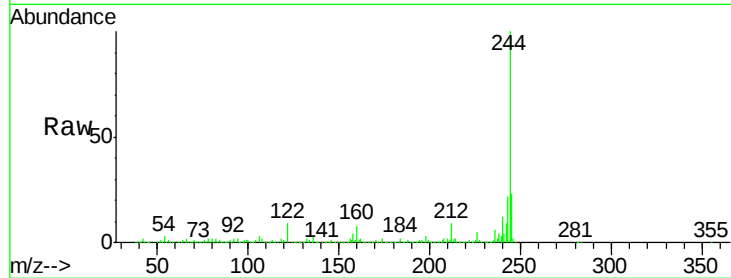

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

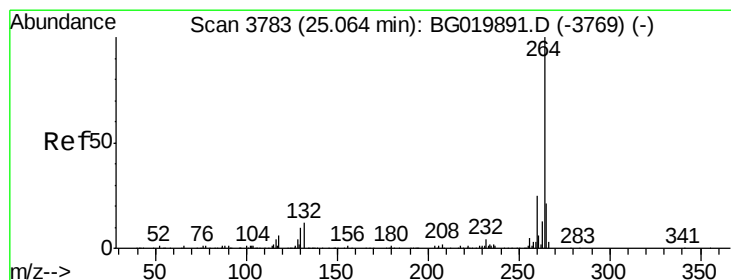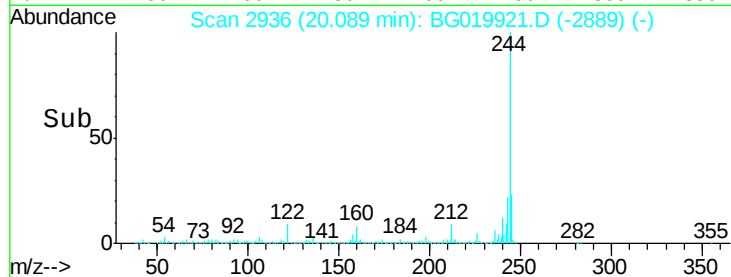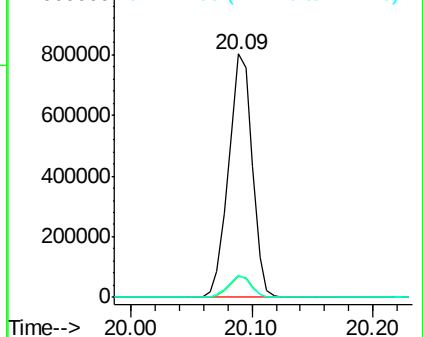

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.04 min Scan# 3779

Delta R.T. -0.05 min

Lab File: BG019921.D

Acq: 5 Dec 2015 1:35


Tgt Ion:264 Resp: 267496

Ion Ratio Lower Upper

264 100

260 23.1 18.5 27.7

265 21.6 17.2 25.8

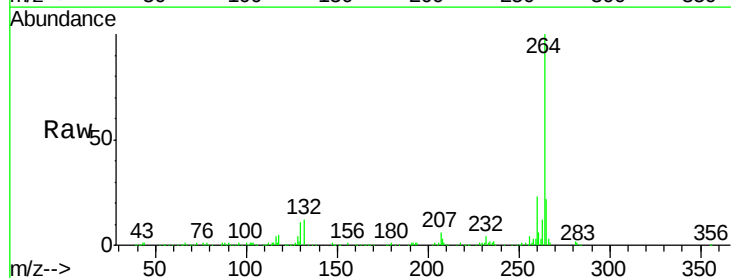

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

