

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120415\
 Data File : BG019933.D
 Acq On : 5 Dec 2015 9:18
 Operator : UM/NP
 Sample : PB87030BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB87030BL

Quant Time: Dec 07 04:06:42 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	32348	20.00	ng	-0.02
21) Naphthalene-d8	10.93	136	133992	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	97337	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	249812	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	314021	20.00	ng	-0.04
86) Perylene-d12	25.04	264	288428	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	214287	119.73	ng	-0.01
7) Phenol-d6	7.26	99	307928	113.95	ng	-0.01
23) Nitrobenzene-d5	9.28	82	199555	76.01	ng	-0.02
41) 2,4,6-Tribromophenol	16.23	330	152066	102.10	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	494800	69.41	ng	-0.02
78) Terphenyl-d14	20.09	244	900400	69.94	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120415\
Data File : BG019933.D
Acq On : 5 Dec 2015 9:18
Operator : UM/NP
Sample : PB87030BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB87030BL

Quant Time: Dec 07 04:06:42 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

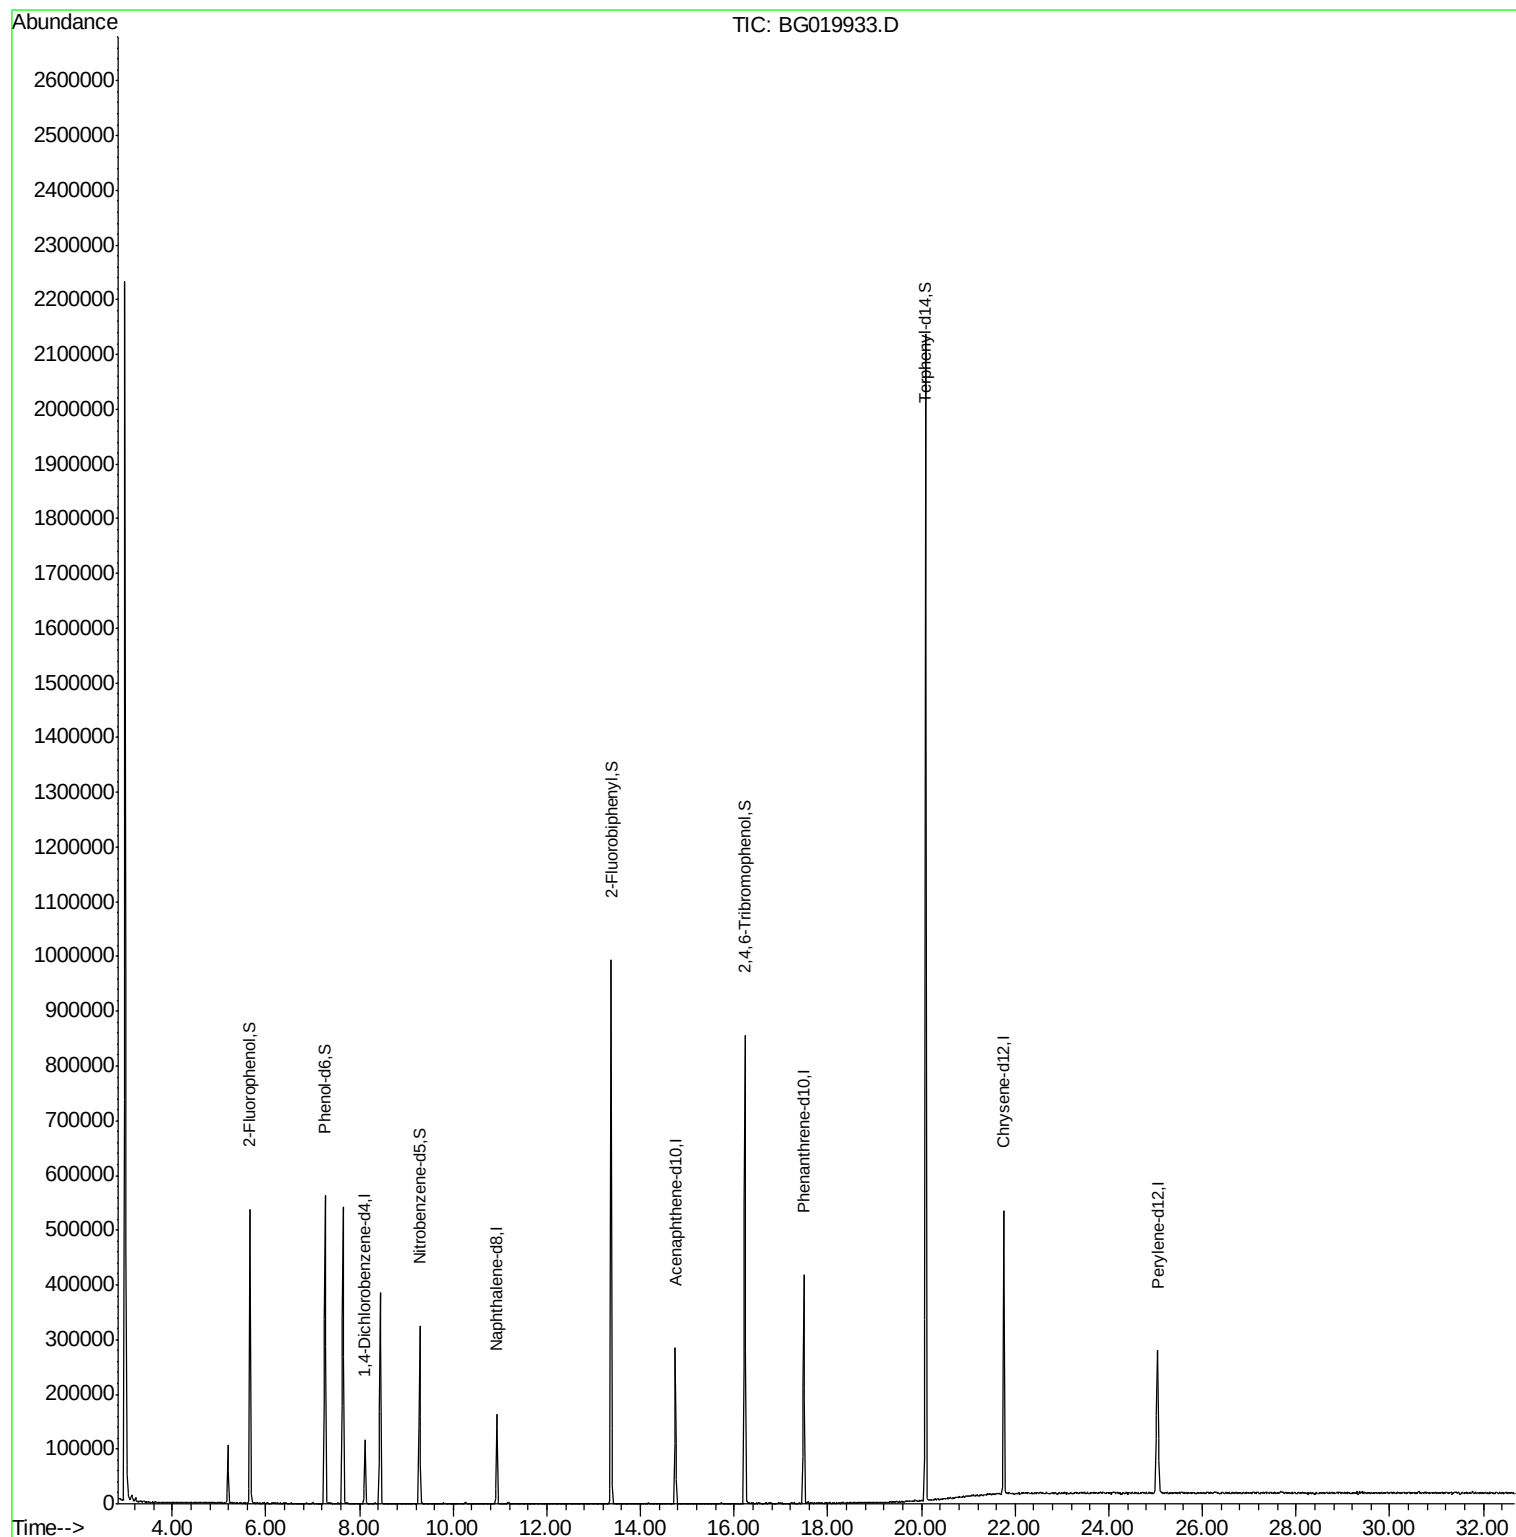

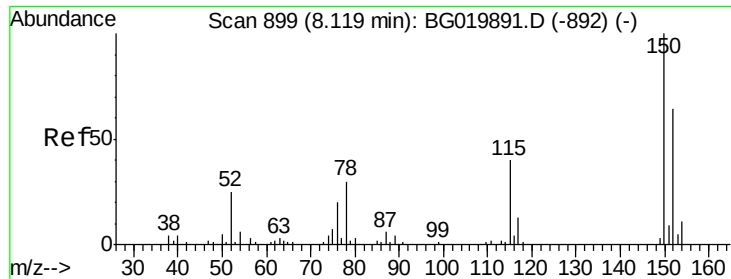


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.11 min Scan# 898
Delta R.T. -0.02 min
Lab File: BG019933.D
Acq: 5 Dec 2015 9:18

Instrument :
BNA_G
ClientSampleId :
PB87030BL

Tot Ion:152 Resp: 32348
Ion Ratio Lower Upper
152 100
150 159.3 115.0 172.4
115 65.1 43.9 65.9

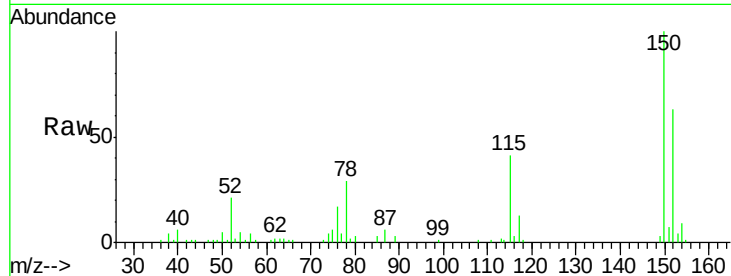


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

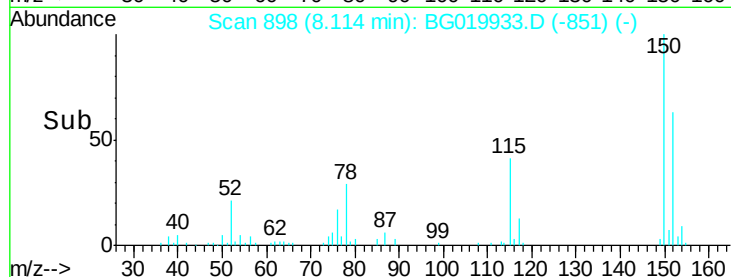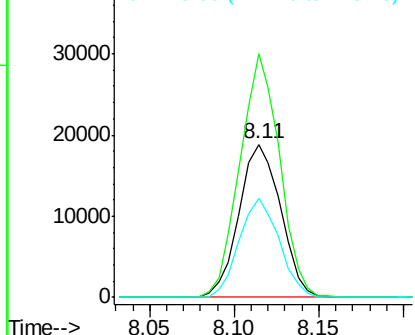



#5


2-Fluorophenol
Concen: 119.73 ng
RT: 5.66 min Scan# 480
Delta R.T. -0.01 min
Lab File: BG019933.D
Acq: 5 Dec 2015 9:18

Tgt Ion:112 Resp: 214287
Ion Ratio Lower Upper
112 100
64 66.1 43.7 65.5#
63 37.8 24.0 36.0#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

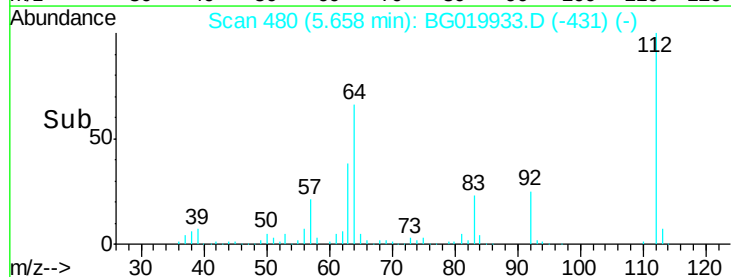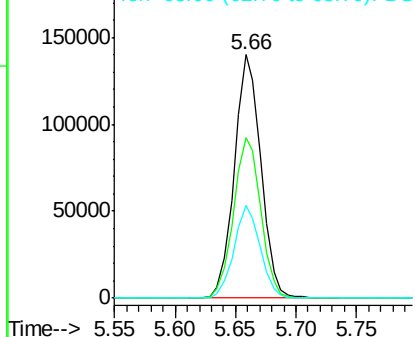

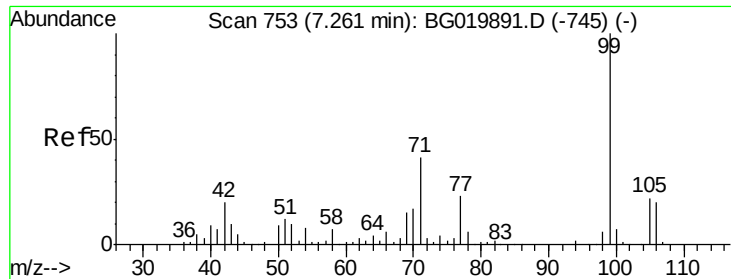

#7

Phenol-d6

Concen: 113.95 ng

RT: 7.26 min Scan# 753

Delta R.T. -0.01 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18

Instrument :

BNA_G

ClientSampleId :

PB87030BL


Tot Ion: 99 Resp: 307928

Ion Ratio Lower Upper

99 100

42 20.1 11.5 17.3#

71 40.0 22.6 34.0#



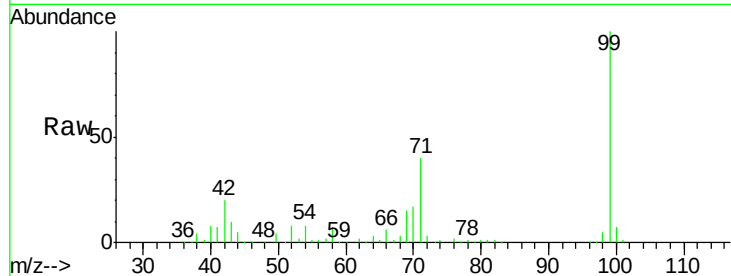


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

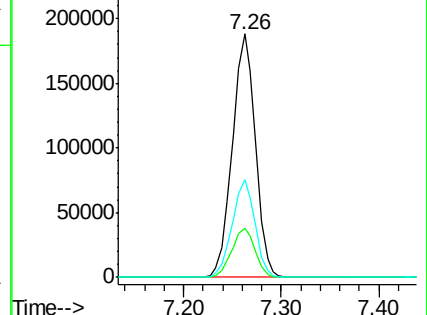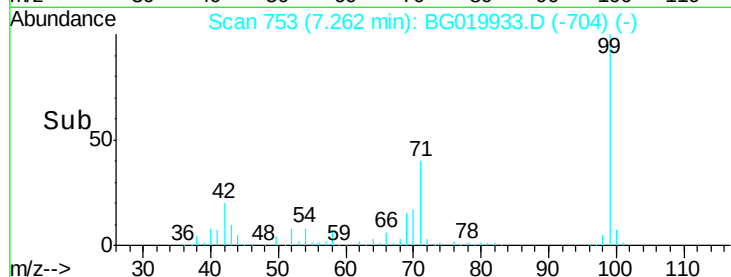

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1378

Delta R.T. -0.02 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18

Tgt Ion: 136 Resp: 133992


Ion Ratio Lower Upper

136 100

137 11.3 8.6 12.8

54 7.6 5.4 8.2

68 6.1 5.3 7.9





Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

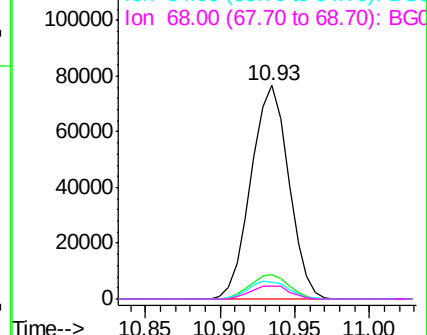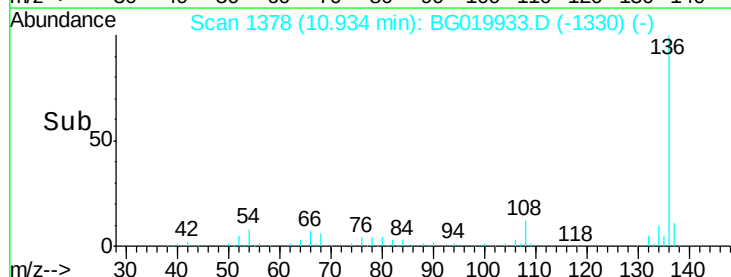


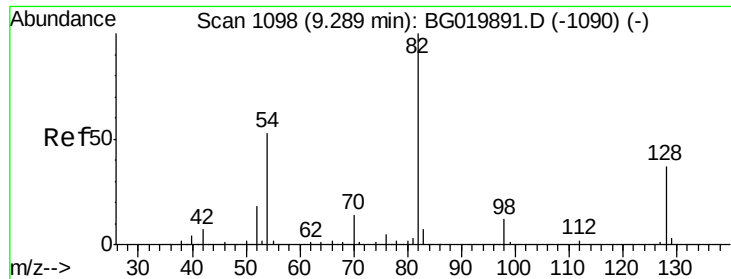




#23
Nitrobenzene-d5
Concen: 76.01 ng
RT: 9.28 min Scan# 1097
Delta R.T. -0.02 min
Lab File: BG019933.D
Acq: 5 Dec 2015 9:18

Instrument :
BNA_G
ClientSampleId :
PB87030BL

Tot Ion	82	Resp	199555
Ion Ratio	100	Lower	Upper
128	37.5	36.7	55.1
54	49.4	33.8	50.8

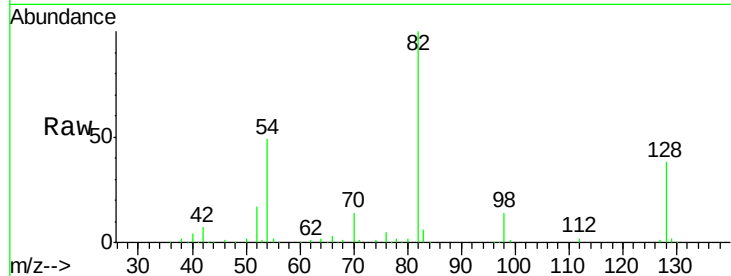


Abundance Ion 82.00 (81.70 to 82.70): BG019891.D (-1090) (-)

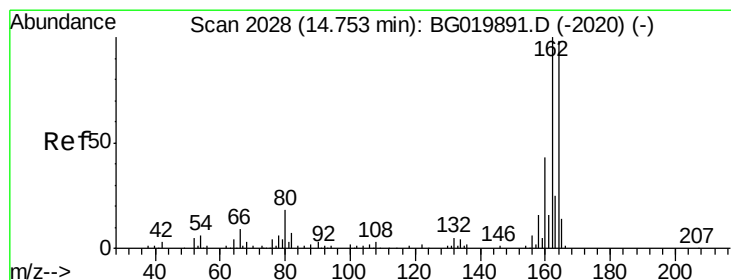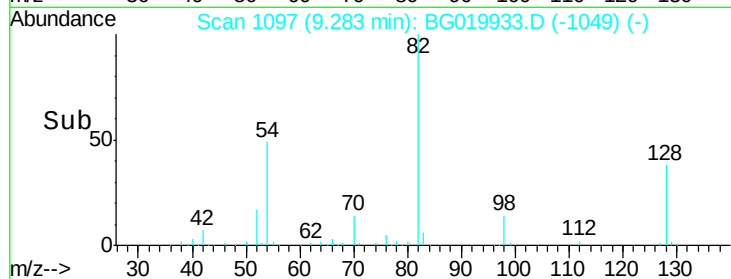
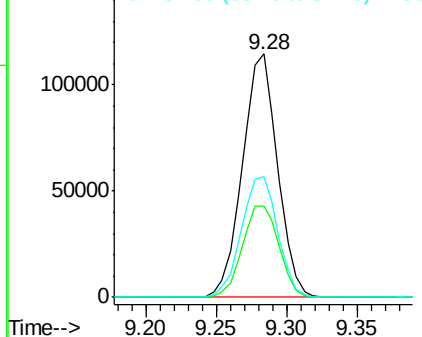



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 2026
Delta R.T. -0.02 min
Lab File: BG019933.D
Acq: 5 Dec 2015 9:18

Tgt Ion	164	Resp	97337
Ion Ratio	100	Lower	Upper
162	104.8	78.8	118.2
160	46.0	36.4	54.6



Abundance Ion 164.00 (163.70 to 164.70): BG019891.D (-2020) (-)

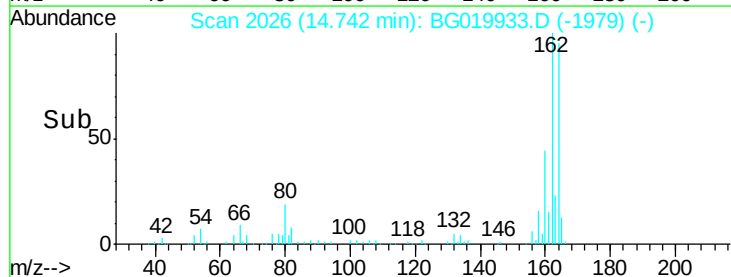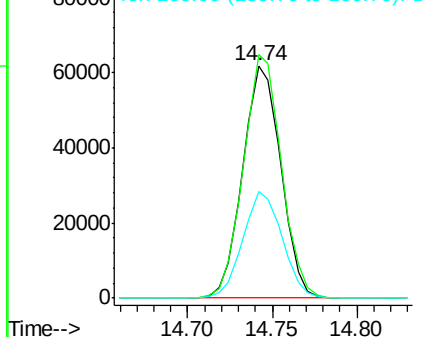


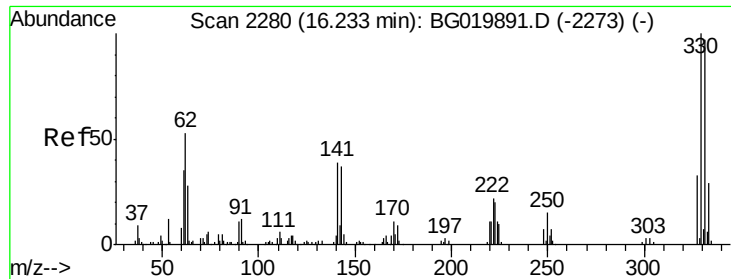




#41
 2,4,6-Tribromophenol
 Concen: 102.10 ng
 RT: 16.23 min Scan# 2279
 Delta R.T. -0.02 min
 Lab File: BG019933.D
 Acq: 5 Dec 2015 9:18

Instrument :
 BNA_G
 ClientSampleId :
 PB87030BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.0	78.1	117.1
141	39.1	28.2	42.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

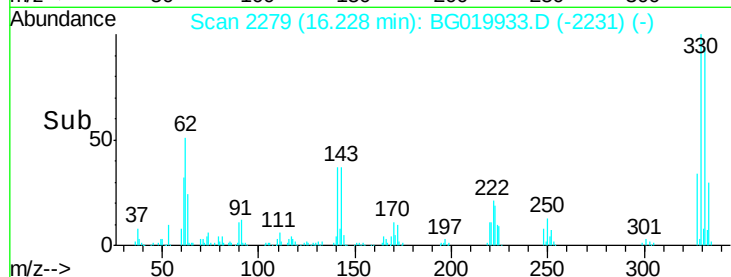
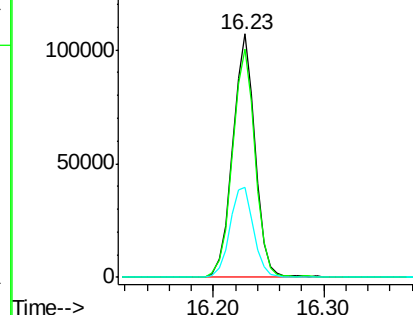



#44
 2-Fluorobiphenyl
 Concen: 69.41 ng
 RT: 13.37 min Scan# 1793
 Delta R.T. -0.02 min
 Lab File: BG019933.D
 Acq: 5 Dec 2015 9:18

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	29.0	43.6
170	24.7	19.9	29.9



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

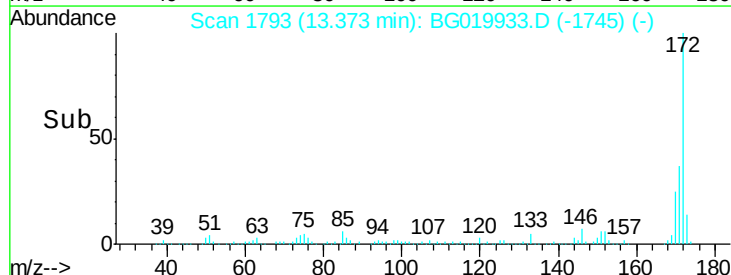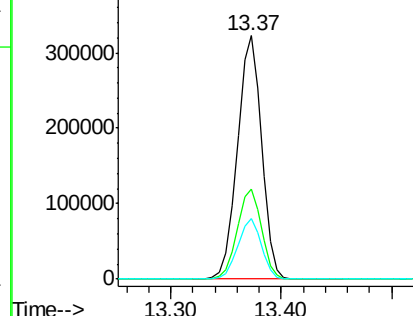

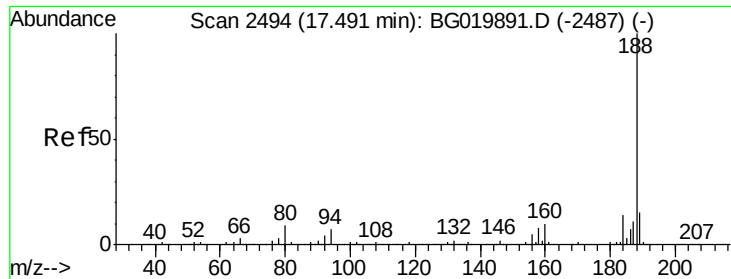

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.49 min Scan# 2493

Delta R.T. -0.02 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18

Instrument :

BNA_G

ClientSampleId :

PB87030BL


Tot Ion:188 Resp: 249812

Ion Ratio Lower Upper

188 100

94 7.3 7.7 11.5#




80 8.3 7.8 11.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

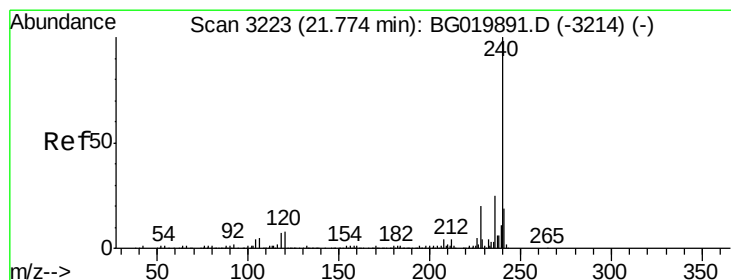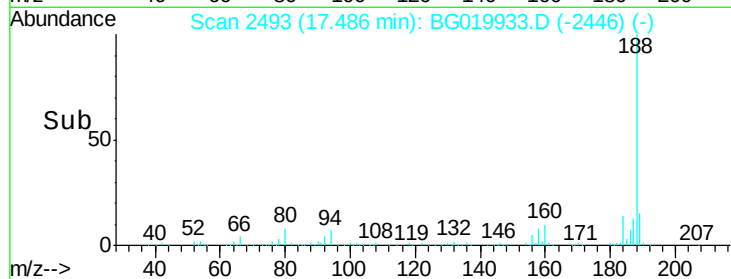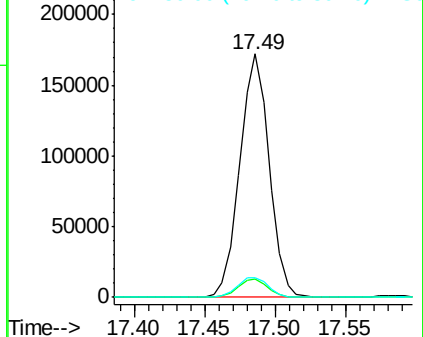

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.76 min Scan# 3220

Delta R.T. -0.04 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18


Tgt Ion:240 Resp: 314021

Ion Ratio Lower Upper

240 100

120 7.5 7.4 11.0



236 25.5 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

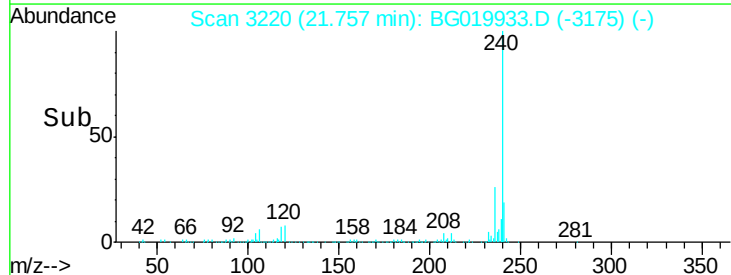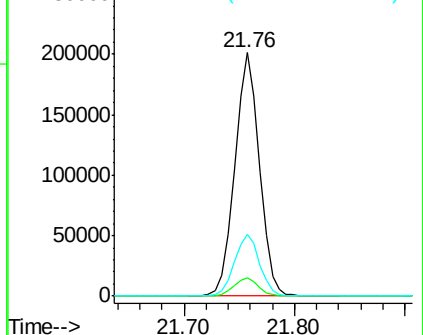

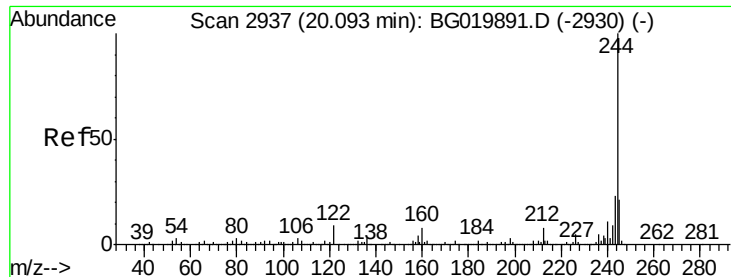

#78

Terphenyl-d14

Concen: 69.94 ng

RT: 20.09 min Scan# 2936

Delta R.T. -0.02 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18

Instrument :

BNA_G

ClientSampleId :

PB87030BL


Tot Ion:244 Resp: 900400

Ion Ratio Lower Upper

244 100

212 8.7 6.9 10.3




122 8.6 10.2 15.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

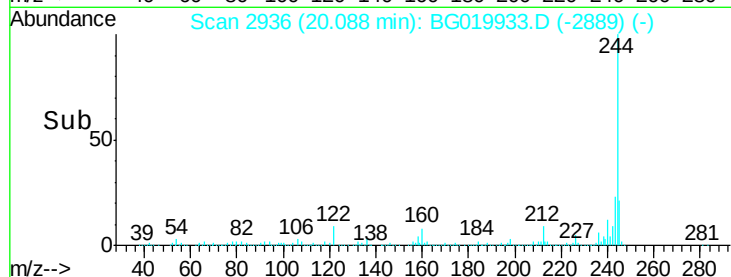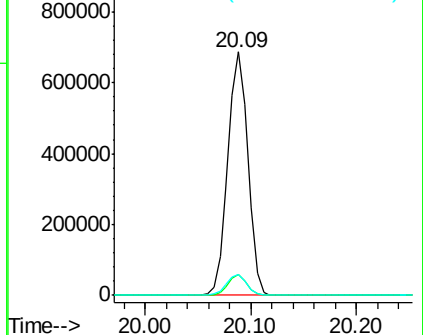

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.04 min Scan# 3779

Delta R.T. -0.05 min

Lab File: BG019933.D

Acq: 5 Dec 2015 9:18


Tgt Ion:264 Resp: 288428

Ion Ratio Lower Upper

264 100

260 24.0 18.5 27.7

265 22.2 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

