
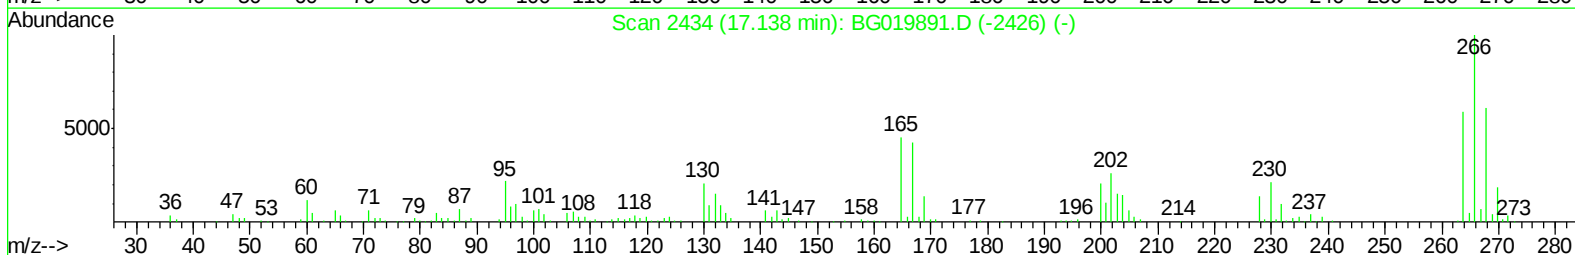
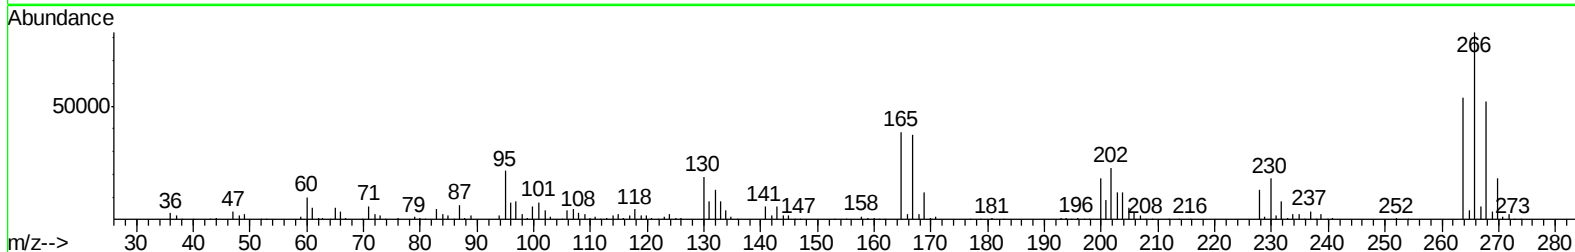


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120415\
Data File : BG019906.D
Acq On : 4 Dec 2015 15:48
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

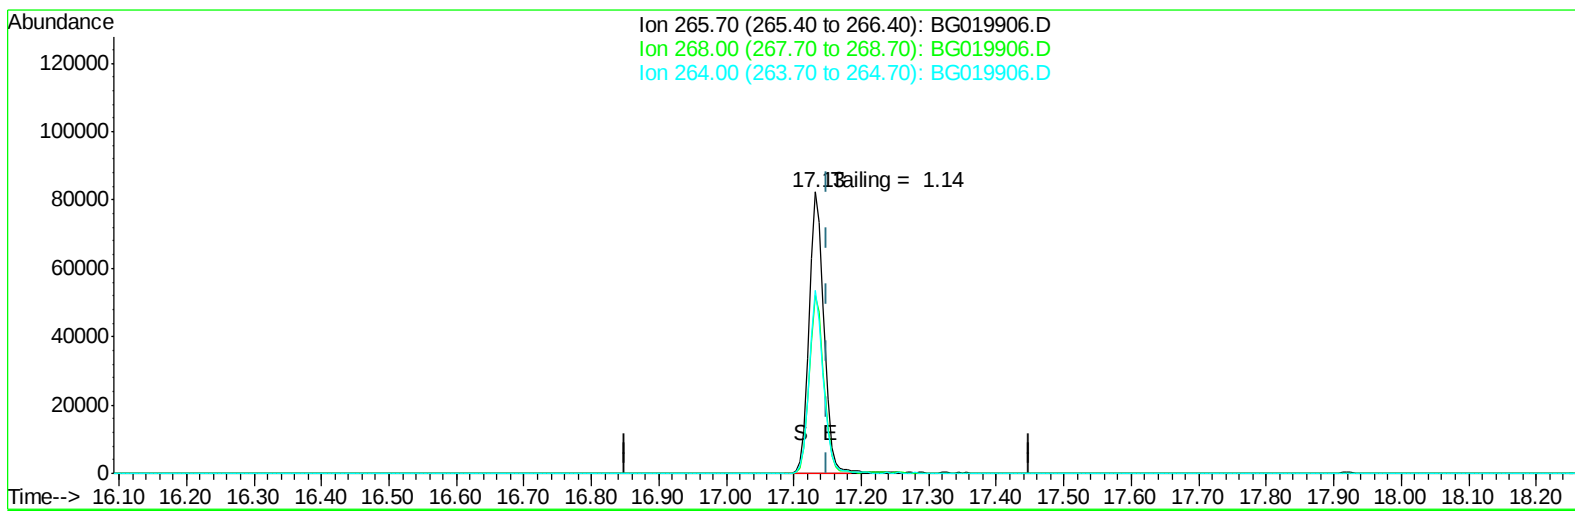

TIC: BG019906.D

(69) Pentachlorophenol (C)




17.132min (-0.018) 0.00ng

response 126580

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	63.36
264.00	60.10	65.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120415\
Data File : BG019906.D
Acq On : 4 Dec 2015 15:48
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

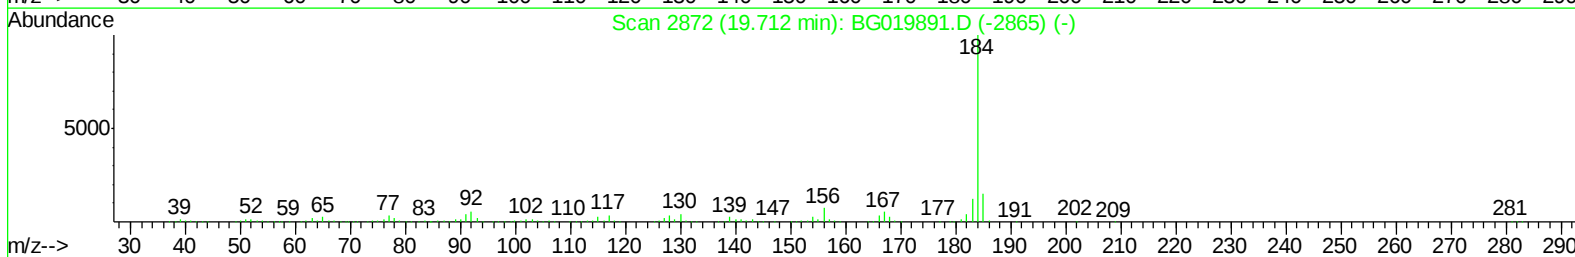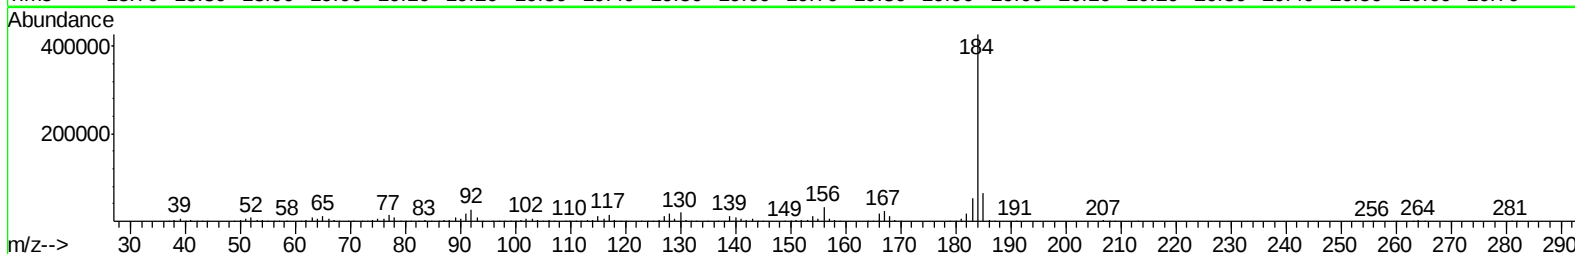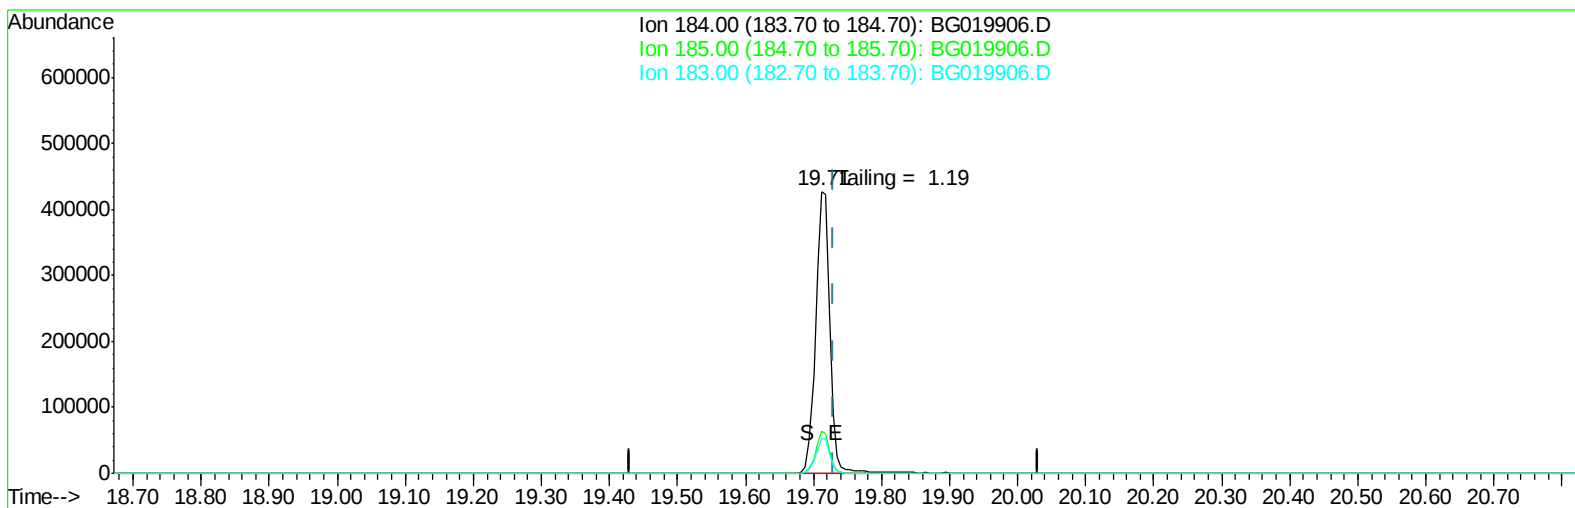

TIC: BG019906.D

(76) Benzidine

19.712min (-0.018) 128775.70ng

response 630268

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.05
183.00	12.60	12.35
0.00	0.00	0.00