
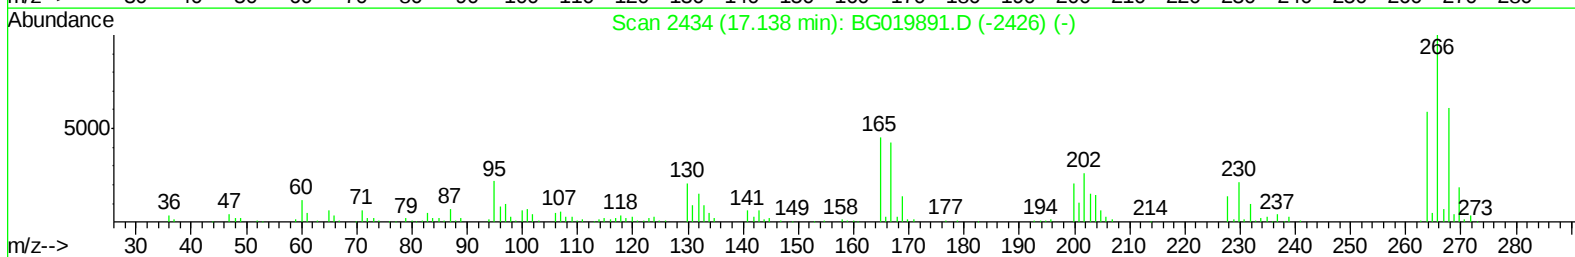
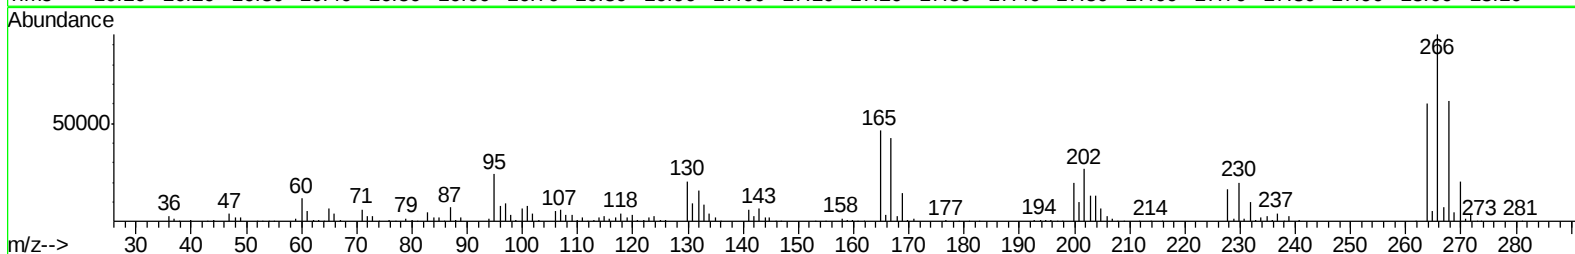


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120415\
Data File : BG019923.D
Acq On : 5 Dec 2015 2:52
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:39:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

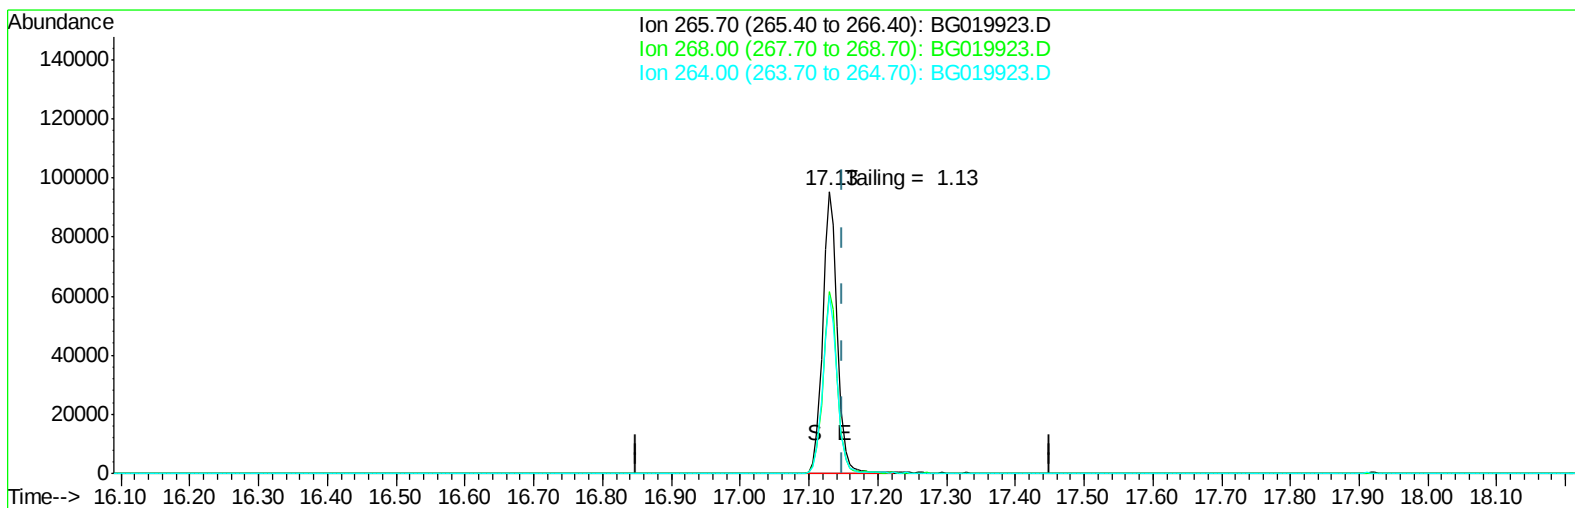

TIC: BG019923.D

(69) Pentachlorophenol (C)




17.129min (-0.021) 0.00ng

response 141228

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	64.77
264.00	60.10	63.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120415\
Data File : BG019923.D
Acq On : 5 Dec 2015 2:52
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:39:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

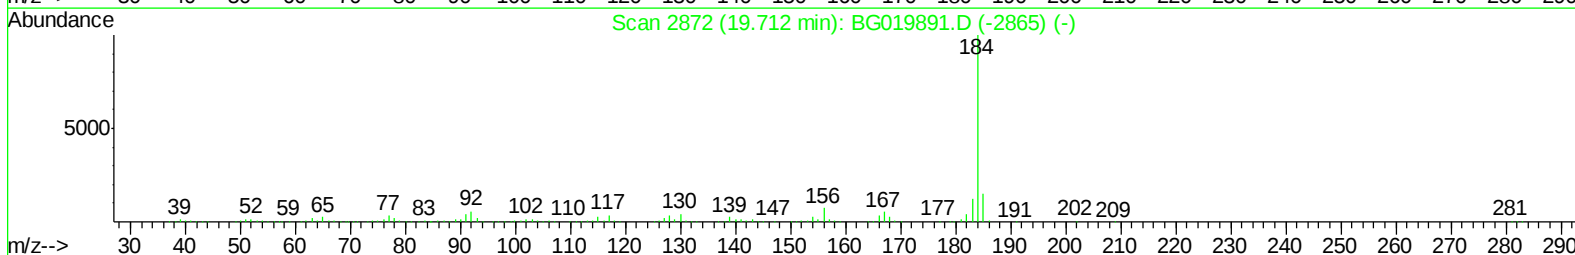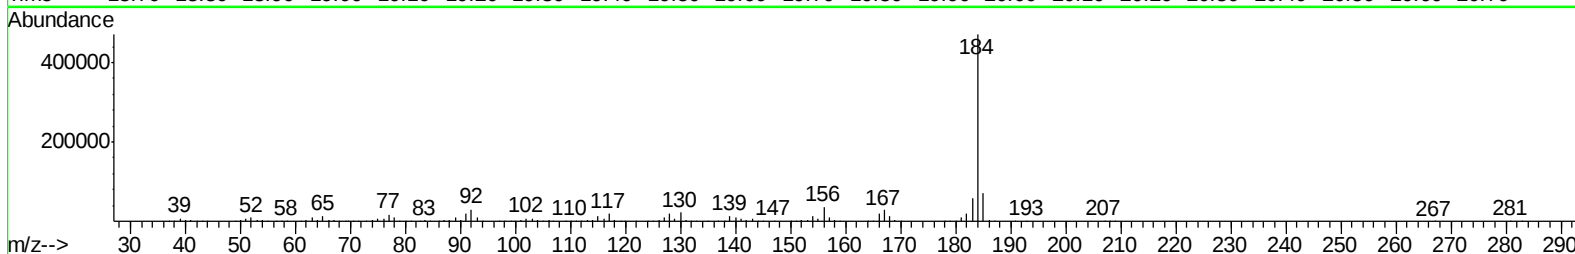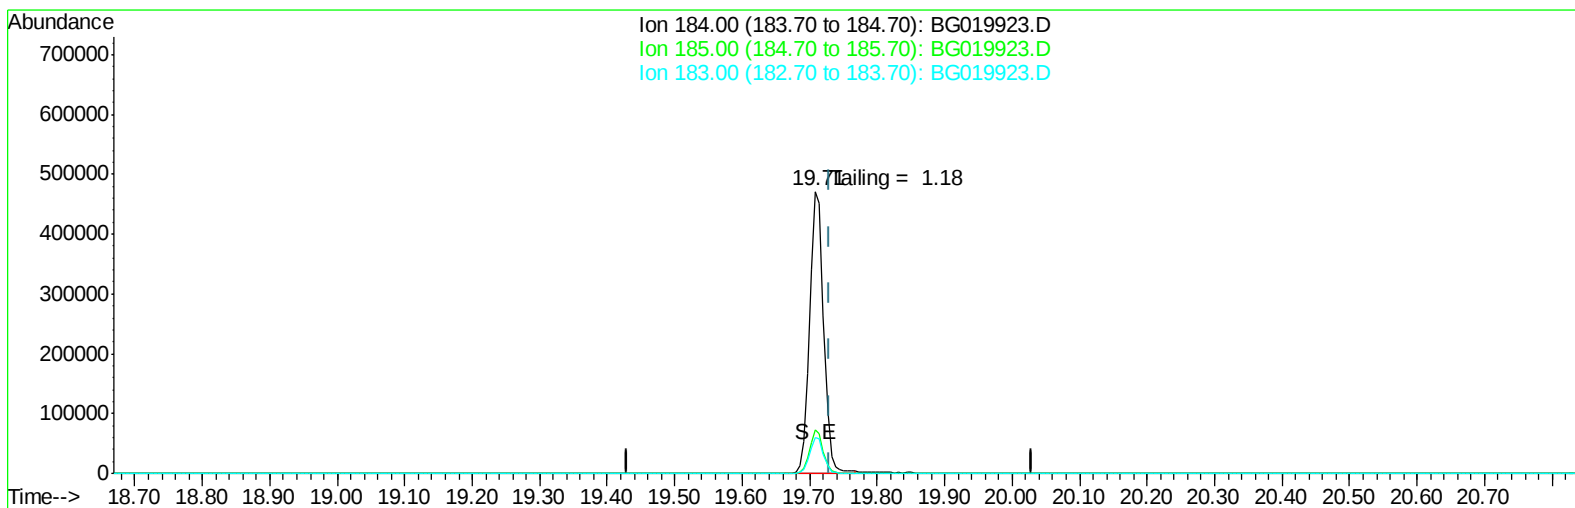

TIC: BG019923.D

(76) Benzidine

19.709min (-0.021) 0.00ng

response 686815

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.34
183.00	12.60	12.65
0.00	0.00	0.00