

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120417\
 Data File : BG031351.D
 Acq On : 4 Dec 2017 18:01
 Operator : SJ/JU
 Sample : PB104670BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB104670BL

Quant Time: Dec 05 04:16:31 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	65621	20.00	ng	-0.02
21) Naphthalene-d8	10.94	136	276671	20.00	ng	-0.02
38) Acenaphthene-d10	14.75	164	174529	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	474679	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	570709	20.00	ng	-0.02
86) Perylene-d12	25.06	264	546887	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	601071	157.07	ng	-0.02
7) Phenol-d6	7.30	99	749192	145.32	ng	0.00
23) Nitrobenzene-d5	9.29	82	428659	91.81	ng	-0.03
41) 2,4,6-Tribromophenol	16.24	330	355580	125.94	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	1237520	101.88	ng	-0.03
78) Terphenyl-d14	20.08	244	2333694	90.29	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120417\
Data File : BG031351.D
Acq On : 4 Dec 2017 18:01
Operator : SJ/JU
Sample : PB104670BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB104670BL

Quant Time: Dec 05 04:16:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

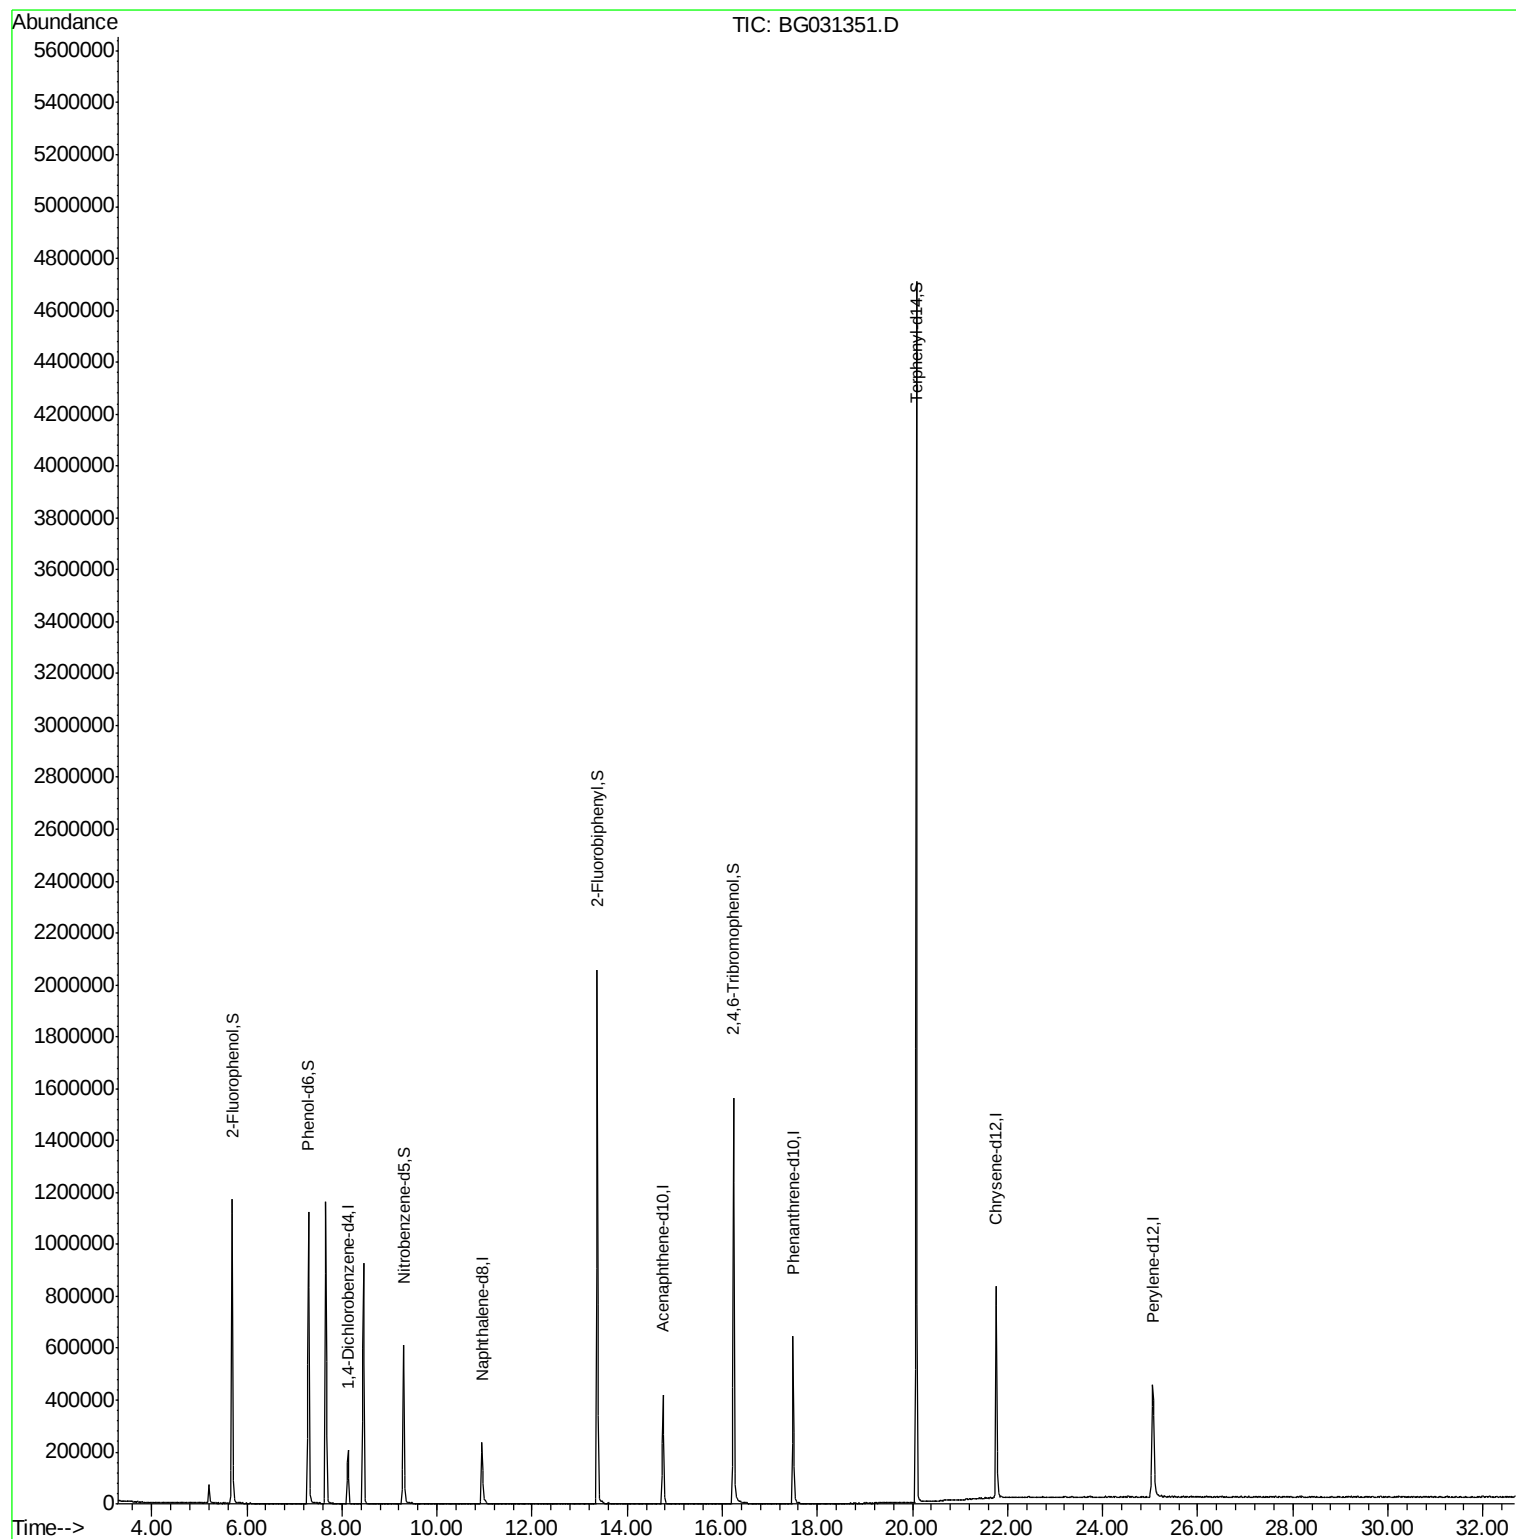




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.13 min Scan# 824
Delta R.T. -0.02 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01

Instrument :
BNA_G
ClientSampleId :
PB104670BL

Tot Ion:152 Resp: 65621
Ion Ratio Lower Upper
152 100
150 162.6 126.6 189.8
115 55.3 53.0 79.4

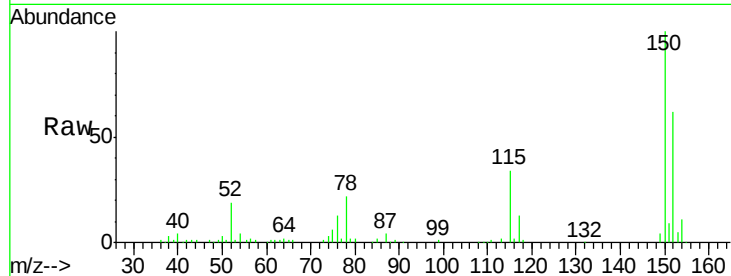


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

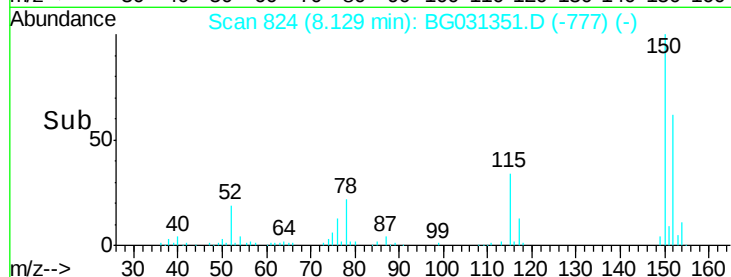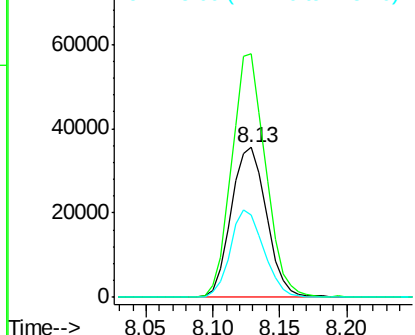



#5


2-Fluorophenol
Concen: 157.07 ng
RT: 5.69 min Scan# 409
Delta R.T. -0.02 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01

Tgt Ion:112 Resp: 601071
Ion Ratio Lower Upper
112 100
64 56.2 56.3 84.5#
63 28.0 30.1 45.1#

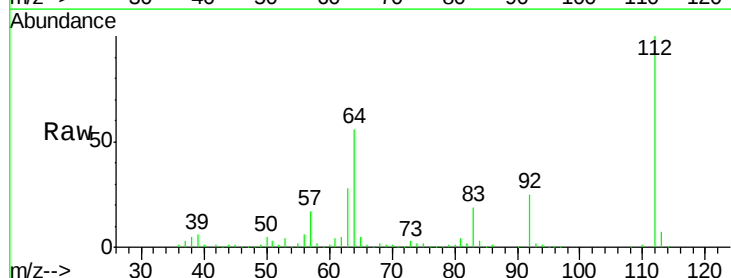

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

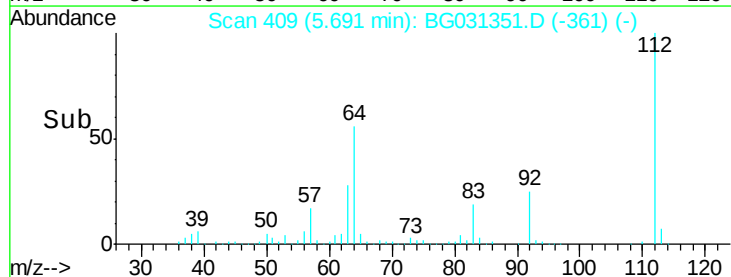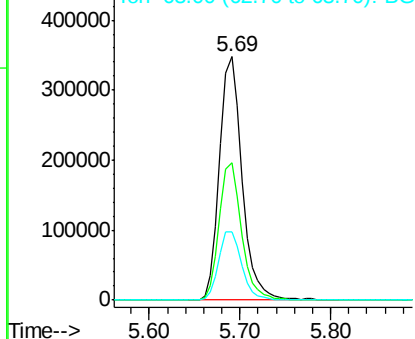

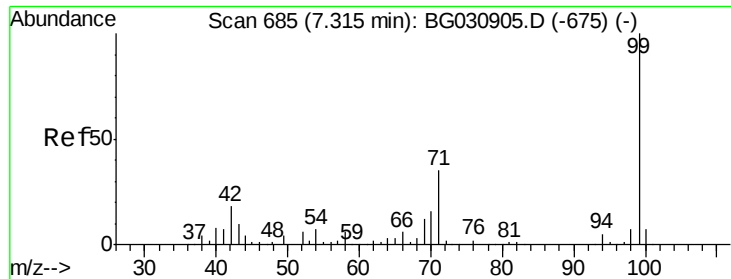

#7

Phenol-d6

Concen: 145.32 ng

RT: 7.30 min Scan# 683

Delta R.T. -0.01 min

Lab File: BG031351.D

Acq: 4 Dec 2017 18:01

Instrument :

BNA_G

ClientSampleId :

PB104670BL


Tot Ion: 99 Resp: 749192

Ion Ratio Lower Upper




99 100

42 16.8 14.1 21.1

71 33.1 26.1 39.1

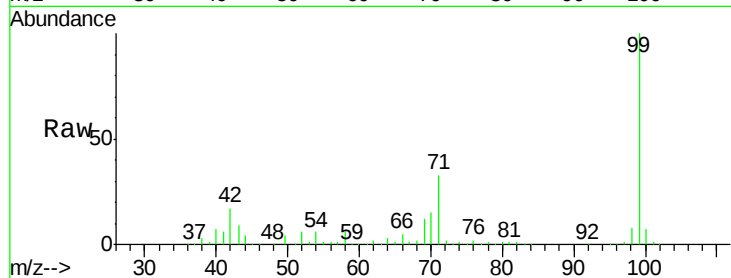

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

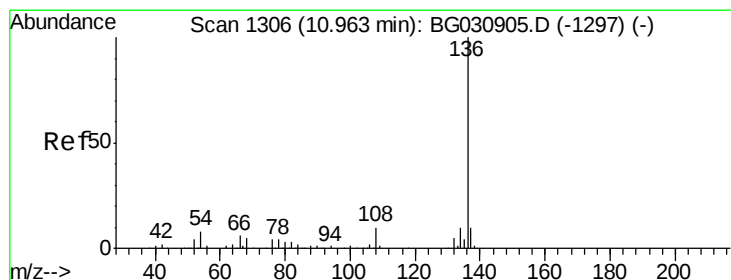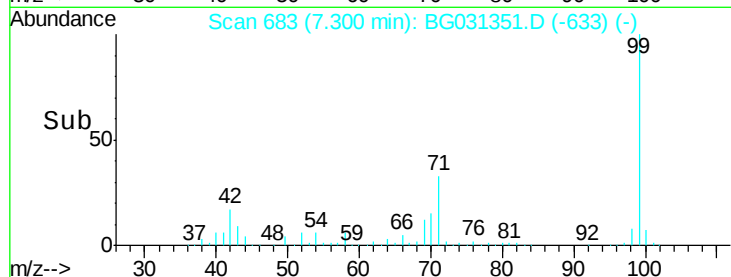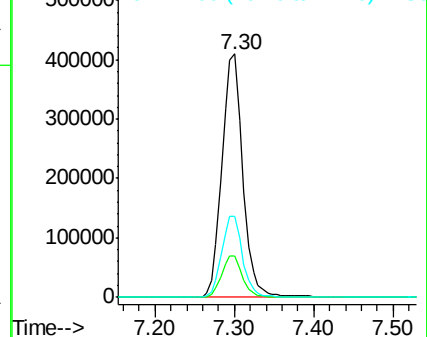

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.94 min Scan# 1303

Delta R.T. -0.02 min

Lab File: BG031351.D

Acq: 4 Dec 2017 18:01

Tgt Ion: 136 Resp: 276671


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 7.3 10.3 15.5#

68 5.3 4.5 6.7

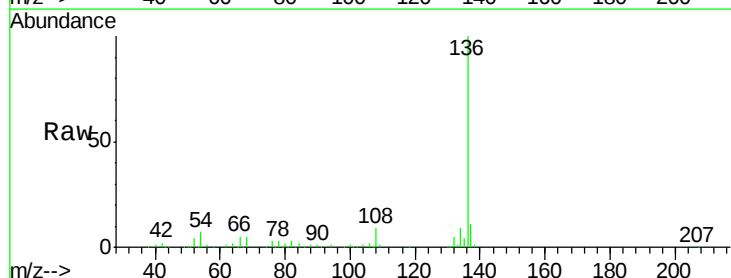

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



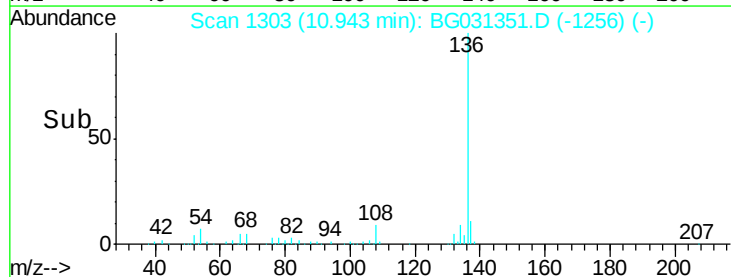
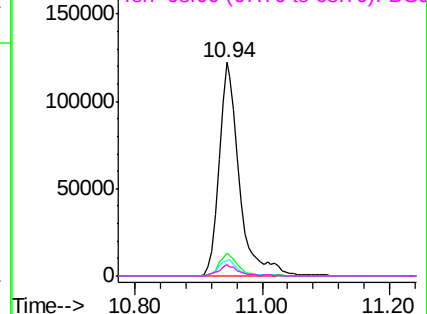


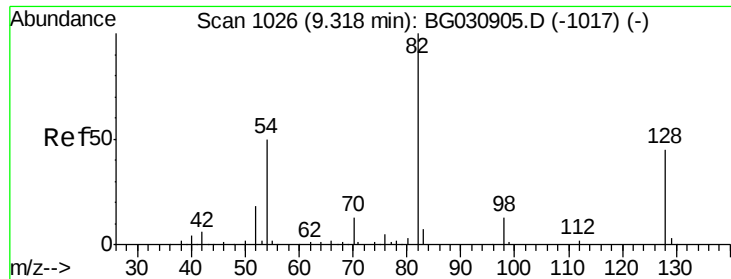

#23
Nitrobenzene-d5
Concen: 91.81 ng
RT: 9.29 min Scan# 1022
Delta R.T. -0.03 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01




Instrument :
BNA_G
ClientSampleId :
PB104670BL


Tot Ion: 82 Resp: 428659
Ion Ratio Lower Upper
82 100
128 45.7 29.7 44.5#
54 48.1 43.1 64.7

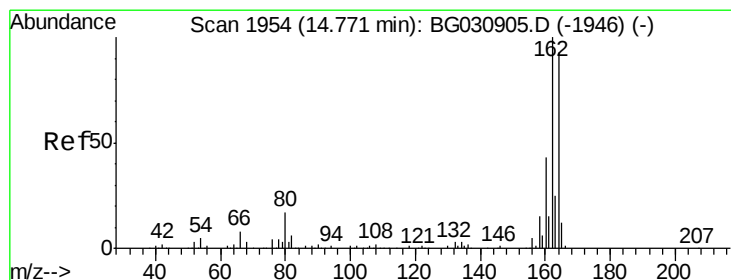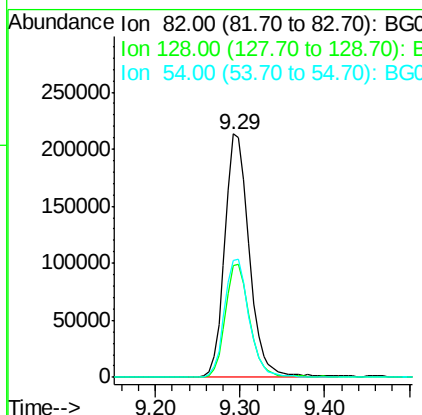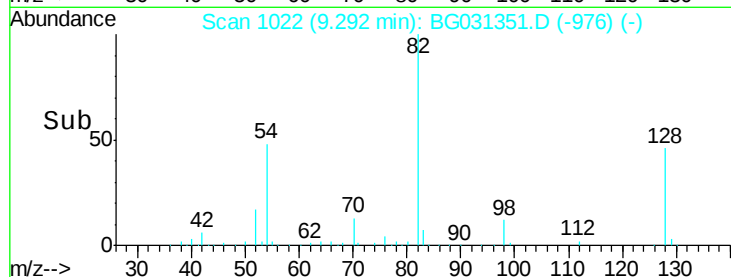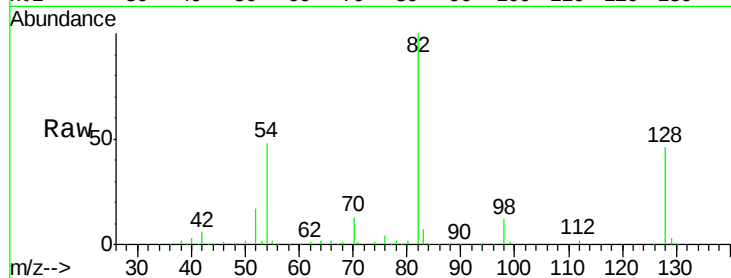

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.02 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01

Tgt Ion:164 Resp: 174529
Ion Ratio Lower Upper
164 100
162 106.0 78.8 118.2
160 46.9 35.4 53.0

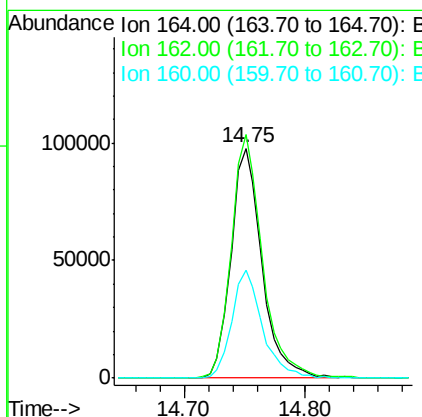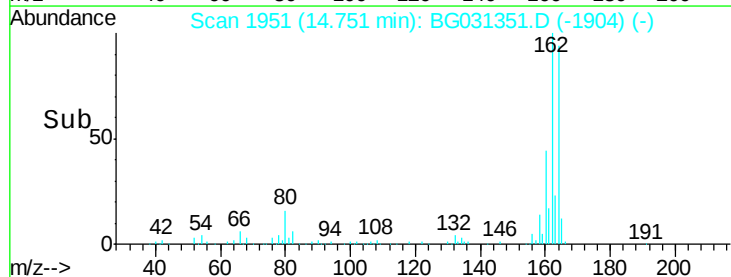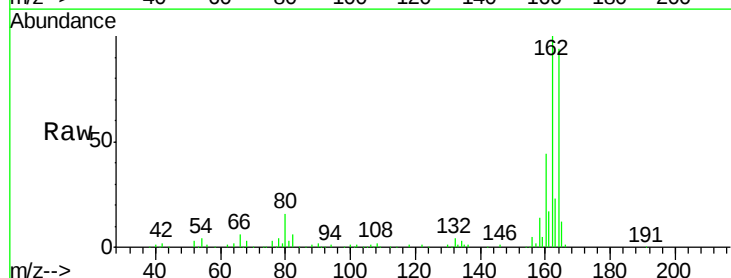


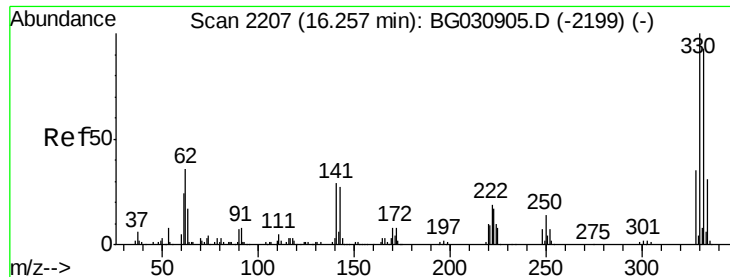




#41
 2,4,6-Tribromophenol
 Concen: 125.94 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.02 min
 Lab File: BG031351.D
 Acq: 4 Dec 2017 18:01

Instrument :
 BNA_G
 ClientSampled :
 PB104670BL

Tot Ion:330 Resp: 355580
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.0 115.6
 141 33.7 25.2 37.8

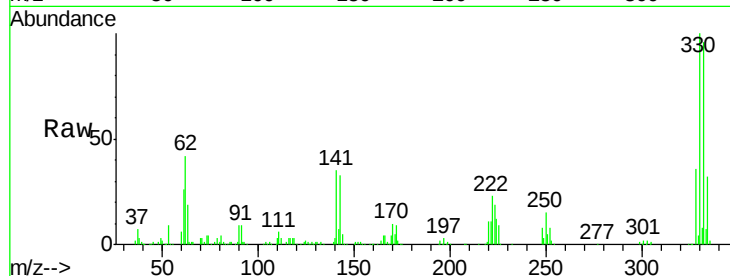


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

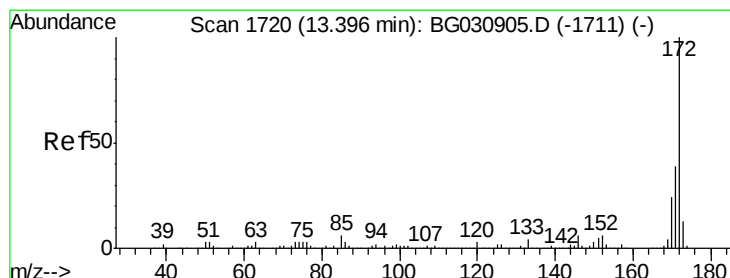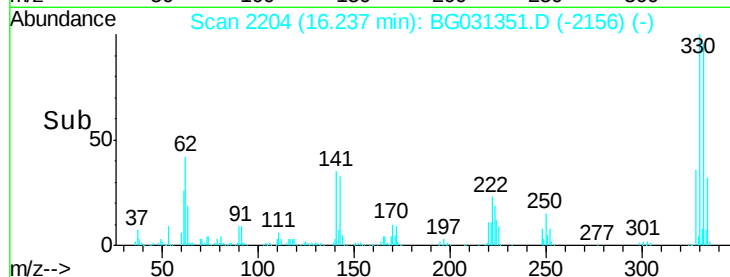
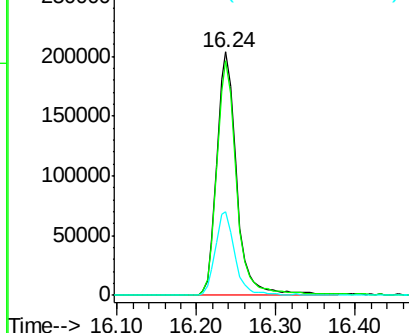


#44
 2-Fluorobiphenyl
 Concen: 101.88 ng
 RT: 13.37 min Scan# 1716
 Delta R.T. -0.03 min
 Lab File: BG031351.D
 Acq: 4 Dec 2017 18:01

Tgt Ion:172 Resp: 1237520
 Ion Ratio Lower Upper
 172 100
 171 37.7 30.0 45.0
 170 24.5 19.5 29.3

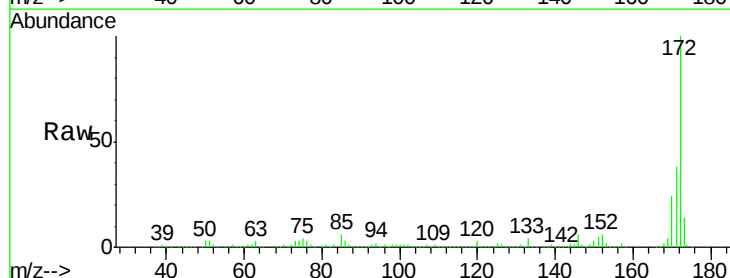

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

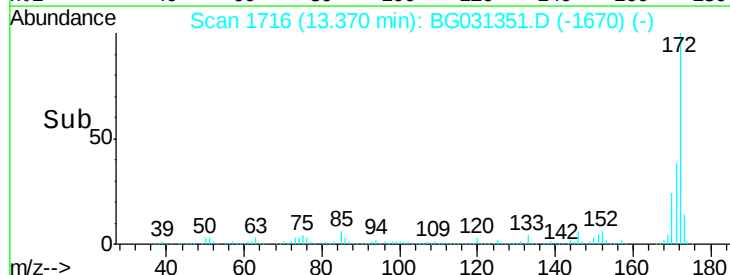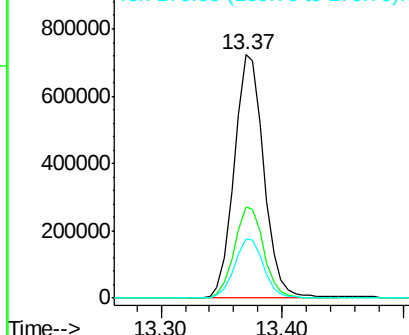







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2417
Delta R.T. -0.02 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01

Instrument :
BNA_G
ClientSampleId :
PB104670BL

Tot Ion:188 Resp: 474679
Ion Ratio Lower Upper
188 100
94 7.5 6.9 10.3
80 8.2 7.7 11.5

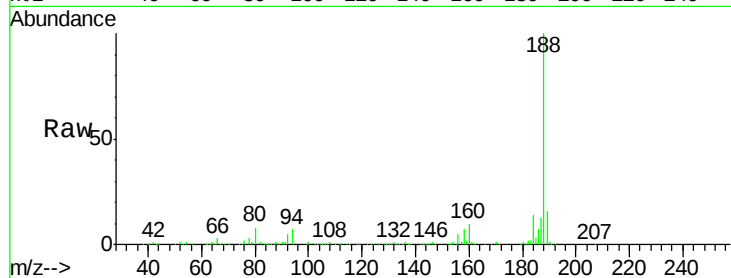


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

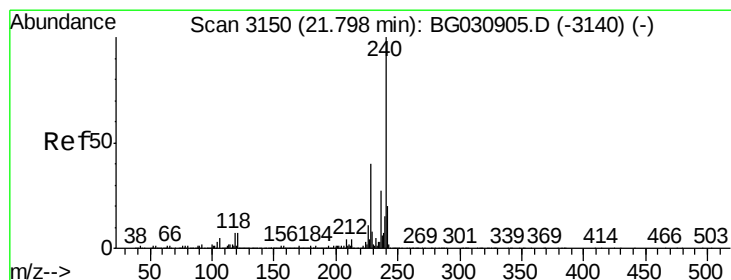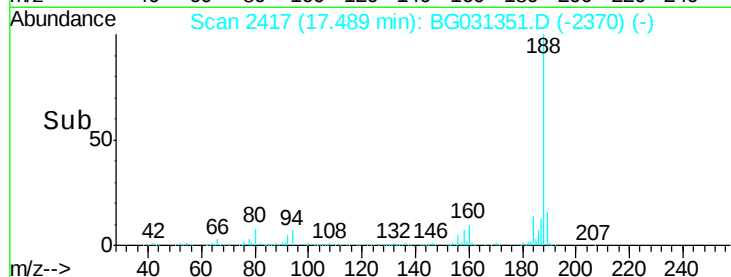
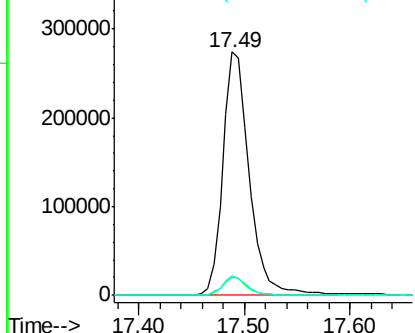


#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.76 min Scan# 3144
Delta R.T. -0.02 min
Lab File: BG031351.D
Acq: 4 Dec 2017 18:01

Tgt Ion:240 Resp: 570709
Ion Ratio Lower Upper
240 100
120 8.1 6.8 10.2
236 25.9 20.9 31.3

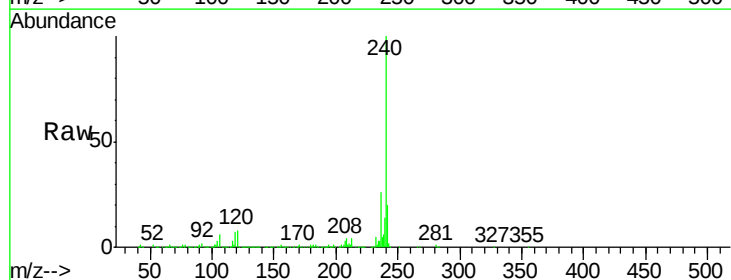

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

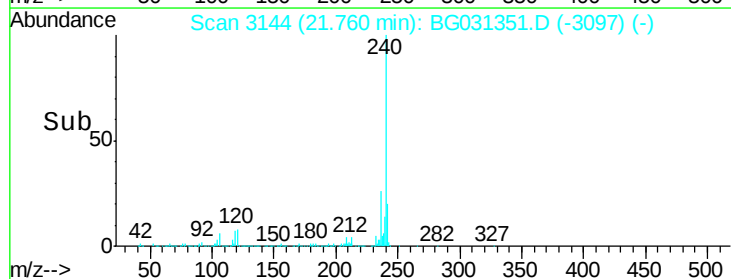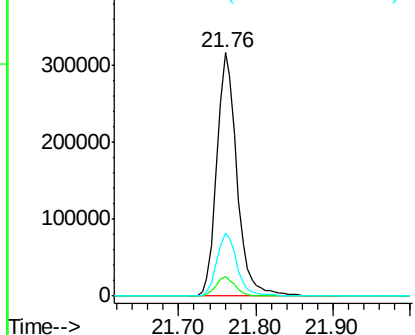



#78

Terphenyl-d14

Concen: 90.29 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.02 min

Lab File: BG031351.D

Acq: 4 Dec 2017 18:01

Instrument :

BNA_G

ClientSampleId :

PB104670BL


Tot Ion:244 Resp: 2333694

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 9.3 7.0 10.4

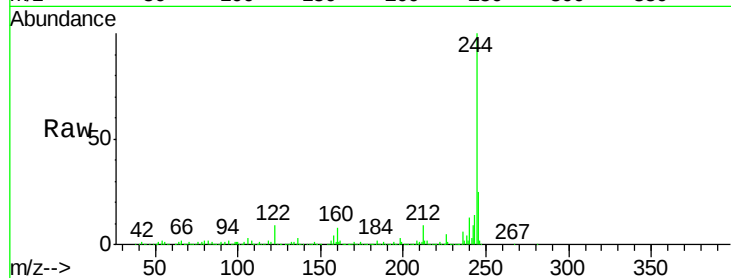

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

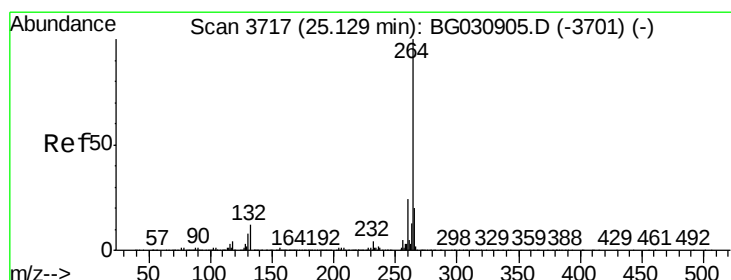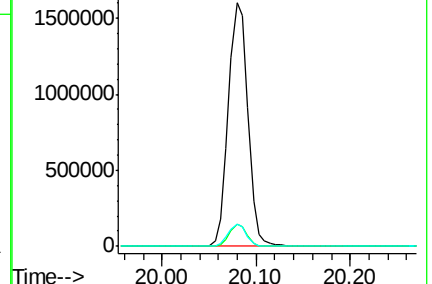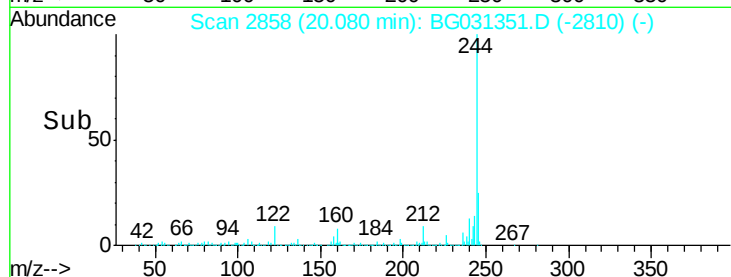

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.06 min Scan# 3705

Delta R.T. -0.04 min

Lab File: BG031351.D

Acq: 4 Dec 2017 18:01


Tgt Ion:264 Resp: 546887

Ion Ratio Lower Upper

264 100

260 25.6 17.4 26.0

265 21.6 17.7 26.5

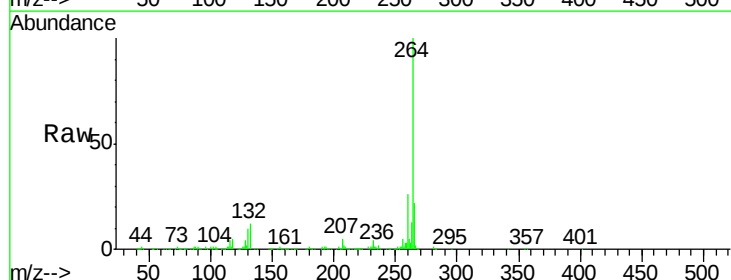

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

